

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 18:25
 Operator : DD\AJ
 Sample : L3993-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 06:31:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	291.7E6	164.3E6	269.087	311.374
Target Compounds							
2) T	3,5-DICHL...	6.499	6.094	9425570	52547090	6.429	64.953 #
3) T	4-Nitroph...	7.108	0.000	9219933	0	17.313	N.D. #
5) T	DICAMBA	7.393	7.046	6032282	9283562	1.434	4.304 #
6) T	MCP	7.626	0.000	9532602	0	2.958	N.D. #
7) T	MCPA	7.686	7.415	338.9E6	1155770	72.524	<MDL #
8) T	DICHLORPROP	0.000	7.736	0	5697140	N.D.	10.069
9) T	2,4-D	8.396	7.940	101.9E6	4648107	89.472	6.390 #
11) T	2,4,5-TP ...	0.000	8.787	0	27579218	N.D.	9.529
12) T	2,4,5-T	9.409	0.000	20632624	0	3.364	N.D. #
14) T	DINOSEB	0.000	10.059	0	9741479	N.D.	4.691
15) T	Picloram	11.001	0.000	11394649	0	1.548	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 18:25
Operator : DD\AJ
Sample : L3993-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 06:31:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

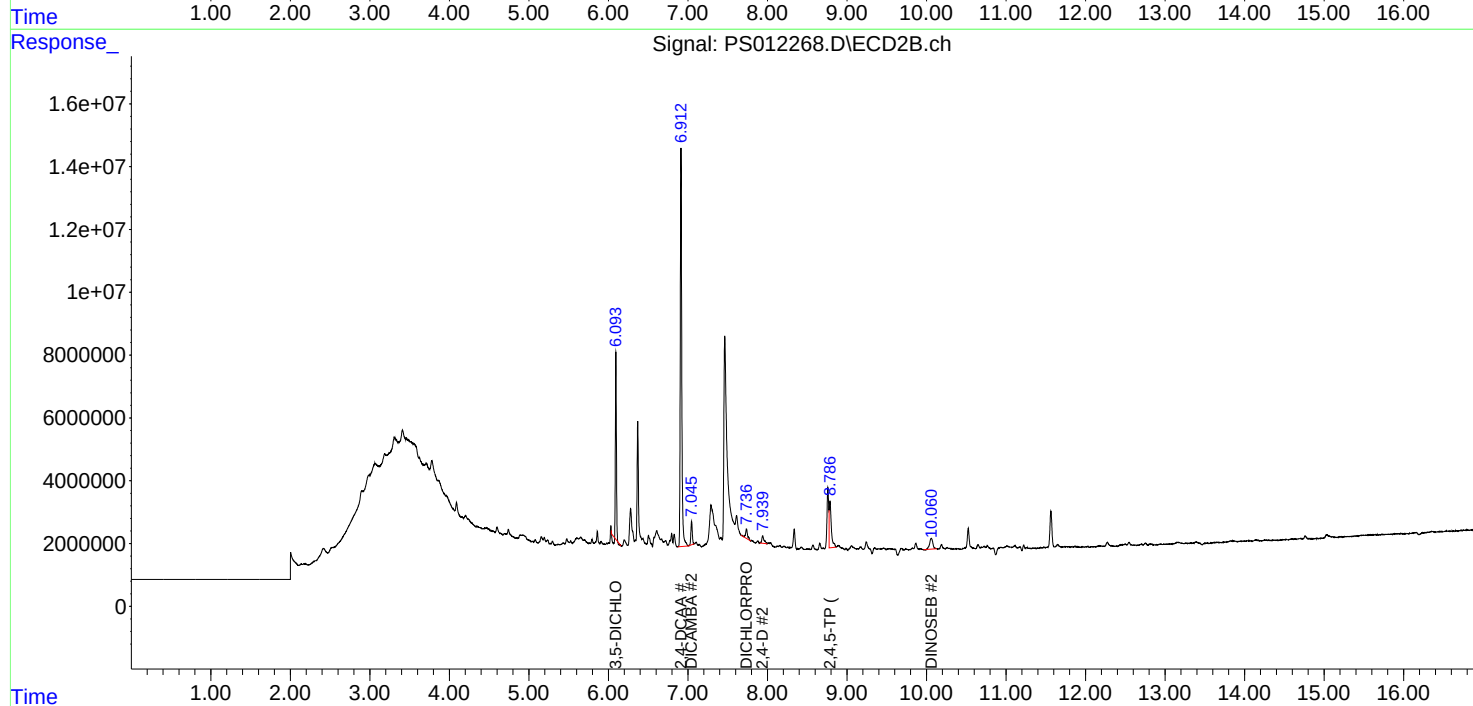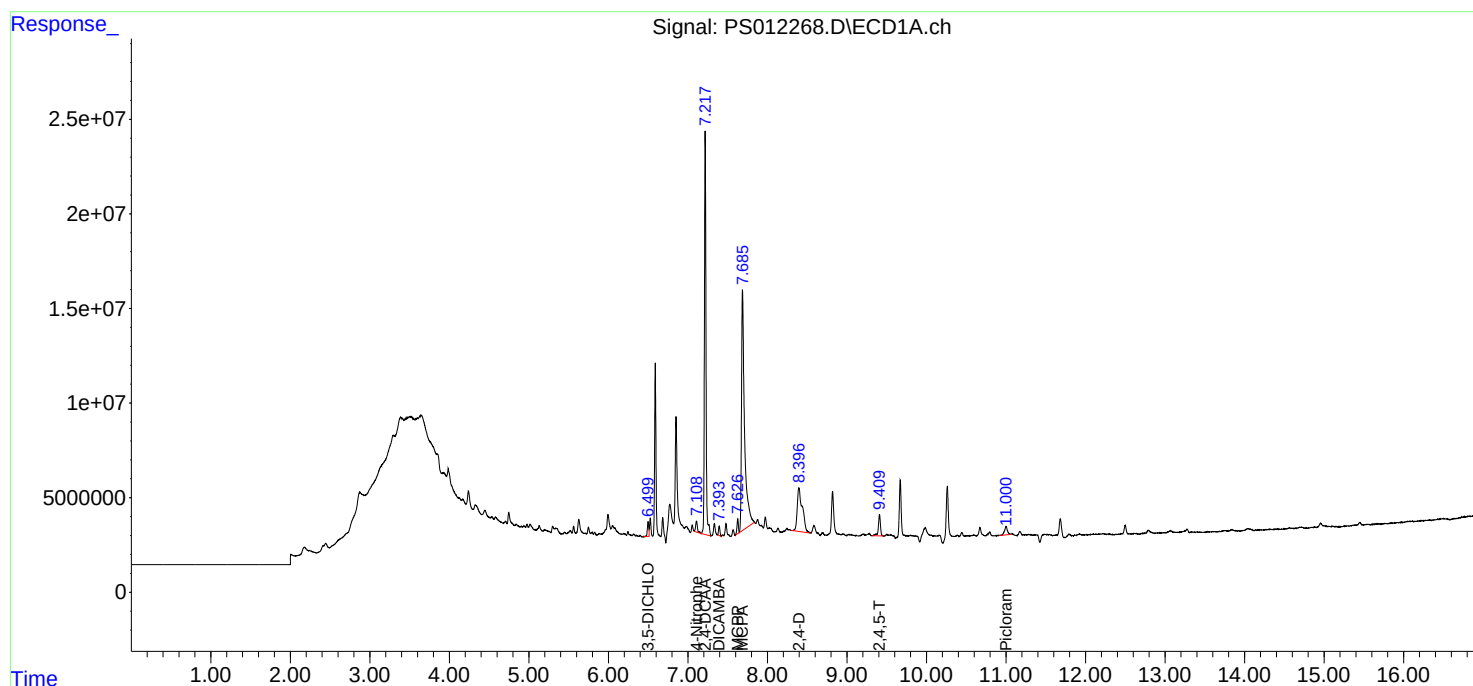


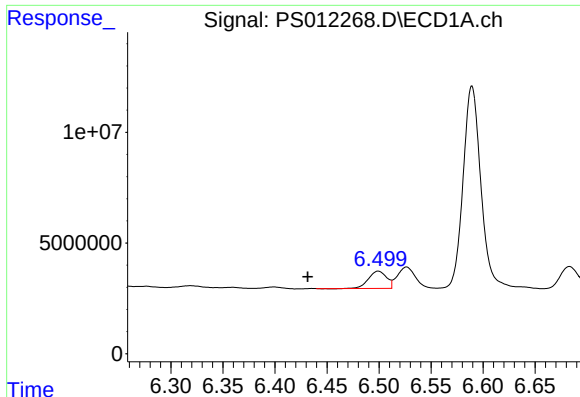

#2 3,5-DICHLORO BENZOIC ACID


R.T.: 6.499 min
Delta R.T.: 0.068 min
Response: 9425570
Conc: 6.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

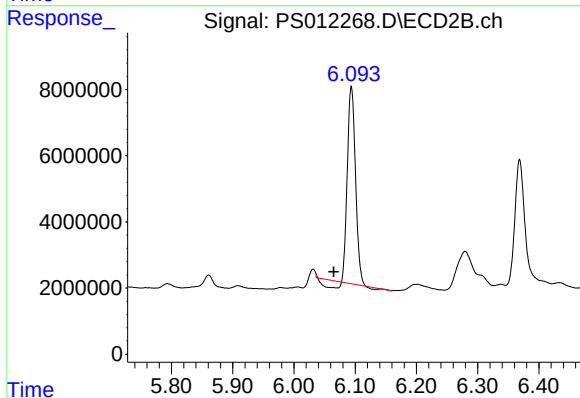


#2 3,5-DICHLORO BENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 52547090
Conc: 64.95 ng/ml

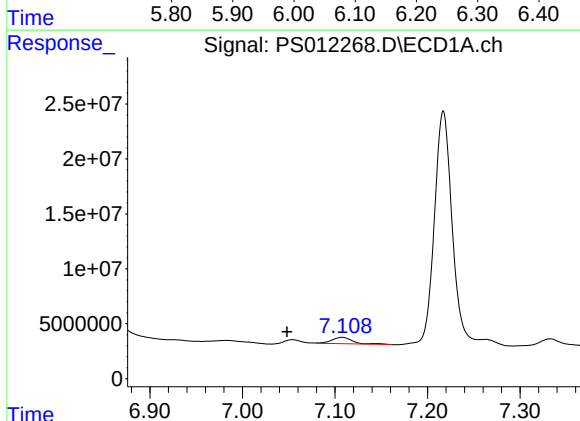


#3 4-Nitrophenol

R.T.: 7.108 min
Delta R.T.: 0.059 min
Response: 9219933
Conc: 17.31 ng/ml

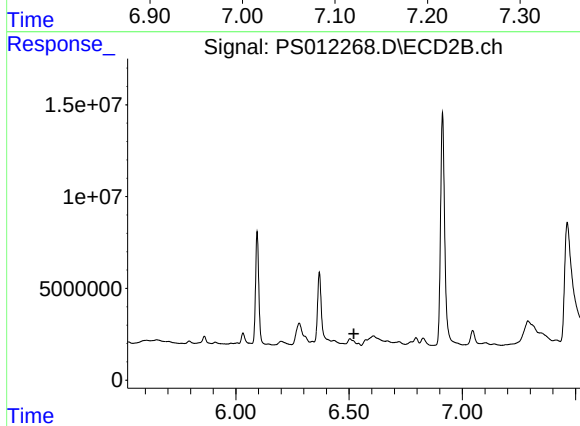

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

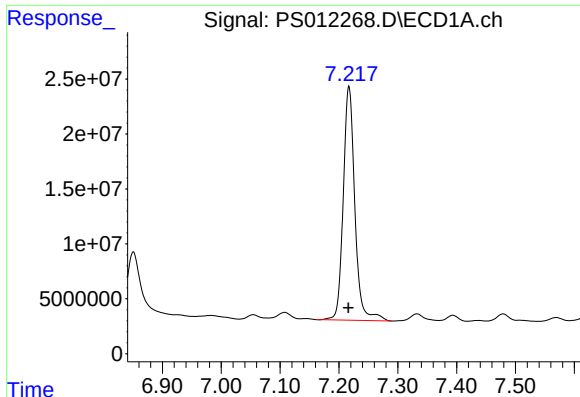

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 291662739
Conc: 269.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

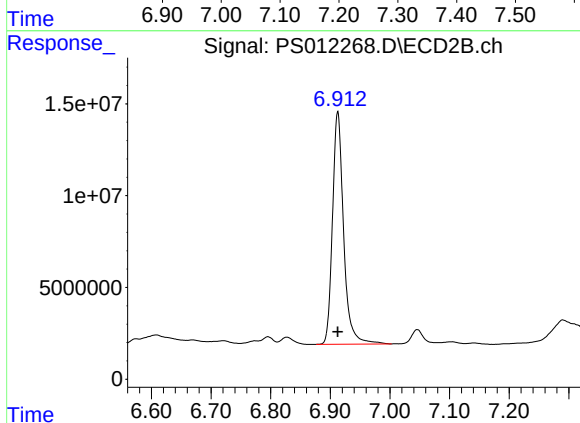


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 164282444
Conc: 311.37 ng/ml

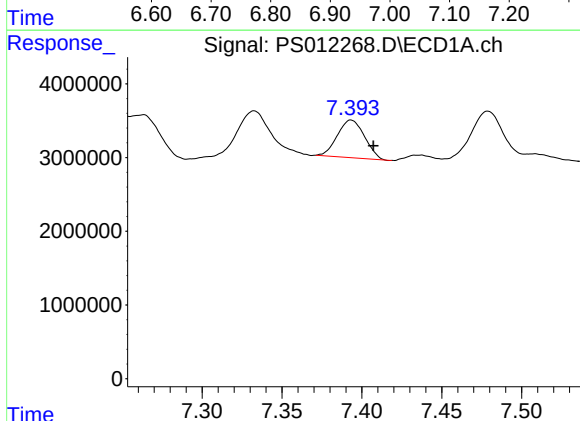


#5 DICAMBA

R.T.: 7.393 min
Delta R.T.: -0.014 min
Response: 6032282
Conc: 1.43 ng/ml

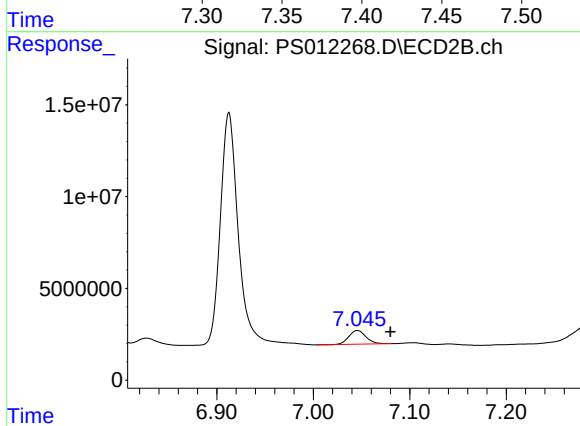

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 9283562
Conc: 4.30 ng/ml

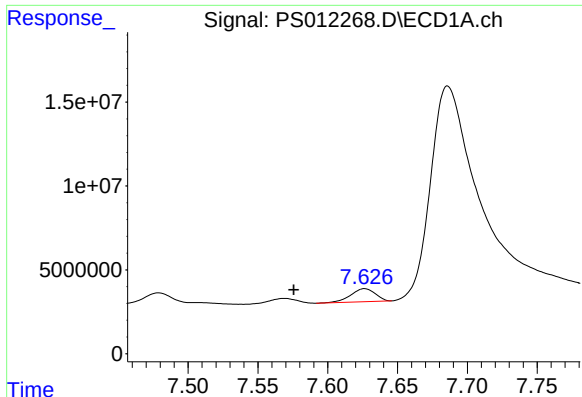

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.051 min
Response: 9532602
Conc: 2.96 ug/ml

Instrument :
ECD_S
ClientSampleId :

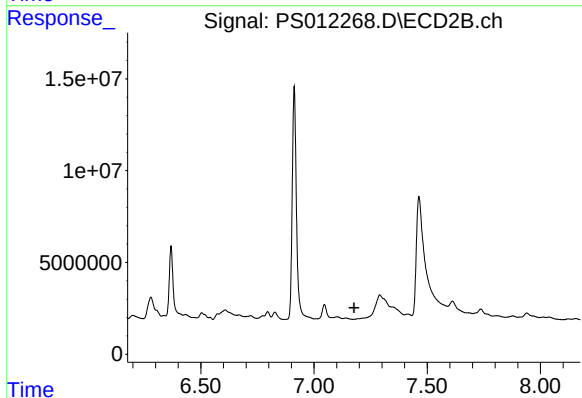


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

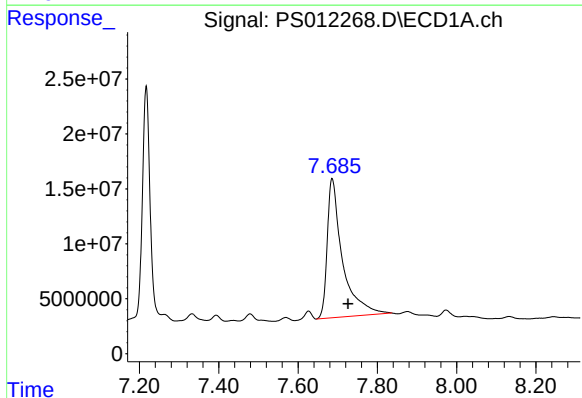


#7 MCPA

R.T.: 7.686 min
Delta R.T.: -0.040 min
Response: 338861084
Conc: 72.52 ug/ml

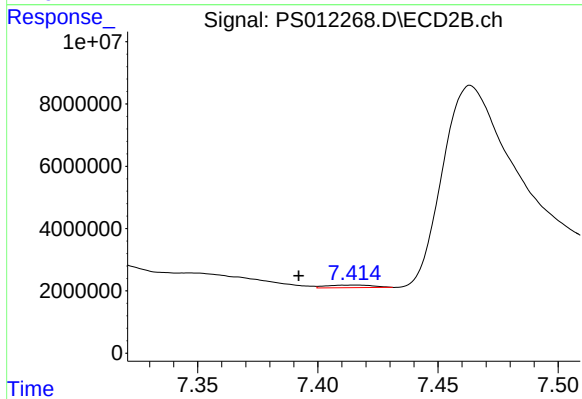

#7 MCPA


R.T.: 7.415 min
Delta R.T.: 0.022 min
Response: 1155770
Conc: N.D.

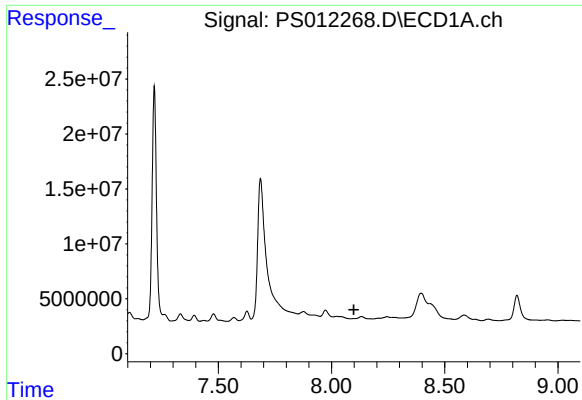

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

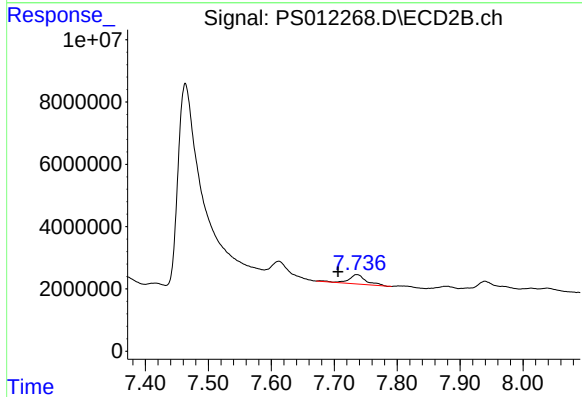


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.030 min
Response: 5697140
Conc: 10.07 ng/ml

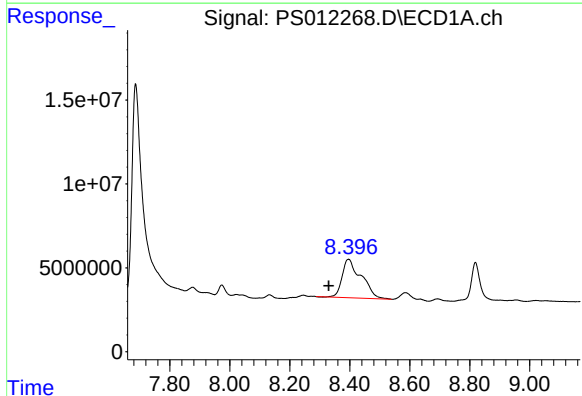


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.066 min
Response: 101904298
Conc: 89.47 ng/ml

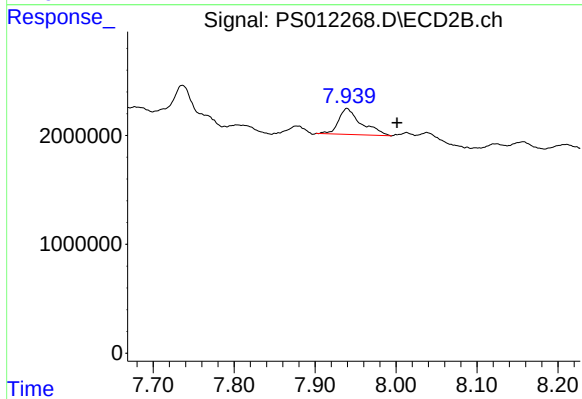

#9 2,4-D


R.T.: 7.940 min
Delta R.T.: -0.062 min
Response: 4648107
Conc: 6.39 ng/ml

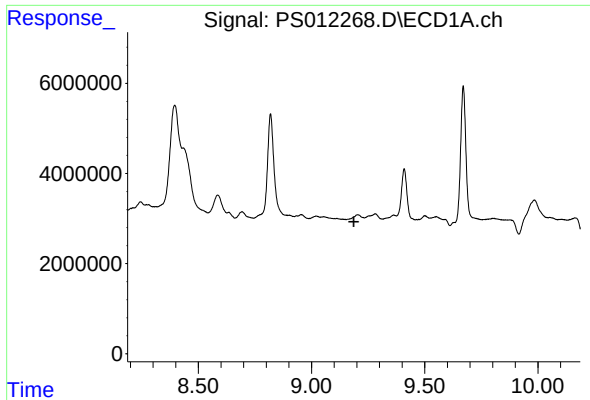

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

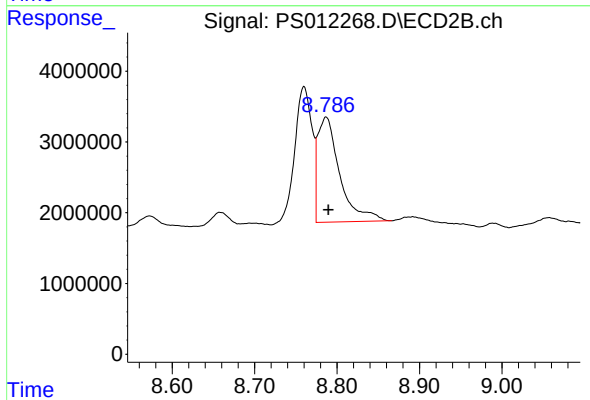


#11 2,4,5-TP (SILVEX)

R.T.: 8.787 min
Delta R.T.: -0.003 min
Response: 27579218
Conc: 9.53 ng/ml

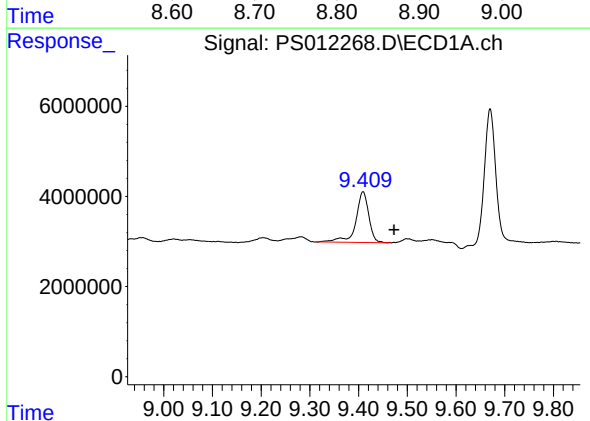


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.064 min
Response: 20632624
Conc: 3.36 ng/ml

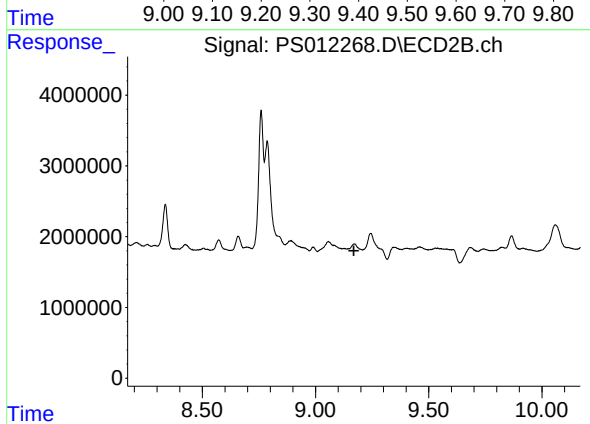

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

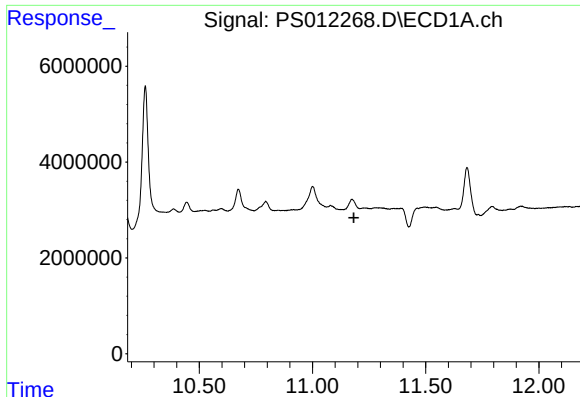

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

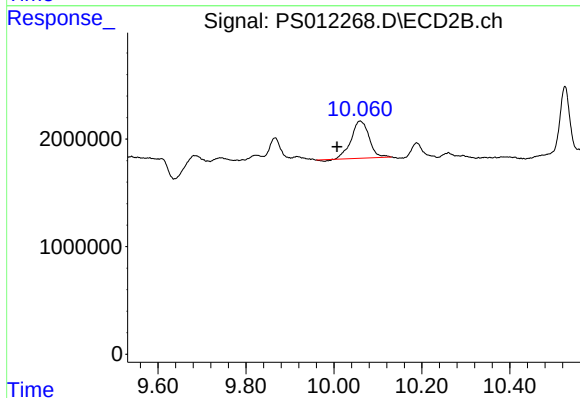


#14 DINOSEB

R.T.: 10.059 min
Delta R.T.: 0.052 min
Response: 9741479
Conc: 4.69 ng/ml

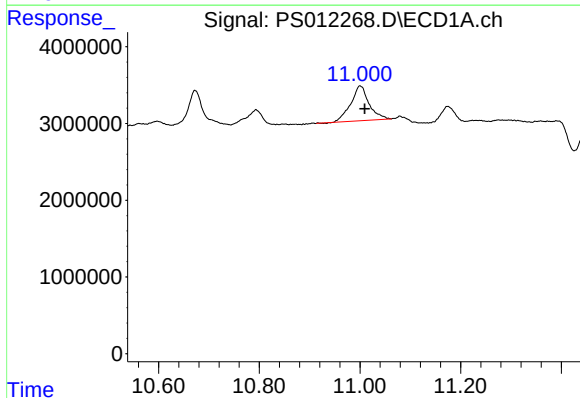

#15 Picloram

R.T.: 11.001 min
Delta R.T.: -0.008 min
Response: 11394649
Conc: 1.55 ng/ml

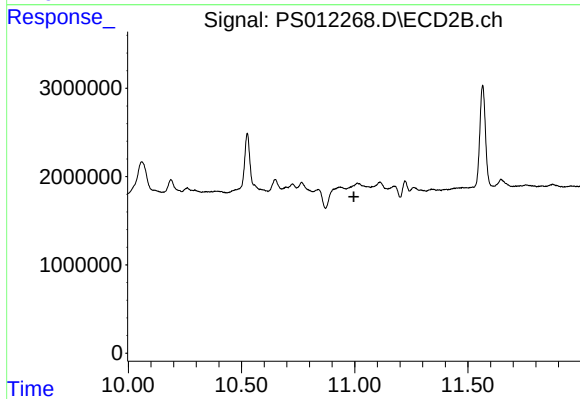

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.996 min
Response: 0
Conc: N.D.