

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 18:48
 Operator : DD\AJ
 Sample : L3993-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 06:32:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	289.3E6	164.4E6	266.885	311.620
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	50166482	N.D.	62.011
3) T	4-Nitroph...	7.107	0.000	7434094	0	13.960	N.D. #
5) T	DICAMBA	7.393	7.046	5976120	9332805	1.420	4.327 #
6) T	MCP	7.626	0.000	9761976	0	3.030	N.D. #
7) T	MCPA	7.687	7.414	323.8E6	1322840	69.300	<MDL #
8) T	DICHLORPROP	0.000	7.737	0	7967719	N.D.	14.082
9) T	2,4-D	8.395	0.000	99368139	0	87.245	N.D. #
11) T	2,4,5-TP ...	0.000	8.760	0	39804540	N.D.	13.753
12) T	2,4,5-T	9.408	0.000	19899817	0	3.245	N.D. #
14) T	DINOSEB	0.000	10.053	0	9259657	N.D.	4.459



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 18:48
Operator : DD\AJ
Sample : L3993-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 06:32:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

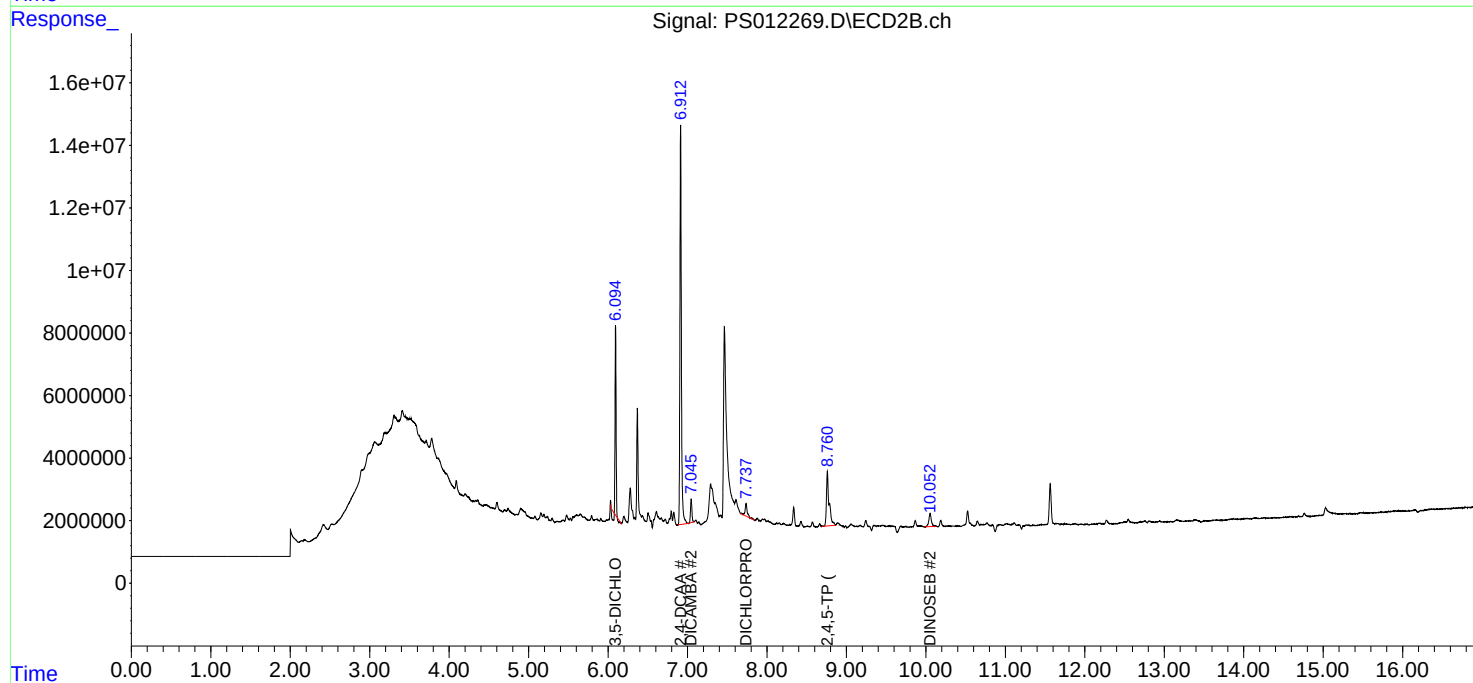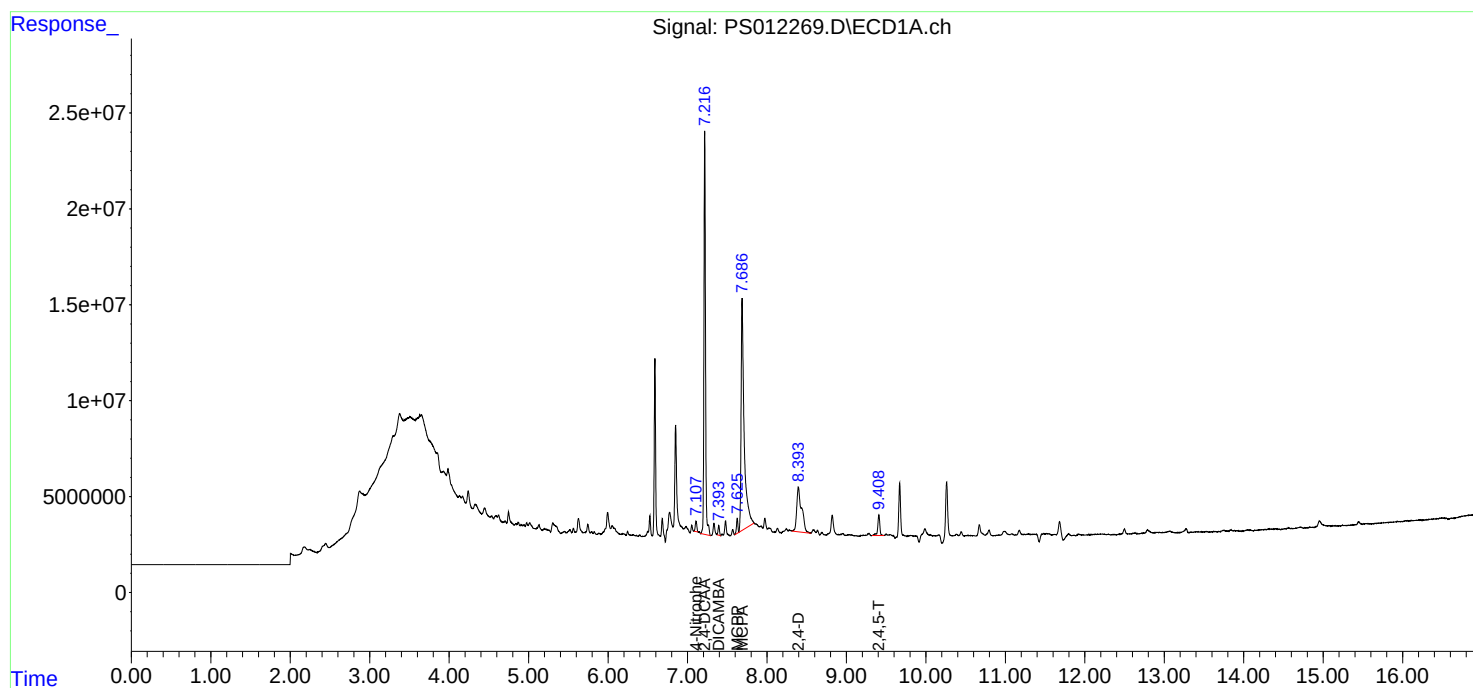


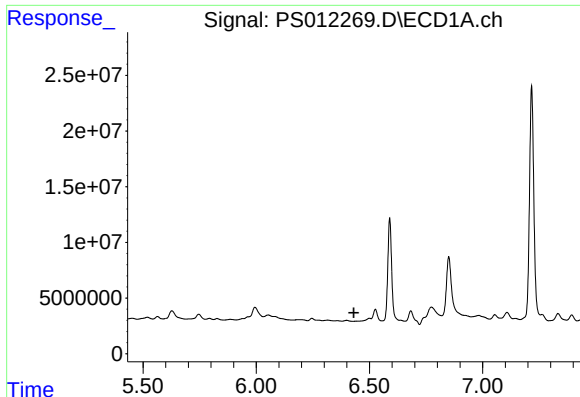

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

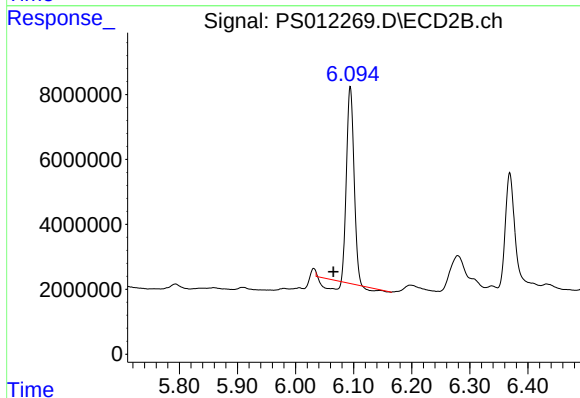


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 50166482
Conc: 62.01 ng/ml

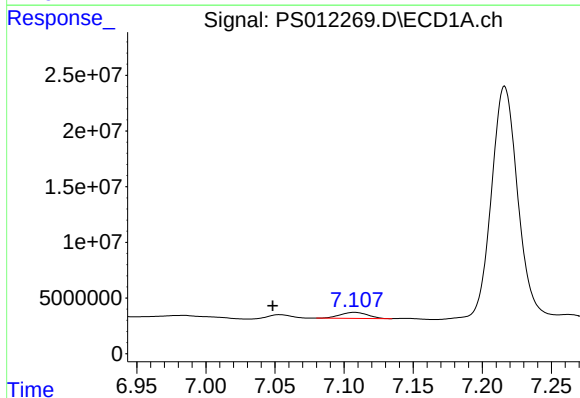


#3 4-Nitrophenol

R.T.: 7.107 min
Delta R.T.: 0.059 min
Response: 7434094
Conc: 13.96 ng/ml

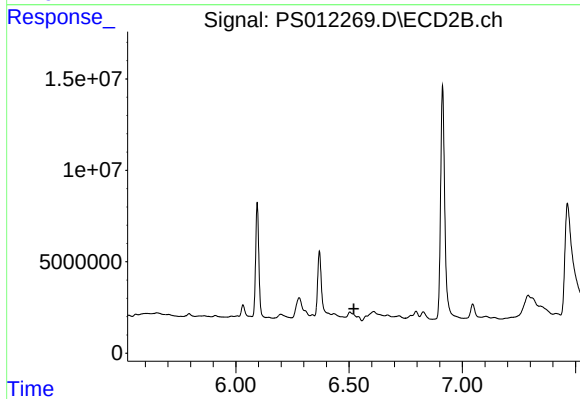

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

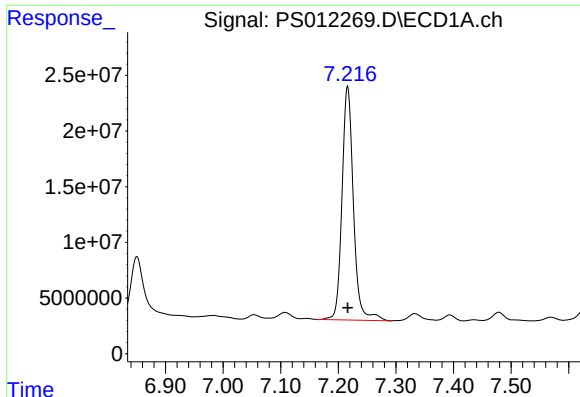

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 289275650
Conc: 266.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

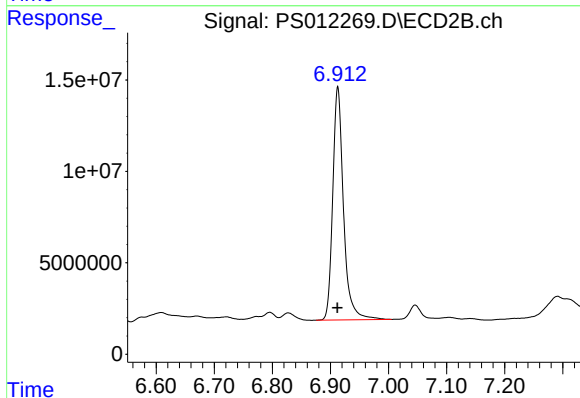


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 164412105
Conc: 311.62 ng/ml

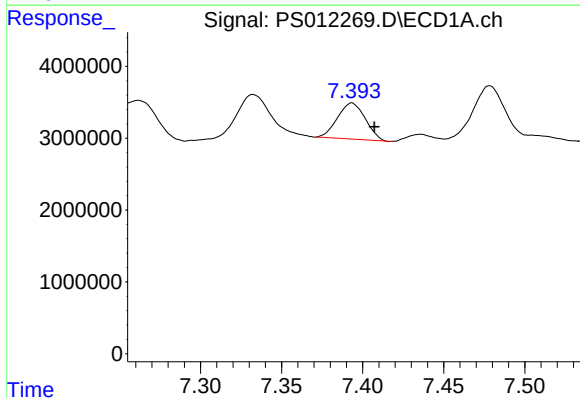


#5 DICAMBA

R.T.: 7.393 min
Delta R.T.: -0.014 min
Response: 5976120
Conc: 1.42 ng/ml

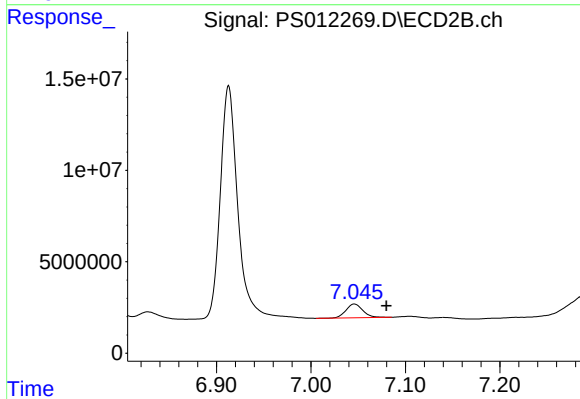

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 9332805
Conc: 4.33 ng/ml

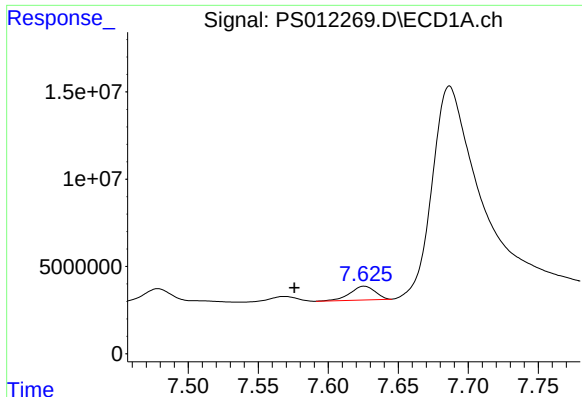

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.050 min
Response: 9761976
Conc: 3.03 ug/ml

Instrument :
ECD_S
ClientSampleId :

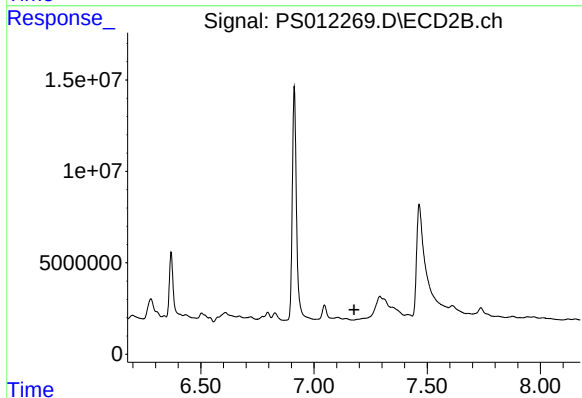


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

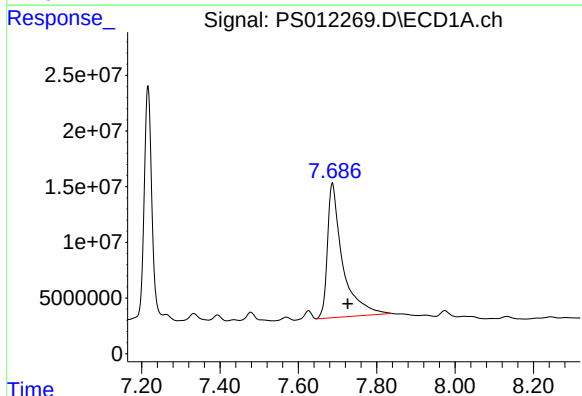


#7 MCPA

R.T.: 7.687 min
Delta R.T.: -0.039 min
Response: 323799720
Conc: 69.30 ug/ml

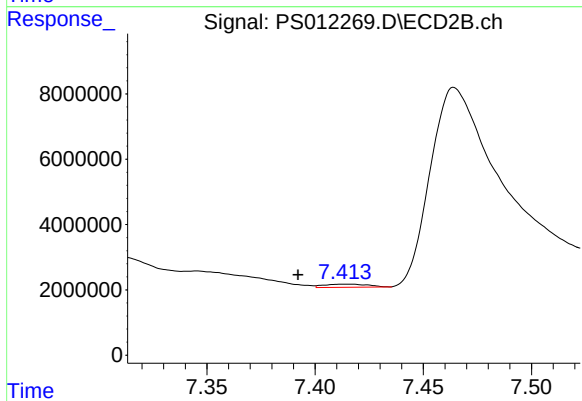

#7 MCPA


R.T.: 7.414 min
Delta R.T.: 0.022 min
Response: 1322840
Conc: N.D.

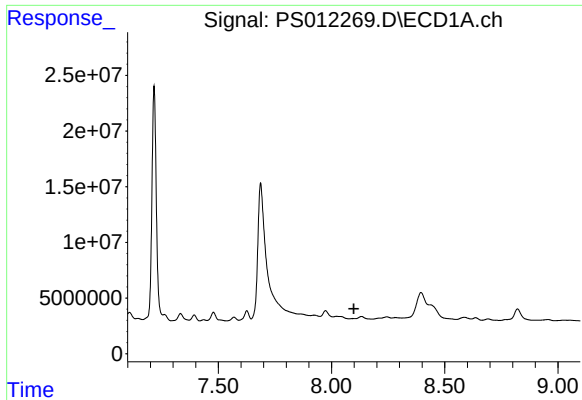

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

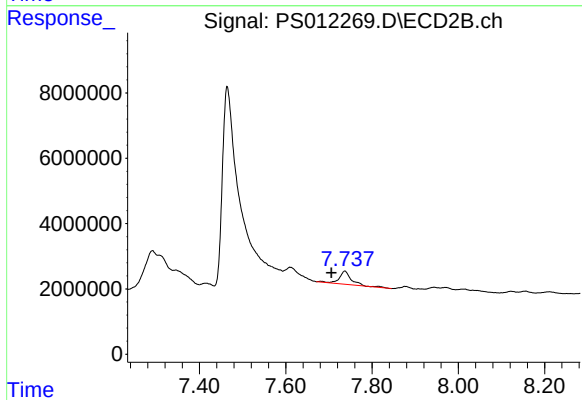


#8 DICHLORPROP

R.T.: 7.737 min
Delta R.T.: 0.031 min
Response: 7967719
Conc: 14.08 ng/ml

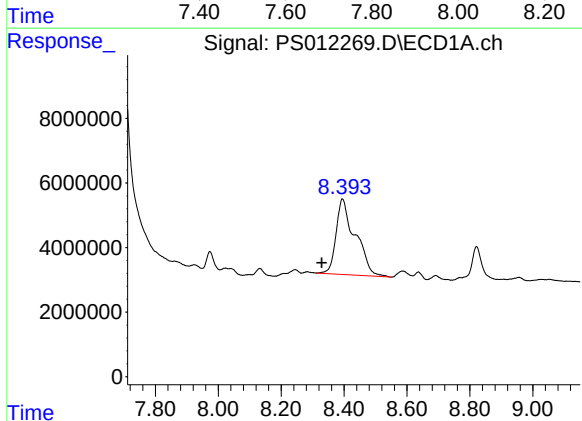


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.066 min
Response: 99368139
Conc: 87.25 ng/ml

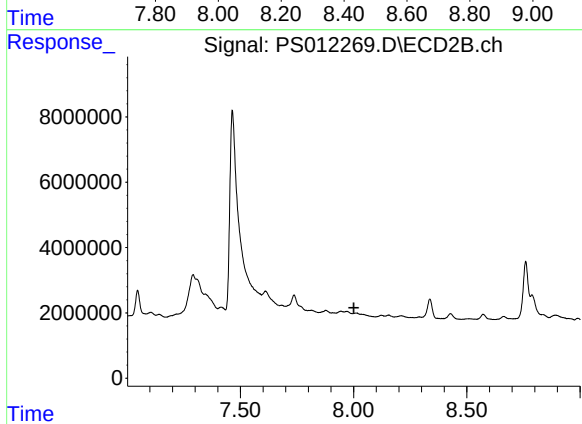

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

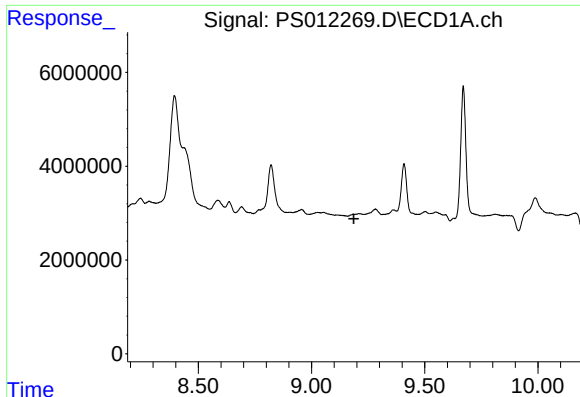

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

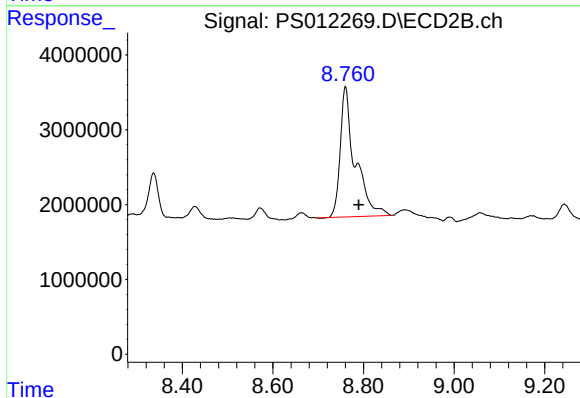


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: -0.029 min
Response: 39804540
Conc: 13.75 ng/ml

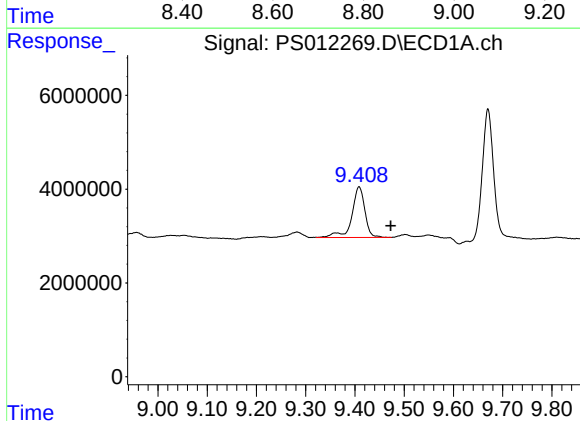


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: -0.064 min
Response: 19899817
Conc: 3.24 ng/ml

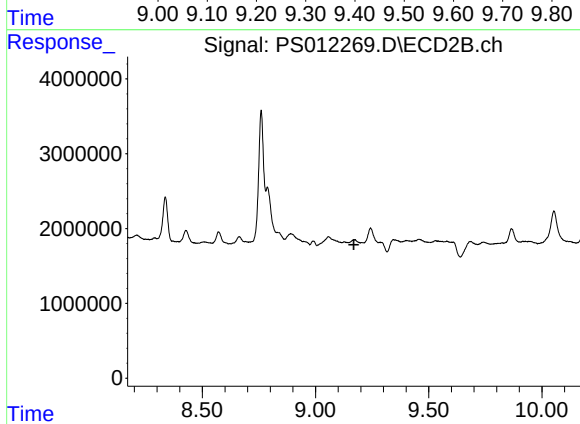

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

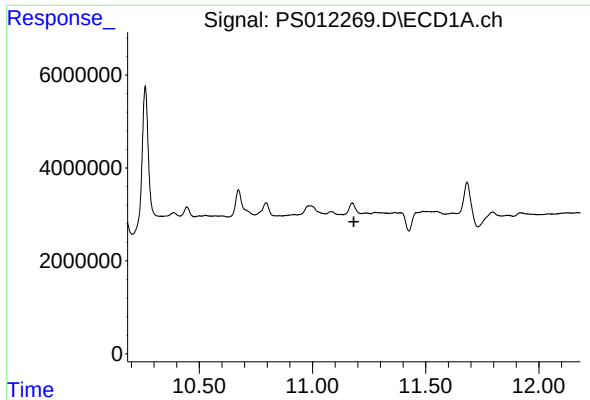

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

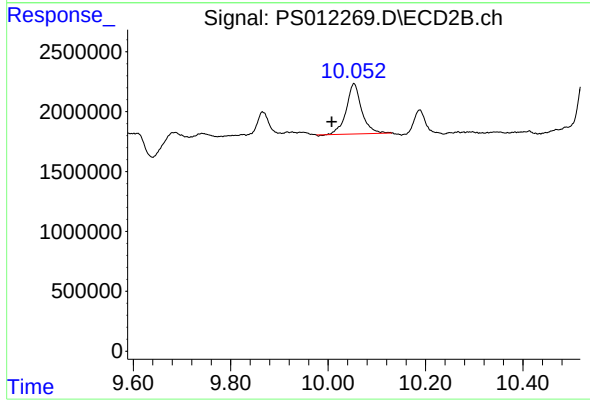

#14 DINOSEB

R.T.: 10.053 min
Delta R.T.: 0.046 min
Response: 9259657
Conc: 4.46 ng/ml