

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 19:11
 Operator : DD\AJ
 Sample : L3993-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 06:32:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	331.5E6	186.7E6	305.864	353.791
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	56065968	N.D.	69.303
3) T	4-Nitroph...	7.107	0.000	7276485	0	13.664	N.D. #
5) T	DICAMBA	7.394	7.046	6858650	10351008	1.630	4.799 #
6) T	MCP	7.626	0.000	11175884	0	3.468	N.D. #
7) T	MCPA	7.690	7.418	266.6E6	1787544	57.063	<MDL #
8) T	DICHLORPROP	0.000	7.738	0	8412166	N.D.	14.867
9) T	2,4-D	8.396	0.000	107.5E6	0	94.358	N.D. #
11) T	2,4,5-TP ...	0.000	8.760	0	38641487	N.D.	13.352
12) T	2,4,5-T	9.409	0.000	18958521	0	3.091	N.D. #
14) T	DINOSEB	0.000	10.054	0	11960540	N.D.	5.759



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 19:11
Operator : DD\AJ
Sample : L3993-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 06:32:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

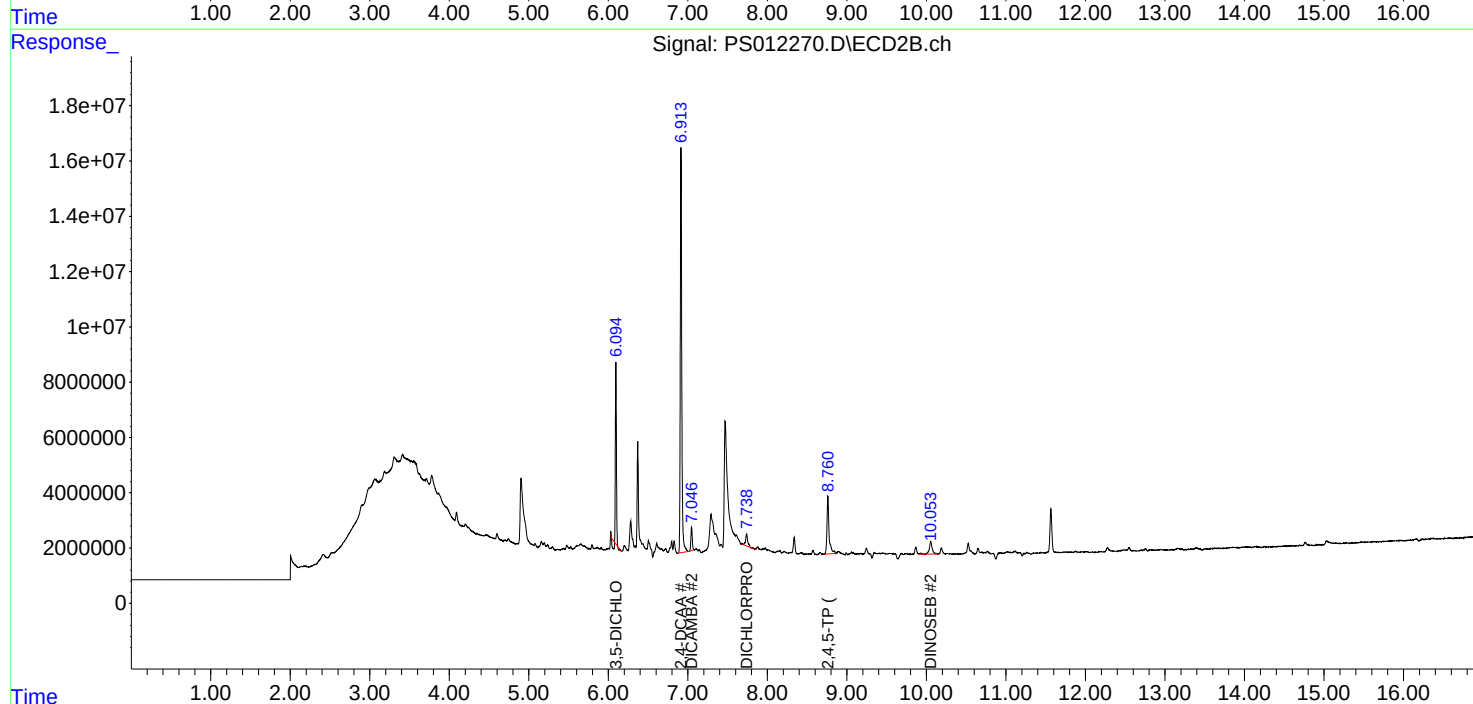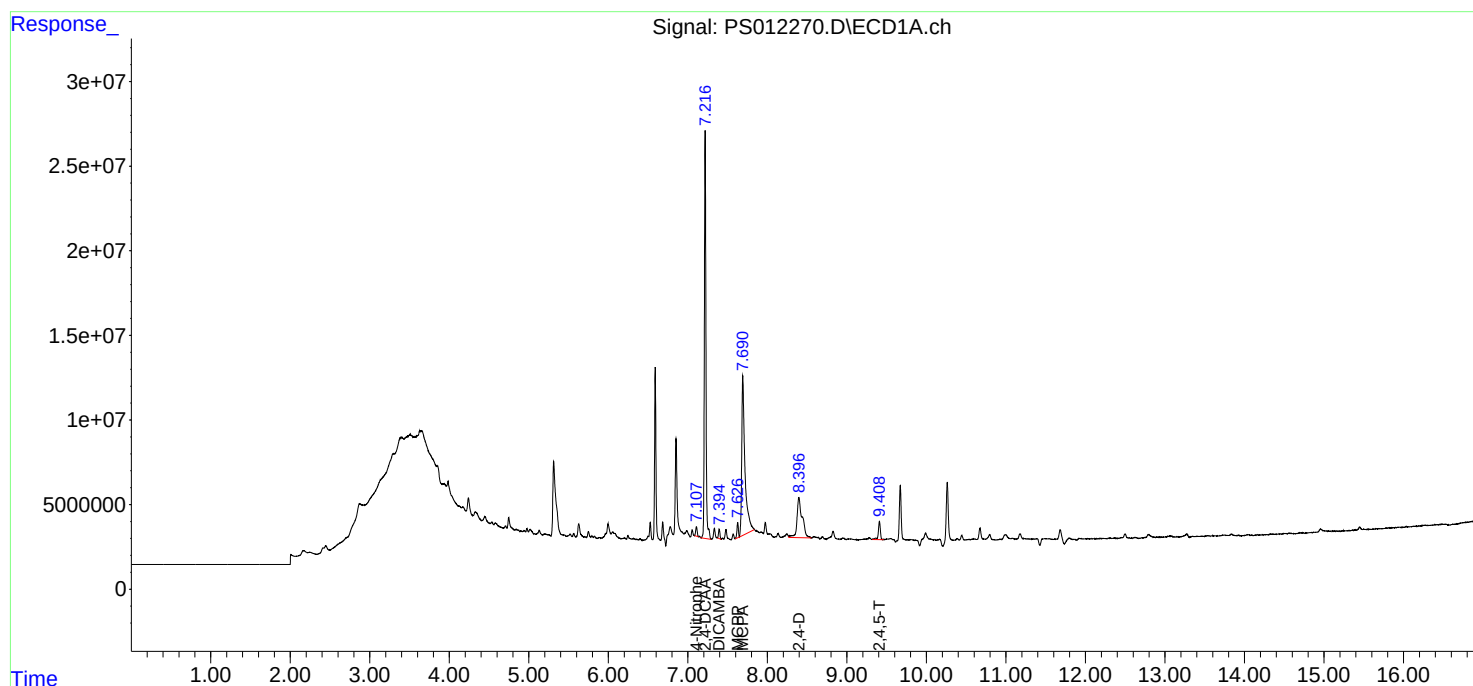


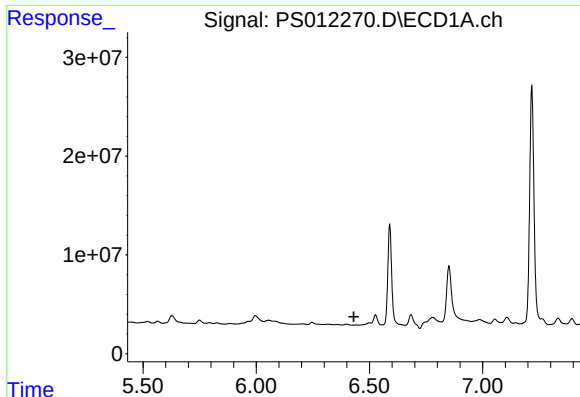

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

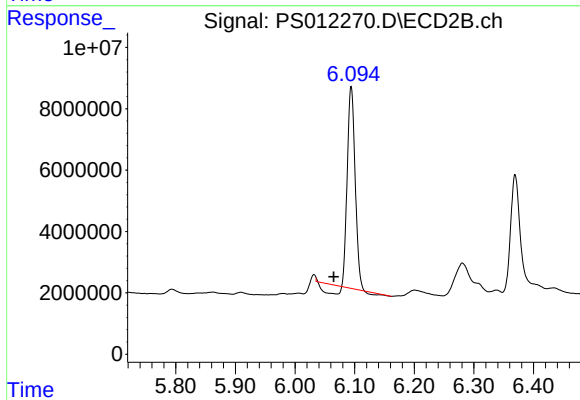


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 56065968
Conc: 69.30 ng/ml

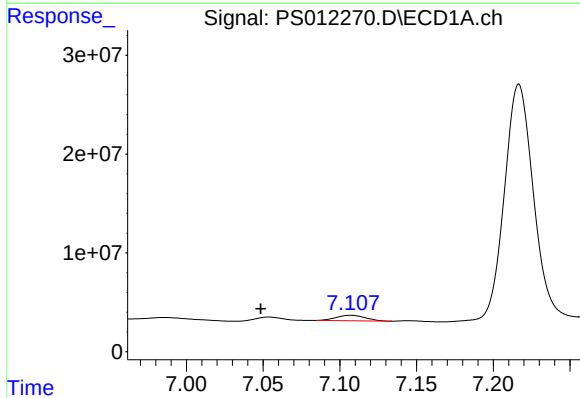


#3 4-Nitrophenol

R.T.: 7.107 min
Delta R.T.: 0.059 min
Response: 7276485
Conc: 13.66 ng/ml

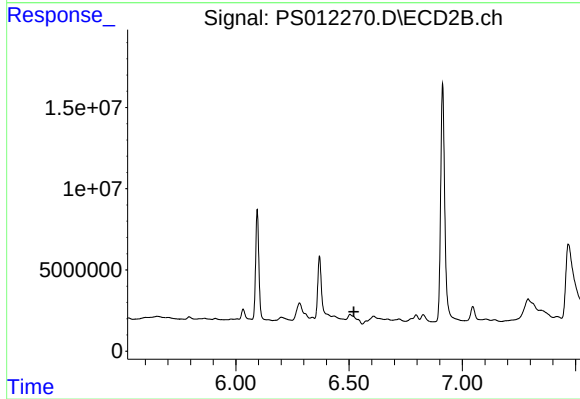

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

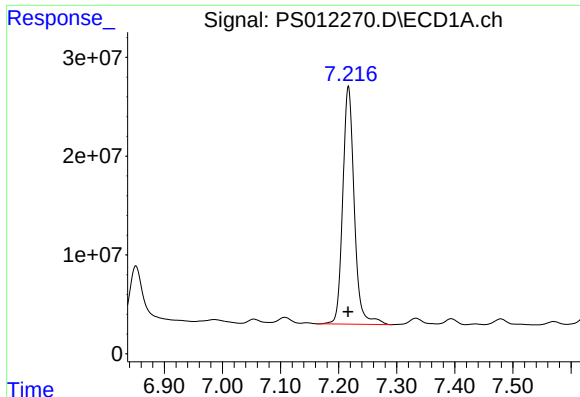

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 331524964
Conc: 305.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

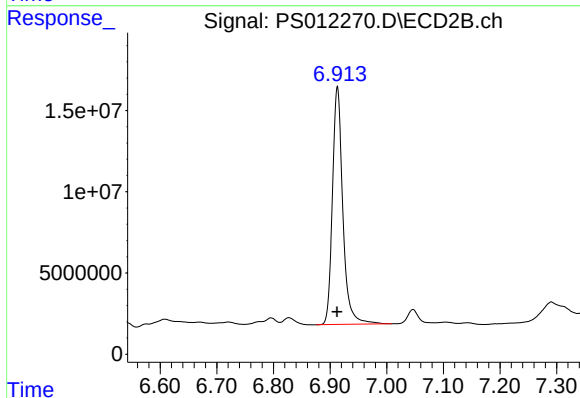


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 186661725
Conc: 353.79 ng/ml

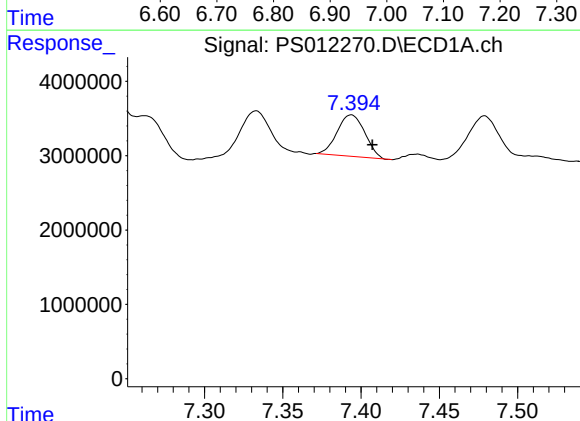


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.014 min
Response: 6858650
Conc: 1.63 ng/ml

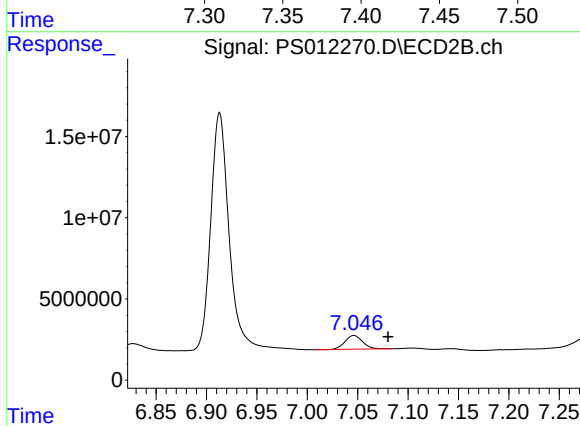

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 10351008
Conc: 4.80 ng/ml

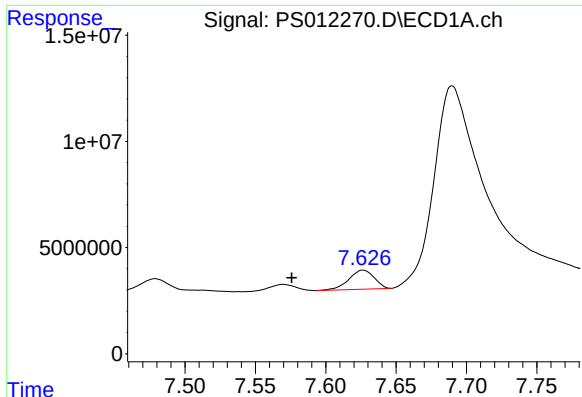

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.051 min
Response: 11175884
Conc: 3.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

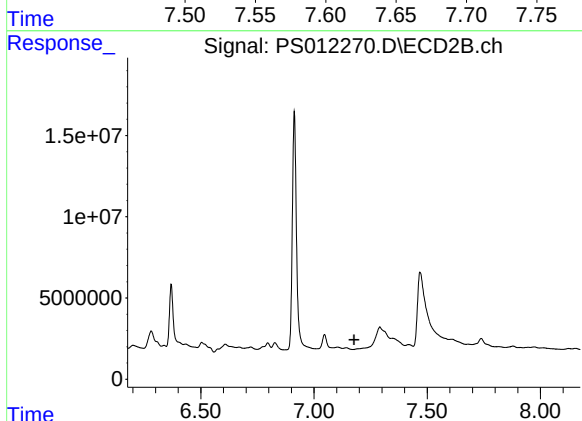


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

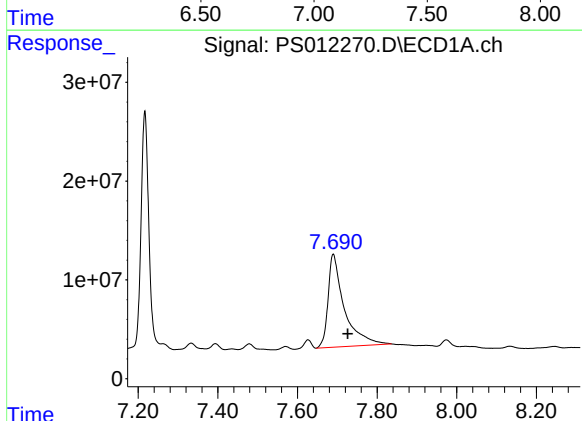


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.036 min
Response: 266622658
Conc: 57.06 ug/ml

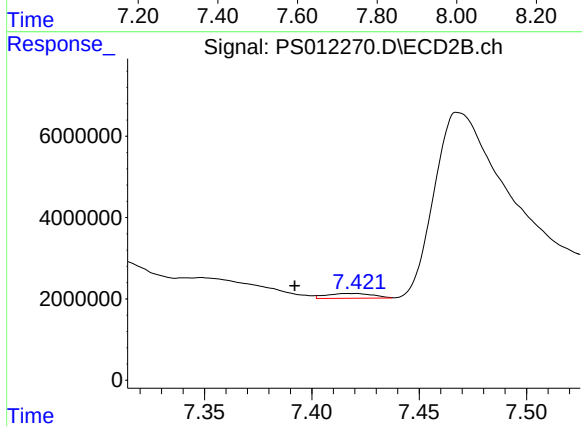

#7 MCPA


R.T.: 7.418 min
Delta R.T.: 0.026 min
Response: 1787544
Conc: N.D.

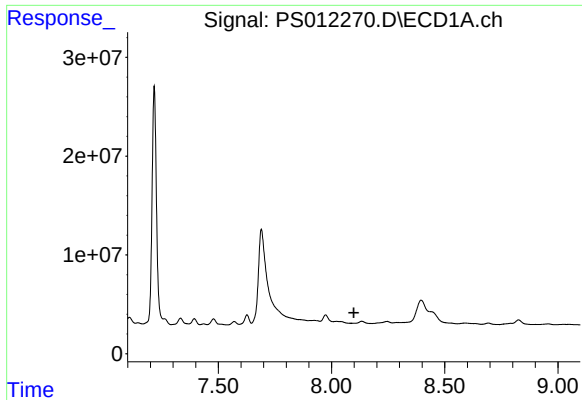

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

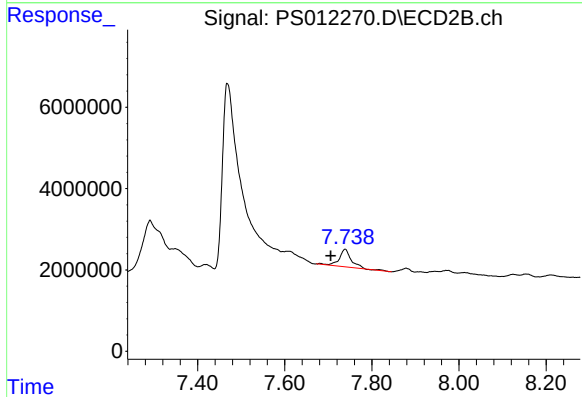


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.032 min
Response: 8412166
Conc: 14.87 ng/ml

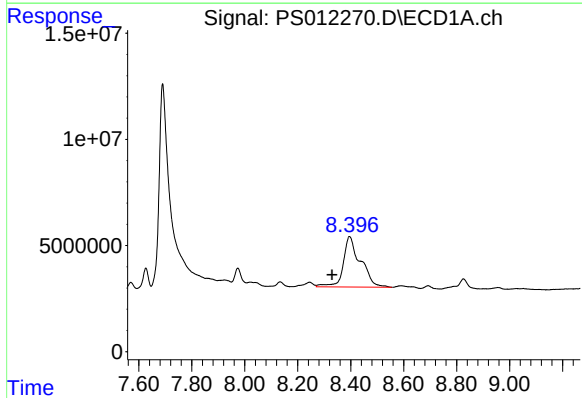


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.066 min
Response: 107469813
Conc: 94.36 ng/ml

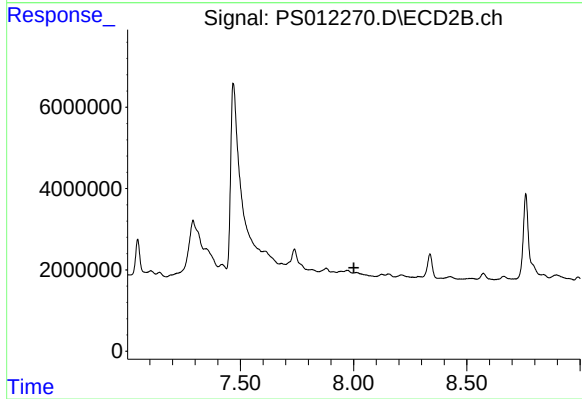

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

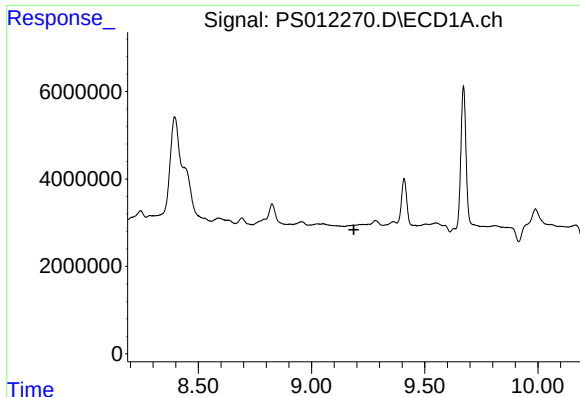

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

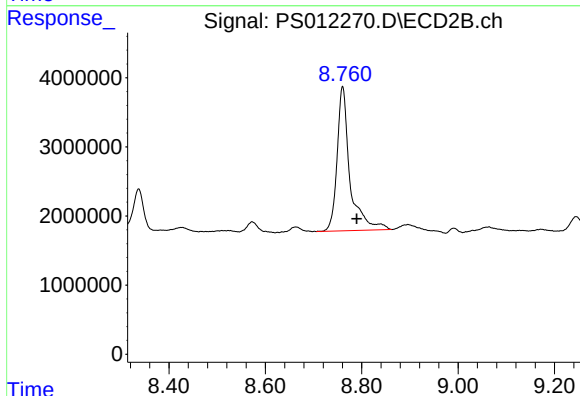


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: -0.029 min
Response: 38641487
Conc: 13.35 ng/ml

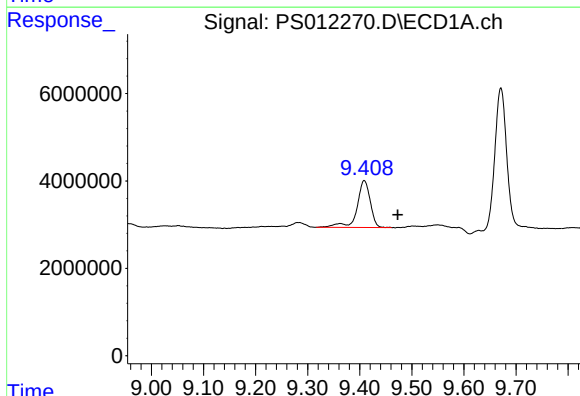


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.064 min
Response: 18958521
Conc: 3.09 ng/ml

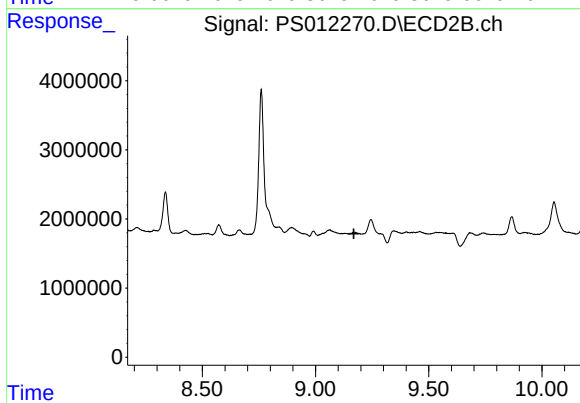

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

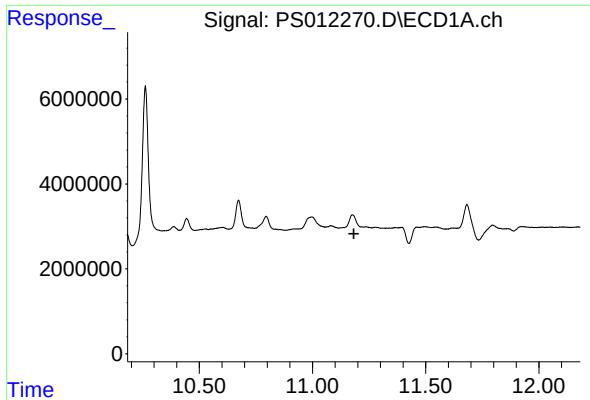

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

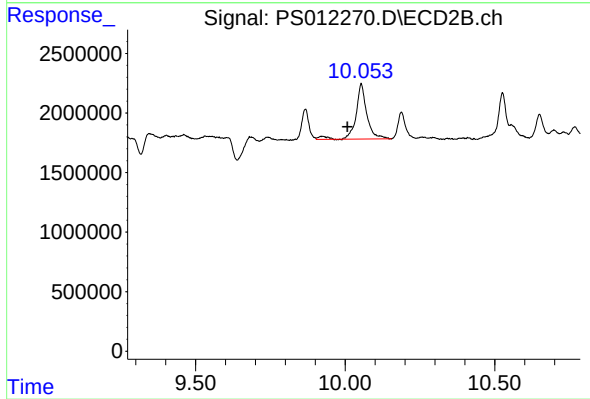

#14 DINOSEB

R.T.: 10.054 min
Delta R.T.: 0.046 min
Response: 11960540
Conc: 5.76 ng/ml