

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091619\
 Data File : PS006750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 19:38
 Operator : SM\AJ
 Sample : K4661-06MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-02-091319MS

Manual Integrations
 APPROVED

Ankita
 9/18/2019 9:38:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 00:46:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.479	5.208	295.5E6	168.2E6	380.428	393.973
Target Compounds							
1) T	Dalapon	2.042	1.752	612.0E6	408.1E6	626.201m	798.556m#
2) T	3,5-DICHL...	4.845	4.511	322.2E6	170.6E6	325.485m	315.215m
5) T	DICAMBA	5.631	5.336	1689.4E6	915.2E6	586.003	570.864
6) T	MCP	5.781	5.418	98753375	48353969	51.912m	45.690m
7) T	MCPA	5.915	5.596	165.9E6	88568805	58.710	50.495m
8) T	DICHLORPROP	6.257	5.874	494.2E6	312.1E6	694.883m	802.032
9) T	2,4-D	6.471	6.143	712.1E6	351.2E6	921.705	736.213m
10) T	Pentachlo...	6.735	6.512	1527.9E6	838.9E6	137.154	139.237
11) T	2,4,5-TP ...	7.269	6.873	3022.2E6	2287.8E6	702.341	1004.986m#
12) T	2,4,5-T	7.540	7.232	3282.0E6	1698.6E6	704.340	787.780m
13) T	2,4-DB	8.069	7.720	422.7E6	217.6E6	694.624	791.306
14) T	DINOSEB	9.162	8.031	404.7E6	154.6E6	116.255	92.302
15) T	Picloram	8.993	8.968	3758.1E6	2075.5E6	557.106	560.856
16) T	DCPA	9.433	8.925	2718.9E6	1505.7E6	481.294	477.970m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091619\
Data File : PS006750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2019 19:38
Operator : SM\AJ
Sample : K4661-06MS
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampled :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 00:46:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

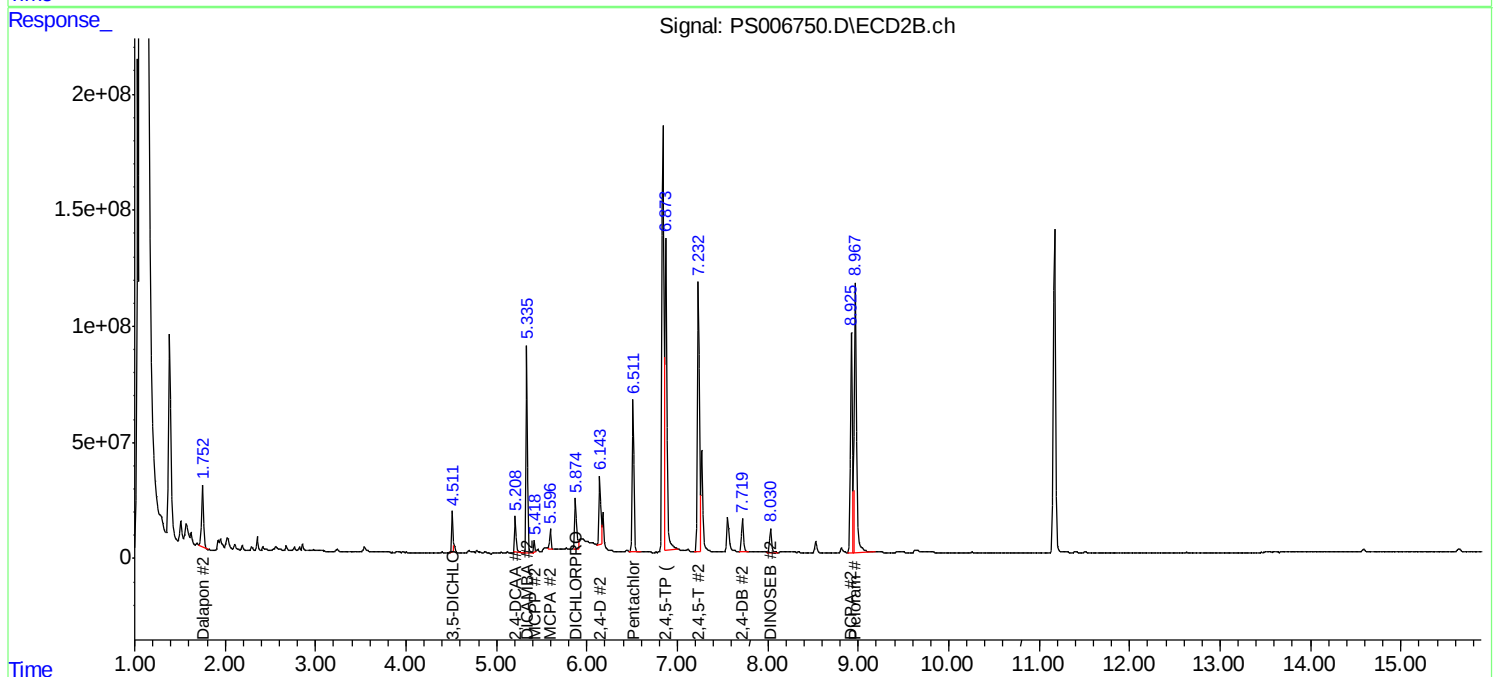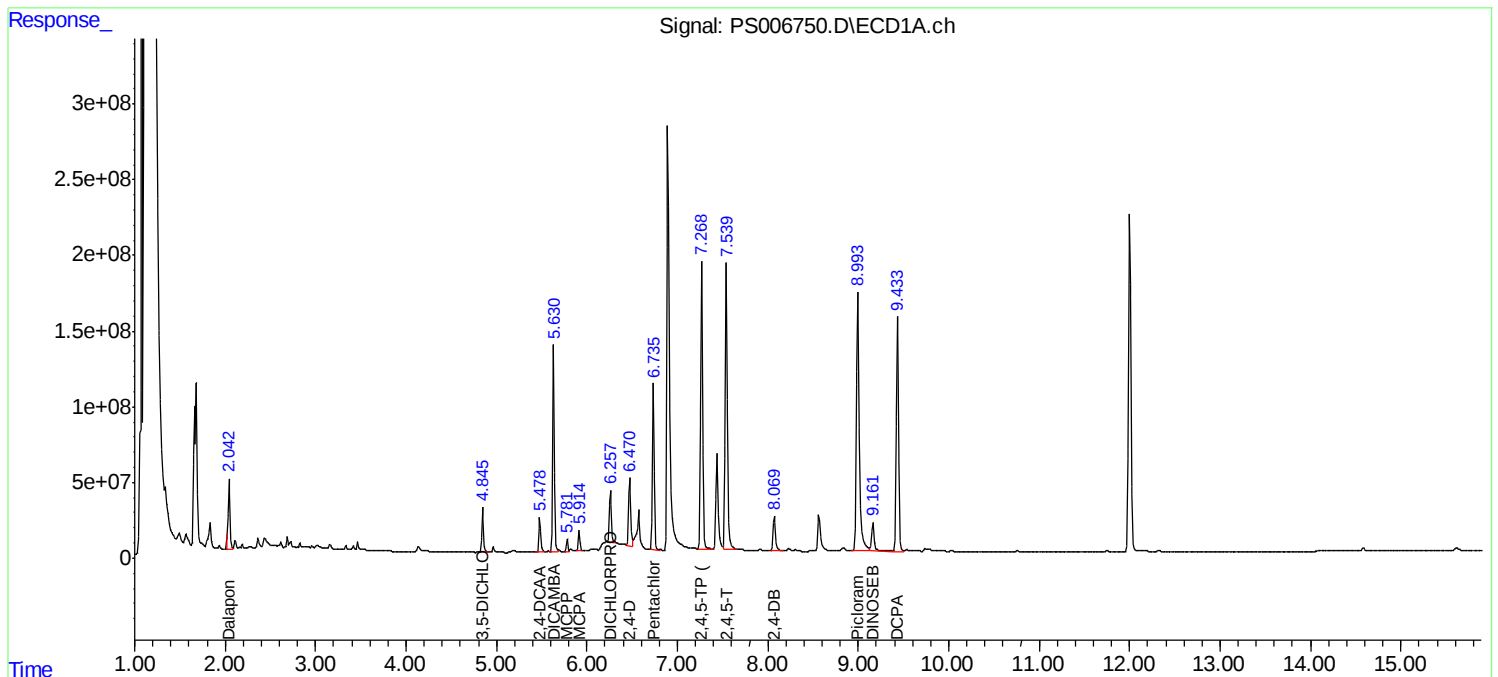

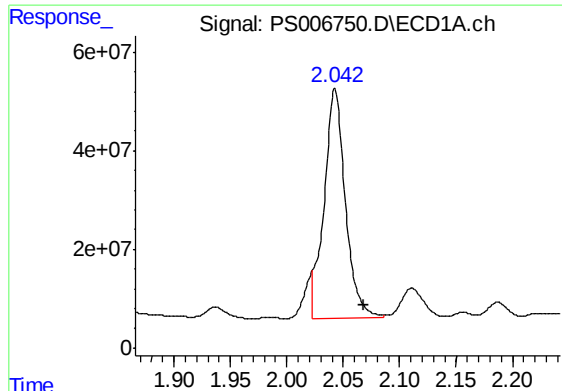


#1 Dalapon

R.T.: 2.042 min
Delta R.T.: -0.026 min
Response: 612048488
Conc: 626.20 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

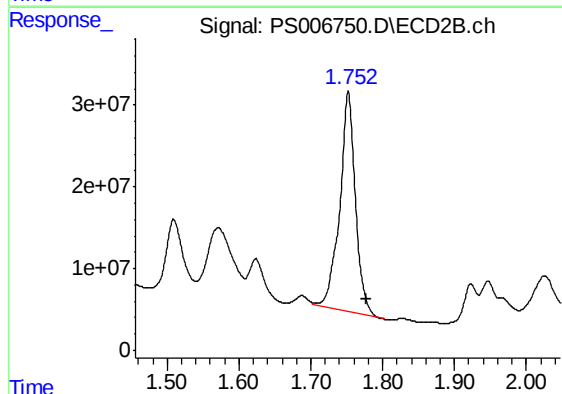


#1 Dalapon

R.T.: 1.752 min
Delta R.T.: -0.026 min
Response: 408100836
Conc: 798.56 ng/ml m

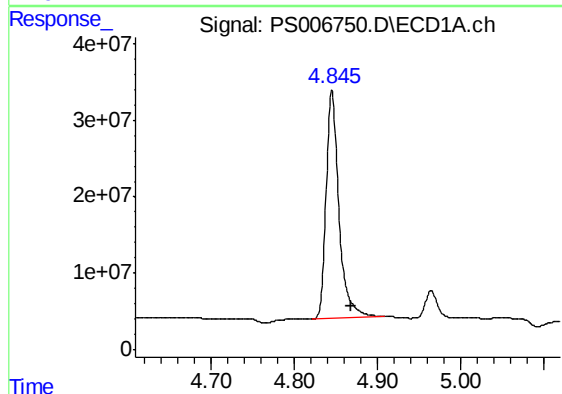


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.845 min
Delta R.T.: -0.023 min
Response: 322223417
Conc: 325.48 ng/ml m

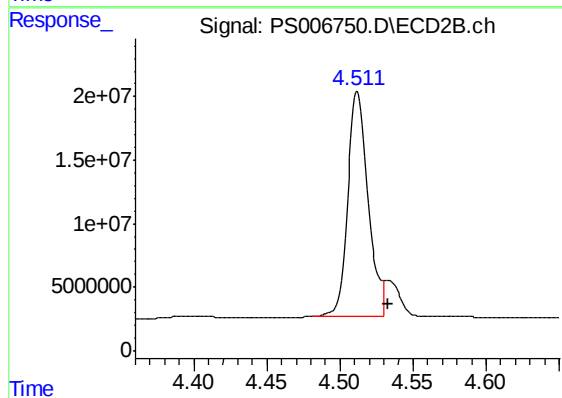

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.511 min
Delta R.T.: -0.022 min
Response: 170610532
Conc: 315.21 ng/ml m

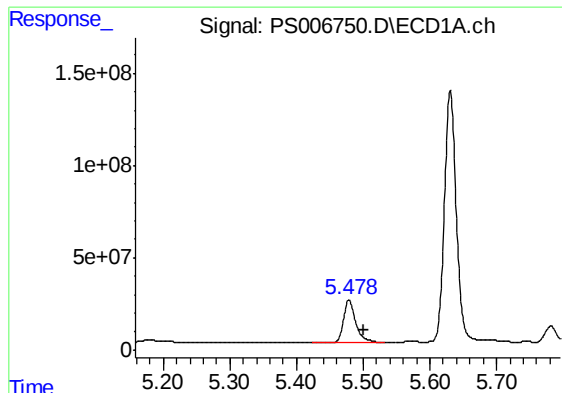


#4 2,4-DCAA

R.T.: 5.479 min
Delta R.T.: -0.022 min
Response: 295548763
Conc: 380.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

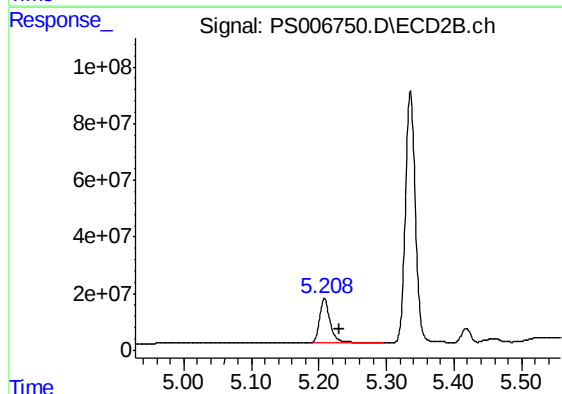


#4 2,4-DCAA

R.T.: 5.208 min
Delta R.T.: -0.022 min
Response: 168227642
Conc: 393.97 ng/ml

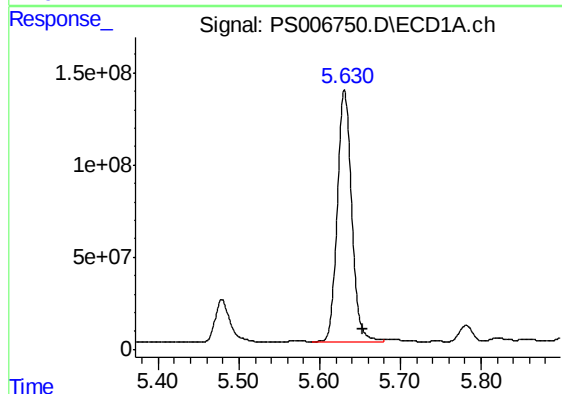


#5 DICAMBA

R.T.: 5.631 min
Delta R.T.: -0.022 min
Response: 1689399345
Conc: 586.00 ng/ml

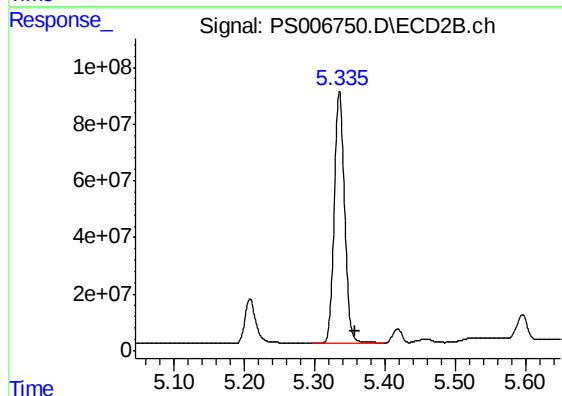

#5 DICAMBA

R.T.: 5.336 min
Delta R.T.: -0.023 min
Response: 915220451
Conc: 570.86 ng/ml

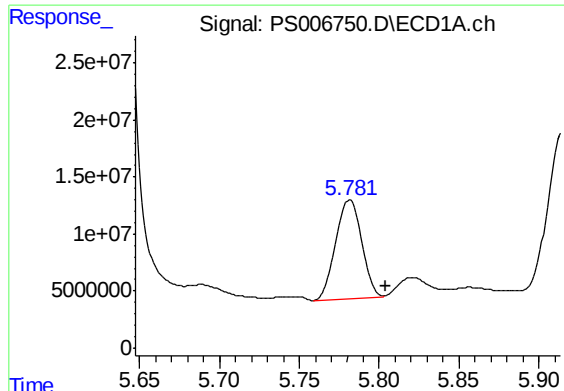


#6 MCPP

R.T.: 5.781 min
Delta R.T.: -0.023 min
Response: 98753375
Conc: 51.91 ug/ml m

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

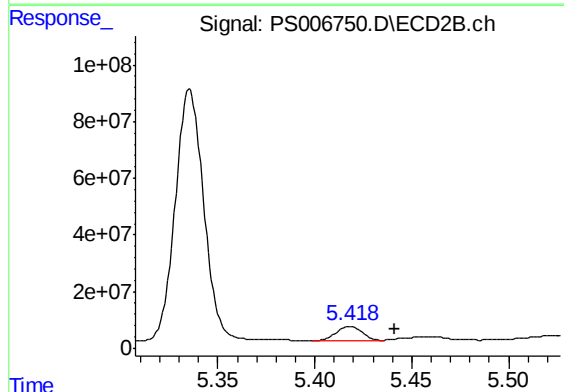


#6 MCPP

R.T.: 5.418 min
Delta R.T.: -0.023 min
Response: 48353969
Conc: 45.69 ug/ml m

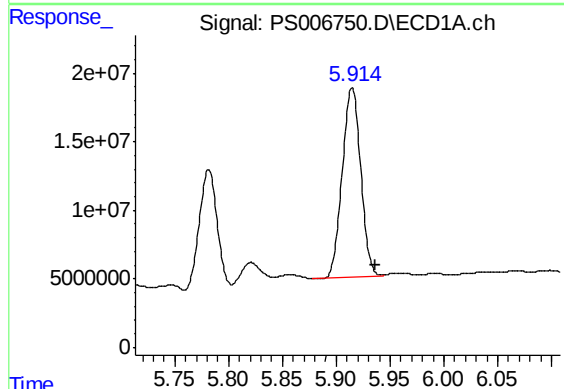


#7 MCPA

R.T.: 5.915 min
Delta R.T.: -0.022 min
Response: 165928517
Conc: 58.71 ug/ml

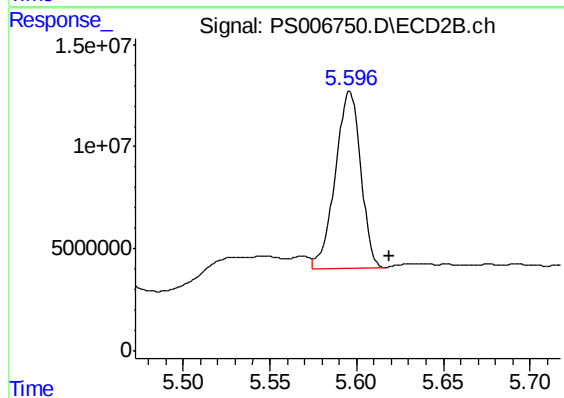

#7 MCPA

R.T.: 5.596 min
Delta R.T.: -0.024 min
Response: 88568805
Conc: 50.50 ug/ml m

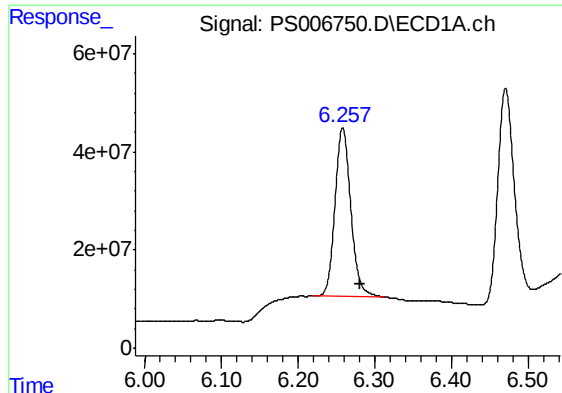


#8 DICHLORPROP

R.T.: 6.257 min
Delta R.T.: -0.024 min
Response: 494179380
Conc: 694.88 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

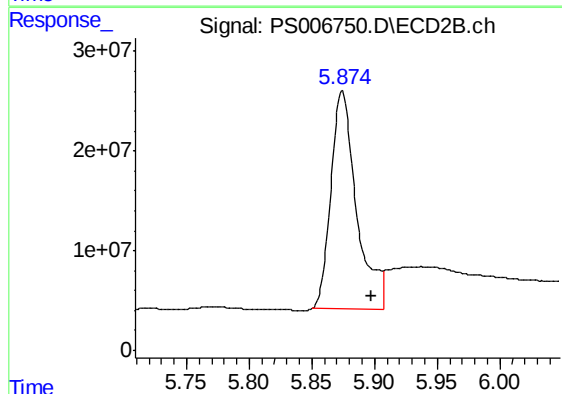


#8 DICHLORPROP

R.T.: 5.874 min
Delta R.T.: -0.023 min
Response: 312139038
Conc: 802.03 ng/ml

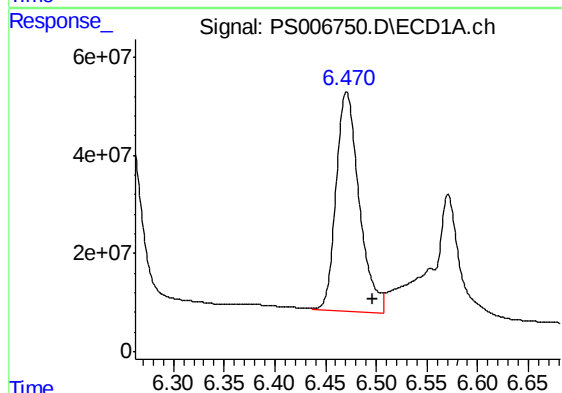


#9 2,4-D

R.T.: 6.471 min
Delta R.T.: -0.026 min
Response: 712130842
Conc: 921.71 ng/ml

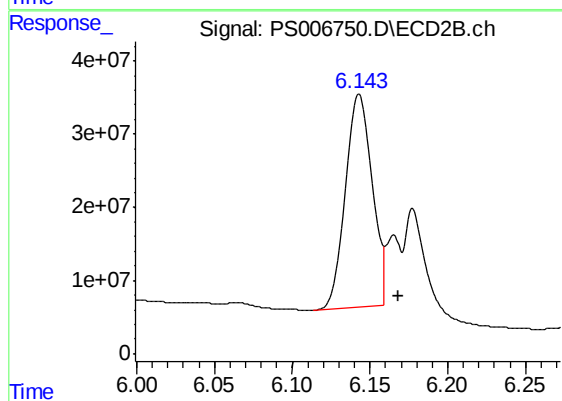

#9 2,4-D

R.T.: 6.143 min
Delta R.T.: -0.026 min
Response: 351164908
Conc: 736.21 ng/ml m

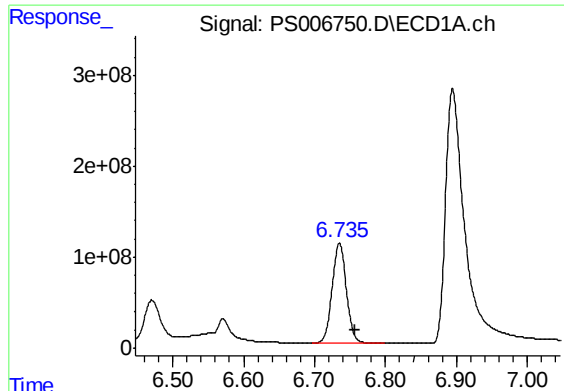


#10 Pentachlorophenol

R.T.: 6.735 min
Delta R.T.: -0.022 min
Response: 1527876561
Conc: 137.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

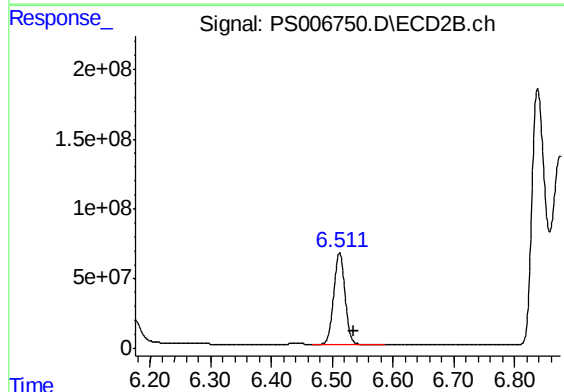


#10 Pentachlorophenol

R.T.: 6.512 min
Delta R.T.: -0.023 min
Response: 838901545
Conc: 139.24 ng/ml

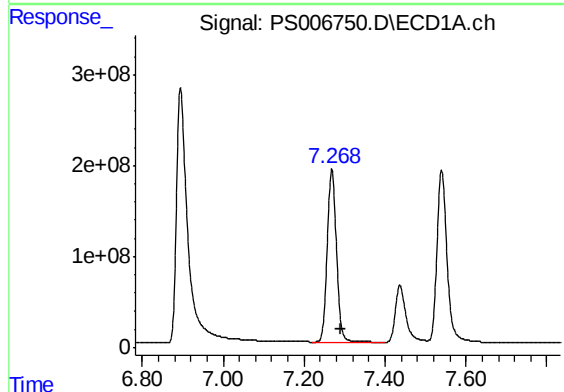


#11 2,4,5-TP (SILVEX)

R.T.: 7.269 min
Delta R.T.: -0.023 min
Response: 3022182795
Conc: 702.34 ng/ml

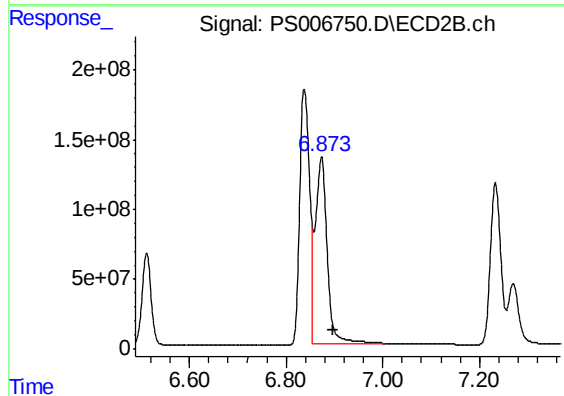

#11 2,4,5-TP (SILVEX)

R.T.: 6.873 min
Delta R.T.: -0.025 min
Response: 2287781850
Conc: 1004.99 ng/ml m

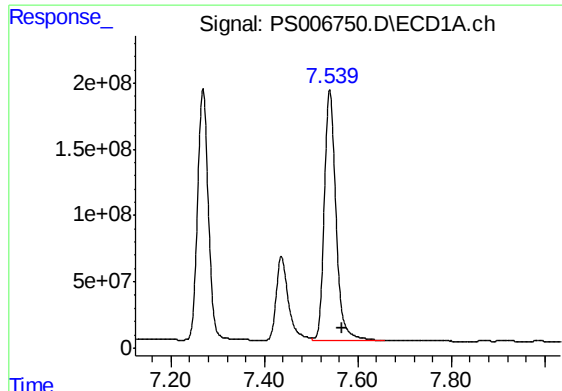


#12 2,4,5-T

R.T.: 7.540 min
Delta R.T.: -0.026 min
Response: 3281969694
Conc: 704.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

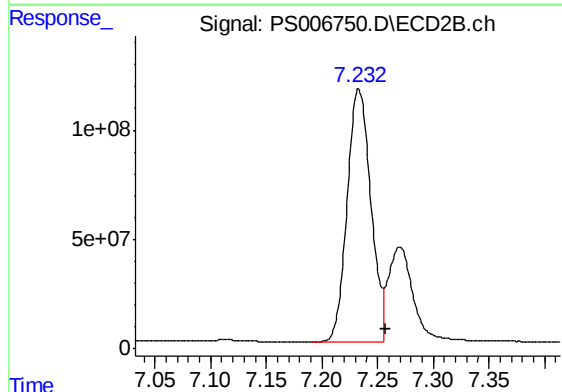


#12 2,4,5-T

R.T.: 7.232 min
Delta R.T.: -0.025 min
Response: 1698580367
Conc: 787.78 ng/ml m

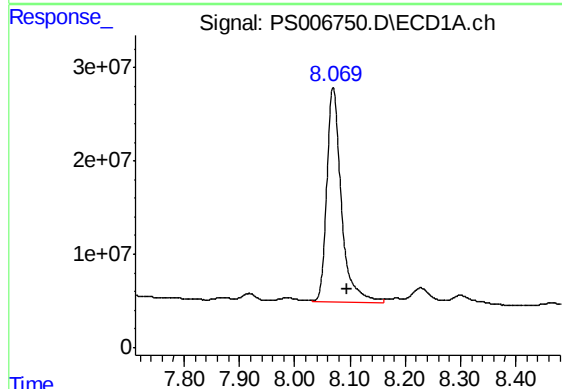


#13 2,4-DB

R.T.: 8.069 min
Delta R.T.: -0.025 min
Response: 422716048
Conc: 694.62 ng/ml

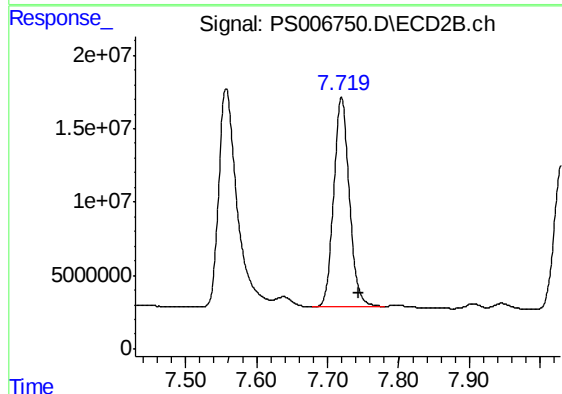

#13 2,4-DB

R.T.: 7.720 min
Delta R.T.: -0.024 min
Response: 217571049
Conc: 791.31 ng/ml

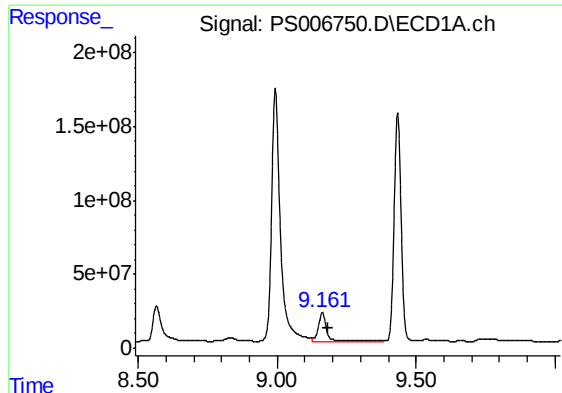


#14 DINOSEB

R.T.: 9.162 min
Delta R.T.: -0.021 min
Response: 404663605
Conc: 116.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS


Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

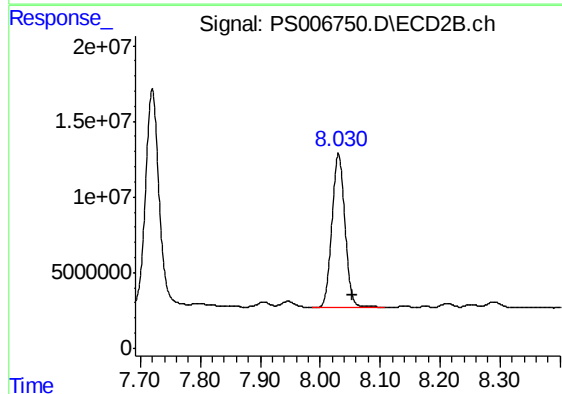


#14 DINOSEB

R.T.: 8.031 min
Delta R.T.: -0.023 min
Response: 154637396
Conc: 92.30 ng/ml

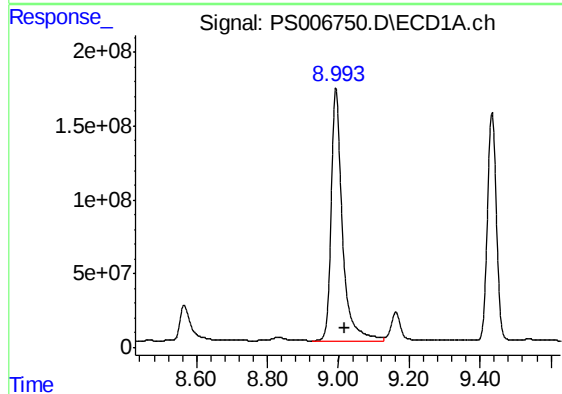


#15 Picloram

R.T.: 8.993 min
Delta R.T.: -0.024 min
Response: 3758066076
Conc: 557.11 ng/ml

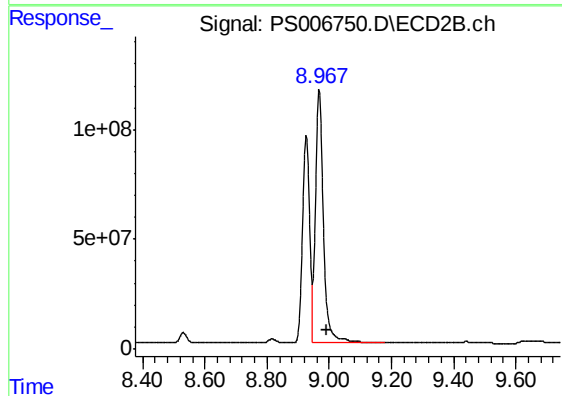

#15 Picloram

R.T.: 8.968 min
Delta R.T.: -0.024 min
Response: 2075509749
Conc: 560.86 ng/ml

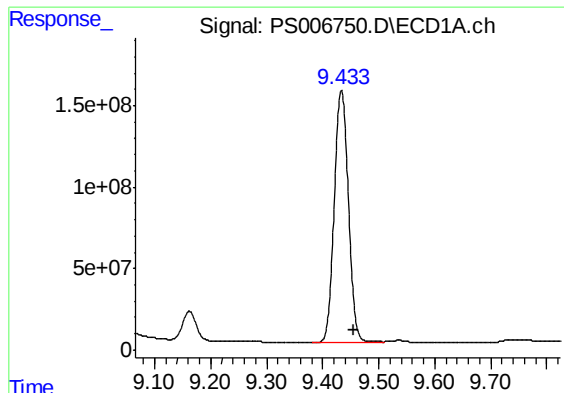


#16 DCPA

R.T.: 9.433 min
Delta R.T.: -0.023 min
Response: 2718905719
Conc: 481.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-091319MS

Manual Integrations
APPROVED

Ankita
9/18/2019 9:38:48 AM

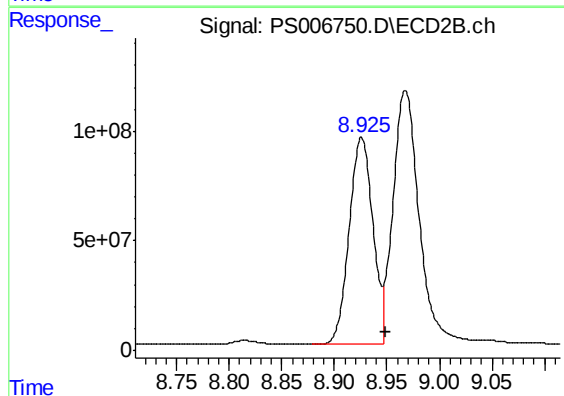

#16 DCPA

R.T.: 8.925 min
Delta R.T.: -0.023 min
Response: 1505715634
Conc: 477.97 ng/ml m