

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091620\
 Data File : PS012279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 11:00
 Operator : DD\AJ
 Sample : L3867-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-02-091420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 12:37:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	239.9E6	142.4E6	221.372	269.861
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	65398024	N.D.	80.838
3) T	4-Nitroph...	7.054	0.000	3232275	0	6.070	N.D. #
5) T	DICAMBA	7.394	7.046	9109760	14462765	2.165	6.706 #
6) T	MCP	7.569	0.000	5960669	0	1.850	N.D. #
7) T	MCPA	7.692	0.000	175.8E6	0	37.633	N.D. #
8) T	DICHLORPROP	0.000	7.736	0	10885498	N.D.	19.239
9) T	2,4-D	8.396	7.941	94193715	6240237	82.702	8.579 #
11) T	2,4,5-TP ...	0.000	8.760	0	27776522	N.D.	9.597
12) T	2,4,5-T	9.408	0.000	15894083	0	2.592	N.D. #
13) T	2,4-DB	0.000	9.738	0	7057937	N.D.	17.347
14) T	DINOSEB	0.000	10.053	0	7607322	N.D.	3.663
15) T	Picloram	0.000	11.026	0	20495275	N.D.	4.834



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091620\
Data File : PS012279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 11:00
Operator : DD\AJ
Sample : L3867-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 12:37:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

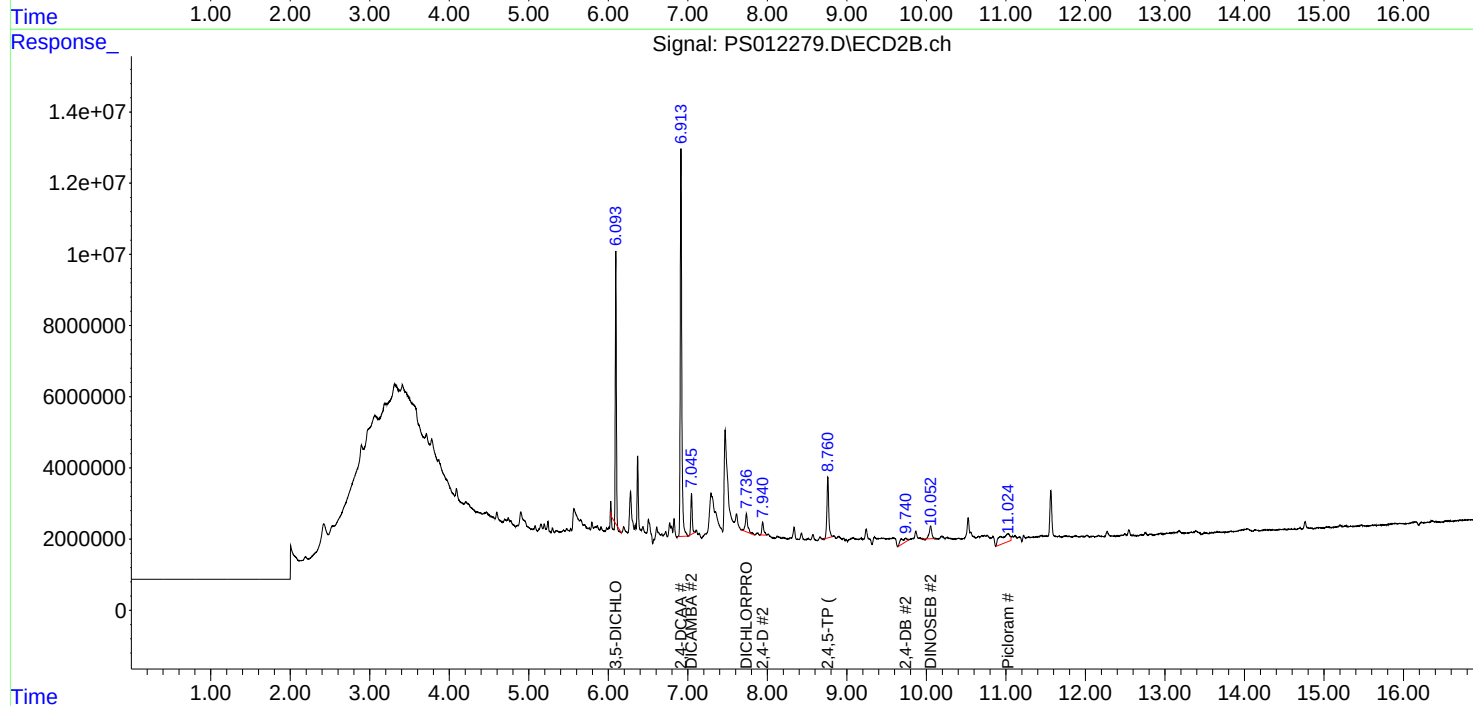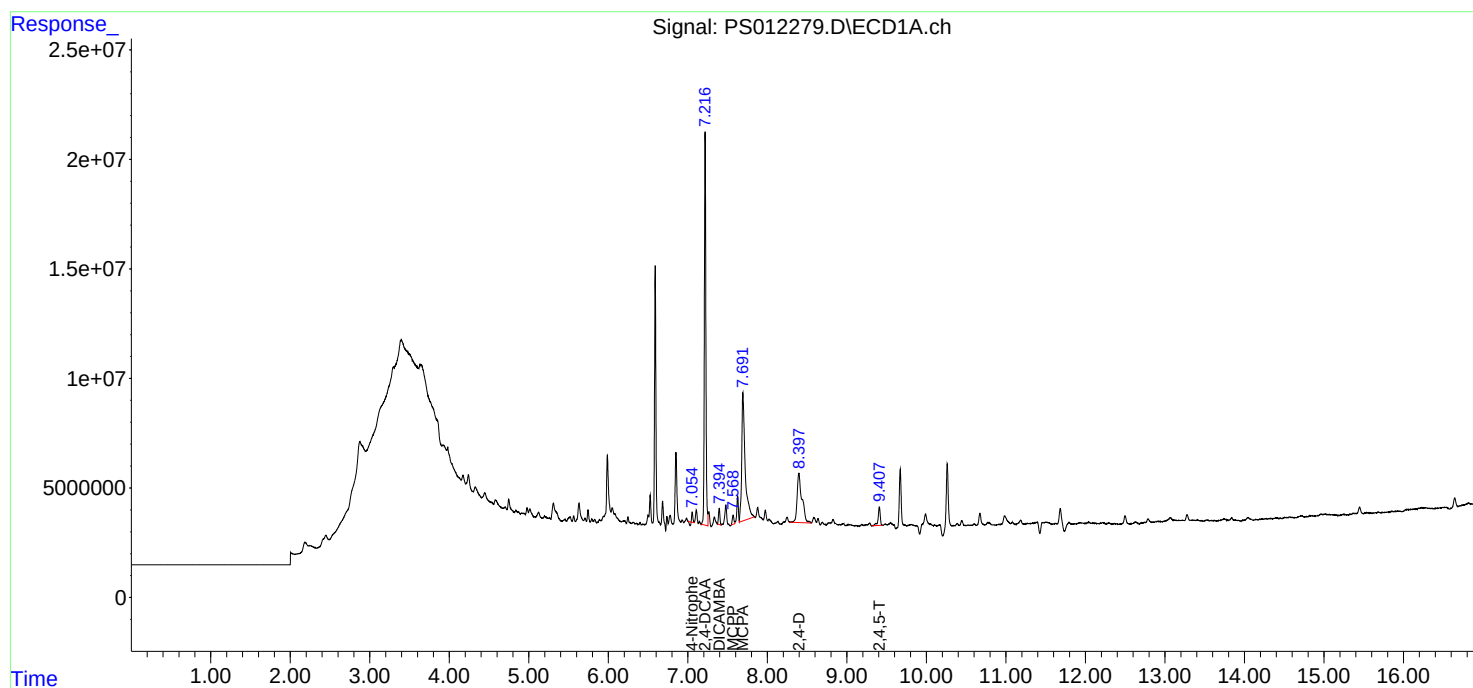


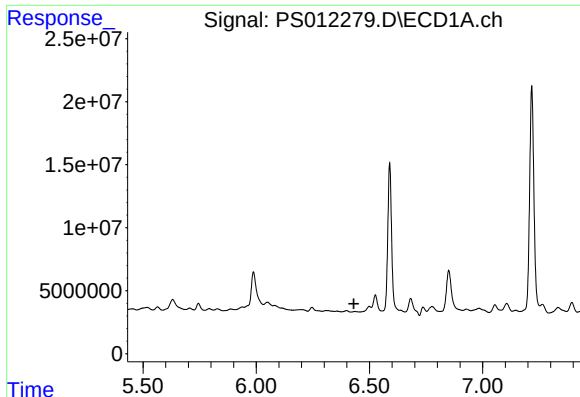

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

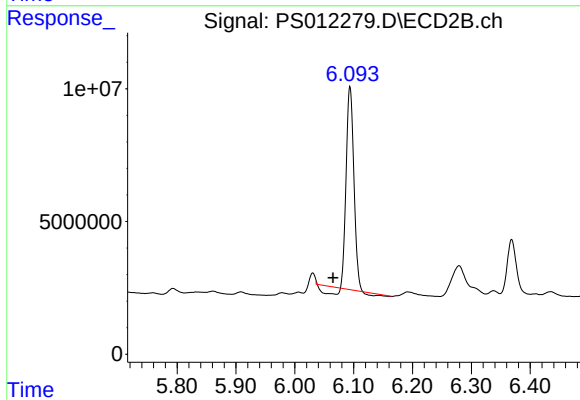


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 65398024
Conc: 80.84 ng/ml

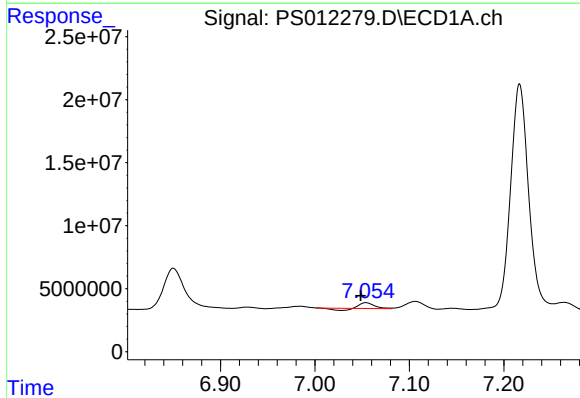


#3 4-Nitrophenol

R.T.: 7.054 min
Delta R.T.: 0.006 min
Response: 3232275
Conc: 6.07 ng/ml

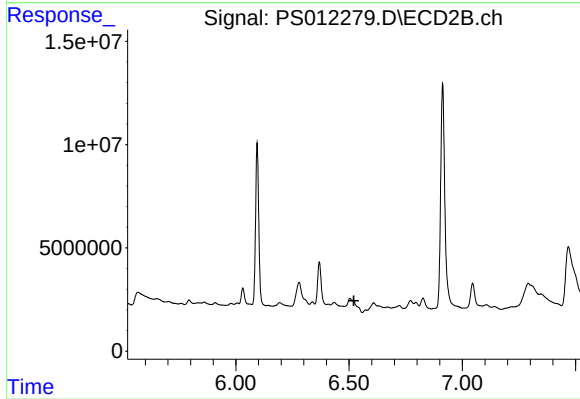

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

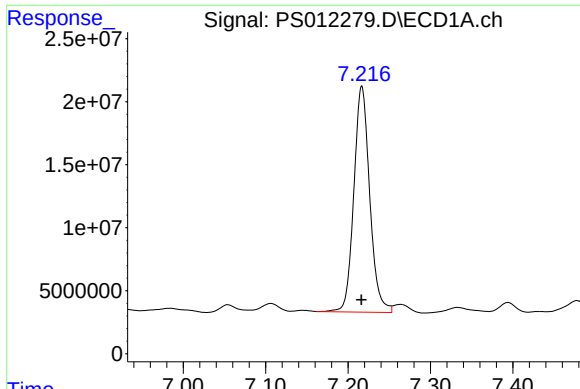

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 239944497
Conc: 221.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

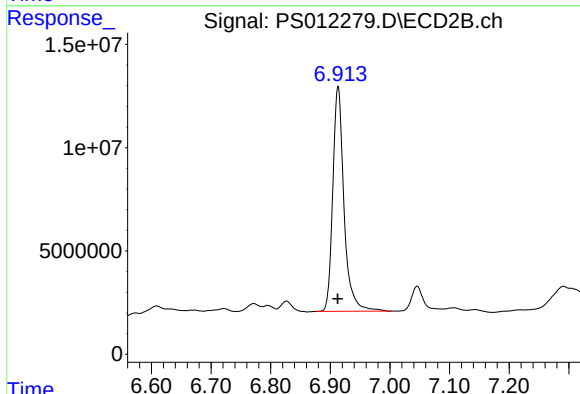


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 142380063
Conc: 269.86 ng/ml

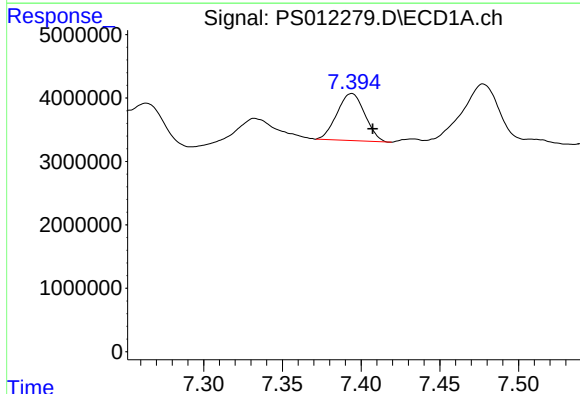


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.013 min
Response: 9109760
Conc: 2.17 ng/ml

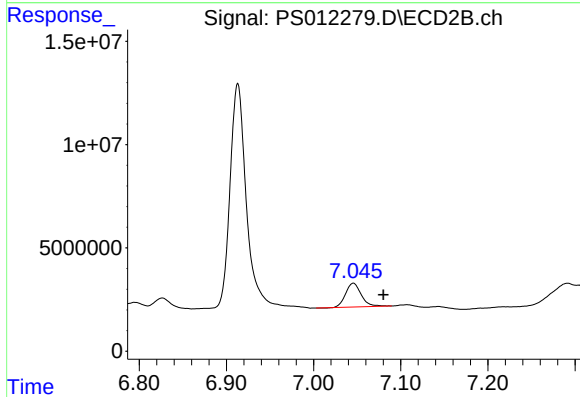

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 14462765
Conc: 6.71 ng/ml

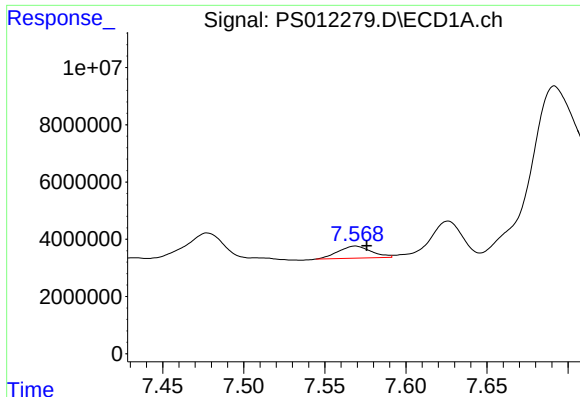

#6 MCPP


R.T.: 7.569 min
Delta R.T.: -0.007 min
Response: 5960669
Conc: 1.85 ug/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

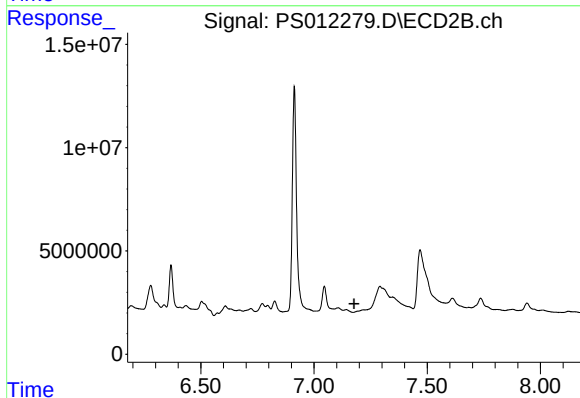


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

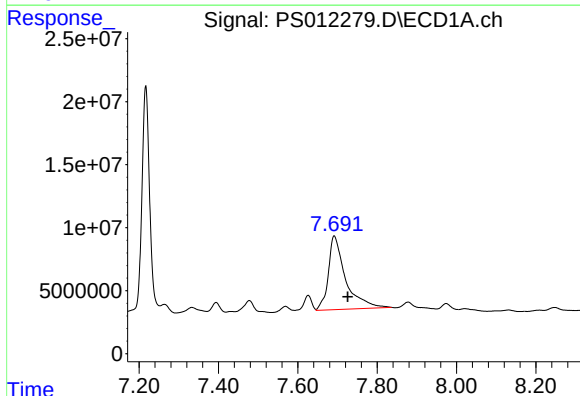


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.034 min
Response: 175836689
Conc: 37.63 ug/ml

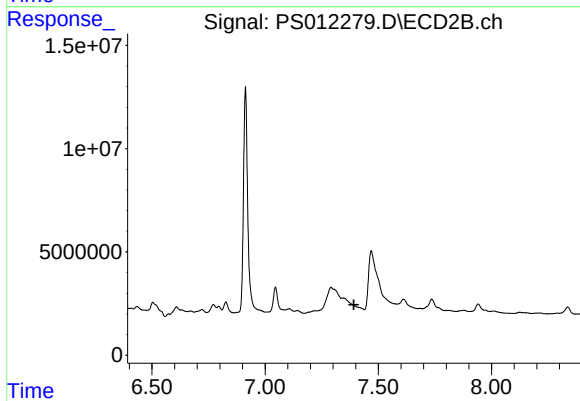

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

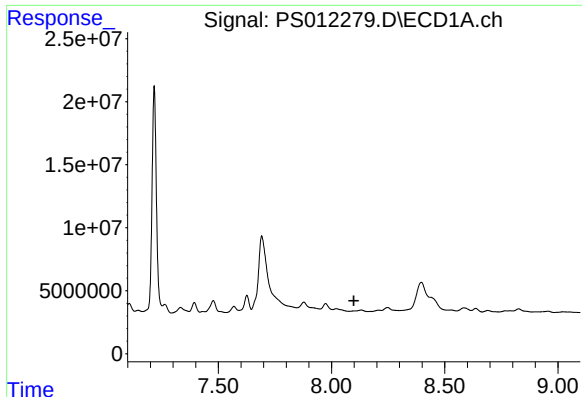

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

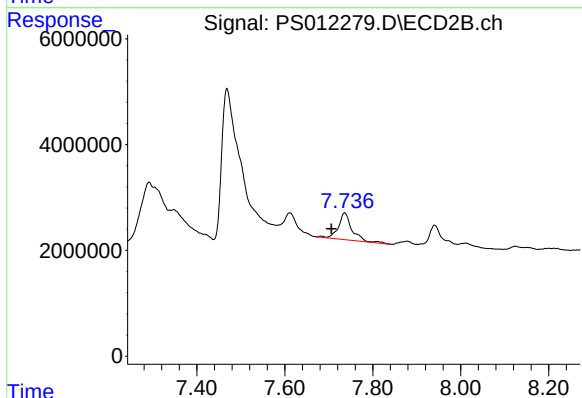


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.030 min
Response: 10885498
Conc: 19.24 ng/ml

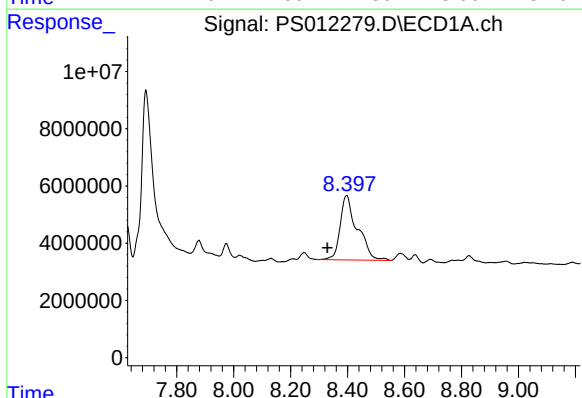


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.067 min
Response: 94193715
Conc: 82.70 ng/ml

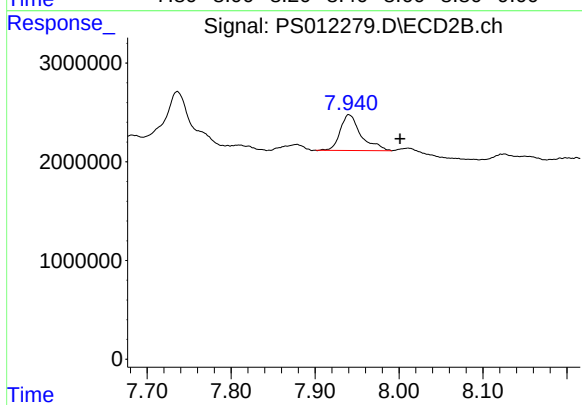

#9 2,4-D


R.T.: 7.941 min
Delta R.T.: -0.061 min
Response: 6240237
Conc: 8.58 ng/ml

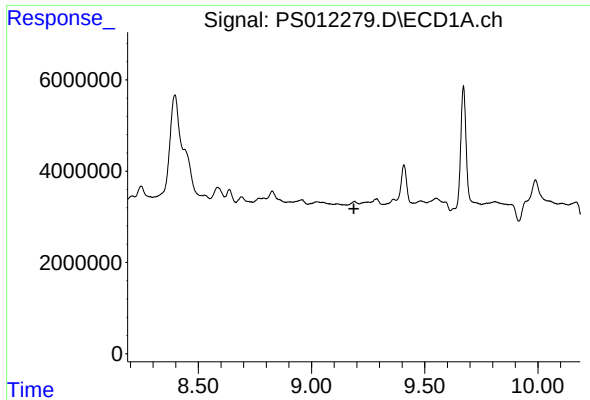

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

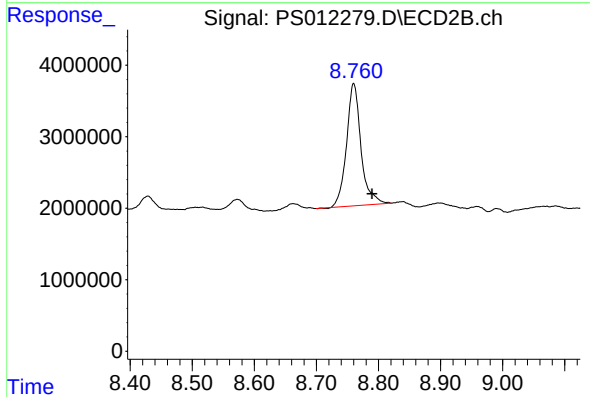


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: -0.029 min
Response: 27776522
Conc: 9.60 ng/ml

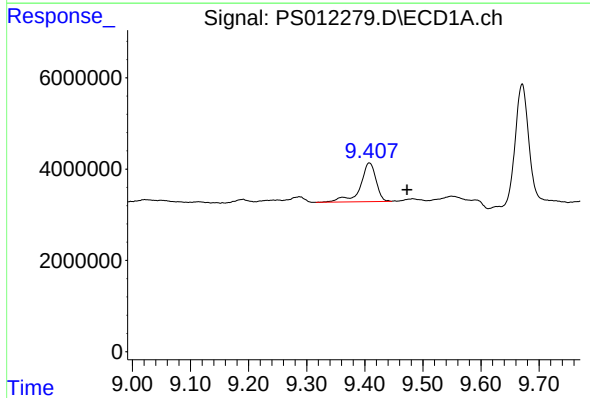


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: -0.065 min
Response: 15894083
Conc: 2.59 ng/ml

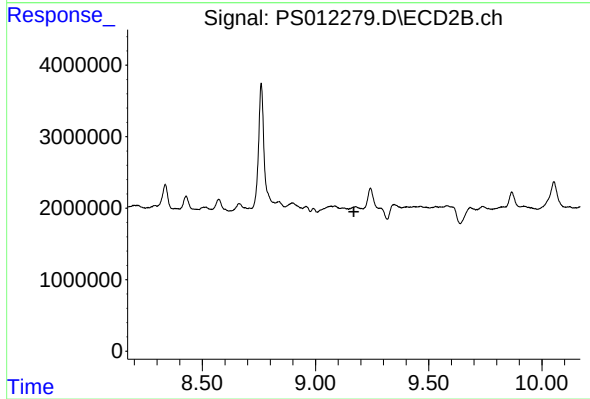

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

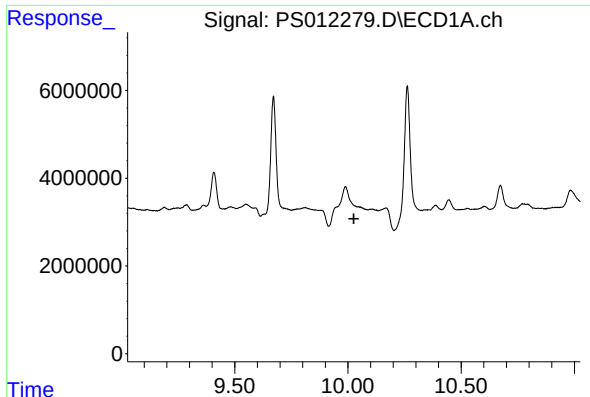

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

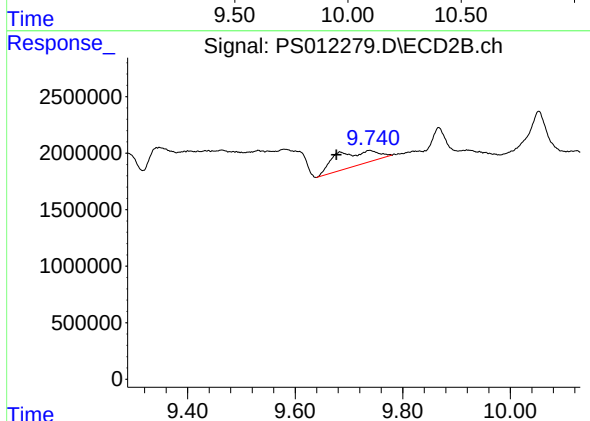


#13 2,4-DB

R.T.: 9.738 min
Delta R.T.: 0.062 min
Response: 7057937
Conc: 17.35 ng/ml

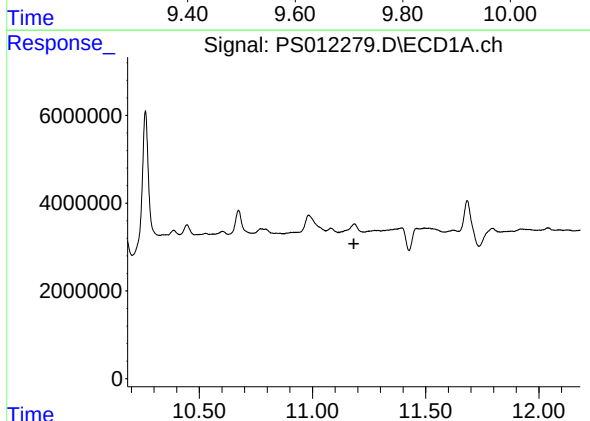


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.183 min
Response: 0
Conc: N.D.

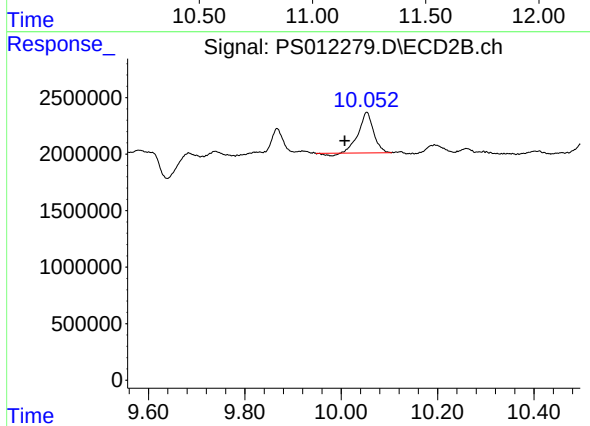

#14 DINOSEB


R.T.: 10.053 min
Delta R.T.: 0.045 min
Response: 7607322
Conc: 3.66 ng/ml

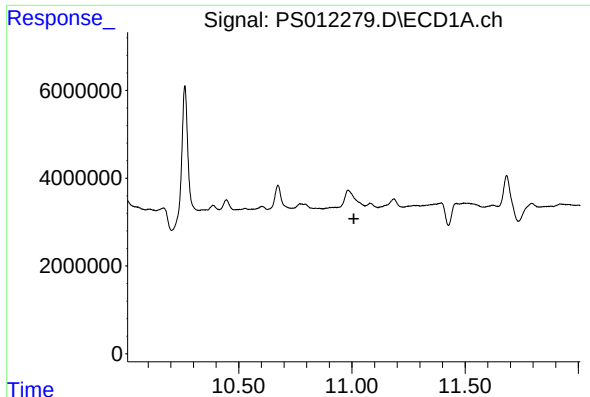

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-091420

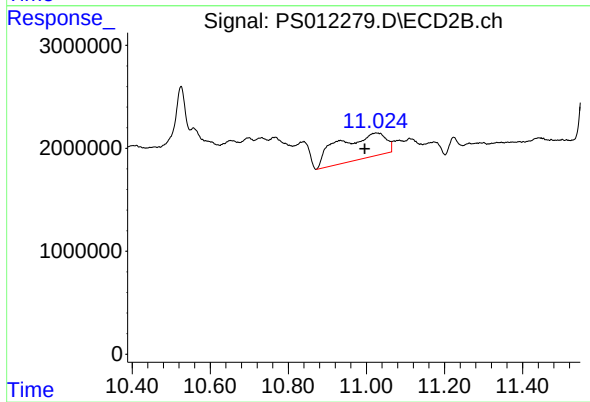

#15 Picloram

R.T.: 11.026 min
Delta R.T.: 0.030 min
Response: 20495275
Conc: 4.83 ng/ml