

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091620\
 Data File : PS012312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 23:38
 Operator : DD\AJ
 Sample : L3998-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-EF-01-TEST1-ABCD-B

Manual Integrations
 APPROVED

Ankita
 9/17/2020 12:03:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:32:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.216	6.911	500.6E6	222.8E6	461.878	422.273m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091620\
Data File : PS012312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 23:38
Operator : DD\AJ
Sample : L3998-03
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-EF-01-TEST1-ABCD-B


Manual Integrations
APPROVED

Ankita
9/17/2020 12:03:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:32:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

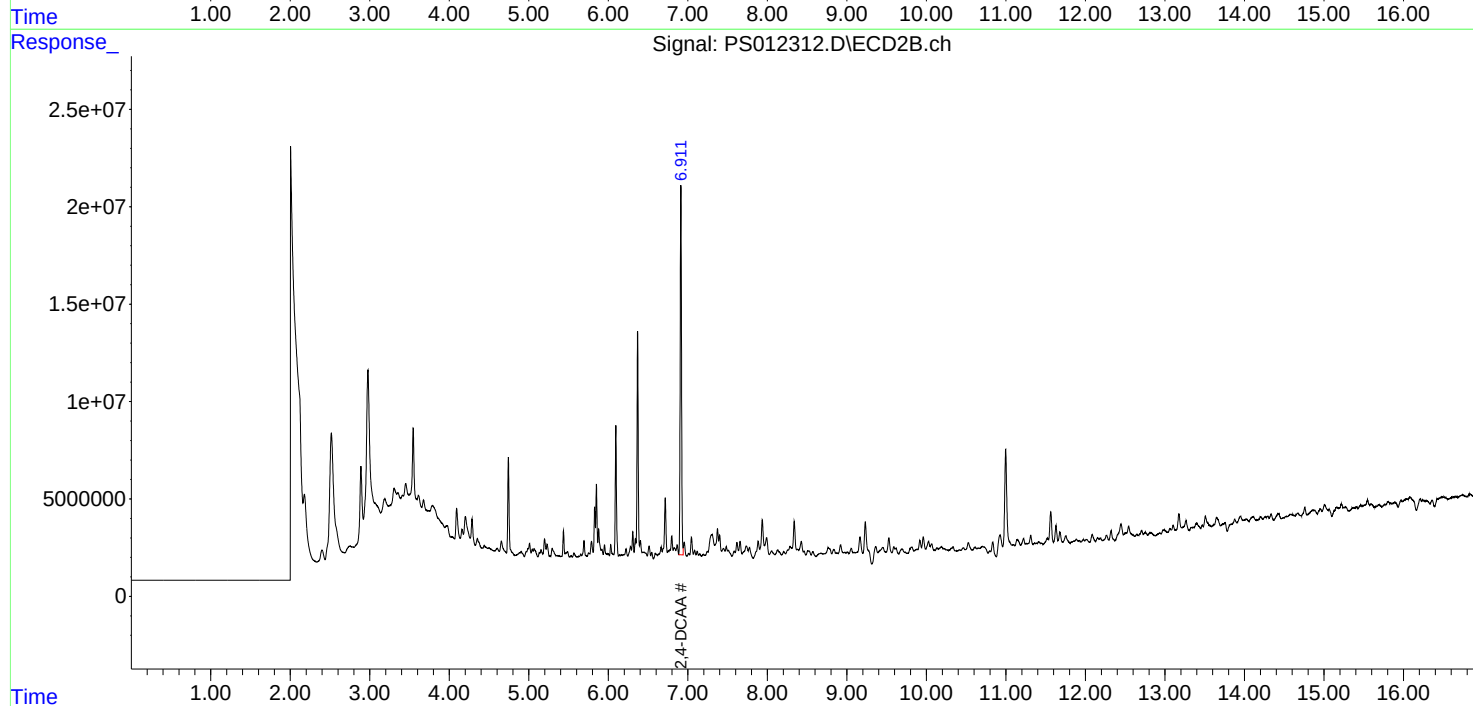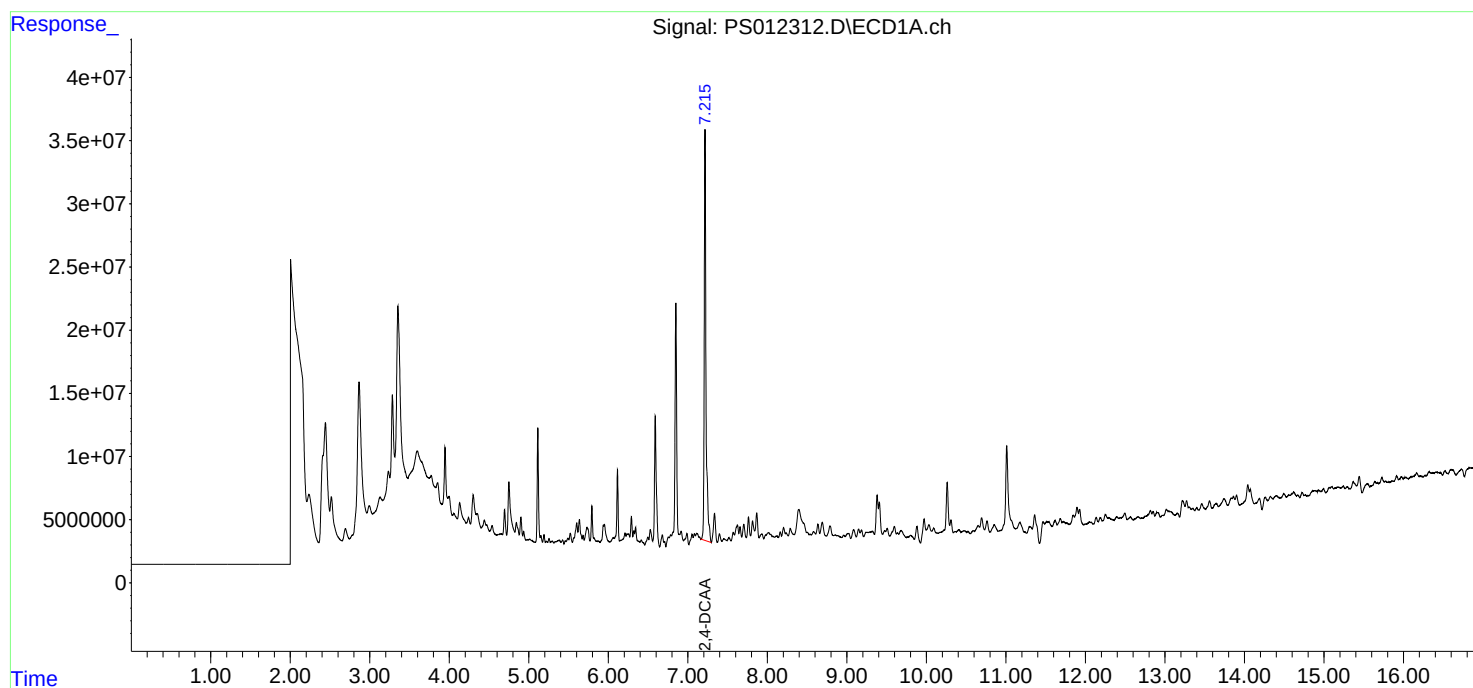

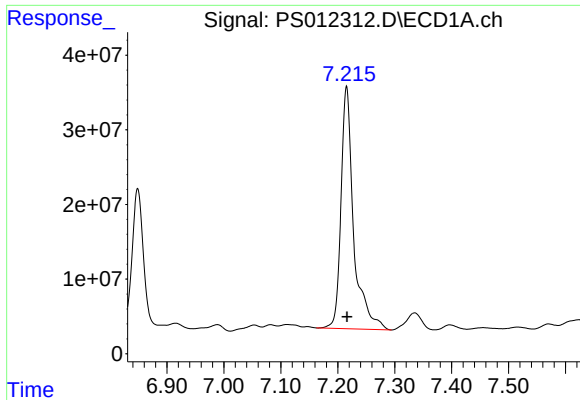


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 500627371
Conc: 461.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-EF-01-TEST1-ABCD-B

Manual Integrations
APPROVED

Ankita
9/17/2020 12:03:56 PM

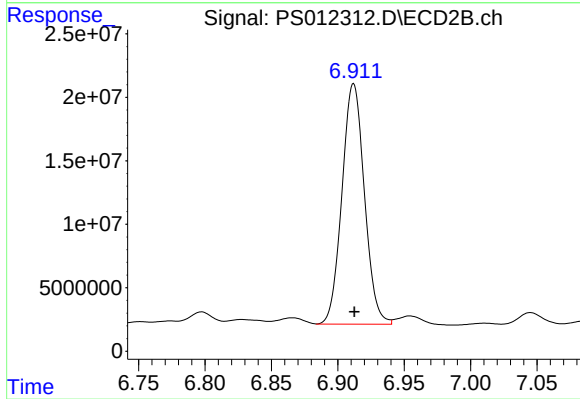

#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 222793624
Conc: 422.27 ng/ml m