

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091621\
 Data File : PS016829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2021 08:35
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:41:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS083121.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 01 10:13:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.186	0.000	3512489	0	2.339	N.D. #
Target Compounds							
3) T	4-Nitroph...	6.970f	0.000	2698066	0	3.489	N.D. #
5) T	DICAMBA	7.371	0.000	7347292	0	1.291	N.D. #
7) T	MCPA	7.633f	0.000	14410203	0	2.460	N.D. #
9) T	2,4-D	8.304	0.000	5705209	0	3.766	N.D. #
10) T	Pentachlo...	8.600	8.258	16708564	6437963	<MDL	<MDL #
11) T	2,4,5-TP ...	9.152	0.000	12606733	0	1.756	N.D. #
12) T	2,4,5-T	9.443	9.002	30761144	9131289	4.299	3.249
13) T	2,4-DB	9.997	0.000	12939957	0	9.362	N.D. #
14) T	DINOSEB	11.140	0.000	21549243	0	3.952	N.D. #
15) T	Picloram	10.971	10.813	546.2E6	205.6E6	61.298	56.100
16) T	DCPA	11.408	10.758	19670643	8513160	1.975	1.962



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091621\
Data File : PS016829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2021 08:35
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:41:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS083121.M
Quant Title : 8080.M
QLast Update : Wed Sep 01 10:13:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

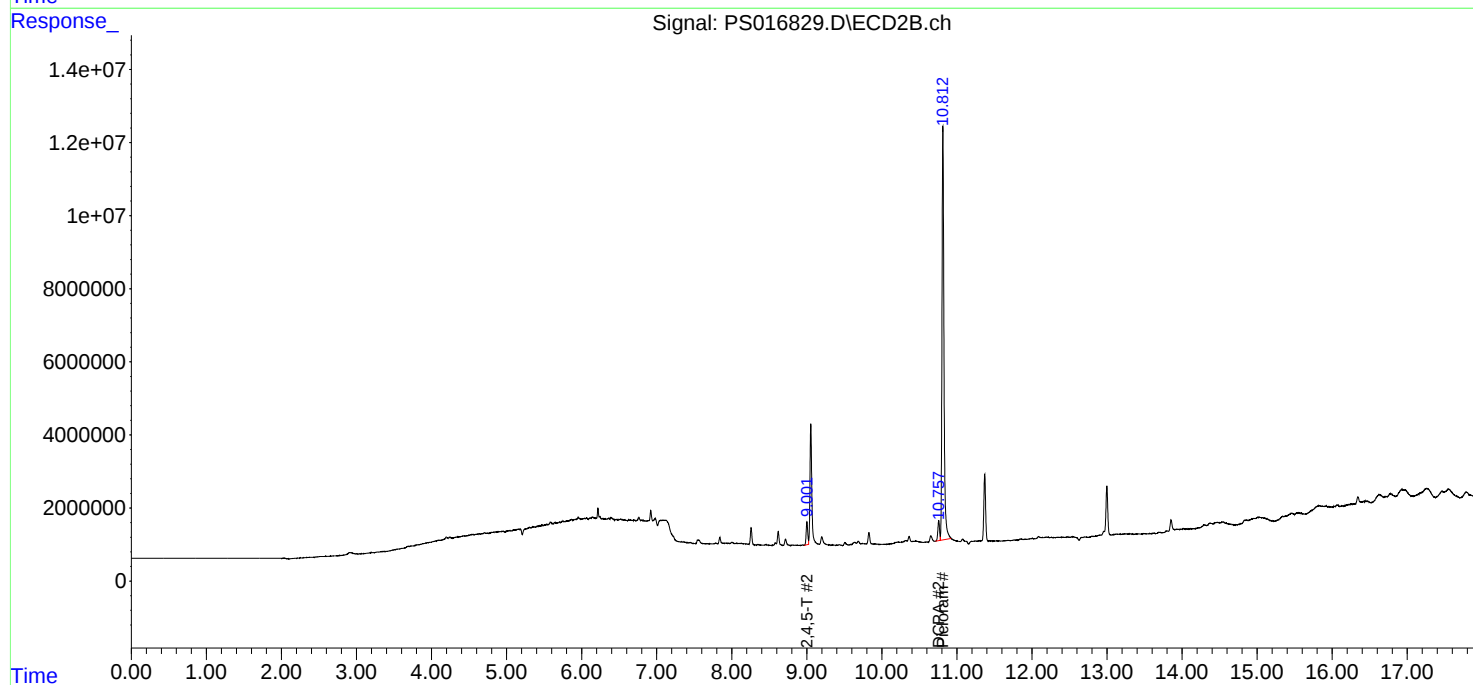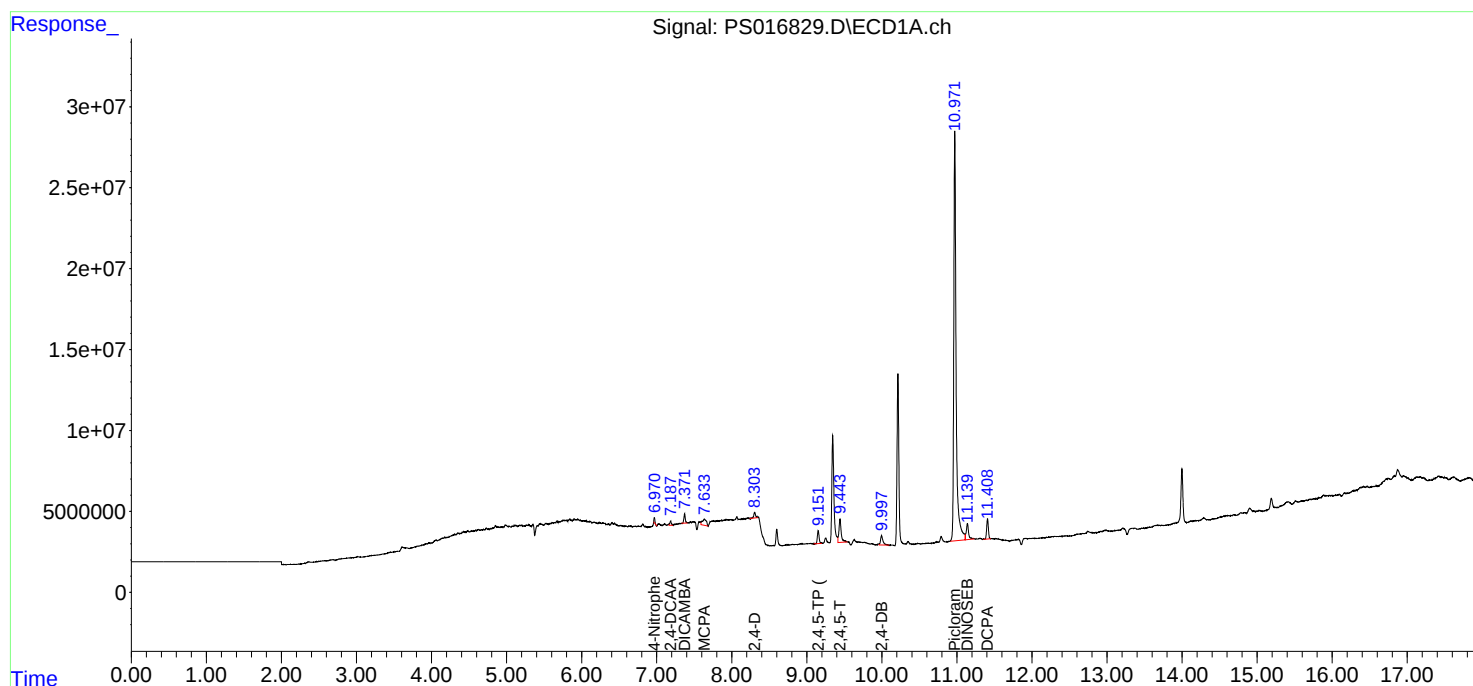


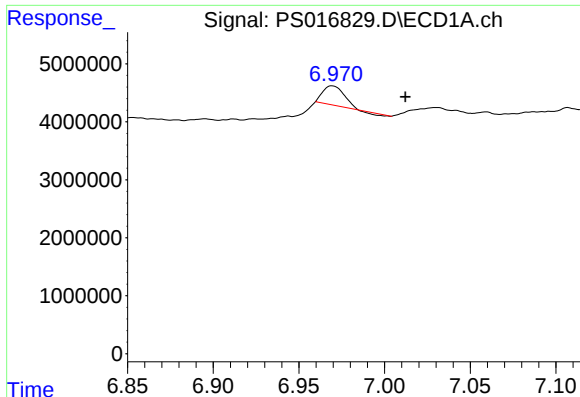

#3 4-Nitrophenol


R.T.: 6.970 min
Delta R.T.: -0.043 min
Response: 2698066
Conc: 3.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

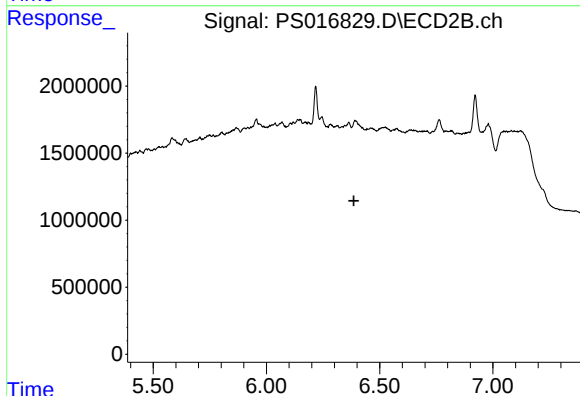


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

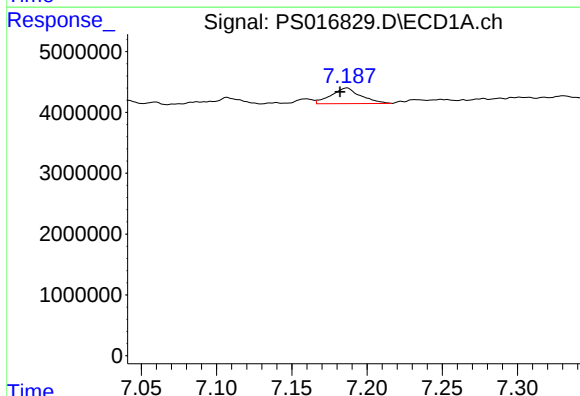


#4 2,4-DCAA

R.T.: 7.186 min
Delta R.T.: 0.004 min
Response: 3512489
Conc: 2.34 ng/ml

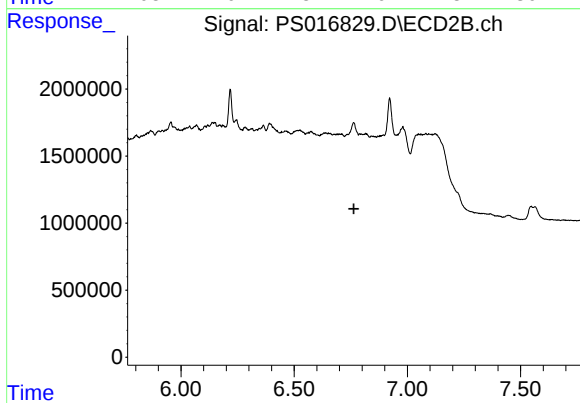

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

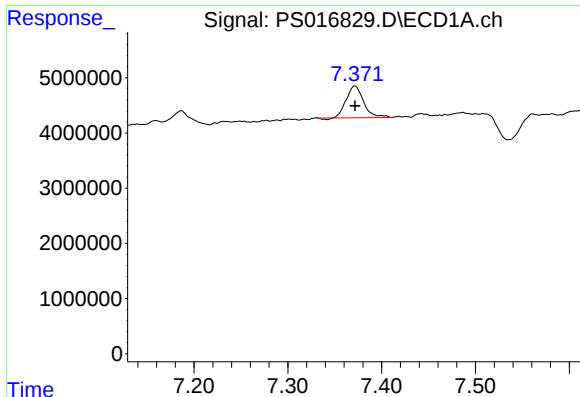

#5 DICAMBA


R.T.: 7.371 min
Delta R.T.: 0.000 min
Response: 7347292
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

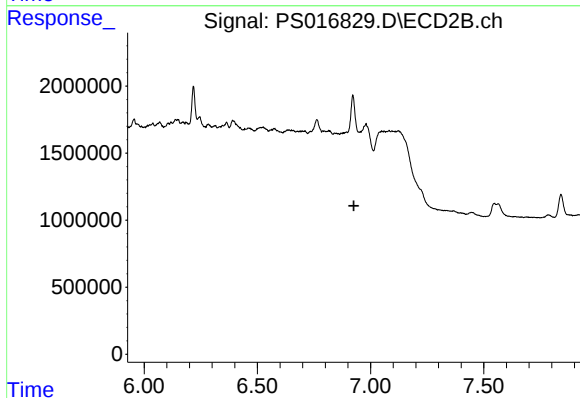


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.926 min
Response: 0
Conc: N.D.

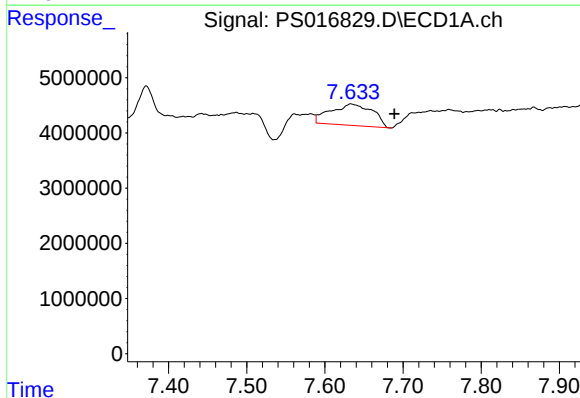


#7 MCPA

R.T.: 7.633 min
Delta R.T.: -0.056 min
Response: 14410203
Conc: 2.46 ug/ml

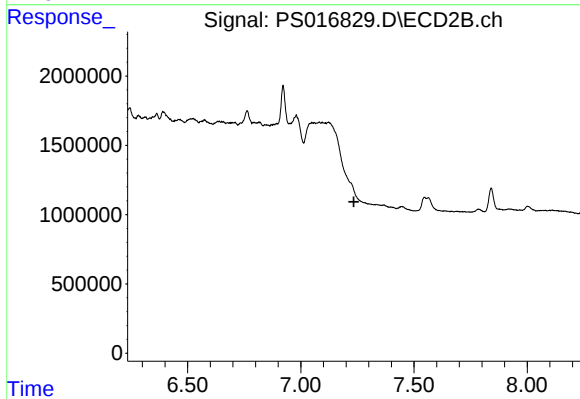

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.234 min
Response: 0
Conc: N.D.

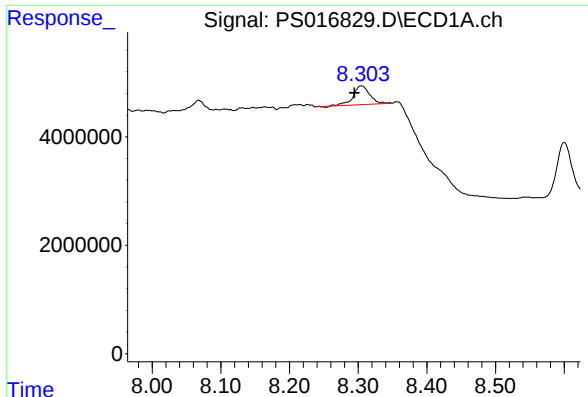

#9 2,4-D


R.T.: 8.304 min
Delta R.T.: 0.010 min
Response: 5705209
Conc: 3.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

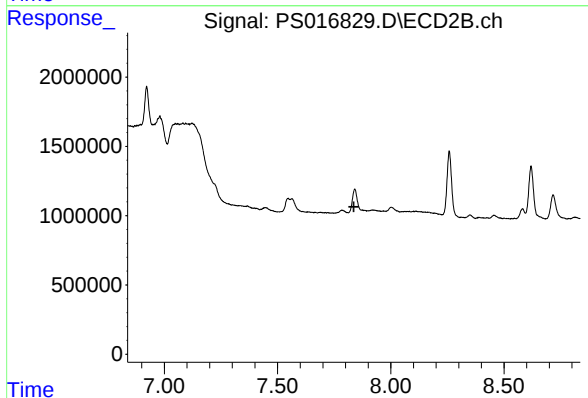


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.837 min
Response: 0
Conc: N.D.

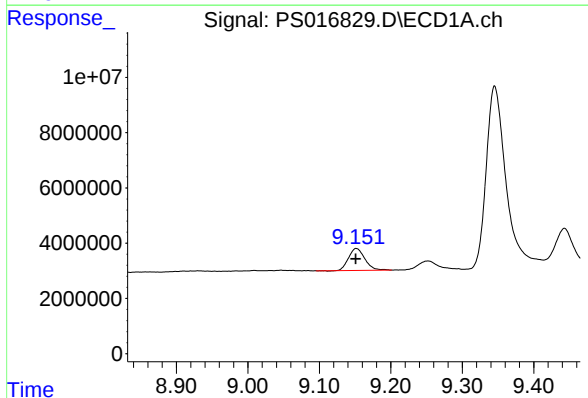


#11 2,4,5-TP (SILVEX)

R.T.: 9.152 min
Delta R.T.: 0.000 min
Response: 12606733
Conc: 1.76 ng/ml

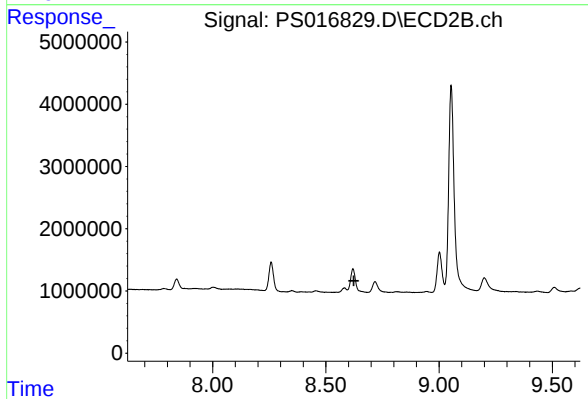

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.624 min
Response: 0
Conc: N.D.

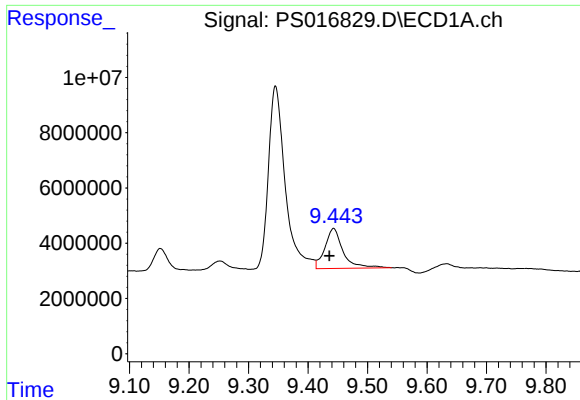

#12 2,4,5-T


R.T.: 9.443 min
Delta R.T.: 0.007 min
Response: 30761144
Conc: 4.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

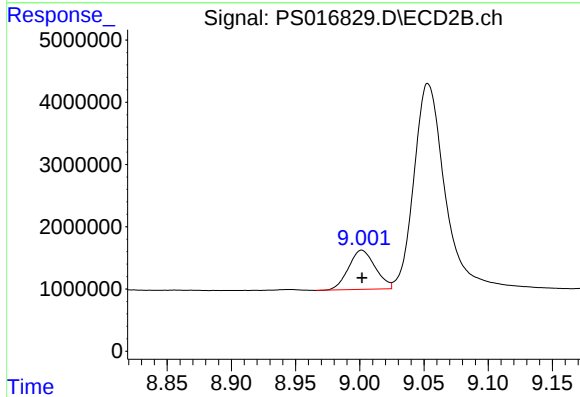


#12 2,4,5-T

R.T.: 9.002 min
Delta R.T.: 0.000 min
Response: 9131289
Conc: 3.25 ng/ml

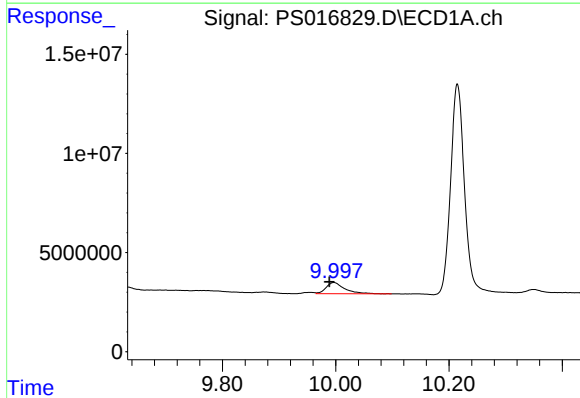


#13 2,4-DB

R.T.: 9.997 min
Delta R.T.: 0.008 min
Response: 12939957
Conc: 9.36 ng/ml

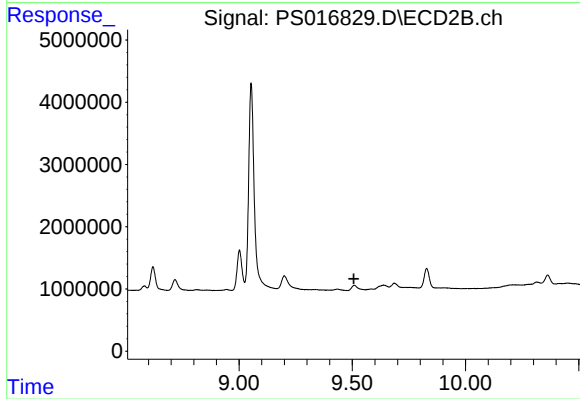

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.507 min
Response: 0
Conc: N.D.

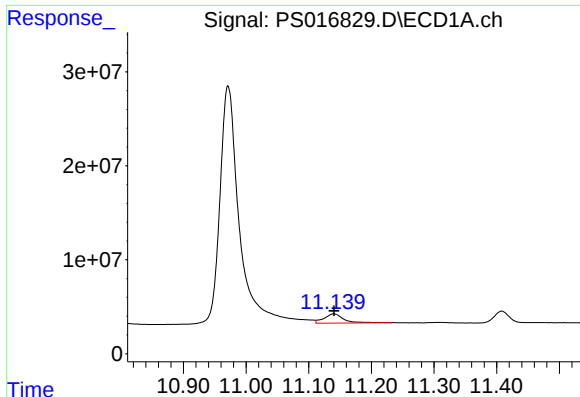

#14 DINOSEB


R.T.: 11.140 min
Delta R.T.: 0.000 min
Response: 21549243
Conc: 3.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

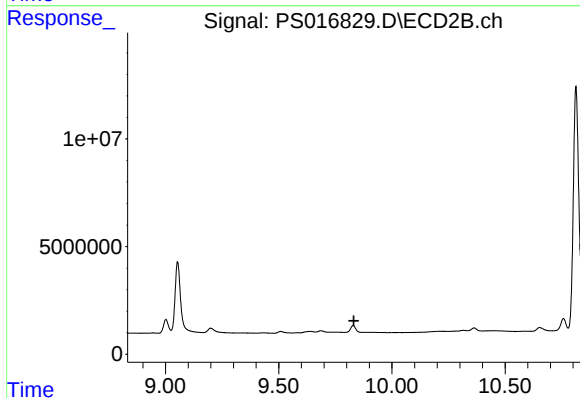


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.832 min
Response: 0
Conc: N.D.

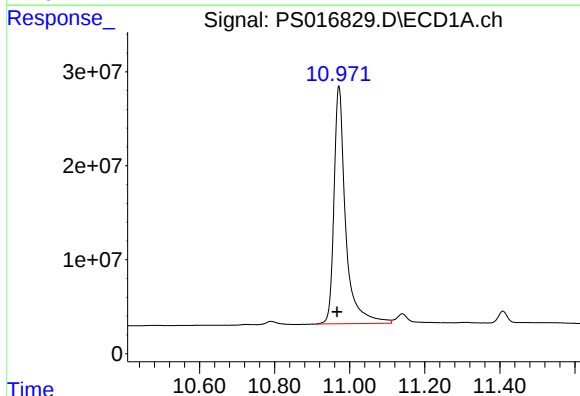


#15 Picloram

R.T.: 10.971 min
Delta R.T.: 0.005 min
Response: 546217231
Conc: 61.30 ng/ml

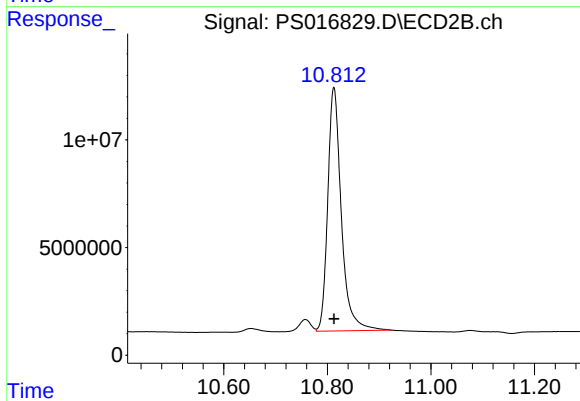

#15 Picloram


R.T.: 10.813 min
Delta R.T.: 0.000 min
Response: 205561654
Conc: 56.10 ng/ml

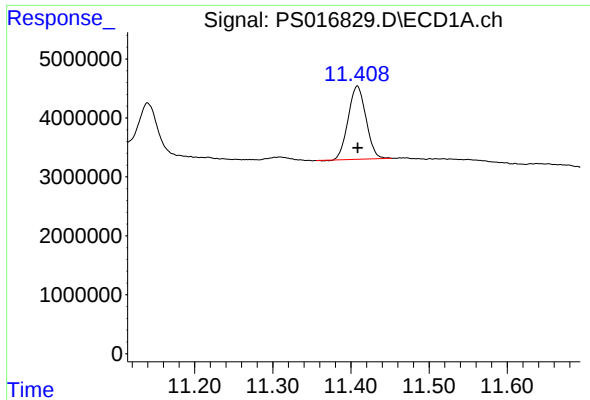

#16 DCPA

R.T.: 11.408 min
Delta R.T.: 0.000 min
Response: 19670643
Conc: 1.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

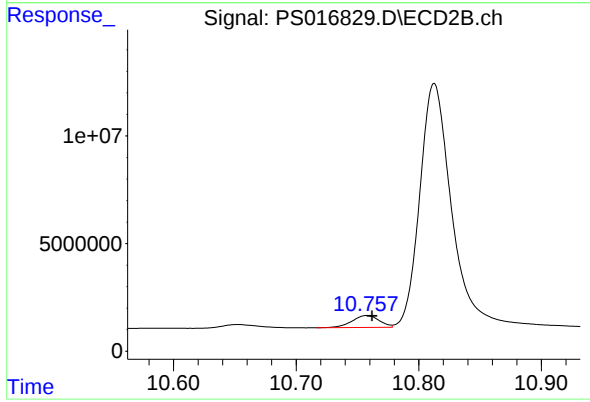

#16 DCPA

R.T.: 10.758 min
Delta R.T.: -0.004 min
Response: 8513160
Conc: 1.96 ng/ml