

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091621\
 Data File : PS016836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2021 11:42
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:43:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS083121.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 01 10:13:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.180	6.762	765.9E6	345.7E6	509.956	666.966 #
Target Compounds							
3) T	4-Nitroph...	6.972f	0.000	3889424	0	5.030	N.D. #
9) T	2,4-D	8.363f	0.000	128.2E6	0	84.642	N.D. #
15) T	Picloram	11.025f	10.847	22158425	10349742	2.487	2.825



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091621\
Data File : PS016836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2021 11:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:43:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS083121.M
Quant Title : 8080.M
QLast Update : Wed Sep 01 10:13:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

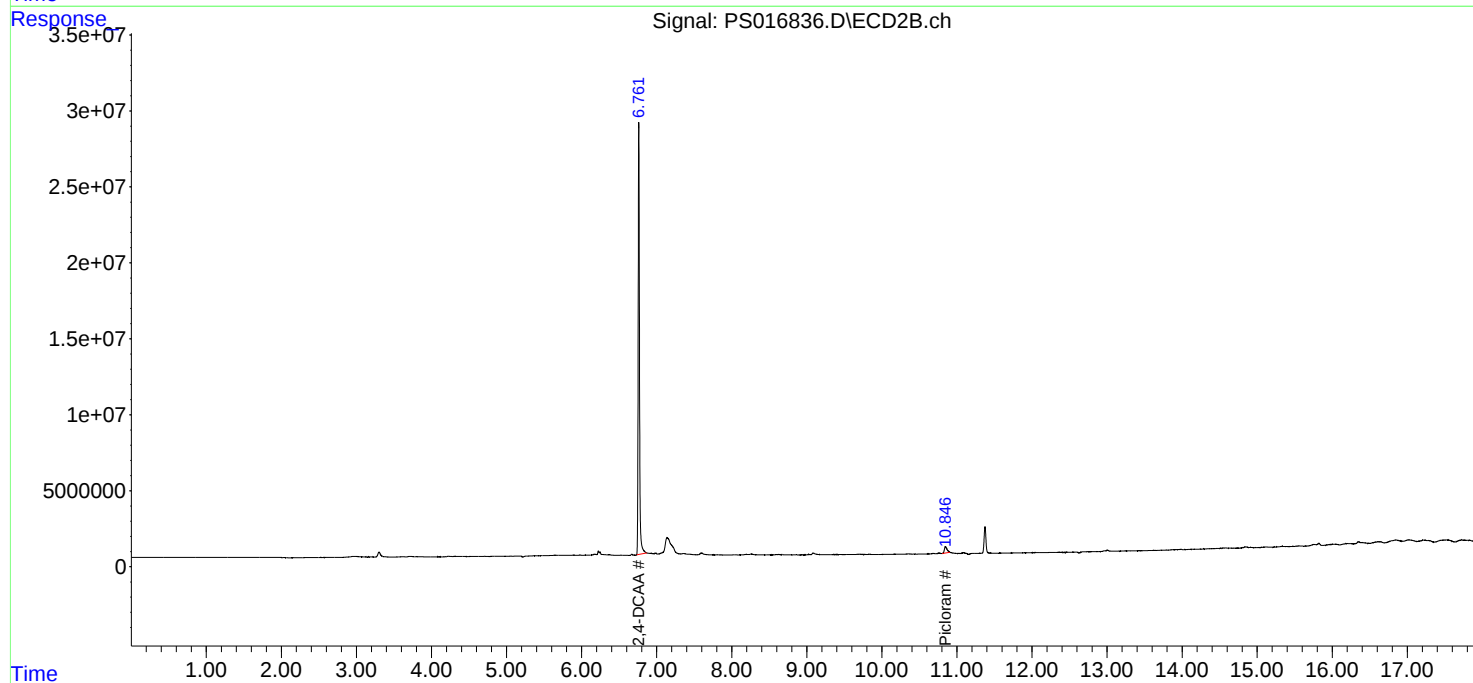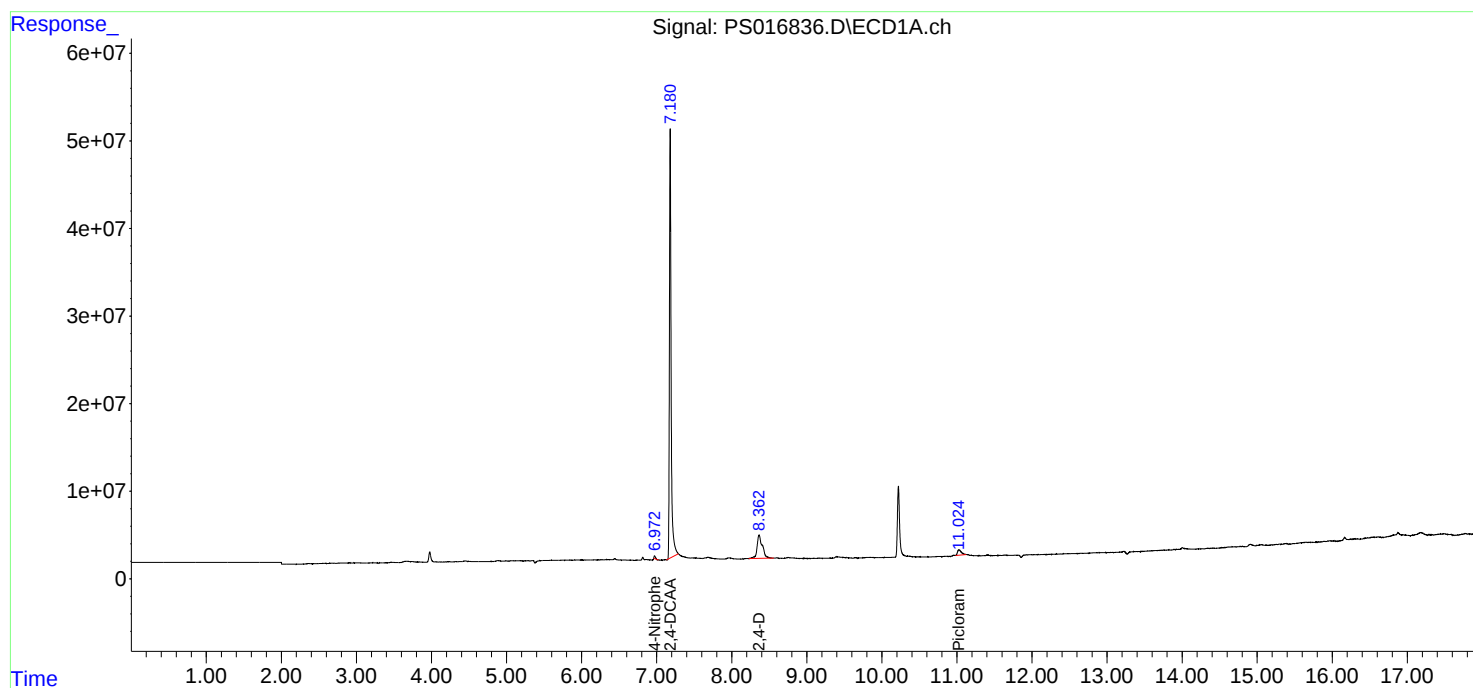


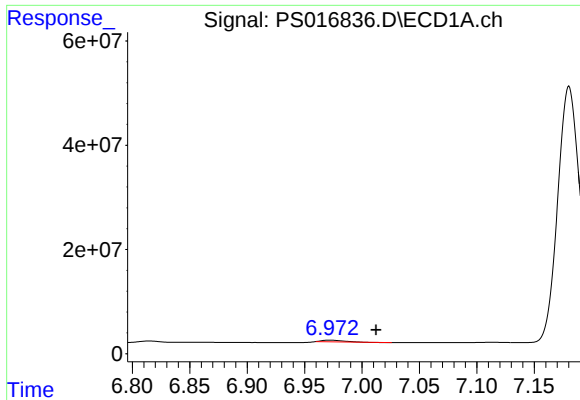

#3 4-Nitrophenol


R.T.: 6.972 min
Delta R.T.: -0.040 min
Response: 3889424
Conc: 5.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

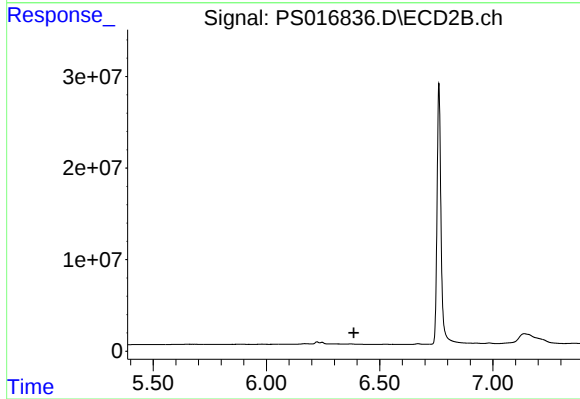


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

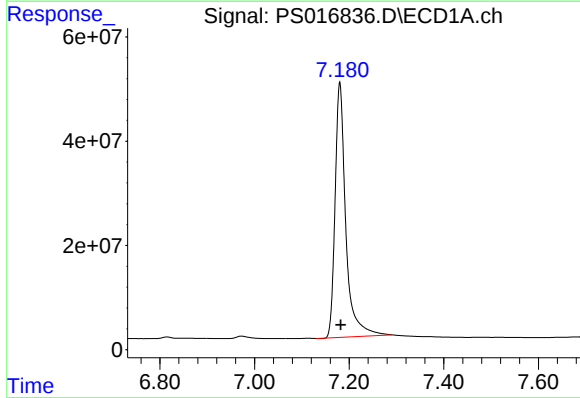


#4 2,4-DCAA

R.T.: 7.180 min
Delta R.T.: -0.002 min
Response: 765883862
Conc: 509.96 ng/ml

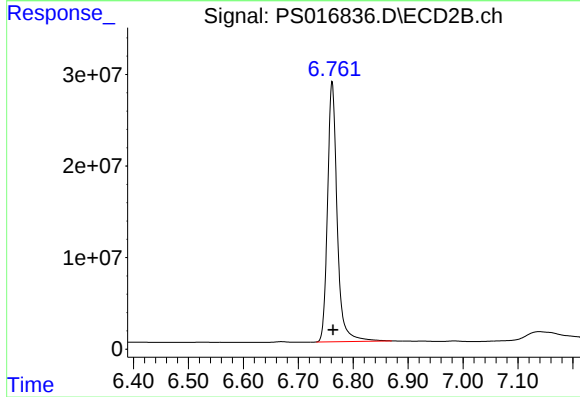

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 345712733
Conc: 666.97 ng/ml

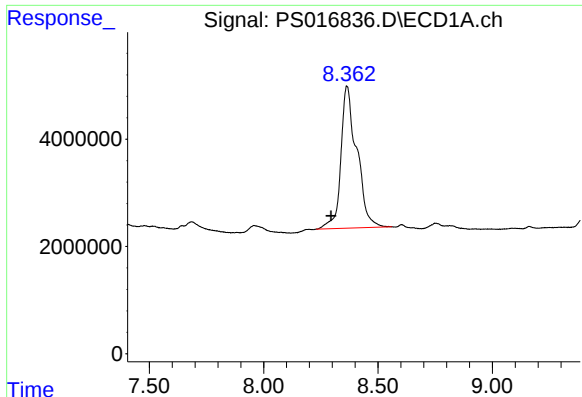

#9 2,4-D


R.T.: 8.363 min
Delta R.T.: 0.069 min
Response: 128212238
Conc: 84.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

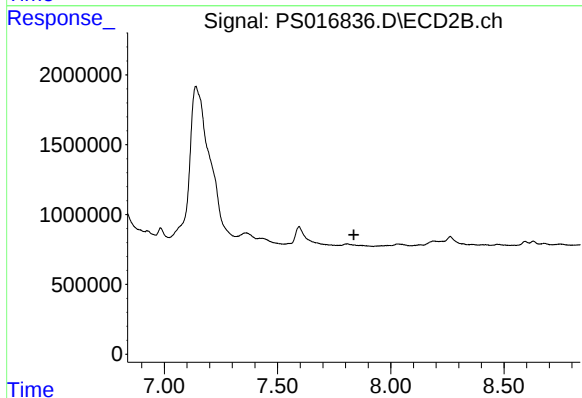


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.837 min
Response: 0
Conc: N.D.

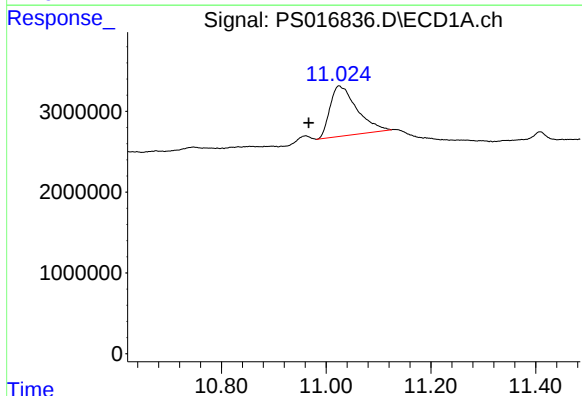

#15 Picloram

R.T.: 11.025 min
Delta R.T.: 0.058 min
Response: 22158425
Conc: 2.49 ng/ml

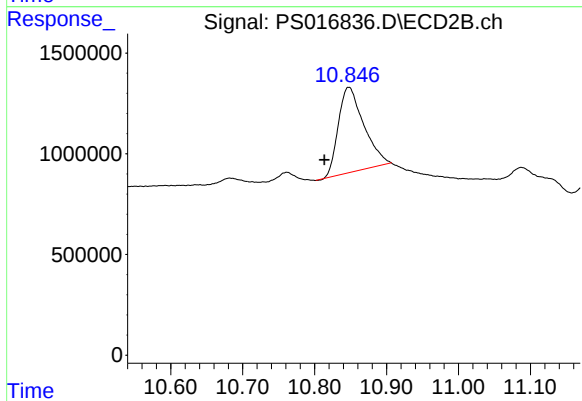

#15 Picloram

R.T.: 10.847 min
Delta R.T.: 0.034 min
Response: 10349742
Conc: 2.82 ng/ml