

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091622\
 Data File : PS020569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 08:59
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 14:39:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.176	6.757	1963.9E6	520.9E6	570.656	611.562
Target Compounds							
1) T	Dalapon	3.040	0.000	953276	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.441f	0.000	144.8E6	0	29.040	N.D. #
3) T	4-Nitroph...	6.963f	0.000	12450029	0	133.576	N.D. #
5) T	DICAMBA	0.000	6.983f	0	23650036	N.D.	6.143
6) T	MCP	0.000	6.983	0	23650036	N.D.	8.189
7) T	MCPA	7.712	7.152f	3043707	23438070	<MDL	5.428 #
9) T	2,4-D	8.364f	0.000	285.0E6	0	61.311	N.D. #
10) T	Pentachlo...	8.613	0.000	2390884	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.159	0.000	2722478	0	<MDL	N.D. #
12) T	2,4,5-T	9.452	0.000	6661372	0	<MDL	N.D. #
13) T	2,4-DB	9.979	0.000	3555362	0	<MDL	N.D. #
15) T	Picloram	11.005	10.843	239.3E6	22685313	7.950	2.817 #
16) T	DCPA	11.402	10.760	7287034	3126469	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091622\
Data File : PS020569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 08:59
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 14:39:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

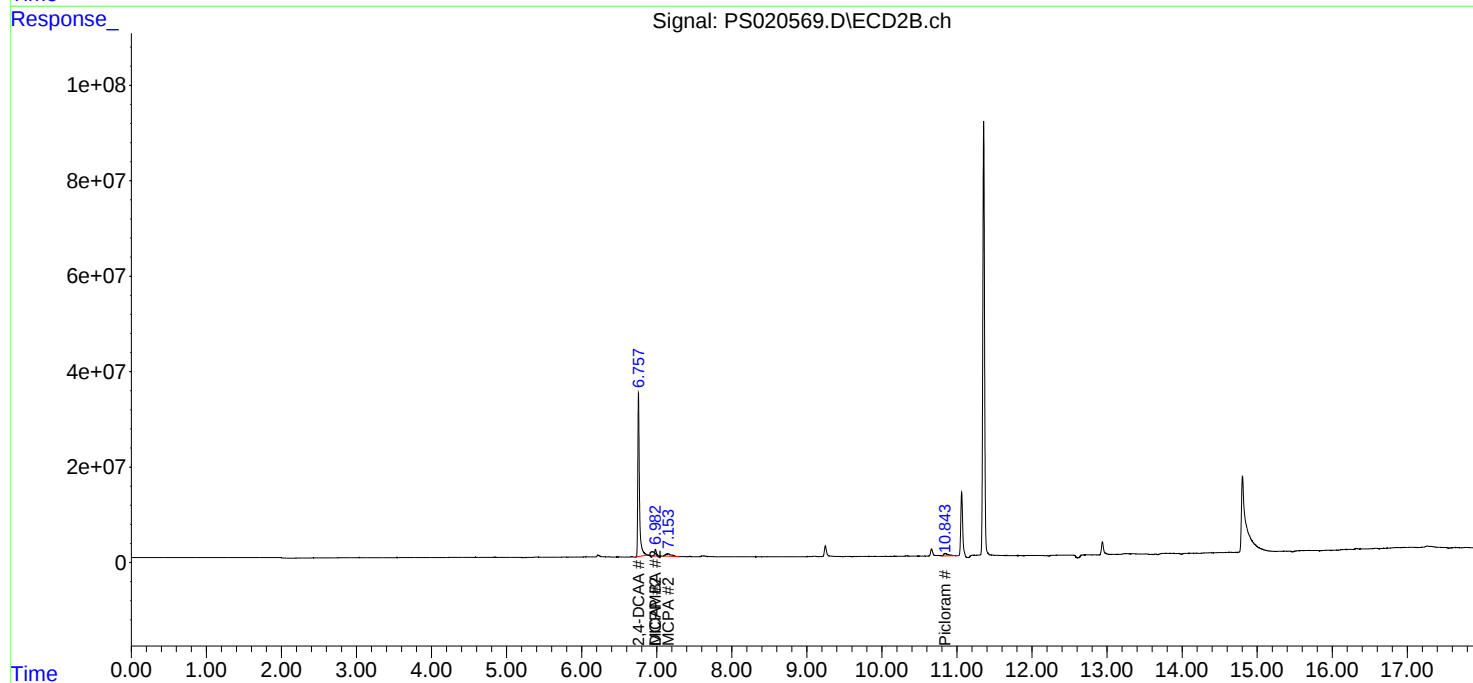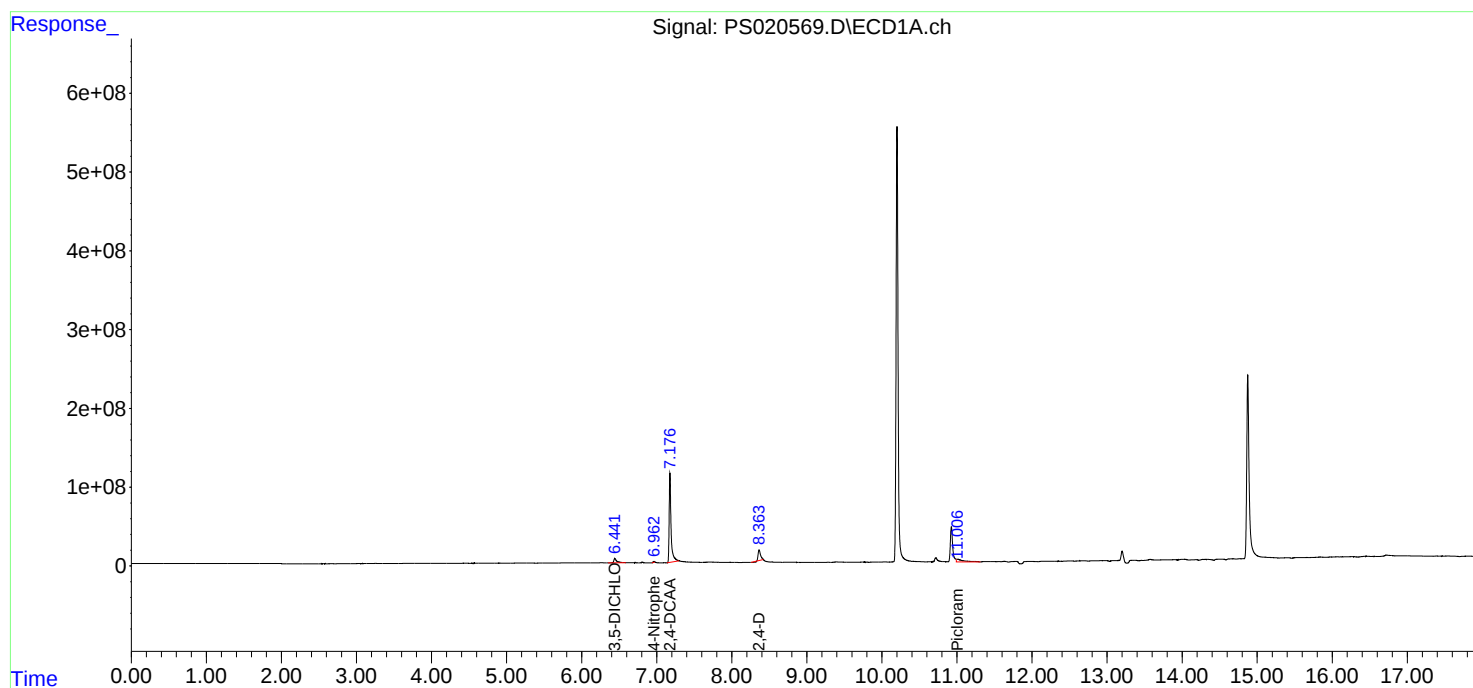


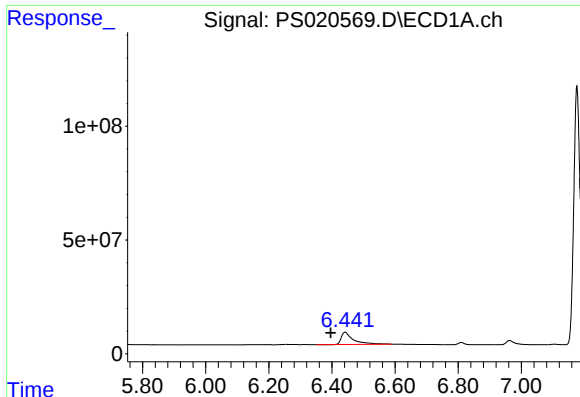

#2 3,5-DICHLORO BENZOIC ACID


R.T.: 6.441 min
Delta R.T.: 0.045 min
Response: 144811721
Conc: 29.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

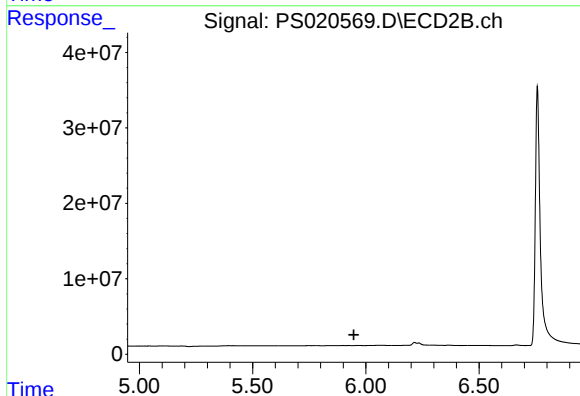


#2 3,5-DICHLORO BENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

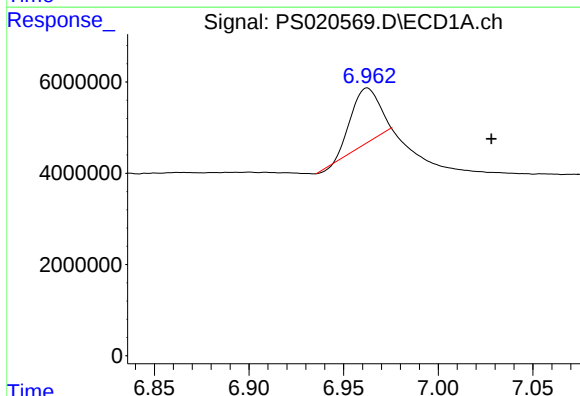


#3 4-Nitrophenol

R.T.: 6.963 min
Delta R.T.: -0.065 min
Response: 12450029
Conc: 133.58 ng/ml

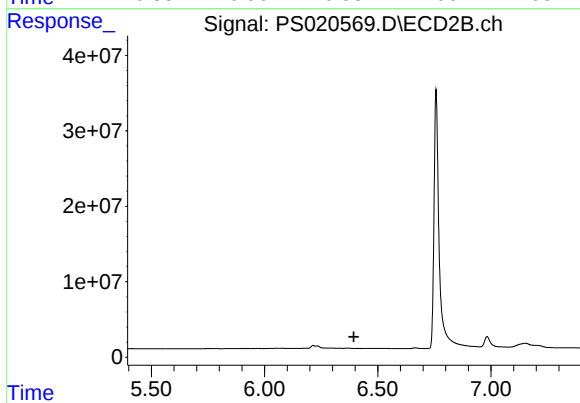

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

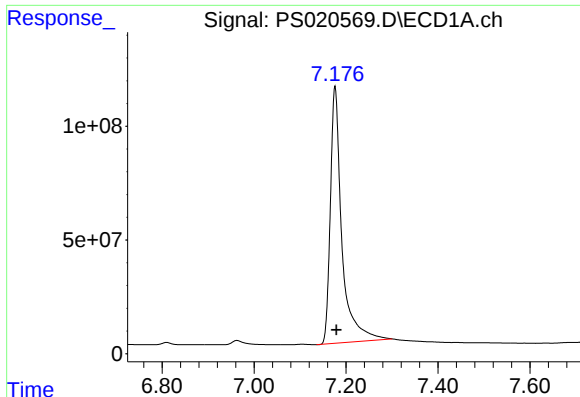

#4 2,4-DCAA


R.T.: 7.176 min
Delta R.T.: -0.003 min
Response: 1963906098
Conc: 570.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

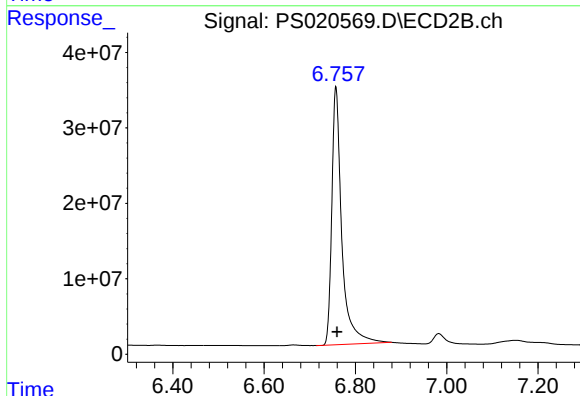


#4 2,4-DCAA

R.T.: 6.757 min
Delta R.T.: -0.003 min
Response: 520864061
Conc: 611.56 ng/ml

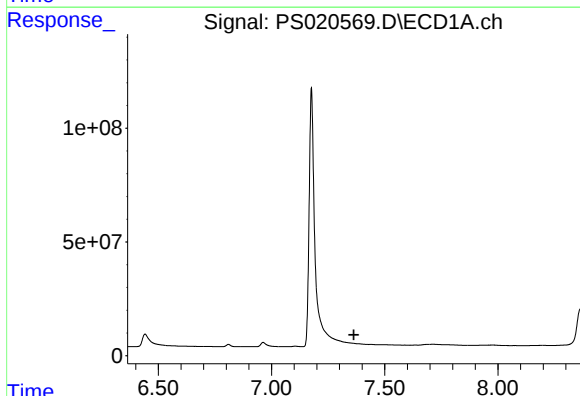


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.363 min
Response: 0
Conc: N.D.

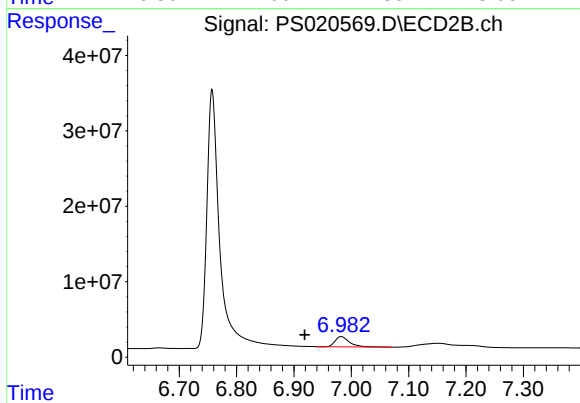

#5 DICAMBA


R.T.: 6.983 min
Delta R.T.: 0.064 min
Response: 23650036
Conc: 6.14 ng/ml

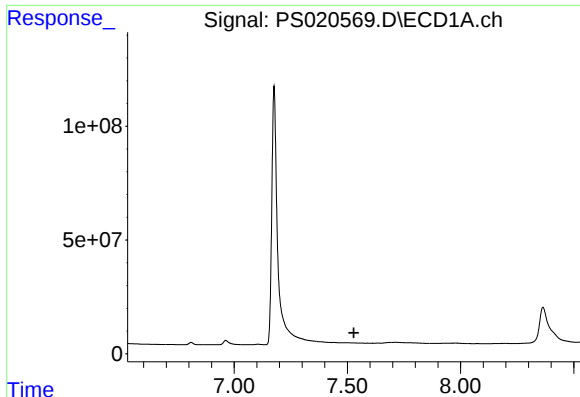

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

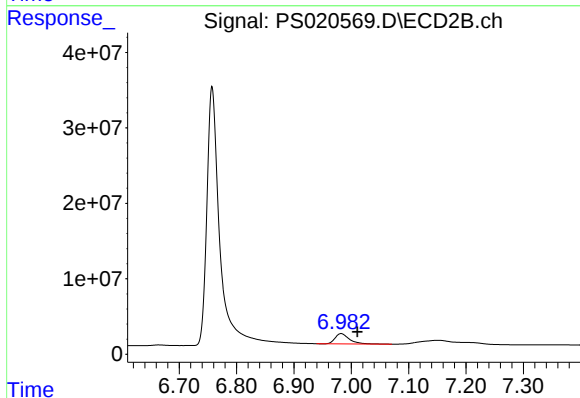


#6 MCPP

R.T.: 6.983 min
Delta R.T.: -0.028 min
Response: 23650036
Conc: 8.19 ug/ml

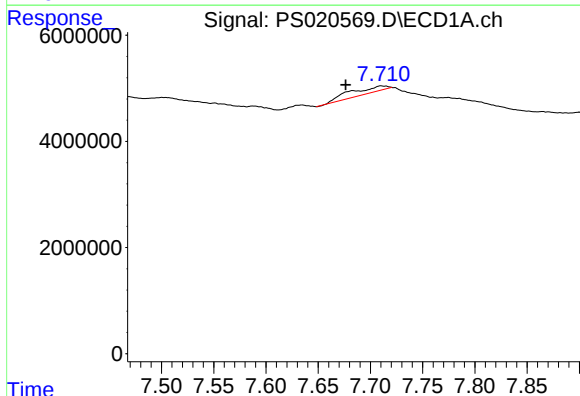


#7 MCPA

R.T.: 7.712 min
Delta R.T.: 0.035 min
Response: 3043707
Conc: N.D.

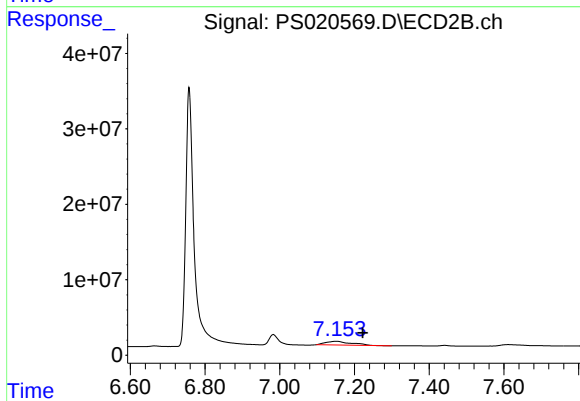

#7 MCPA


R.T.: 7.152 min
Delta R.T.: -0.070 min
Response: 23438070
Conc: 5.43 ug/ml

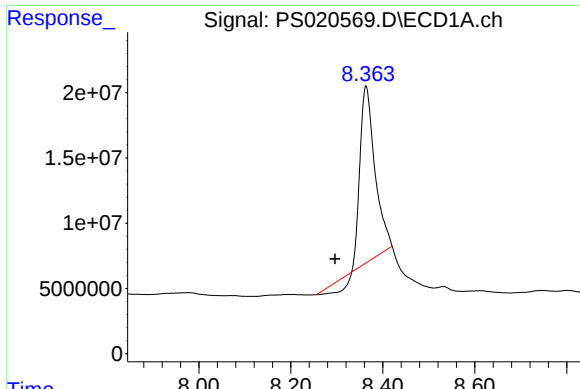

#9 2,4-D


R.T.: 8.364 min
Delta R.T.: 0.067 min
Response: 284977088
Conc: 61.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

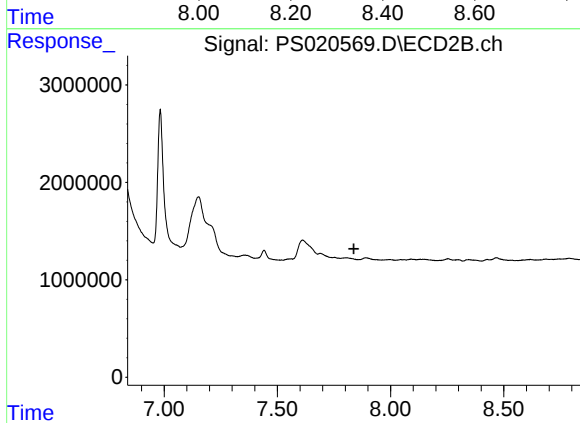


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

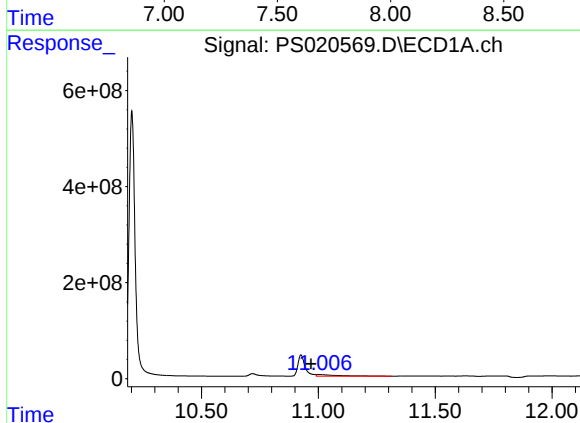

#15 Picloram

R.T.: 11.005 min
Delta R.T.: 0.037 min
Response: 239253432
Conc: 7.95 ng/ml

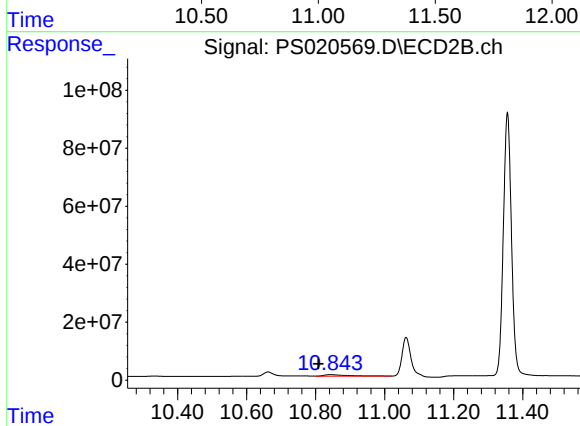

#15 Picloram

R.T.: 10.843 min
Delta R.T.: 0.035 min
Response: 22685313
Conc: 2.82 ng/ml