

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091622\
 Data File : PS020579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 14:00
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 17:54:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.178	6.759	1649.9E6	452.7E6	479.405	531.573
Target Compounds							
1) T	Dalapon	3.035	0.000	640731	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.445f	0.000	1753266	0	<MDL	N.D. #
7) T	MCPA	7.638	0.000	1046918	0	<MDL	N.D. #
9) T	2,4-D	8.359f	0.000	139.5E6	0	30.014	N.D. #
10) T	Pentachlo...	8.592	0.000	1928522	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.154	0.000	2508867	0	<MDL	N.D. #
12) T	2,4,5-T	9.418	0.000	7312858	0	<MDL	N.D. #
13) T	2,4-DB	9.947	0.000	917029	0	<MDL	N.D. #
14) T	DINOSEB	11.122	0.000	5969386	0	<MDL	N.D. #
15) T	Picloram	10.956	10.873f	27273476	1986499	<MDL	<MDL #
16) T	DCPA	11.395	0.000	4556827	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091622\
Data File : PS020579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 14:00
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 17:54:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

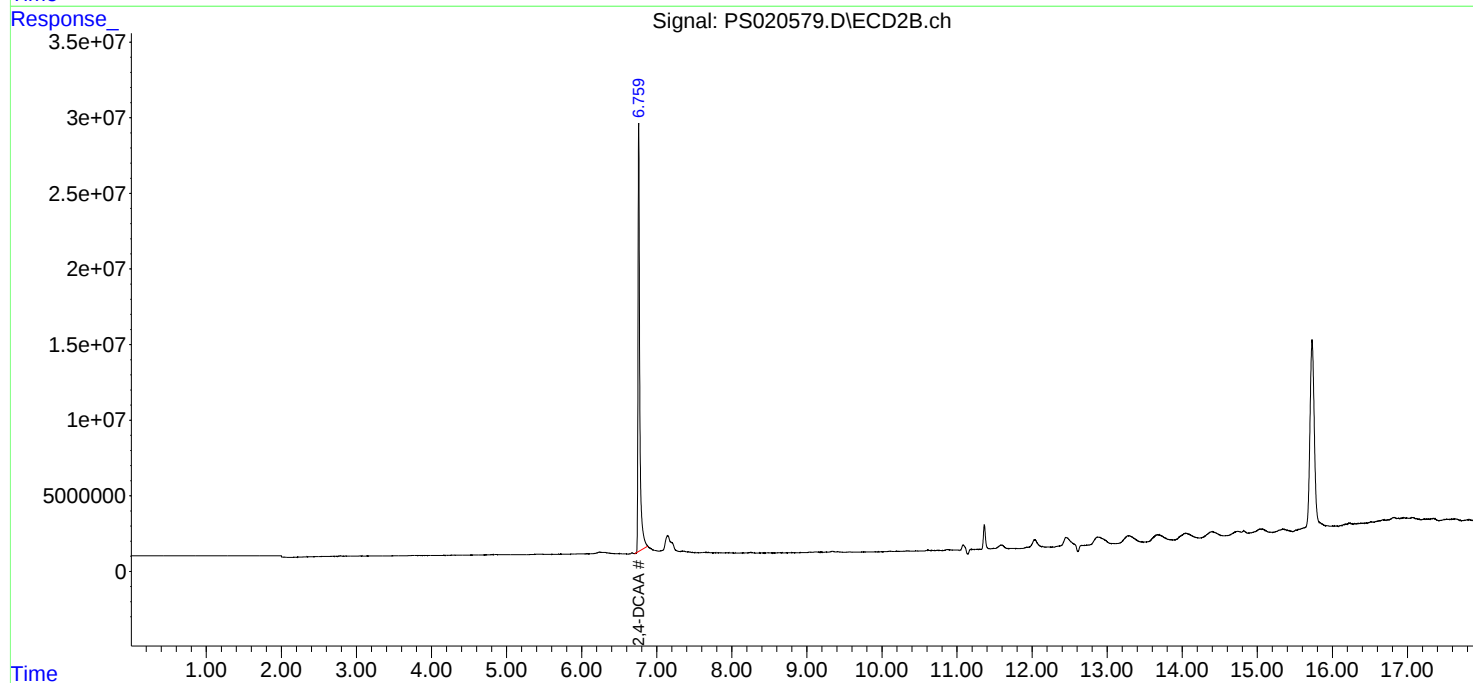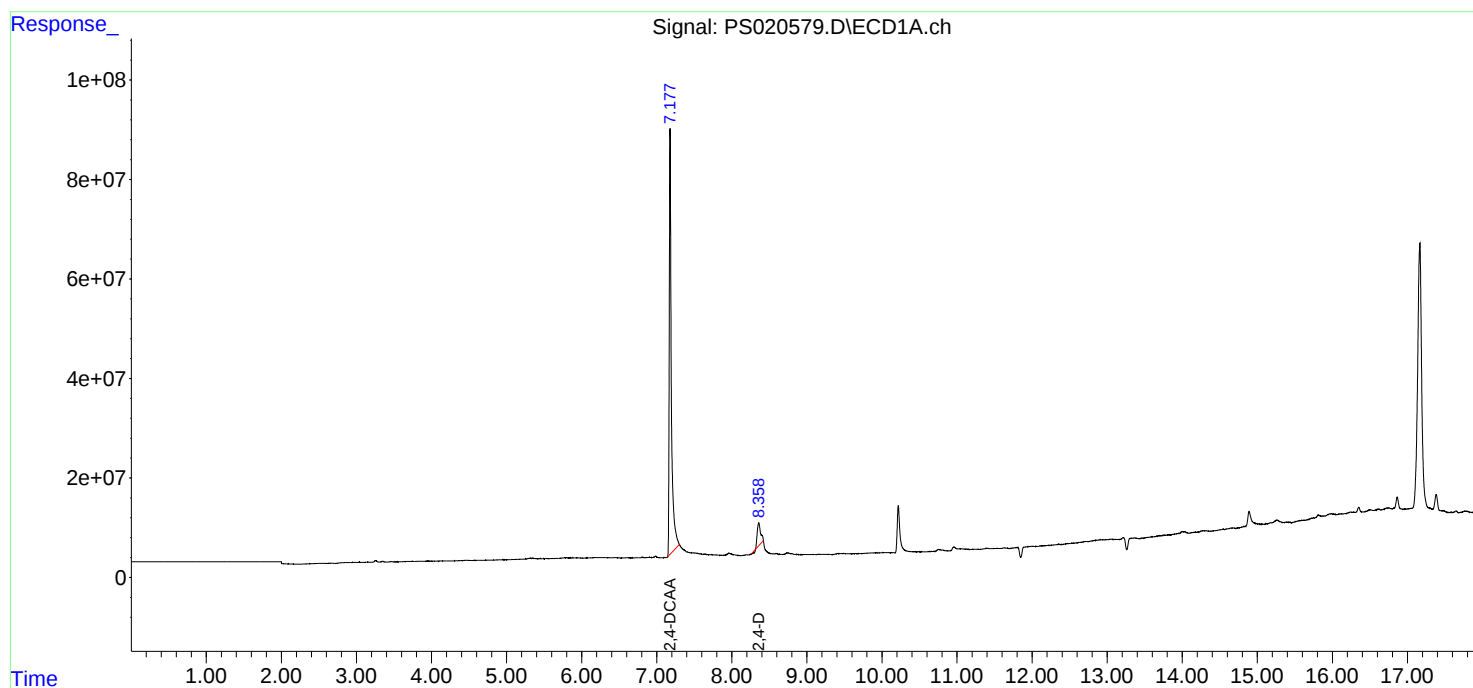


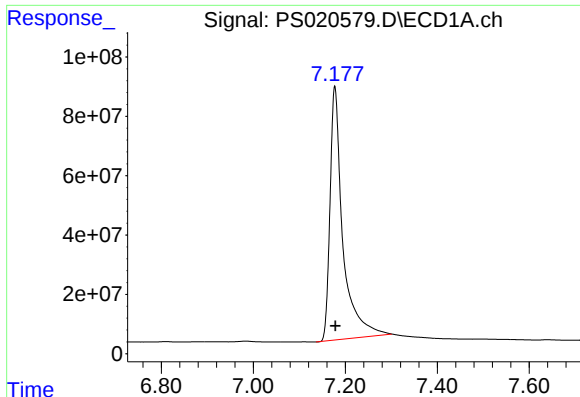

#4 2,4-DCAA


R.T.: 7.178 min
Delta R.T.: -0.001 min
Response: 1649866306
Conc: 479.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

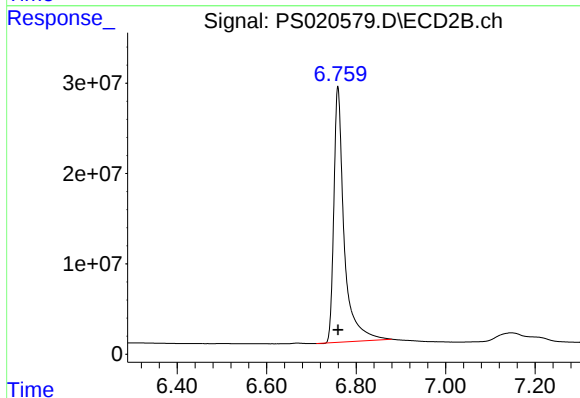


#4 2,4-DCAA

R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 452738149
Conc: 531.57 ng/ml

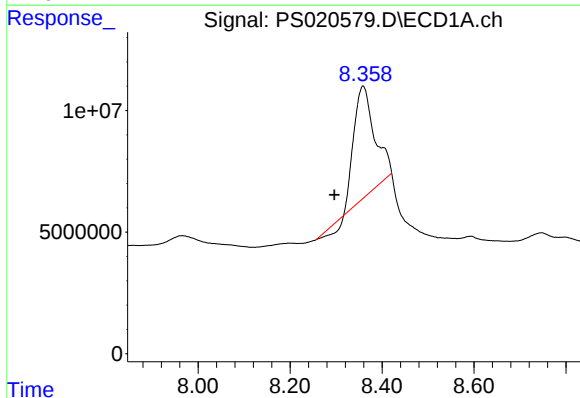

#9 2,4-D

R.T.: 8.359 min
Delta R.T.: 0.062 min
Response: 139507884
Conc: 30.01 ng/ml

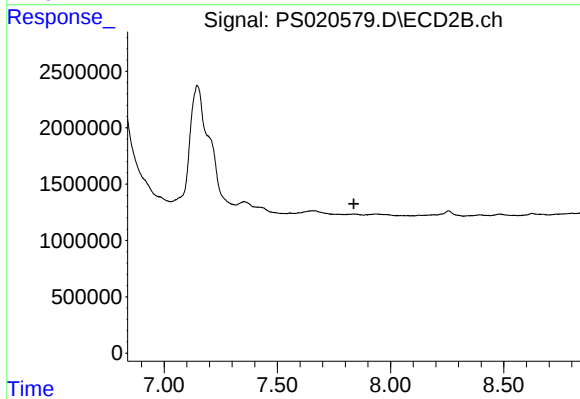

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.