

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091624\
 Data File : PS027693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 13:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:12:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.109	7.630	1240.6E6	479.7E6	498.721	484.005
Target Compounds							
1) T	Dalapon	2.539	0.000	19005982	0	4.587	N.D. #
2) T	3,5-DICHL...	0.000	6.633f	0	1376962	N.D.	<MDL
3) T	4-Nitroph...	6.910	0.000	3762854	0	2.222	N.D. #
5) T	DICAMBA	0.000	7.820	0	9362110	N.D.	2.125
8) T	DICHLORPROP	0.000	8.575f	0	706540	N.D.	<MDL
10) T	Pentachlo...	8.482	9.328f	3433693	560763	<MDL	<MDL #
11) T	2,4,5-TP ...	9.051	9.750	4860033	1153094	<MDL	<MDL #
12) T	2,4,5-T	9.345	10.164	3761642	3379899	<MDL	<MDL #
13) T	2,4-DB	9.923	0.000	1903260	0	<MDL	N.D. #
14) T	DINOSEB	11.080	11.099	4519505	1218662	<MDL	<MDL #
15) T	Picloram	10.902	12.188	64576545	11026208	3.452	2.373 #
16) T	DCPA	11.380	12.135	8459391	4604110	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091624\
Data File : PS027693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 13:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:12:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

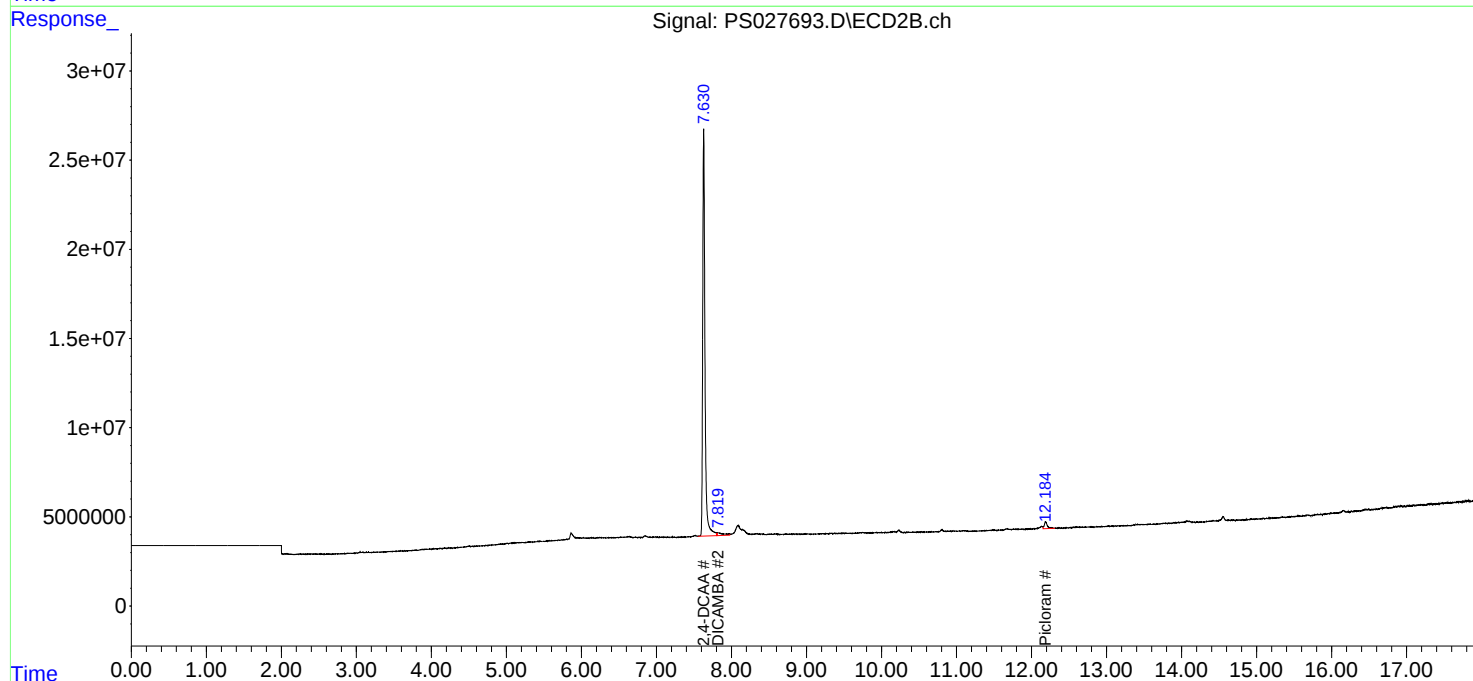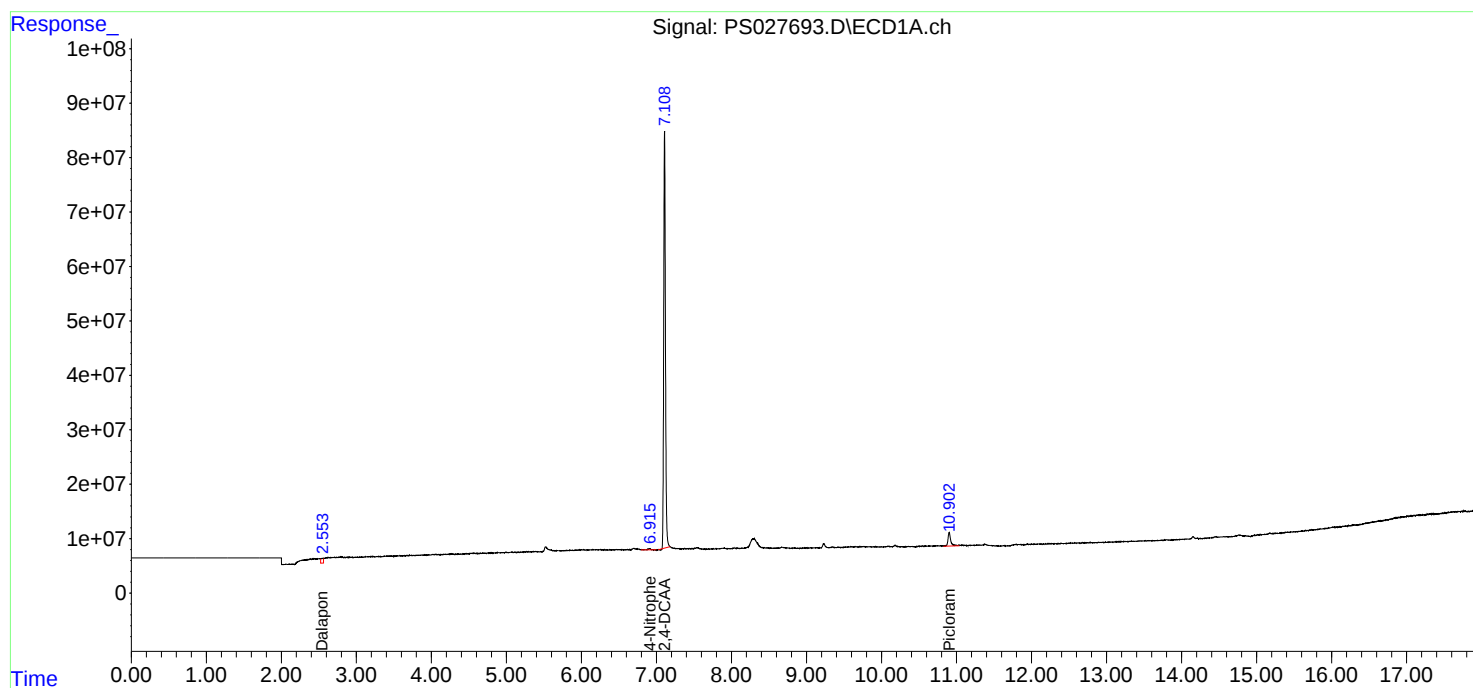


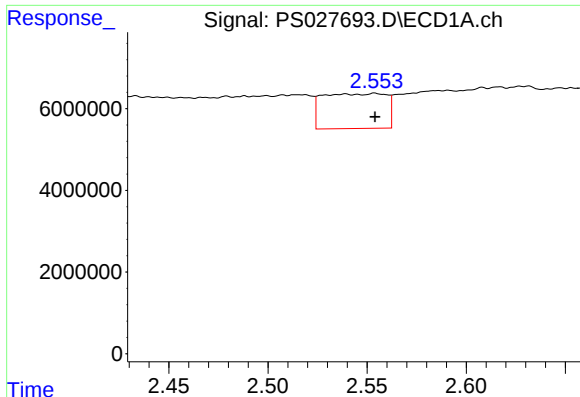

#1 Dalapon


R.T.: 2.539 min
Delta R.T.: -0.015 min
Response: 19005982
Conc: 4.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

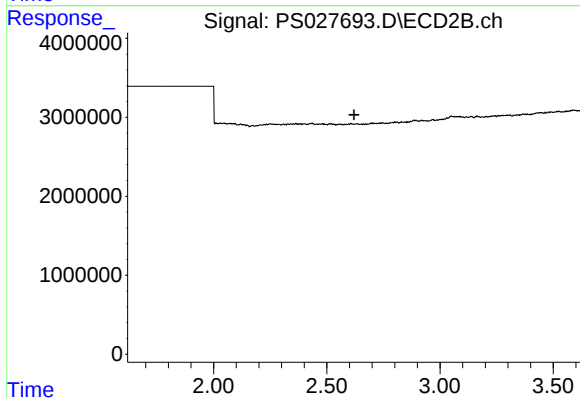


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

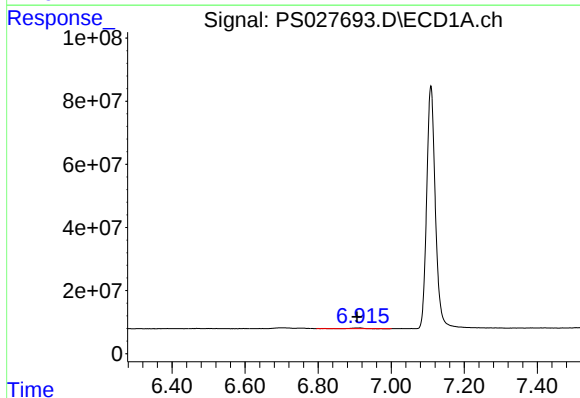


#3 4-Nitrophenol

R.T.: 6.910 min
Delta R.T.: 0.003 min
Response: 3762854
Conc: 2.22 ng/ml

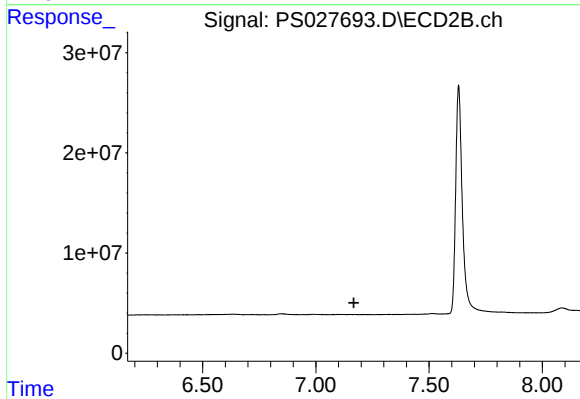

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

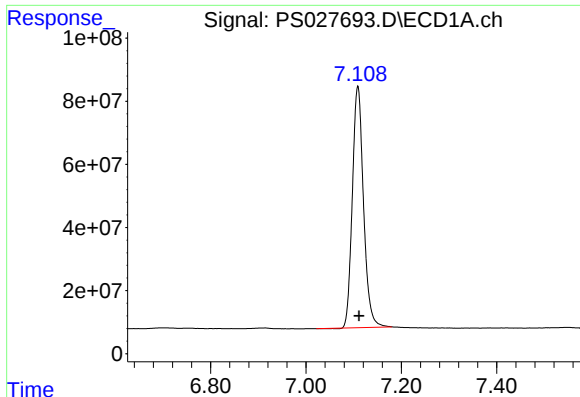

#4 2,4-DCAA


R.T.: 7.109 min
Delta R.T.: -0.003 min
Response: 1240622268
Conc: 498.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

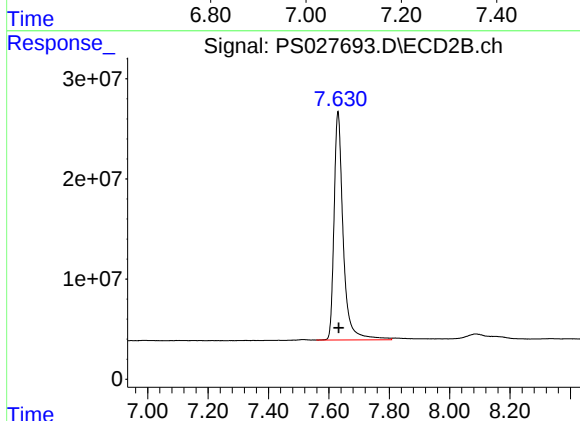


#4 2,4-DCAA

R.T.: 7.630 min
Delta R.T.: -0.003 min
Response: 479664752
Conc: 484.00 ng/ml

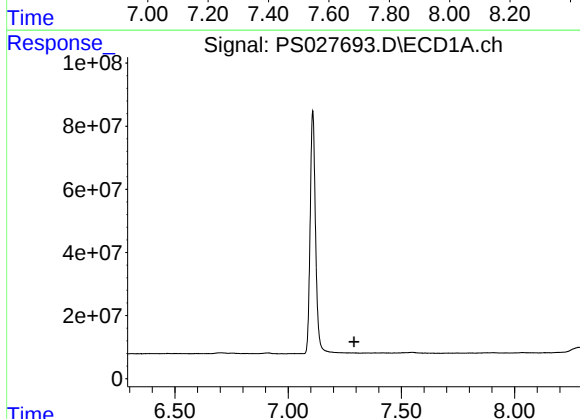


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.291 min
Response: 0
Conc: N.D.

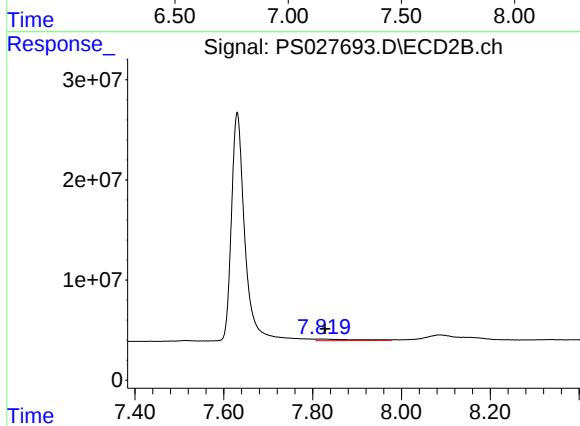

#5 DICAMBA


R.T.: 7.820 min
Delta R.T.: -0.008 min
Response: 9362110
Conc: 2.12 ng/ml

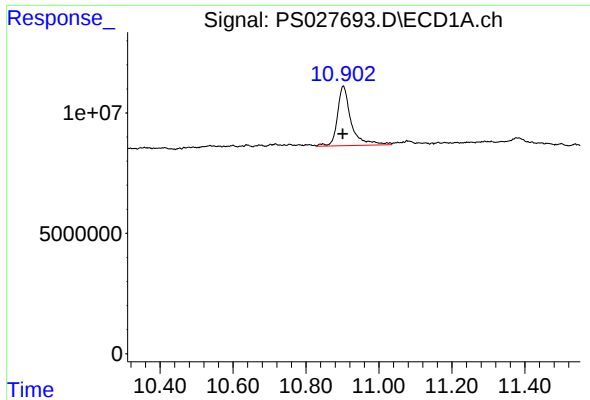

#15 Picloram

R.T.: 10.902 min
Delta R.T.: 0.002 min
Response: 64576545
Conc: 3.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

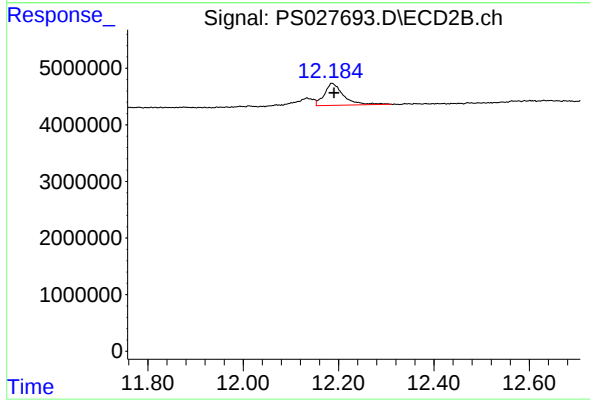

#15 Picloram

R.T.: 12.188 min
Delta R.T.: -0.003 min
Response: 11026208
Conc: 2.37 ng/ml