

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091624\
 Data File : PS027696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 16:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:15:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.110	7.628	1272.7E6	679.5E6	511.607	685.616 #
Target Compounds							
1) T	Dalapon	2.525f	0.000	20922683	0	5.050	N.D. #
2) T	3,5-DICHL...	6.290	0.000	410110	0	<MDL	N.D. #
3) T	4-Nitroph...	6.910	7.136f	8277572	79237	4.889	<MDL #
6) T	MCP	0.000	7.974f	0	19264125	N.D.	5.869
8) T	DICHLORPROP	7.979	8.574f	4344397	2797273	1.639	2.504 #
9) T	2,4-D	8.198	0.000	16287133	0	5.314	N.D. #
10) T	Pentachlo...	8.492	9.370	999323	1048086	<MDL	<MDL #
11) T	2,4,5-TP ...	9.046	9.707f	1444876	9525364	<MDL	1.589 #
13) T	2,4-DB	9.896	0.000	452375	0	<MDL	N.D. #
14) T	DINOSEB	11.063	0.000	2750308	0	<MDL	N.D. #
15) T	Picloram	10.904	12.182	5392530	982297	<MDL	<MDL #
16) T	DCPA	11.363	12.182f	3643192	982297	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091624\
Data File : PS027696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 16:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:15:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

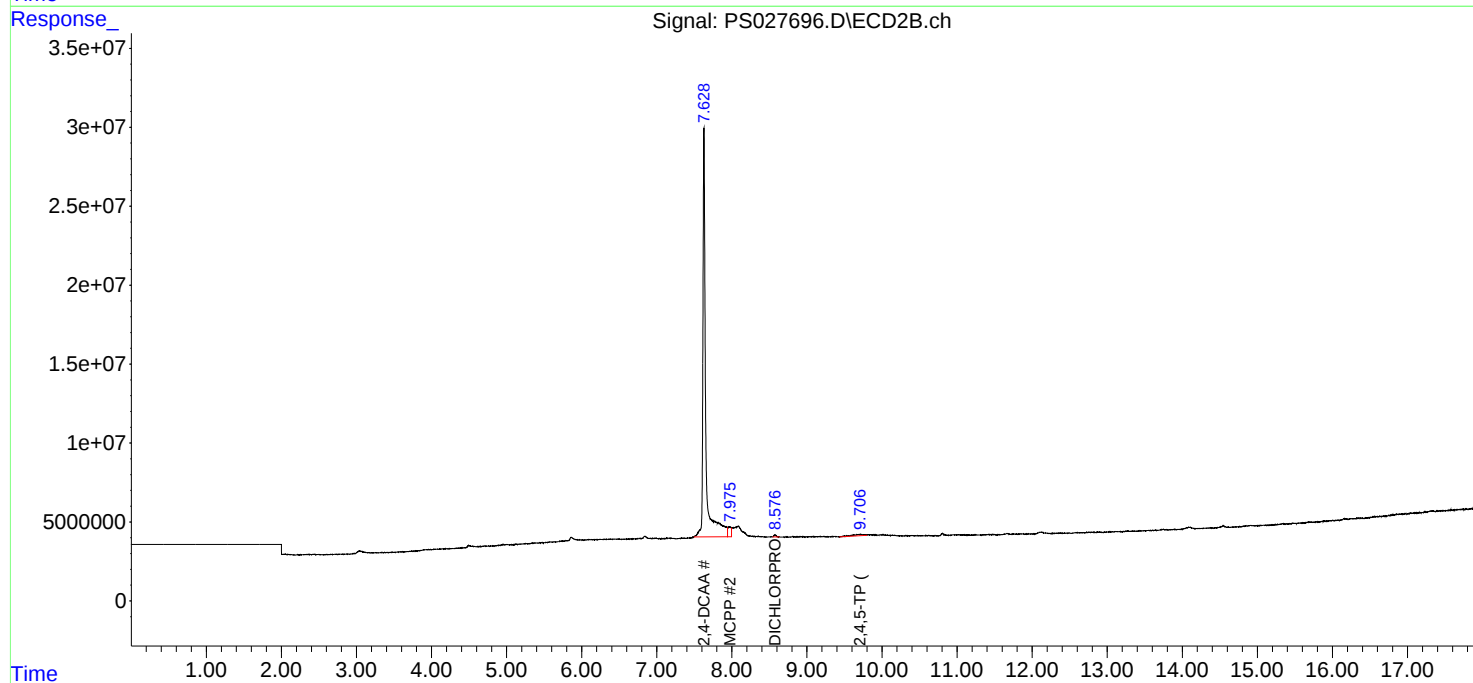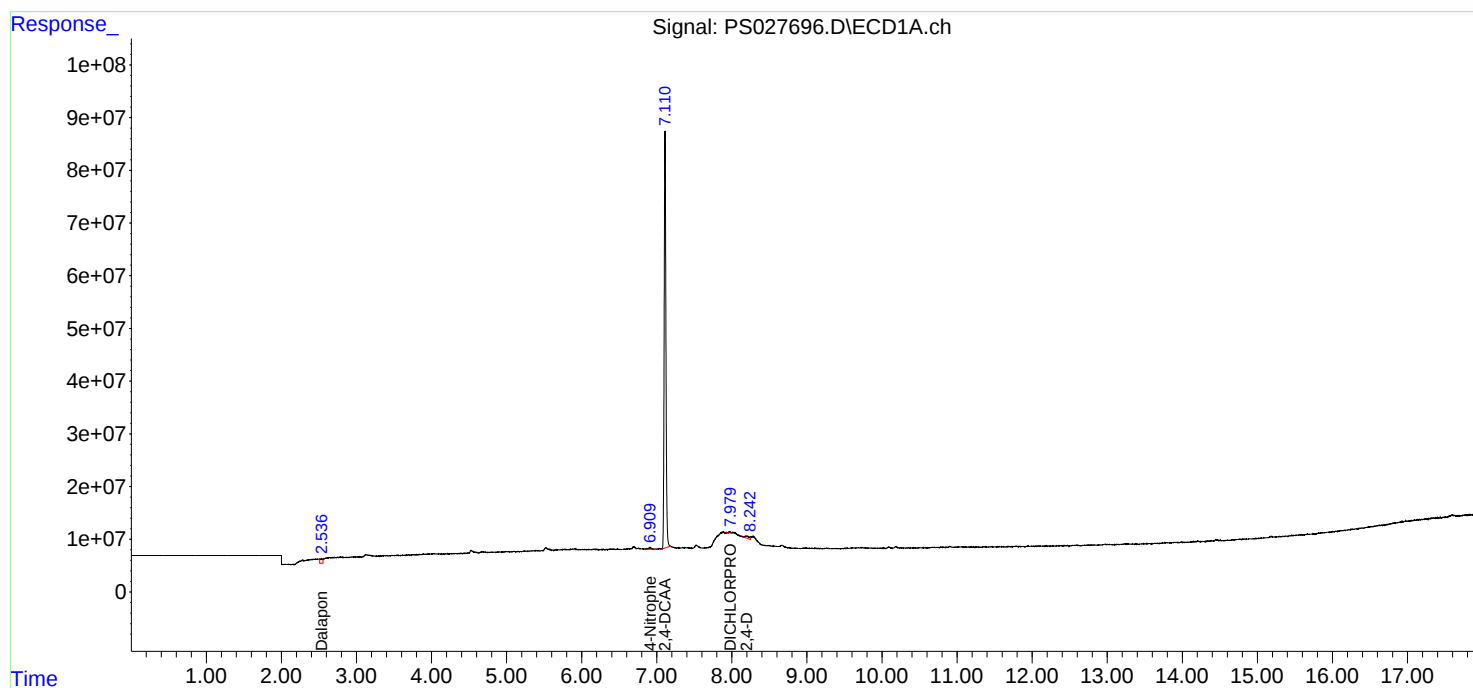


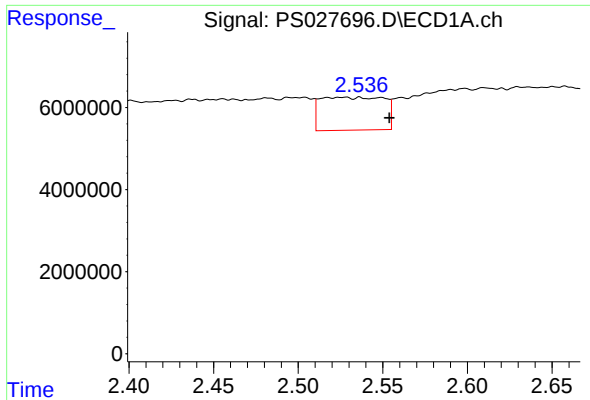

#1 Dalapon


R.T.: 2.525 min
Delta R.T.: -0.029 min
Response: 20922683
Conc: 5.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

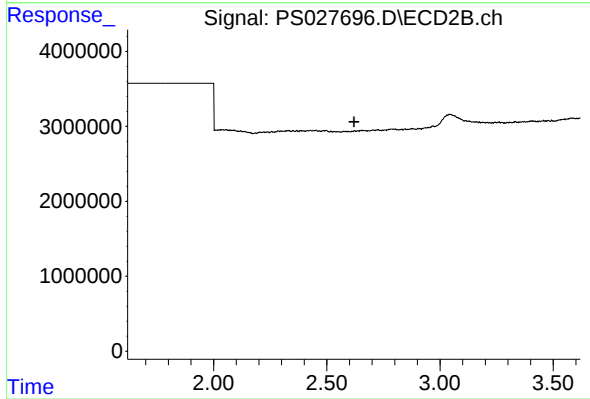


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

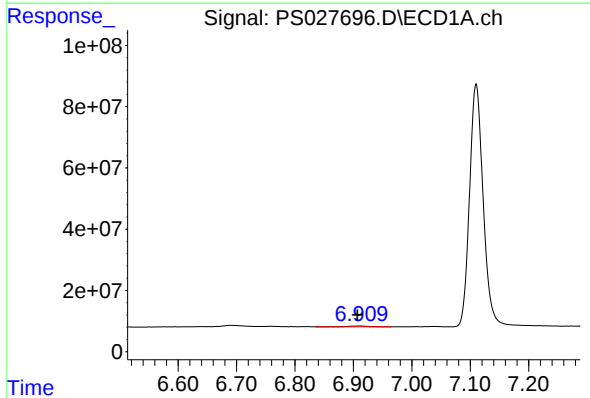


#3 4-Nitrophenol

R.T.: 6.910 min
Delta R.T.: 0.004 min
Response: 8277572
Conc: 4.89 ng/ml

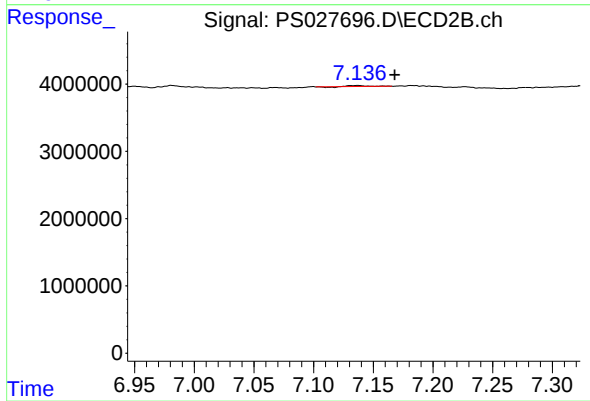

#3 4-Nitrophenol


R.T.: 7.136 min
Delta R.T.: -0.033 min
Response: 79237
Conc: N.D.

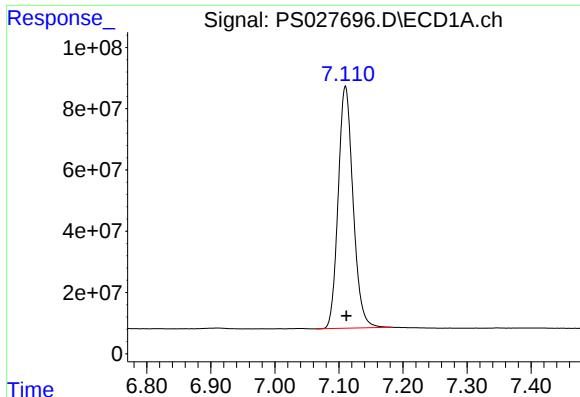

#4 2,4-DCAA


R.T.: 7.110 min
Delta R.T.: -0.001 min
Response: 1272676647
Conc: 511.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

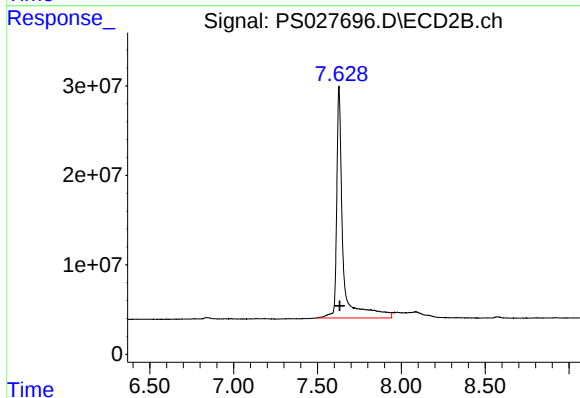


#4 2,4-DCAA

R.T.: 7.628 min
Delta R.T.: -0.005 min
Response: 679468280
Conc: 685.62 ng/ml

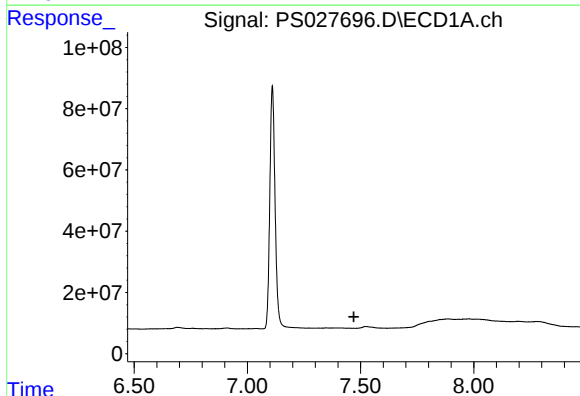


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.471 min
Response: 0
Conc: N.D.

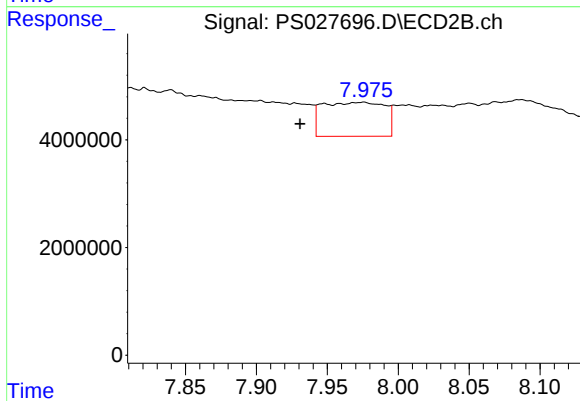

#6 MCP


R.T.: 7.974 min
Delta R.T.: 0.043 min
Response: 19264125
Conc: 5.87 ug/ml

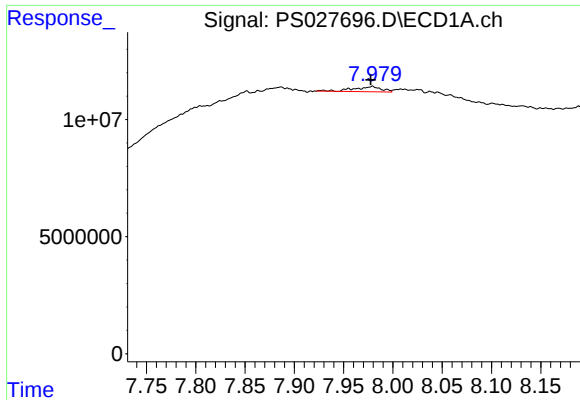

#8 DICHLORPROP


R.T.: 7.979 min
Delta R.T.: 0.000 min
Response: 4344397
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

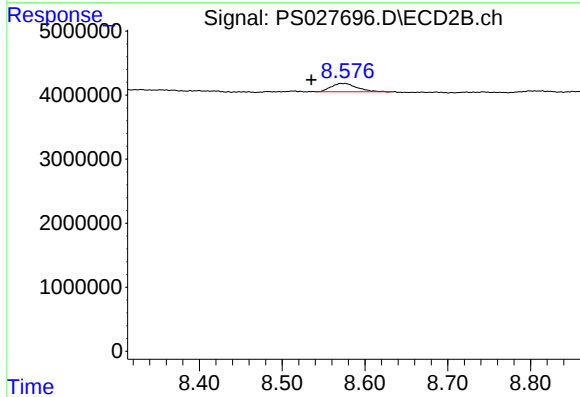


#8 DICHLORPROP

R.T.: 8.574 min
Delta R.T.: 0.038 min
Response: 2797273
Conc: 2.50 ng/ml

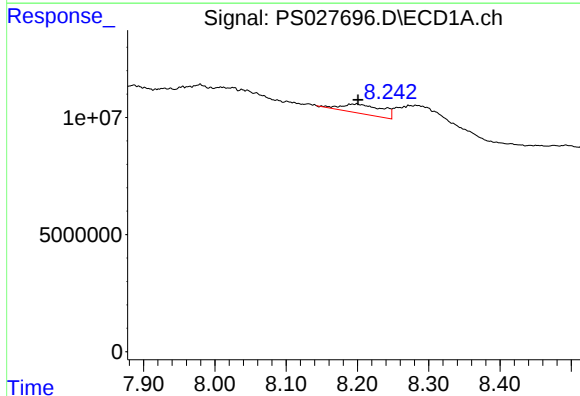


#9 2,4-D

R.T.: 8.198 min
Delta R.T.: -0.003 min
Response: 16287133
Conc: 5.31 ng/ml

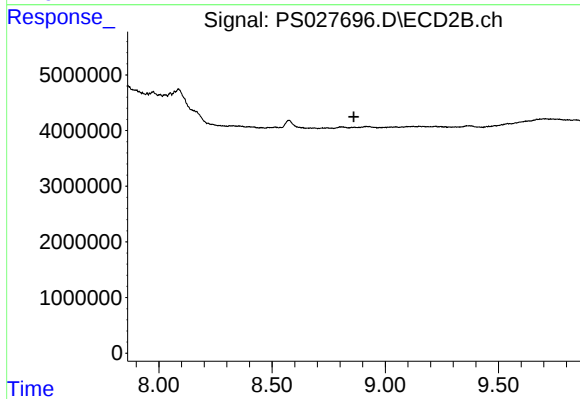

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.861 min
Response: 0
Conc: N.D.

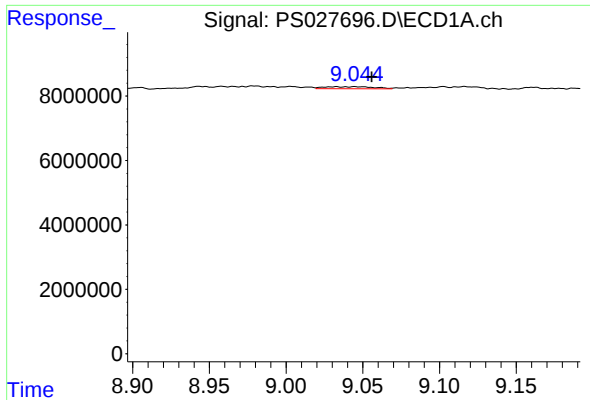

#11 2,4,5-TP (SILVEX)

R.T.: 9.046 min
Delta R.T.: -0.010 min
Response: 1444876
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

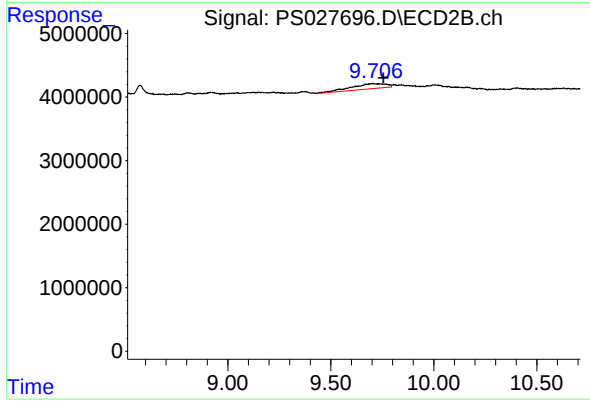

#11 2,4,5-TP (SILVEX)

R.T.: 9.707 min
Delta R.T.: -0.048 min
Response: 9525364
Conc: 1.59 ng/ml