

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091718\
 Data File : PS001779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 01:12
 Operator : EI\SJ
 Sample : J4898-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 07:12:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.494	10.992	29758958	26908845	132.666	105.933
Target Compounds							
1) T	Dalapon	2.925	2.404	32713897	26845400	100.606	90.873
5) T	DICAMBA	0.000	11.236	0	24299010	N.D.	27.245 #
6) T	MCP	12.183	11.503	16257203	1586812	25.512	2.693 #
8) T	DICHLORPROP	12.911	0.000	1037194	0	4.469	N.D. #
10) T	Pentachlo...	13.733	13.439	2627711	1083894	0.855	0.316 #
12) T	2,4,5-T	0.000	14.565	0	1197236	N.D.	1.084 #
13) T	2,4-DB	15.779	15.243	19124537	13452054	117.435	81.271 #
14) T	DINOSEB	17.228	15.735	4916613	4645569	5.898	4.901
15) T	Picloram	17.056	0.000	1141533	0	0.656	N.D. #
16) T	DCPA	0.000	16.933	0	5530411	N.D.	2.998 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091718\
Data File : PS001779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 01:12
Operator : EI\SJ
Sample : J4898-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 07:12:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

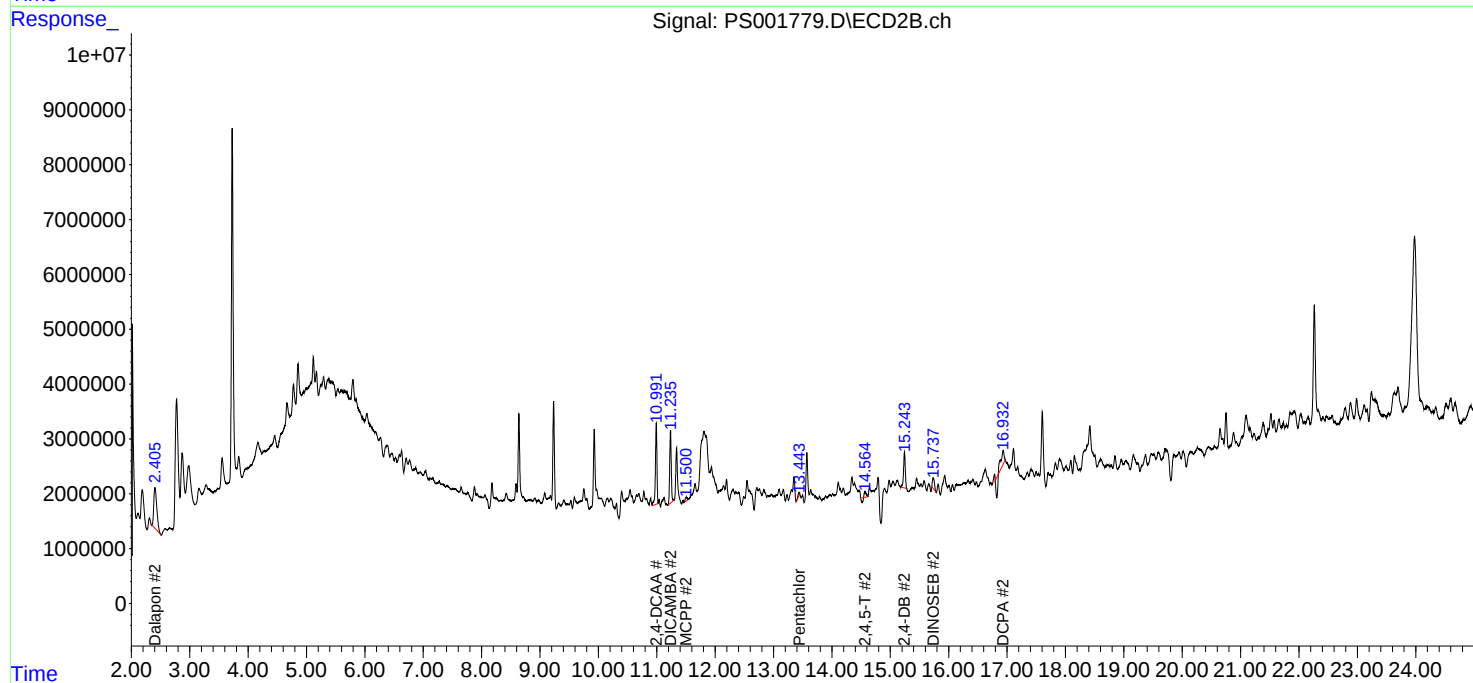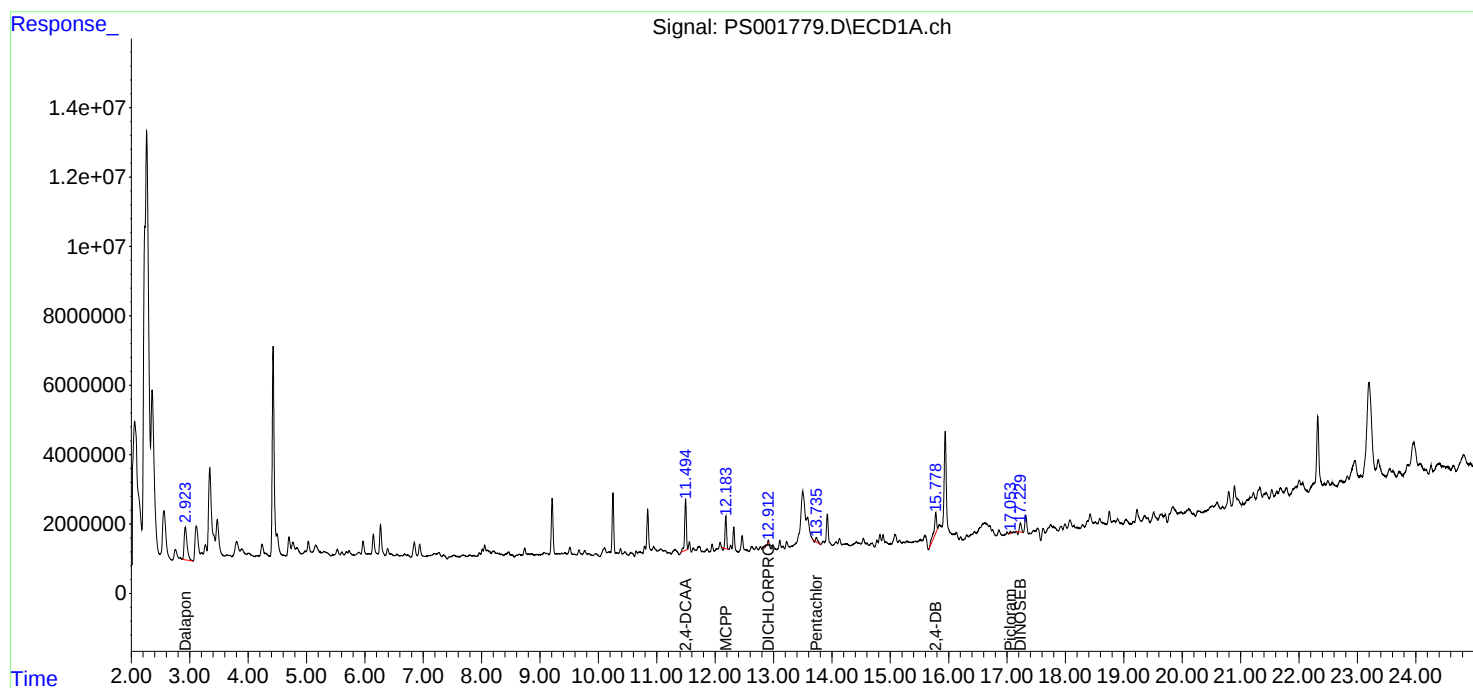


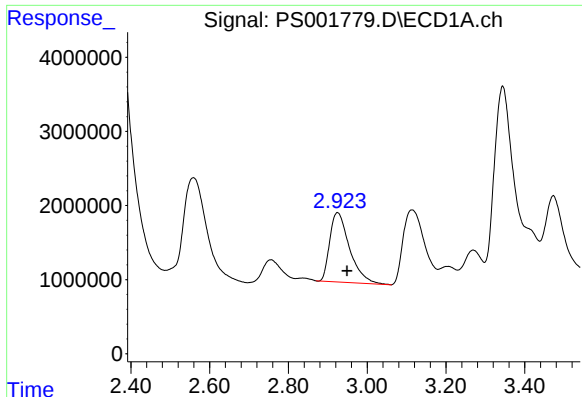

#1 Dalapon


R.T.: 2.925 min
Delta R.T.: -0.024 min
Response: 32713897
Conc: 100.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

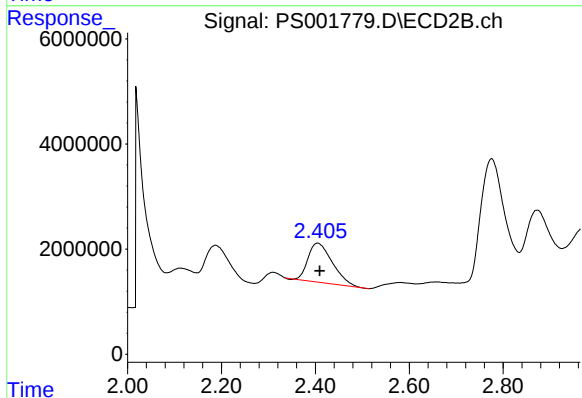


#1 Dalapon

R.T.: 2.404 min
Delta R.T.: -0.005 min
Response: 26845400
Conc: 90.87 ng/ml

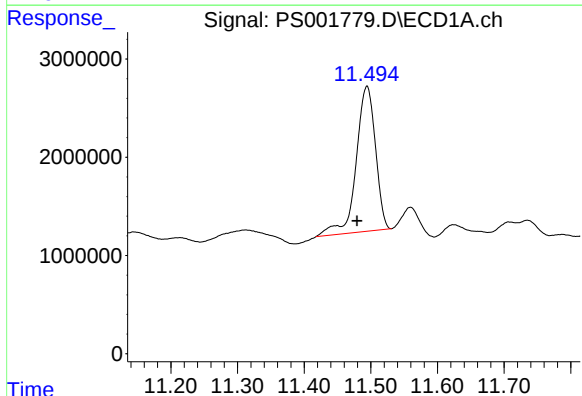


#4 2,4-DCAA

R.T.: 11.494 min
Delta R.T.: 0.014 min
Response: 29758958
Conc: 132.67 ng/ml

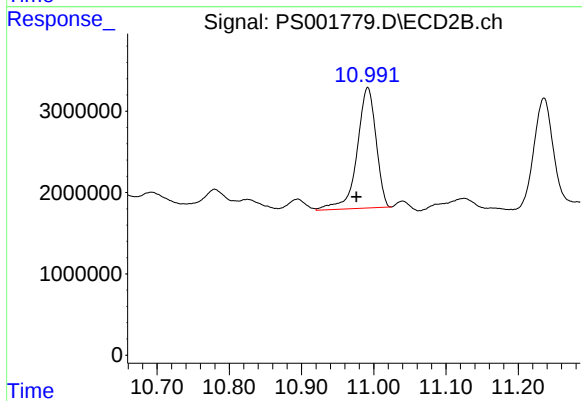

#4 2,4-DCAA


R.T.: 10.992 min
Delta R.T.: 0.016 min
Response: 26908845
Conc: 105.93 ng/ml

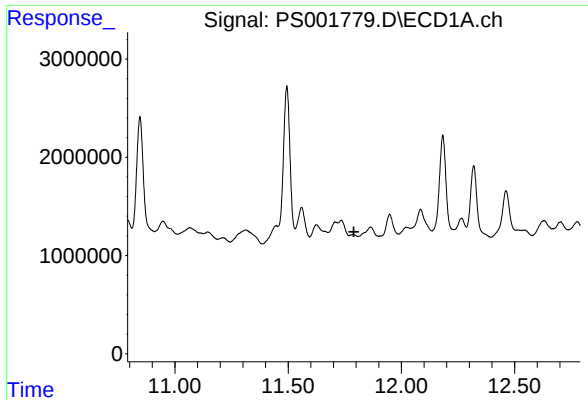

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

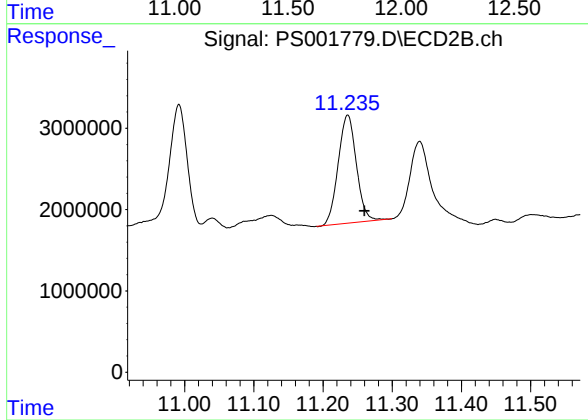


#5 DICAMBA

R.T.: 11.236 min
Delta R.T.: -0.024 min
Response: 24299010
Conc: 27.24 ng/ml

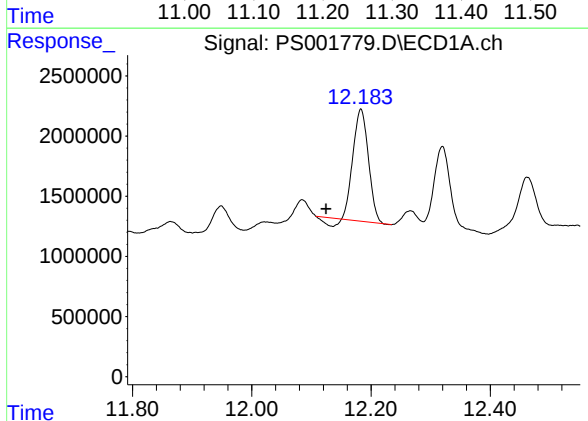


#6 MCP

R.T.: 12.183 min
Delta R.T.: 0.058 min
Response: 16257203
Conc: 25.51 ug/ml

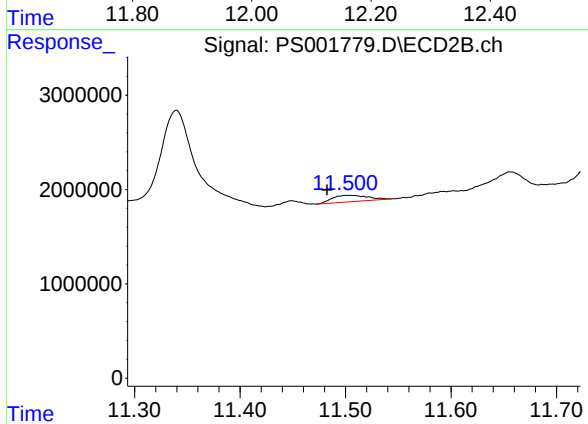

#6 MCP


R.T.: 11.503 min
Delta R.T.: 0.020 min
Response: 1586812
Conc: 2.69 ug/ml

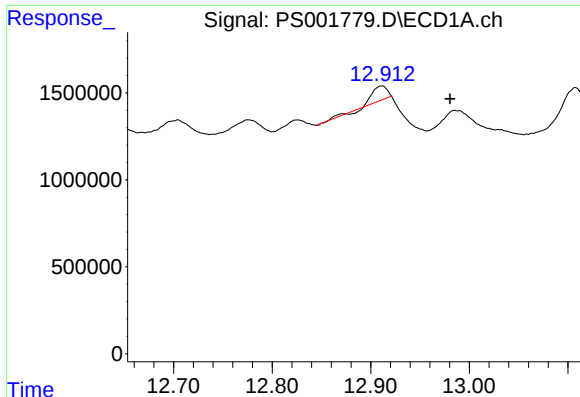

#8 DICHLORPROP


R.T.: 12.911 min
Delta R.T.: -0.070 min
Response: 1037194
Conc: 4.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

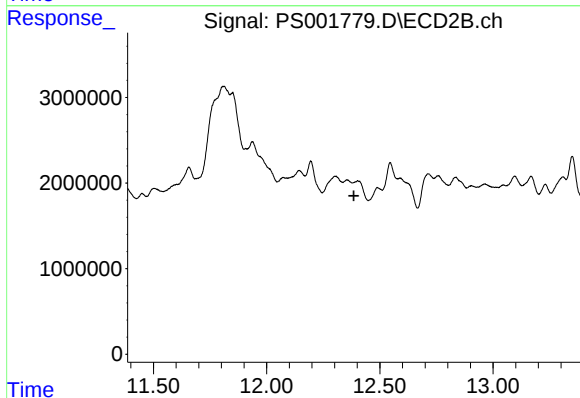


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.386 min
Response: 0
Conc: N.D.

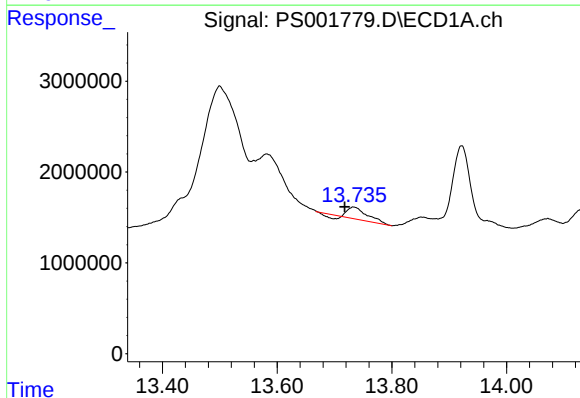


#10 Pentachlorophenol

R.T.: 13.733 min
Delta R.T.: 0.016 min
Response: 2627711
Conc: 0.86 ng/ml

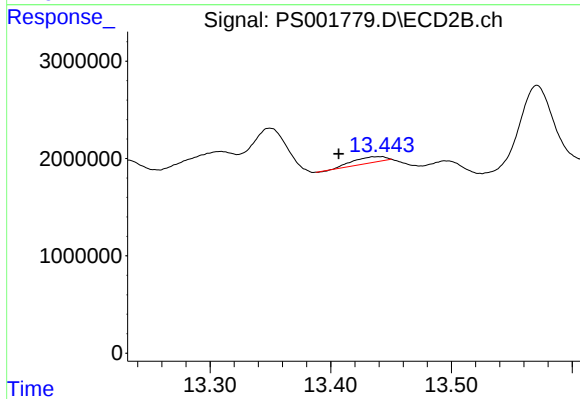

#10 Pentachlorophenol


R.T.: 13.439 min
Delta R.T.: 0.032 min
Response: 1083894
Conc: 0.32 ng/ml

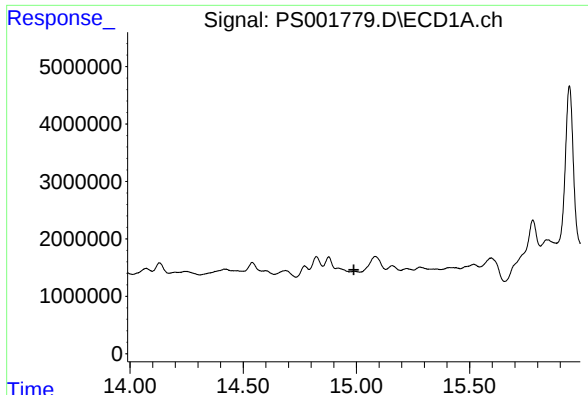

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

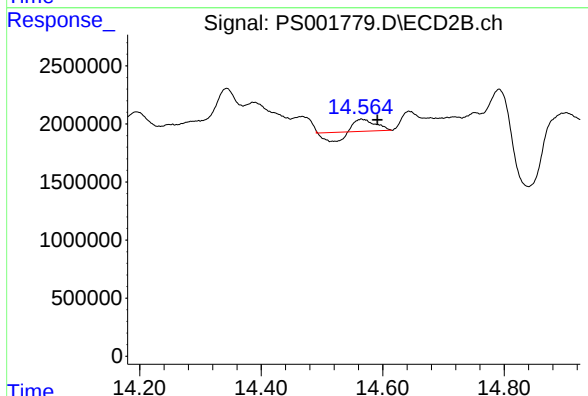


#12 2,4,5-T

R.T.: 14.565 min
Delta R.T.: -0.026 min
Response: 1197236
Conc: 1.08 ng/ml

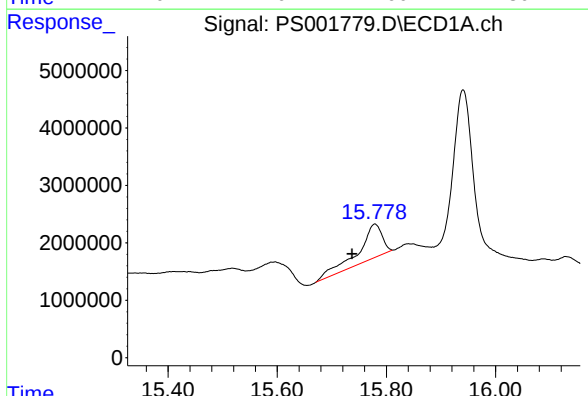


#13 2,4-DB

R.T.: 15.779 min
Delta R.T.: 0.042 min
Response: 19124537
Conc: 117.43 ng/ml

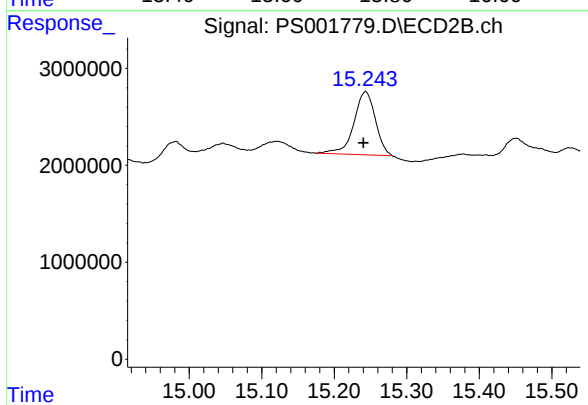

#13 2,4-DB


R.T.: 15.243 min
Delta R.T.: 0.003 min
Response: 13452054
Conc: 81.27 ng/ml

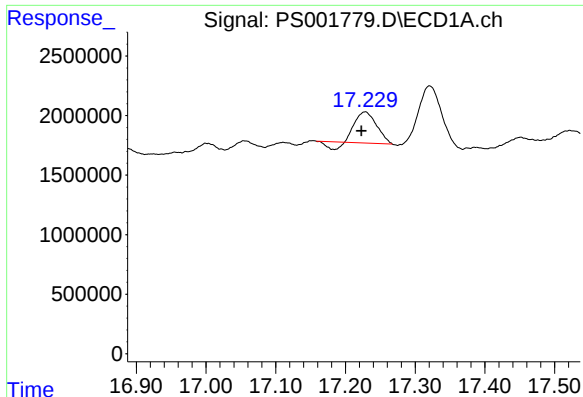

#14 DINOSEB


R.T.: 17.228 min
Delta R.T.: 0.005 min
Response: 4916613
Conc: 5.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

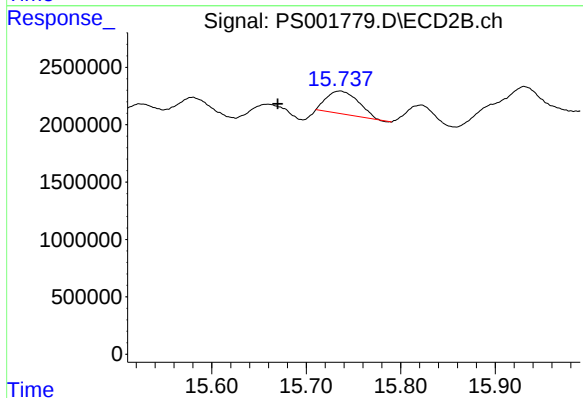


#14 DINOSEB

R.T.: 15.735 min
Delta R.T.: 0.066 min
Response: 4645569
Conc: 4.90 ng/ml

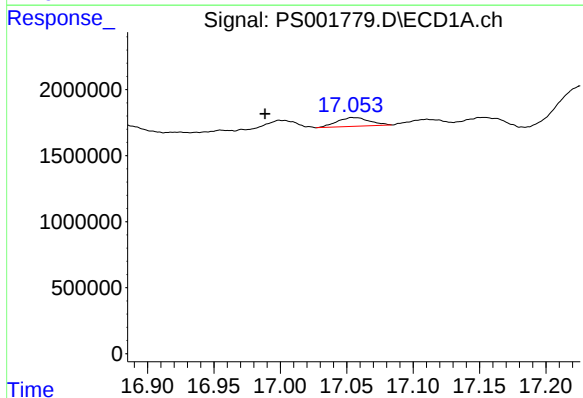


#15 Picloram

R.T.: 17.056 min
Delta R.T.: 0.067 min
Response: 1141533
Conc: 0.66 ng/ml

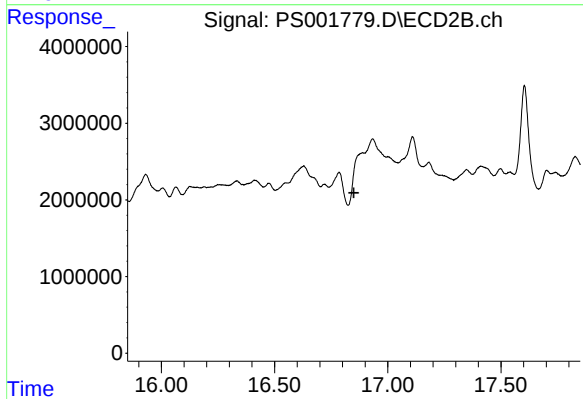

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.850 min
Response: 0
Conc: N.D.

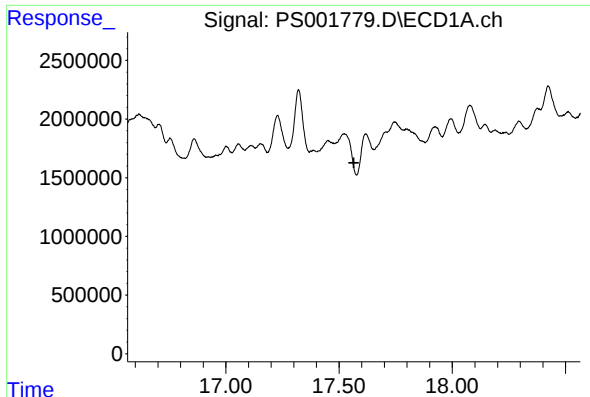

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

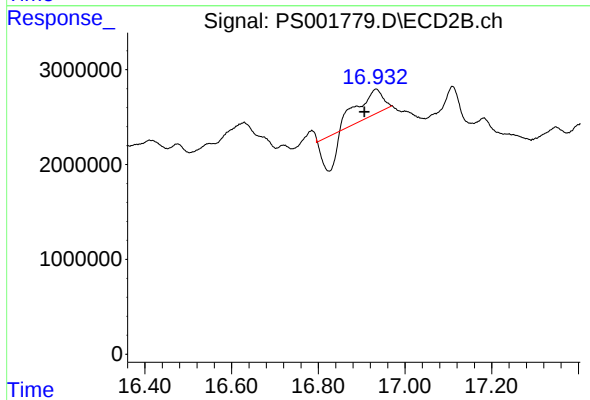

#16 DCPA

R.T.: 16.933 min
Delta R.T.: 0.027 min
Response: 5530411
Conc: 3.00 ng/ml