

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091719\
 Data File : PS006781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2019 13:05
 Operator : SM\AJ
 Sample : K4859-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 IDW-DECON-WATER-091119

Manual Integrations
 APPROVED

Ankita
 9/19/2019 9:05:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 06:53:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.480	5.207	276.6E6	143.1E6	356.006	335.130m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091719\
Data File : PS006781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2019 13:05
Operator : SM\AJ
Sample : K4859-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
IDW-DECON-WATER-091119


Manual Integrations
APPROVED

Ankita
9/19/2019 9:05:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 06:53:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

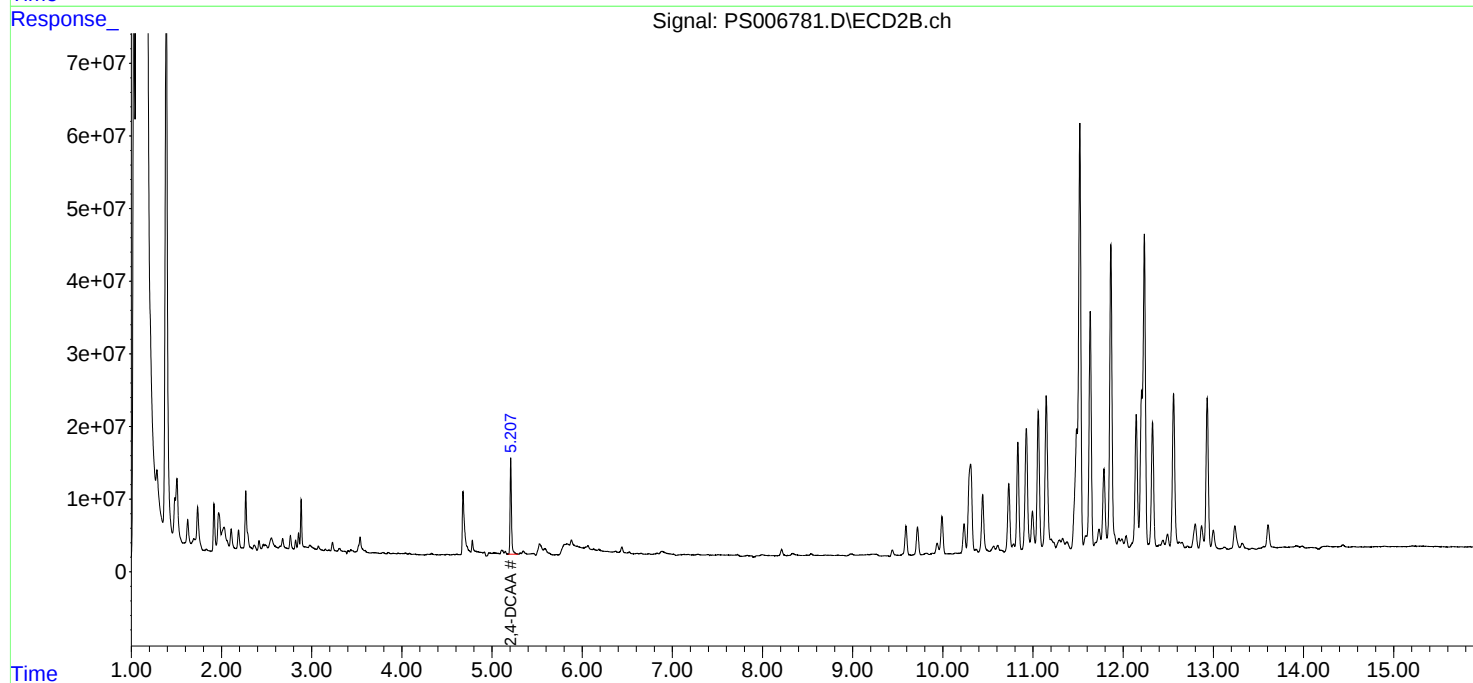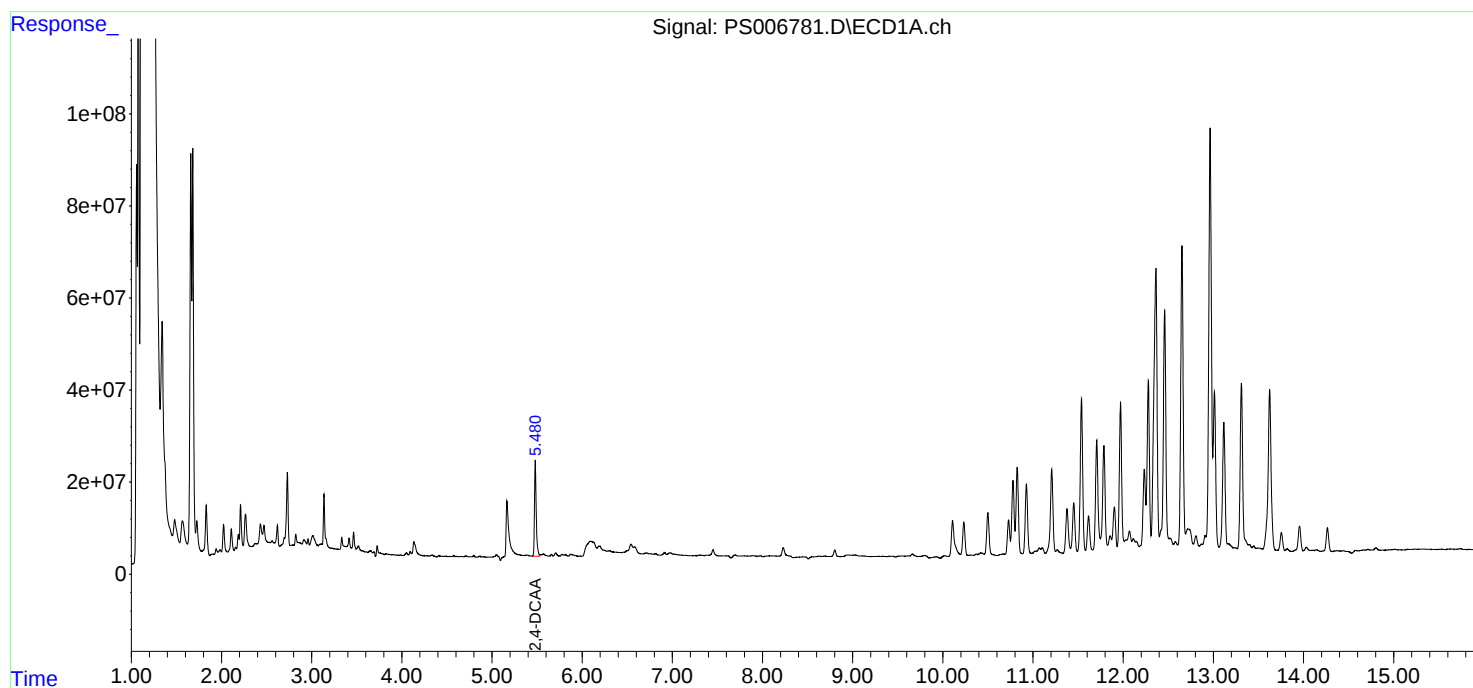

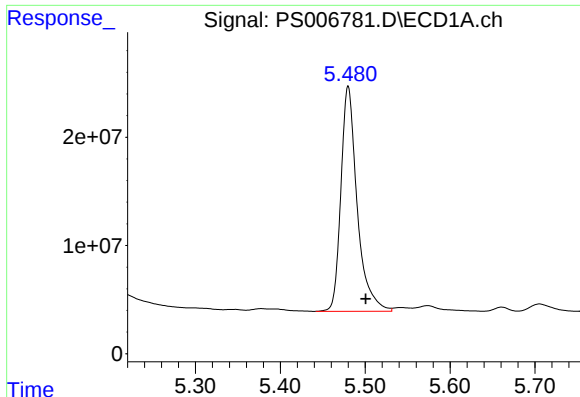


#4 2,4-DCAA

R.T.: 5.480 min
Delta R.T.: -0.021 min
Response: 276575545
Conc: 356.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
IDW-DECON-WATER-091119

Manual Integrations
APPROVED

Ankita
9/19/2019 9:05:05 AM

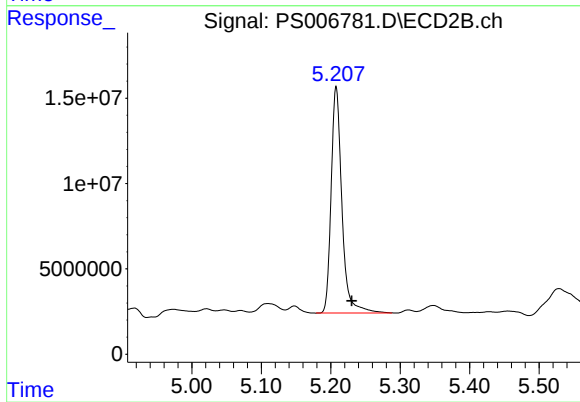

#4 2,4-DCAA

R.T.: 5.207 min
Delta R.T.: -0.023 min
Response: 143101183
Conc: 335.13 ng/ml m