

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
 Data File : PS012347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2020 17:56
 Operator : DD\AJ
 Sample : PB131666BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 05:12:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	563.9E6	307.4E6	520.281	582.559
Target Compounds							
1) T	Dalapon	0.000	2.589	0	5087641	N.D.	7.643
2) T	3,5-DICHL...	0.000	6.095	0	35379486	N.D.	43.732
3) T	4-Nitroph...	6.991	0.000	4737963	0	8.897	N.D. #
5) T	DICAMBA	0.000	7.047	0	7015798	N.D.	3.253
6) T	MCPD	7.626	0.000	9890652	0	3.070	N.D. #
7) T	MCPA	7.762	7.373	20537275	24499082	4.395	8.718 #
8) T	DICHLORPROP	0.000	7.745	0	8310460	N.D.	14.688
9) T	2,4-D	8.396	7.973	98741202	3309668	86.695	4.550 #
10) T	Pentachlo...	8.692	8.427	12924700	4088197	<MDL	<MDL #
12) T	2,4,5-T	9.409	0.000	24370584	0	3.974	N.D. #
15) T	Picloram	0.000	11.025	0	14356222	N.D.	3.386
16) T	DCPA	0.000	10.936	0	18386436	N.D.	5.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
Data File : PS012347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2020 17:56
Operator : DD\AJ
Sample : PB131666BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 05:12:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

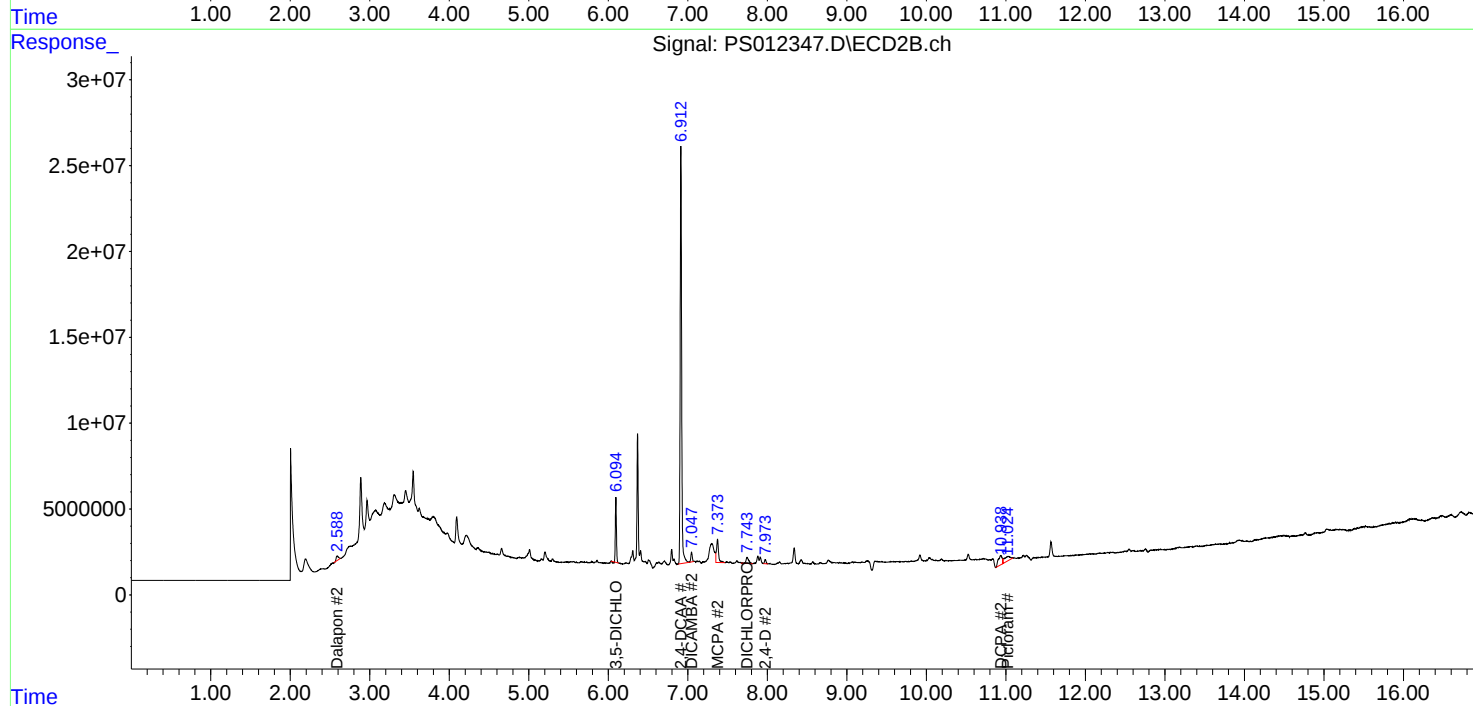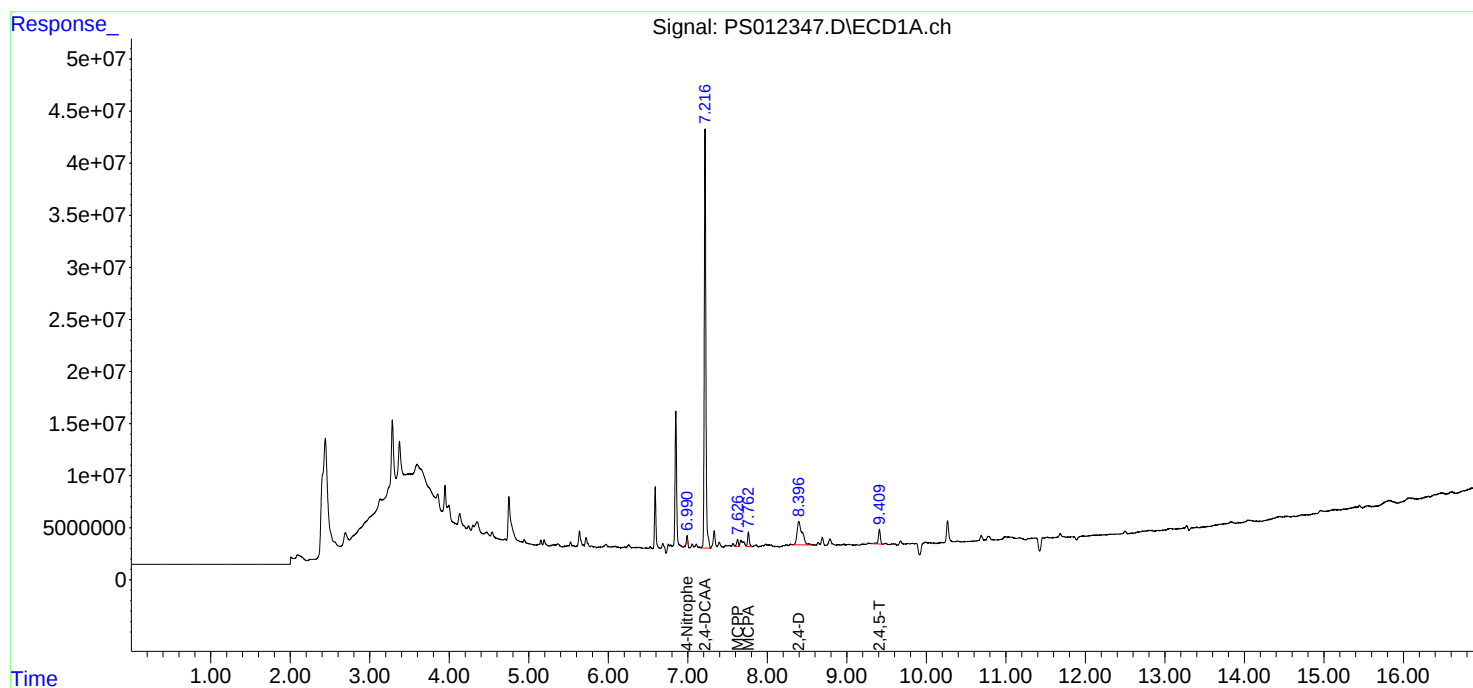


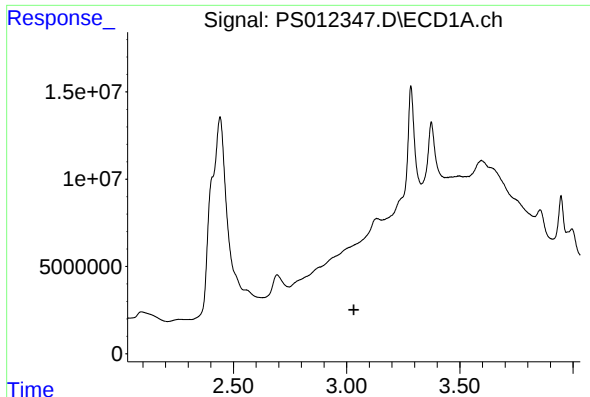

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

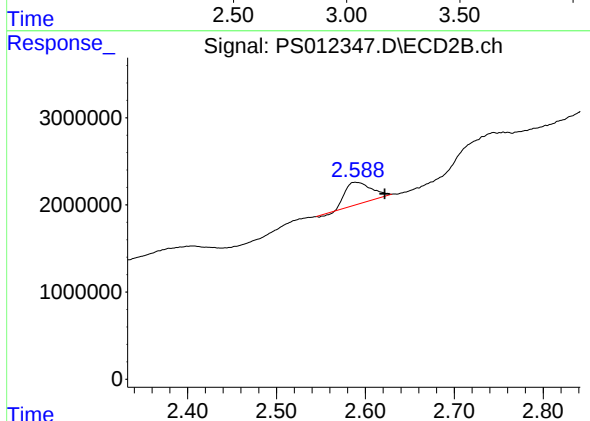


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.033 min
Response: 5087641
Conc: 7.64 ng/ml

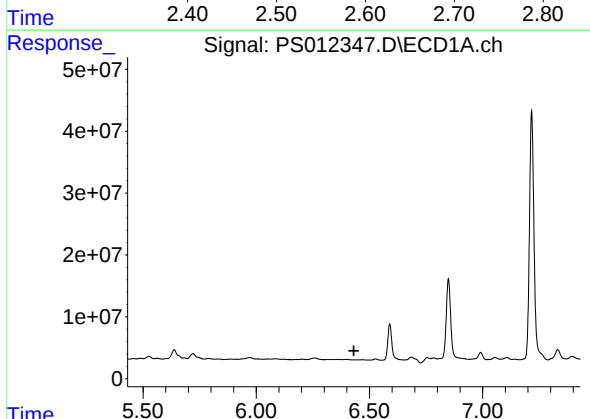


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

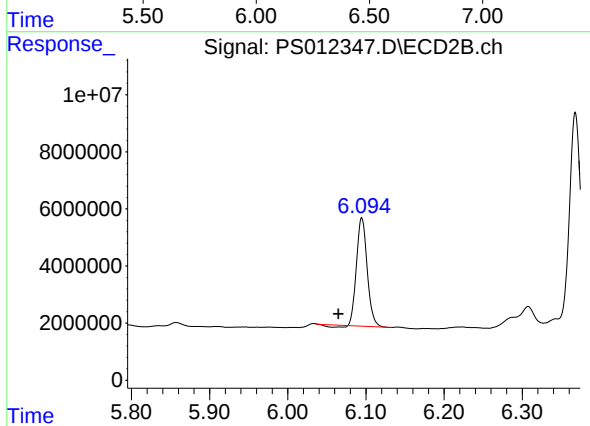

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.030 min
Response: 35379486
Conc: 43.73 ng/ml

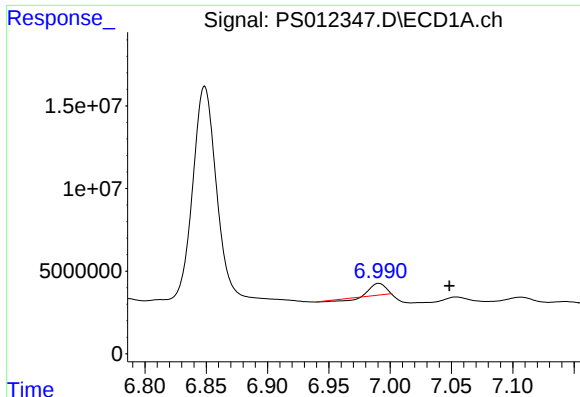

#3 4-Nitrophenol


R.T.: 6.991 min
Delta R.T.: -0.058 min
Response: 4737963
Conc: 8.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

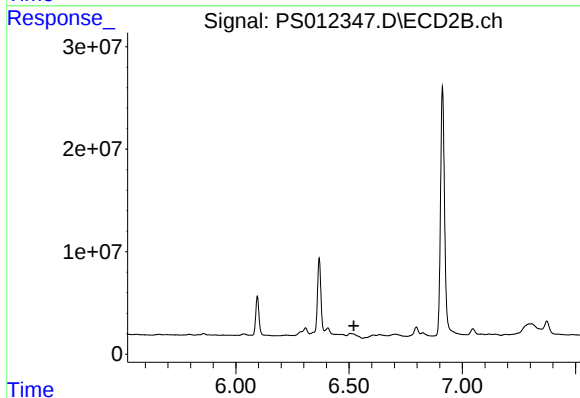


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

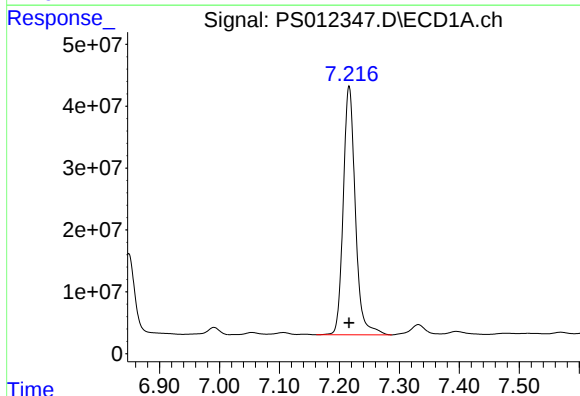


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 563930585
Conc: 520.28 ng/ml

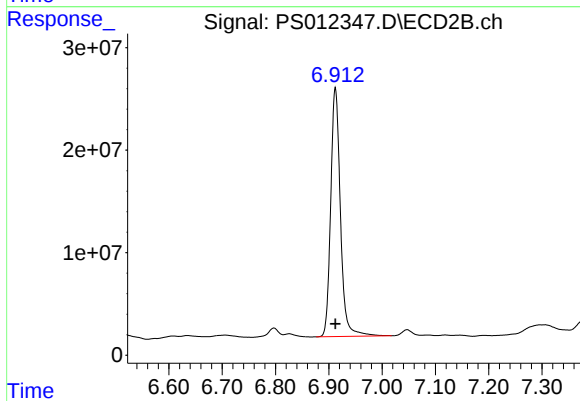

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 307360963
Conc: 582.56 ng/ml

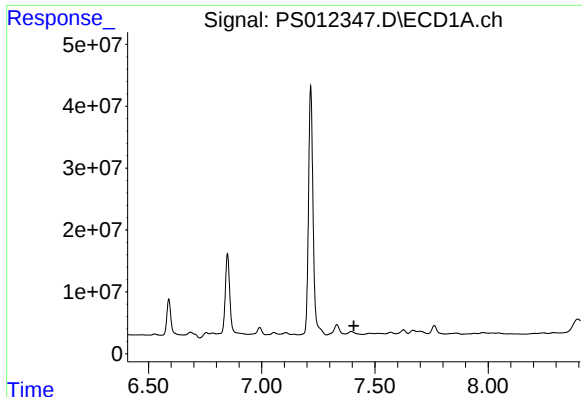

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

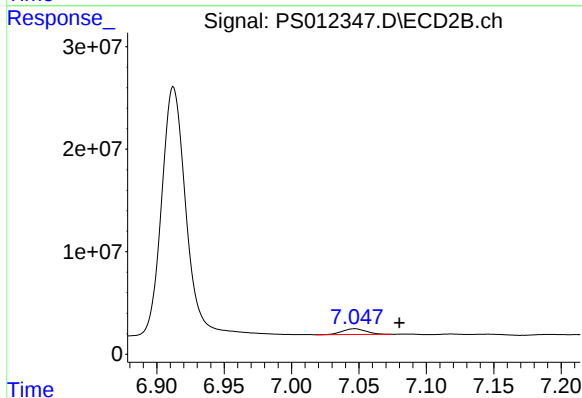


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.033 min
Response: 7015798
Conc: 3.25 ng/ml

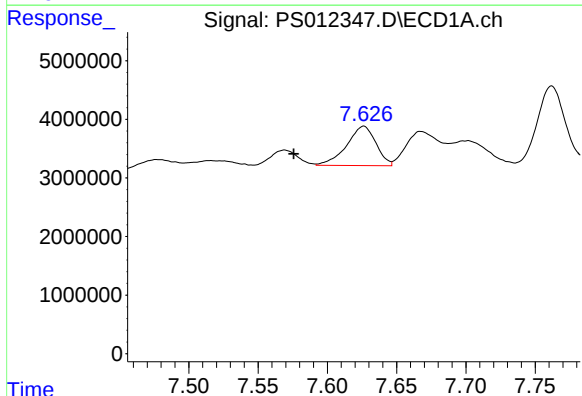


#6 MCP

R.T.: 7.626 min
Delta R.T.: 0.050 min
Response: 9890652
Conc: 3.07 ug/ml

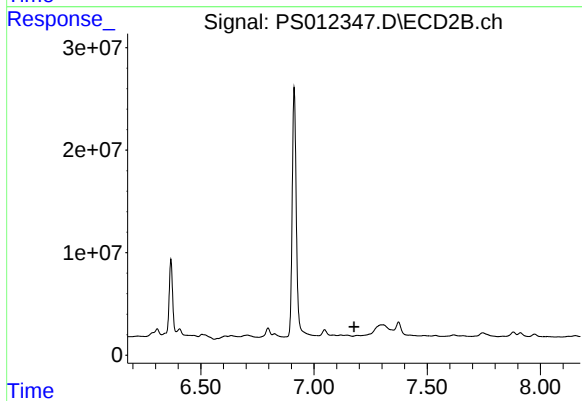

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.177 min
Response: 0
Conc: N.D.

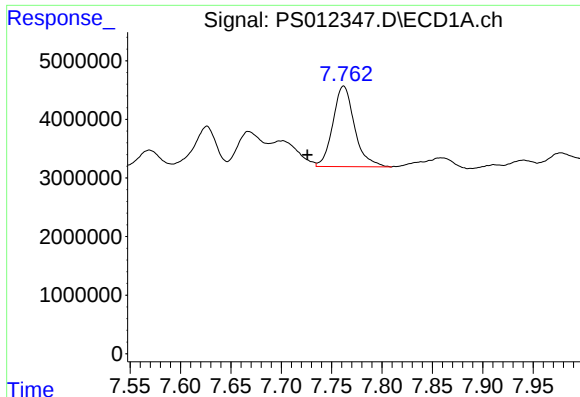

#7 MCPA


R.T.: 7.762 min
Delta R.T.: 0.036 min
Response: 20537275
Conc: 4.40 ug/ml

Instrument :
ECD_S
ClientSampleId :

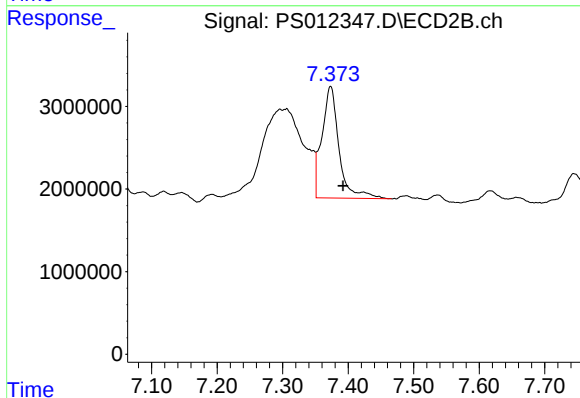


#7 MCPA

R.T.: 7.373 min
Delta R.T.: -0.019 min
Response: 24499082
Conc: 8.72 ug/ml

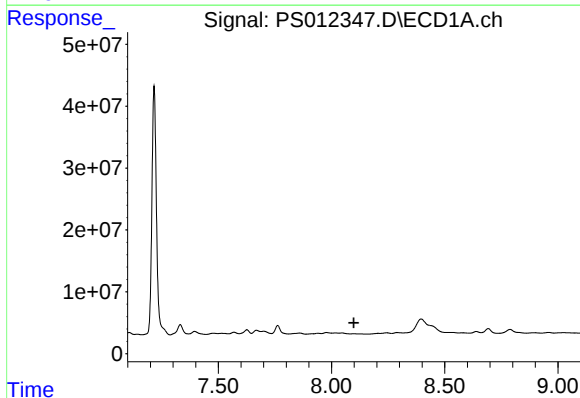


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.099 min
Response: 0
Conc: N.D.

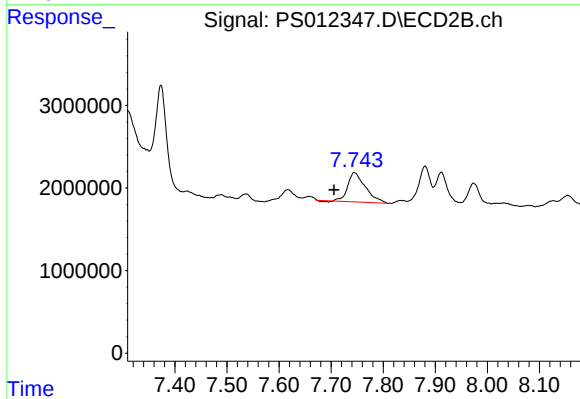

#8 DICHLORPROP


R.T.: 7.745 min
Delta R.T.: 0.039 min
Response: 8310460
Conc: 14.69 ng/ml

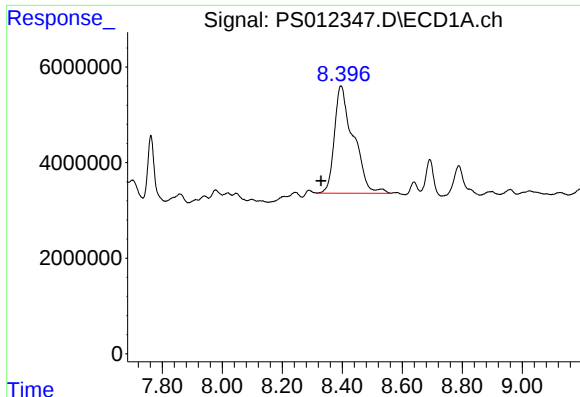

#9 2,4-D


R.T.: 8.396 min
Delta R.T.: 0.066 min
Response: 98741202
Conc: 86.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

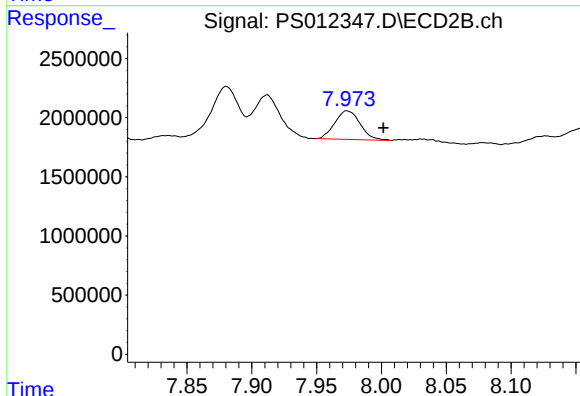


#9 2,4-D

R.T.: 7.973 min
Delta R.T.: -0.028 min
Response: 3309668
Conc: 4.55 ng/ml

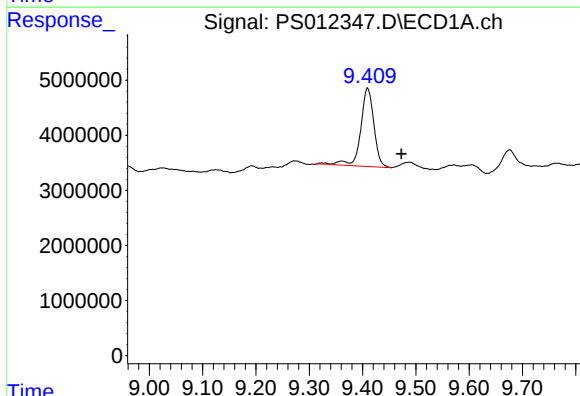


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.063 min
Response: 24370584
Conc: 3.97 ng/ml

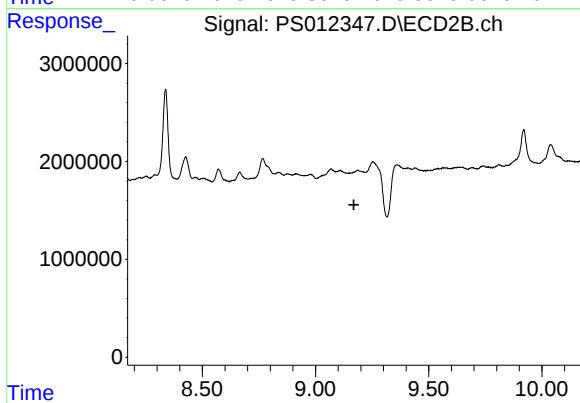

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

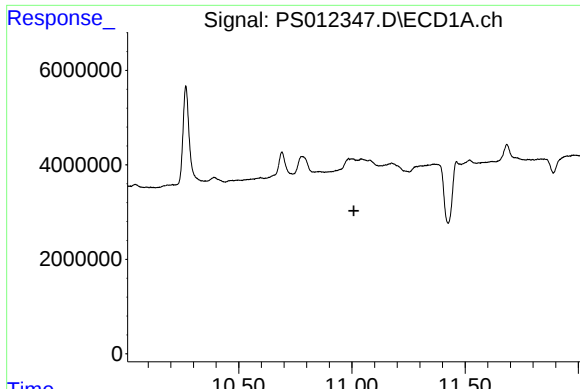

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

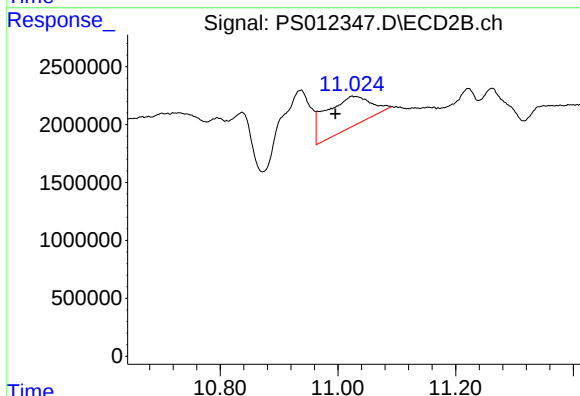


#15 Picloram

R.T.: 11.025 min
Delta R.T.: 0.029 min
Response: 14356222
Conc: 3.39 ng/ml

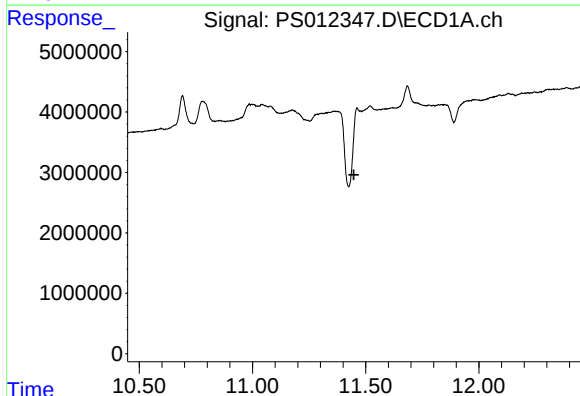

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.448 min
Response: 0
Conc: N.D.

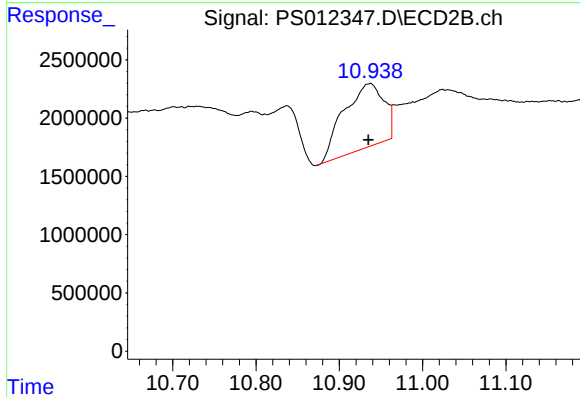

#16 DCPA

R.T.: 10.936 min
Delta R.T.: 0.002 min
Response: 18386436
Conc: 5.06 ng/ml