

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
 Data File : PS012352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2020 19:51
 Operator : DD\AJ
 Sample : L3868-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 05:14:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	319.7E6	180.4E6	294.979	341.930
Target Compounds							
1) T	Dalapon	2.996	2.588	14184488	9745608	11.555	14.640 #
2) T	3,5-DICHL...	0.000	6.095	0	7493306	N.D.	9.262
7) T	MCPA	7.675	7.369	12292905	9040723	2.631	3.217
8) T	DICHLORPROP	0.000	7.748	0	8810919	N.D.	15.572
9) T	2,4-D	8.397	0.000	91852174	0	80.646	N.D. #
15) T	Picloram	0.000	10.940	0	5551289	N.D.	1.309
16) T	DCPA	0.000	10.940	0	5551289	N.D.	1.527



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
Data File : PS012352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2020 19:51
Operator : DD\AJ
Sample : L3868-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 05:14:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

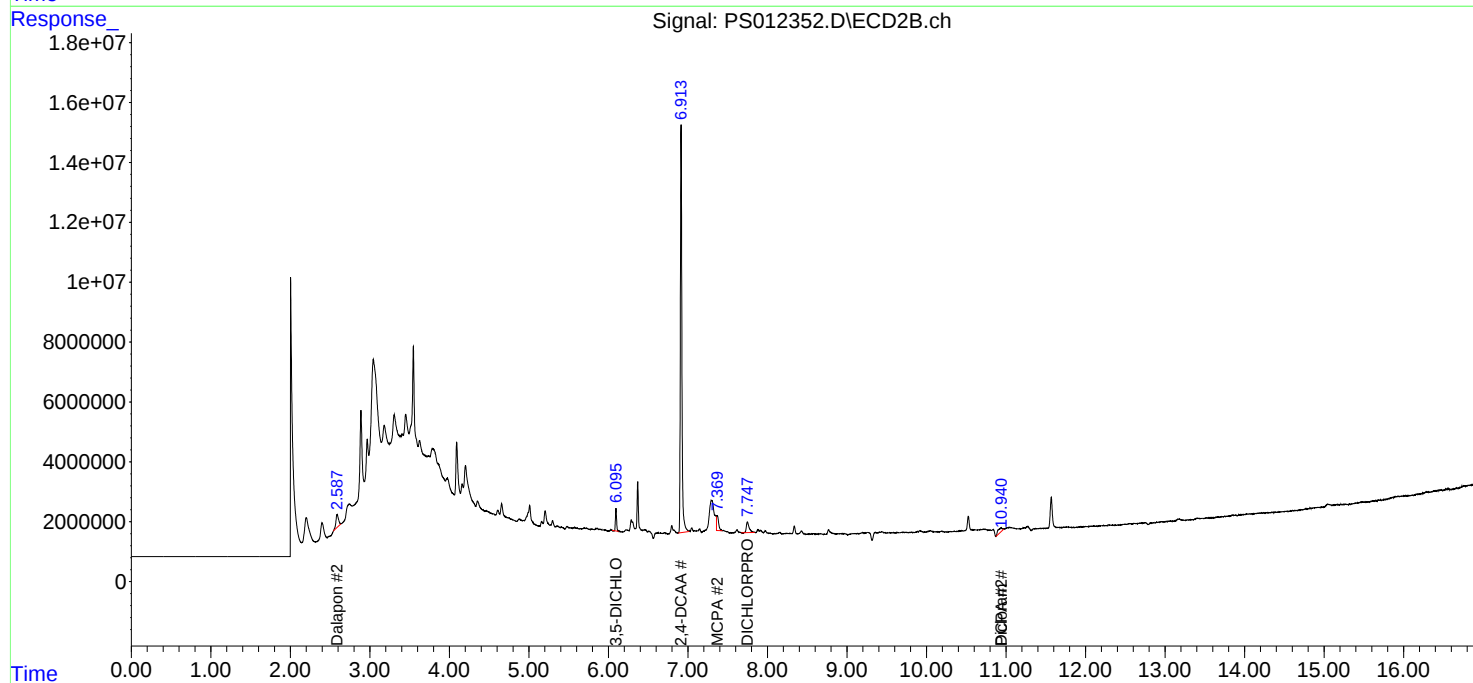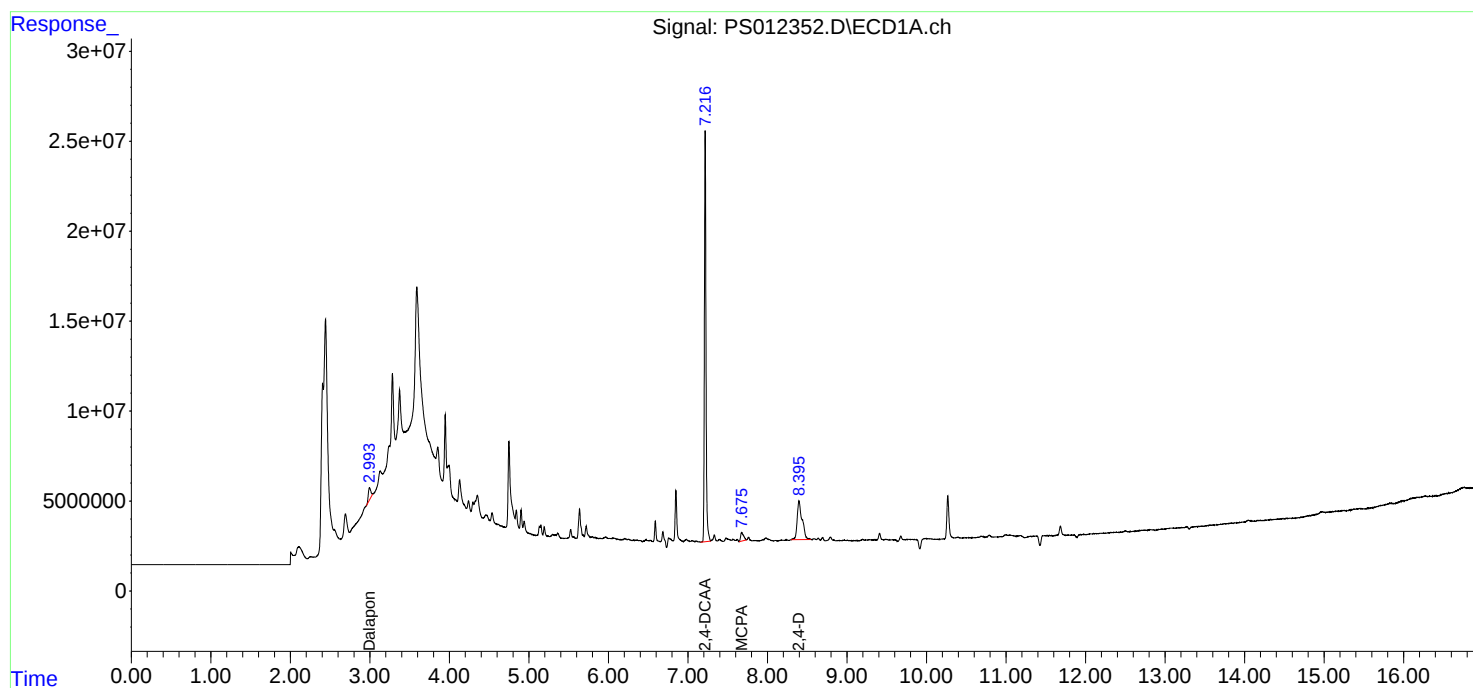


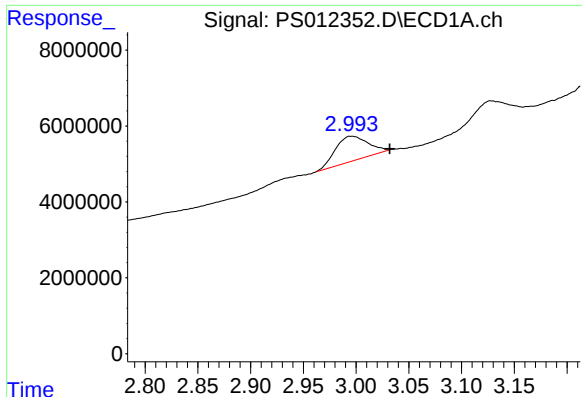

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.036 min
Response: 14184488
Conc: 11.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

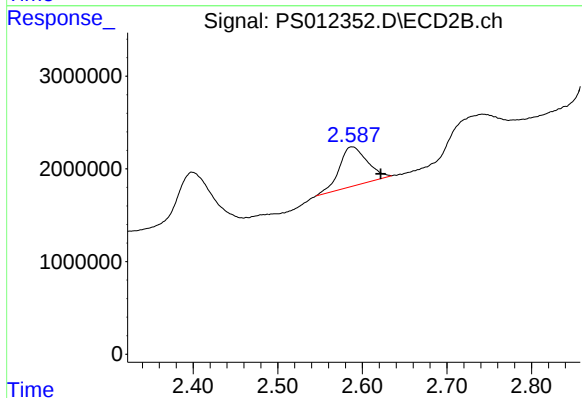


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.034 min
Response: 9745608
Conc: 14.64 ng/ml

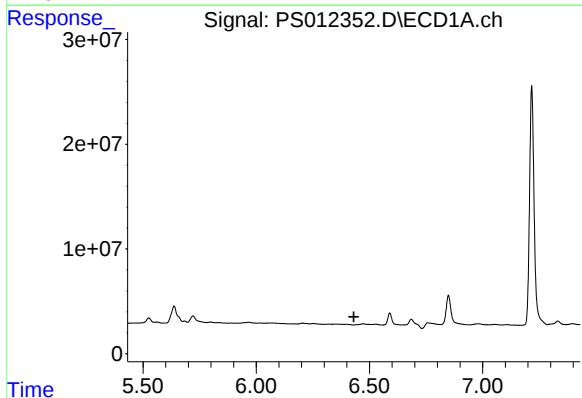


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.431 min
Response: 0
Conc: N.D.

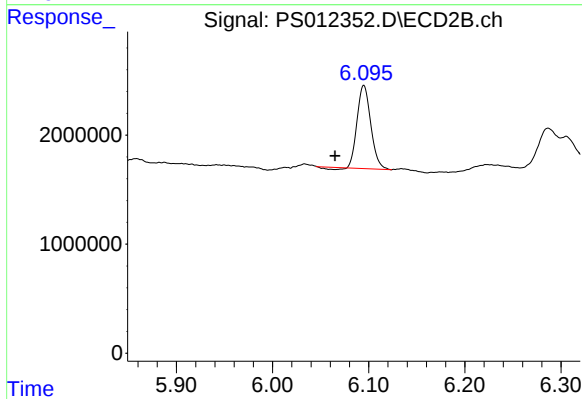

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.030 min
Response: 7493306
Conc: 9.26 ng/ml

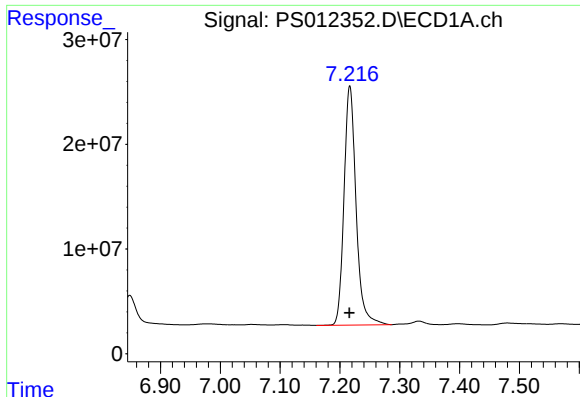

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 319726190
Conc: 294.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

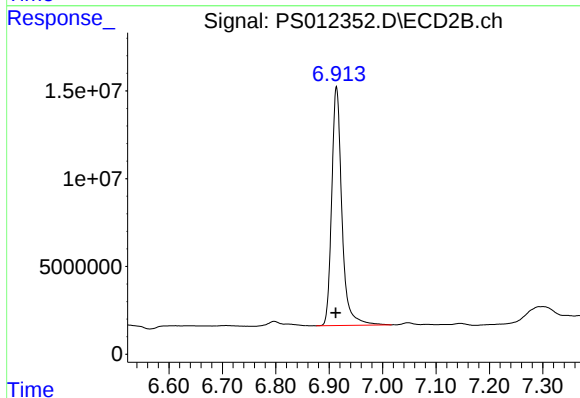


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.001 min
Response: 180404087
Conc: 341.93 ng/ml

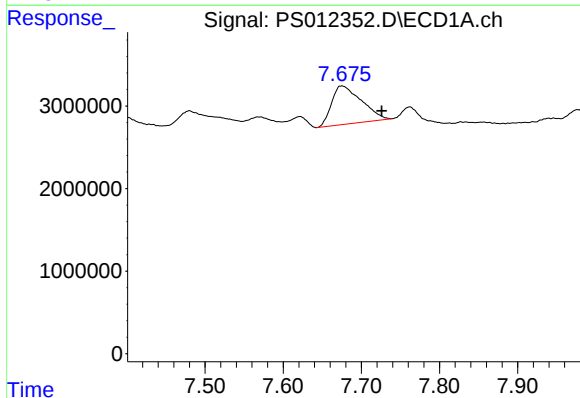


#7 MCPA

R.T.: 7.675 min
Delta R.T.: -0.051 min
Response: 12292905
Conc: 2.63 ug/ml

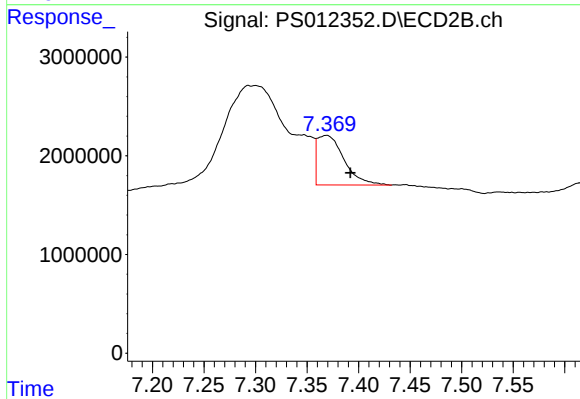

#7 MCPA


R.T.: 7.369 min
Delta R.T.: -0.023 min
Response: 9040723
Conc: 3.22 ug/ml

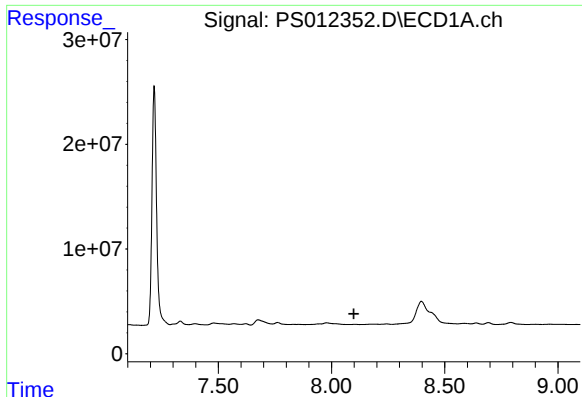

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

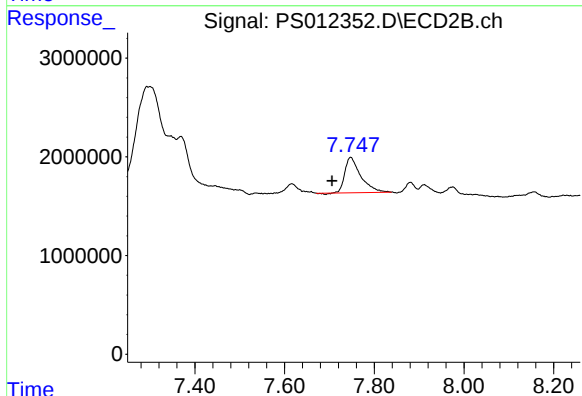


#8 DICHLORPROP

R.T.: 7.748 min
Delta R.T.: 0.042 min
Response: 8810919
Conc: 15.57 ng/ml

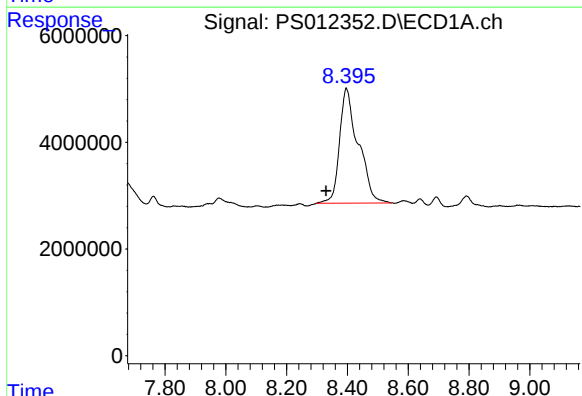


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.067 min
Response: 91852174
Conc: 80.65 ng/ml

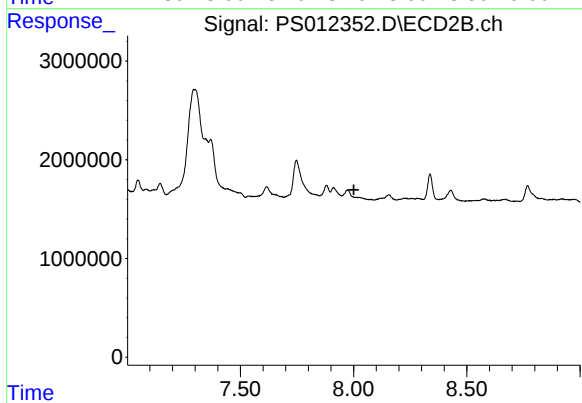

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

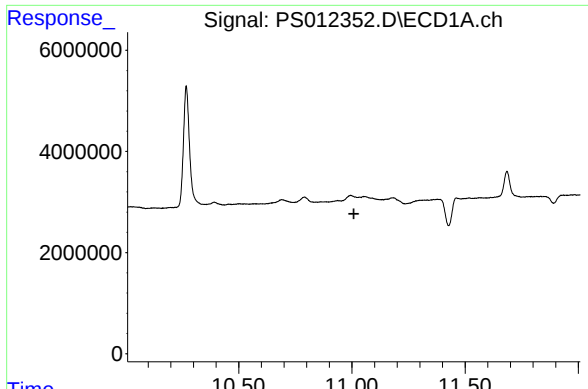

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

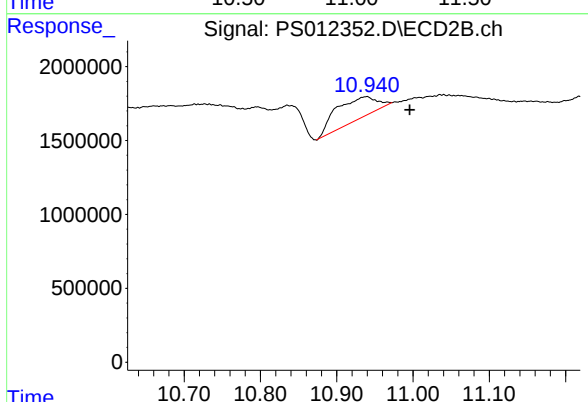


#15 Picloram

R.T.: 10.940 min
Delta R.T.: -0.056 min
Response: 5551289
Conc: 1.31 ng/ml

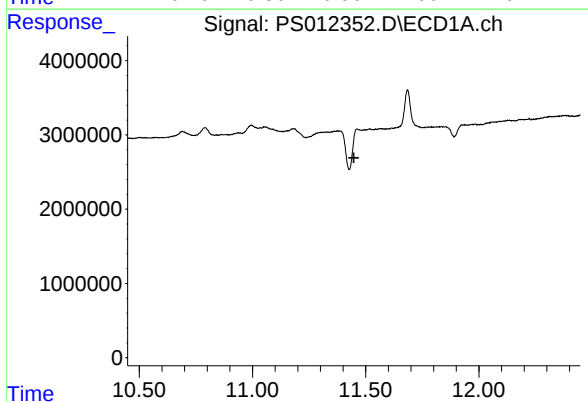

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.448 min
Response: 0
Conc: N.D.

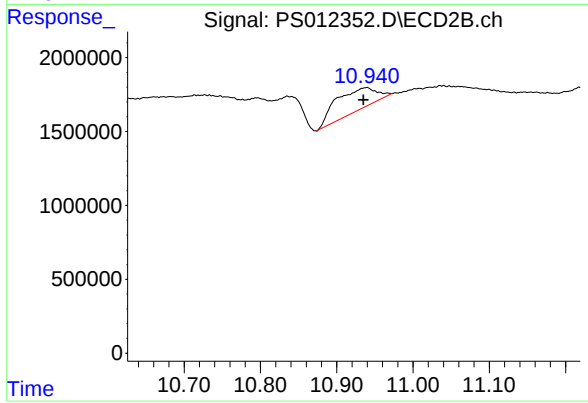

#16 DCPA

R.T.: 10.940 min
Delta R.T.: 0.005 min
Response: 5551289
Conc: 1.53 ng/ml