

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
 Data File : PS012356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2020 21:23
 Operator : DD\AJ
 Sample : L4015-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 05:15:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	424.4E6	236.4E6	391.551	448.108
Target Compounds							
1) T	Dalapon	0.000	2.596	0	8285624	N.D.	12.447
2) T	3,5-DICHL...	0.000	6.094	0	75457089	N.D.	93.272
3) T	4-Nitroph...	7.054	0.000	2902019	0	5.449	N.D. #
5) T	DICAMBA	7.393	7.045	9450118	14398219	2.246	6.676 #
6) T	MCPD	7.570	0.000	5280348	0	1.639	N.D. #
7) T	MCPA	7.699	7.419	132.4E6	4044046	28.332	1.439 #
8) T	DICHLORPROP	0.000	7.737	0	17103454	N.D.	30.228
9) T	2,4-D	8.397	0.000	96700050	0	84.902	N.D. #
11) T	2,4,5-TP ...	0.000	8.793	0	9423869	N.D.	3.256
12) T	2,4,5-T	9.409	0.000	21383974	0	3.487	N.D. #
14) T	DINOSEB	0.000	10.052	0	10855673	N.D.	5.227
15) T	Picloram	0.000	11.017	0	6260749	N.D.	1.477
16) T	DCPA	0.000	10.935	0	7373703	N.D.	2.029



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
Data File : PS012356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2020 21:23
Operator : DD\AJ
Sample : L4015-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 05:15:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

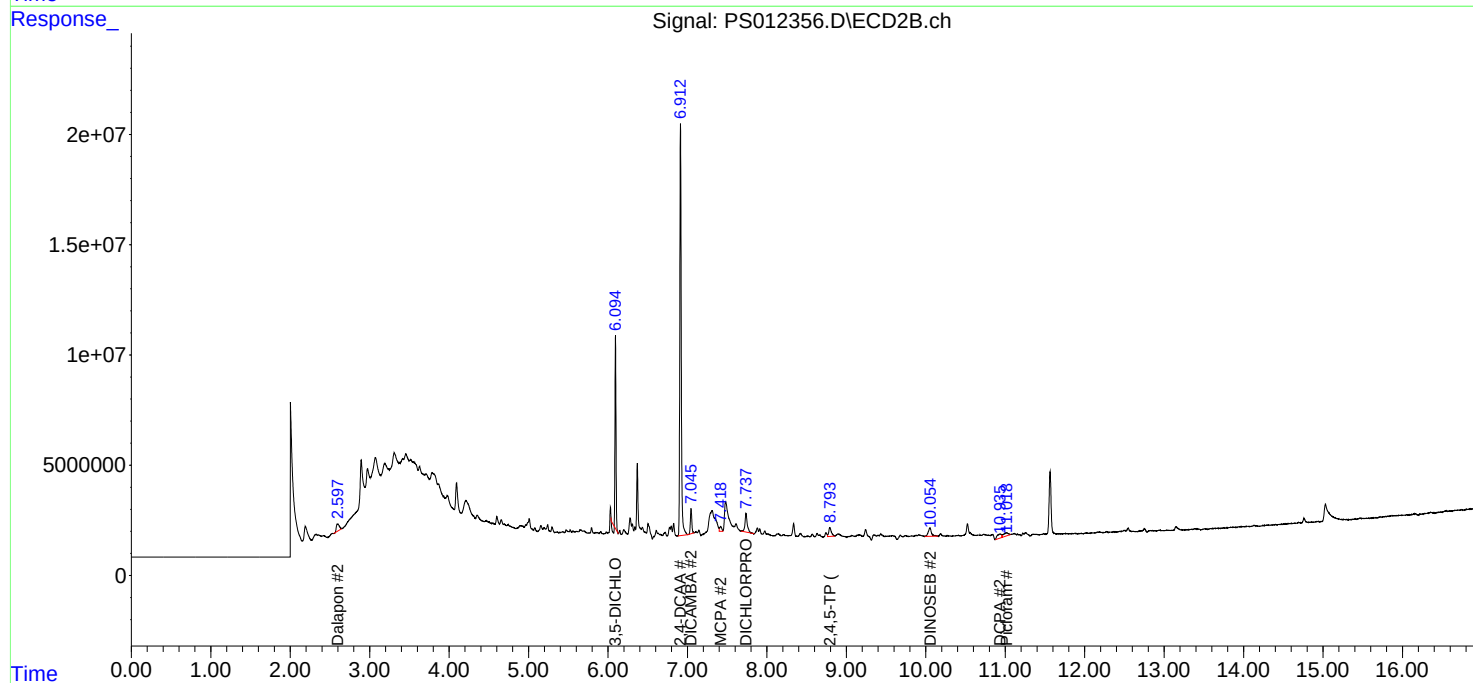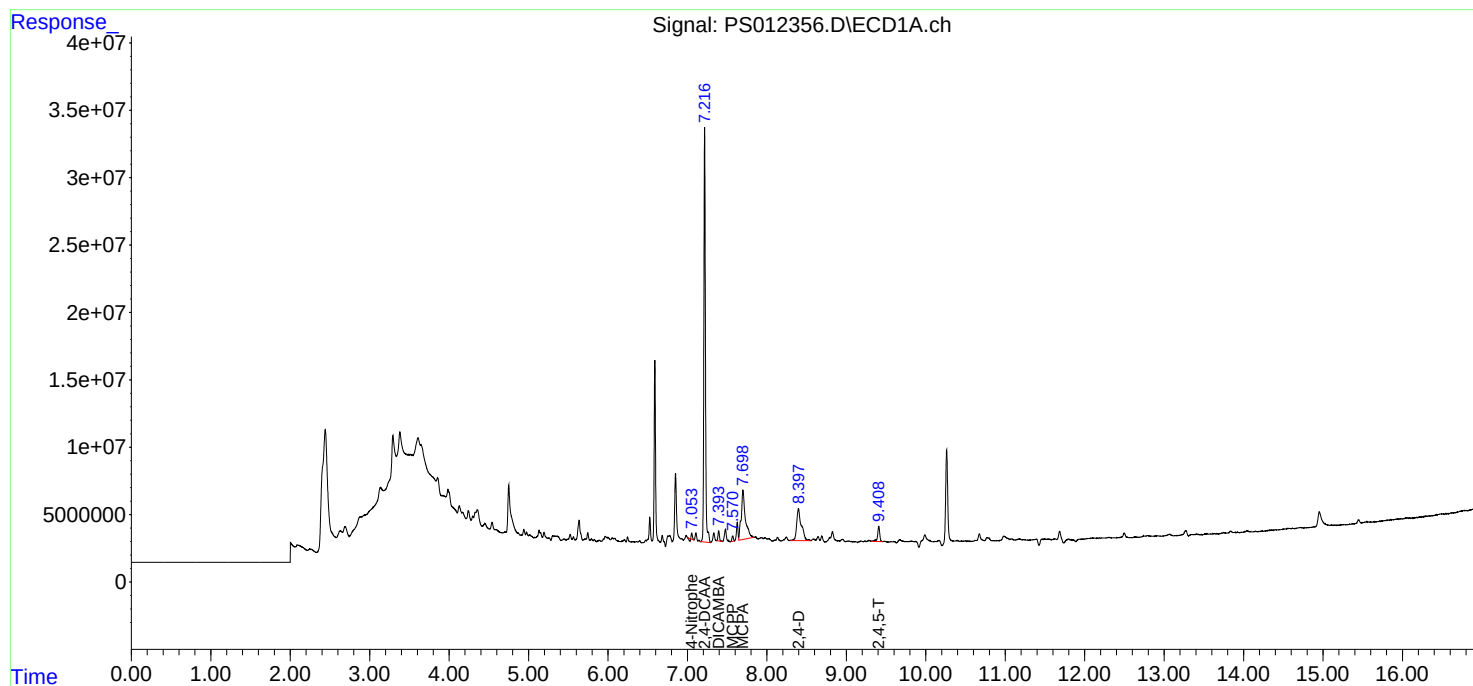


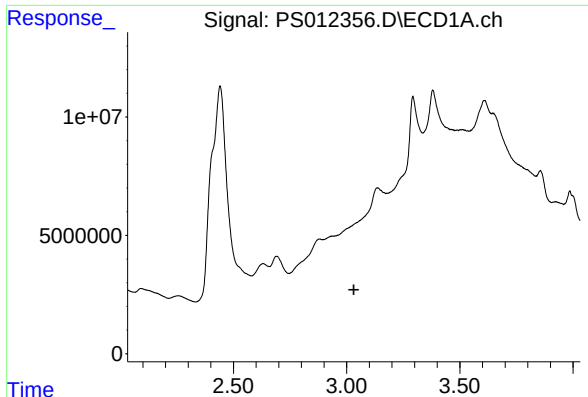

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

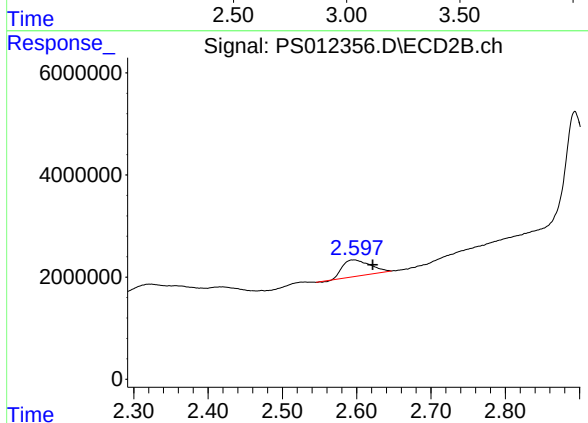


#1 Dalapon

R.T.: 2.596 min
Delta R.T.: -0.025 min
Response: 8285624
Conc: 12.45 ng/ml

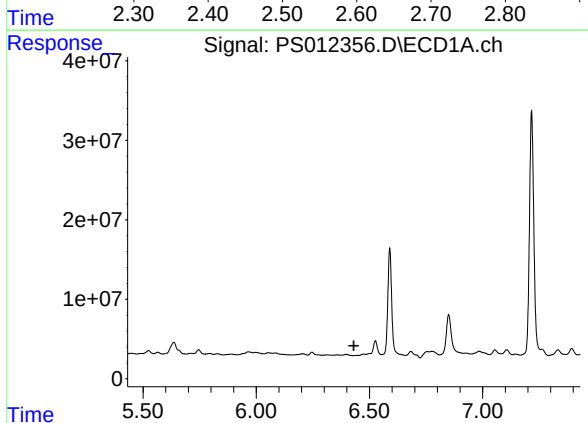


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

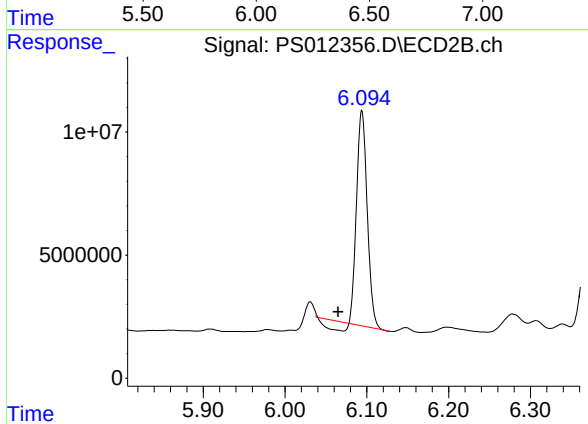

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 75457089
Conc: 93.27 ng/ml

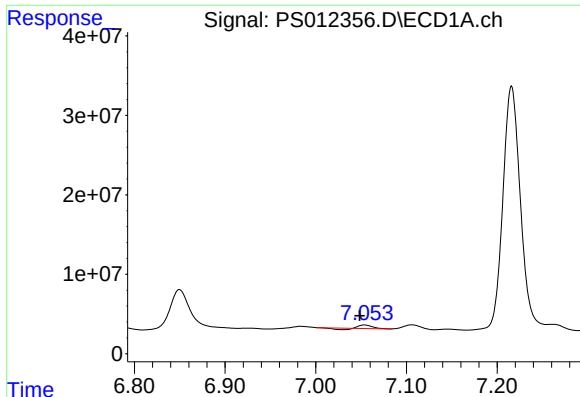

#3 4-Nitrophenol


R.T.: 7.054 min
Delta R.T.: 0.005 min
Response: 2902019
Conc: 5.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

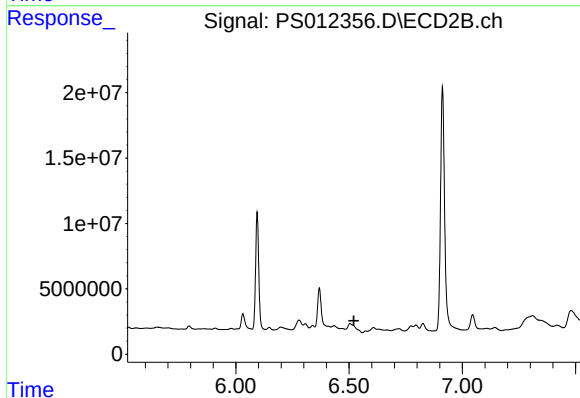


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

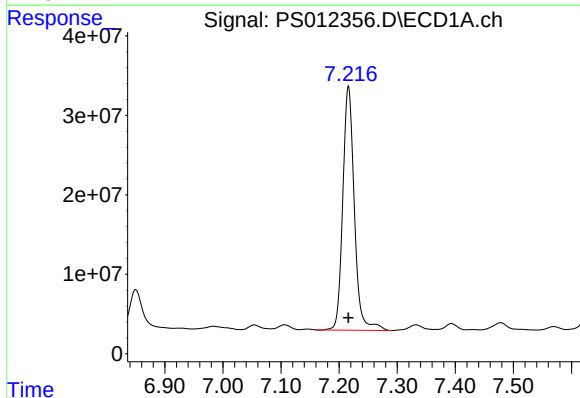


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 424400159
Conc: 391.55 ng/ml

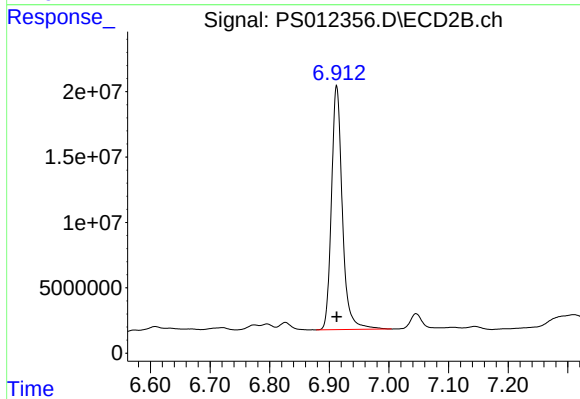

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 236424047
Conc: 448.11 ng/ml

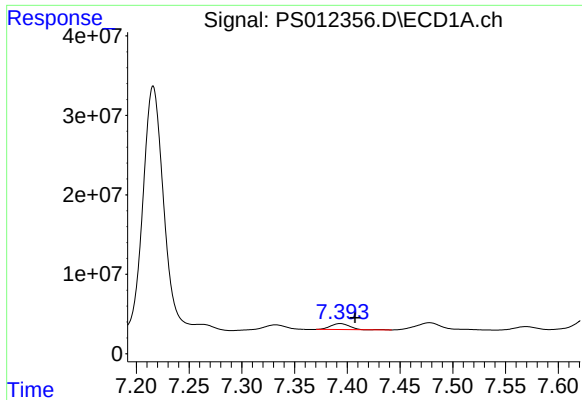

#5 DICAMBA


R.T.: 7.393 min
Delta R.T.: -0.014 min
Response: 9450118
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

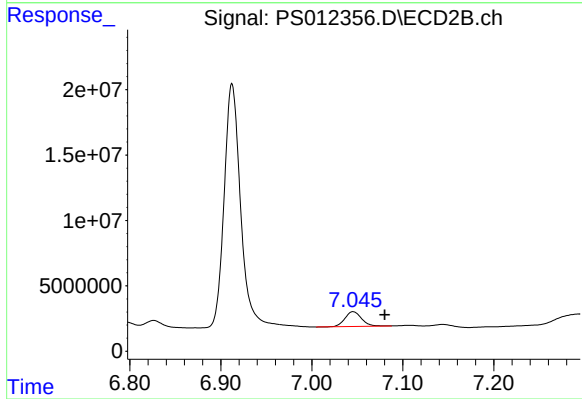


#5 DICAMBA

R.T.: 7.045 min
Delta R.T.: -0.035 min
Response: 14398219
Conc: 6.68 ng/ml

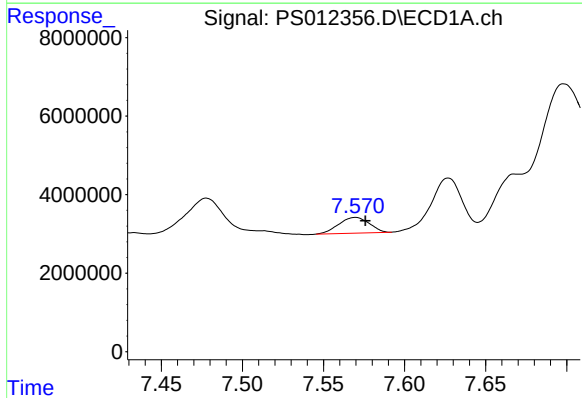


#6 MCP

R.T.: 7.570 min
Delta R.T.: -0.006 min
Response: 5280348
Conc: 1.64 ug/ml

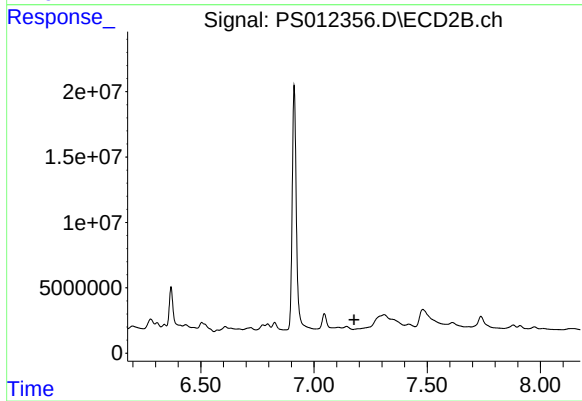

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.177 min
Response: 0
Conc: N.D.

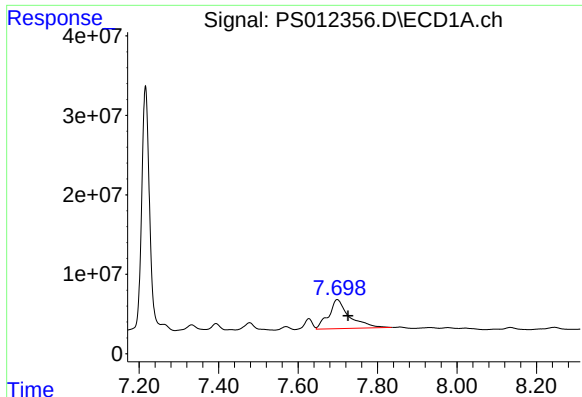

#7 MCPA


R.T.: 7.699 min
Delta R.T.: -0.027 min
Response: 132378844
Conc: 28.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

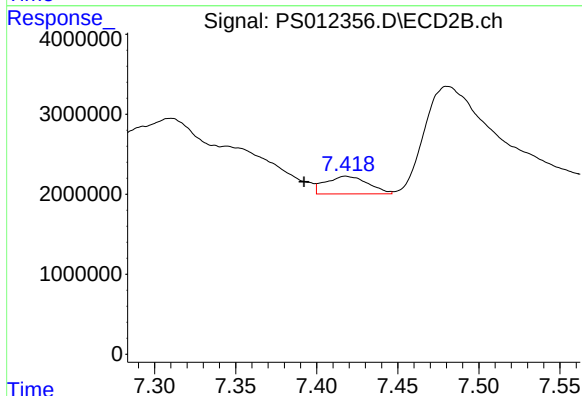


#7 MCPA

R.T.: 7.419 min
Delta R.T.: 0.026 min
Response: 4044046
Conc: 1.44 ug/ml

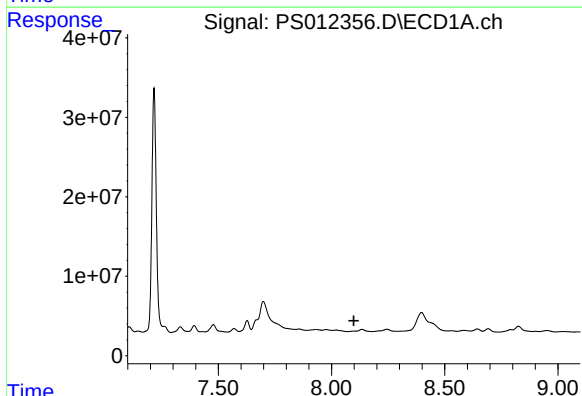


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.099 min
Response: 0
Conc: N.D.

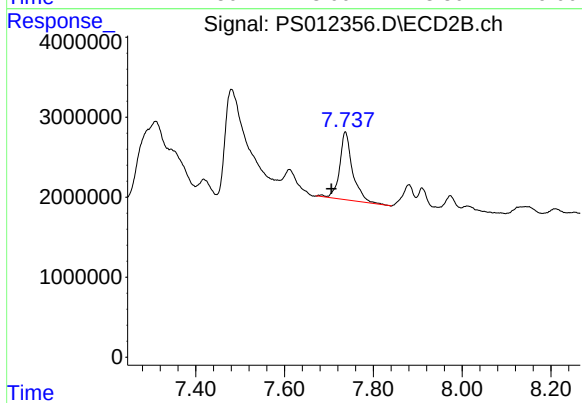

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.031 min
Response: 17103454
Conc: 30.23 ng/ml

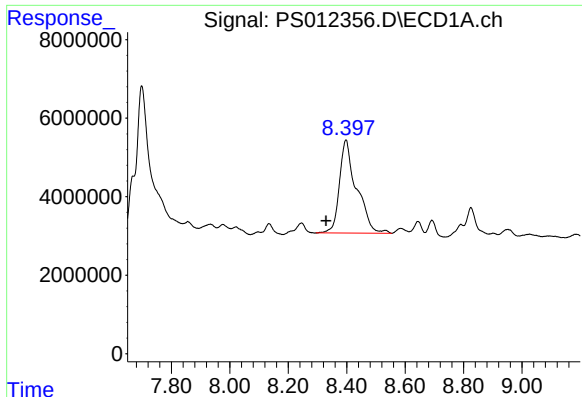

#9 2,4-D


R.T.: 8.397 min
Delta R.T.: 0.068 min
Response: 96700050
Conc: 84.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

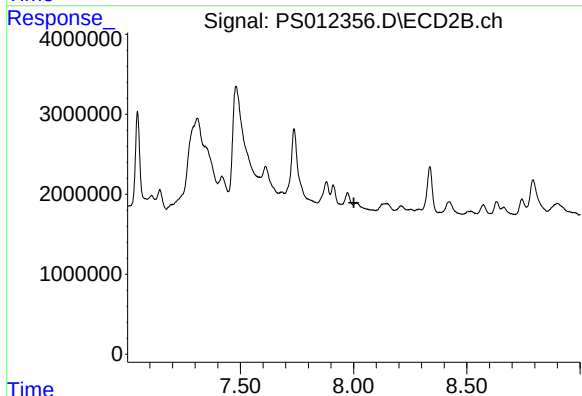


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

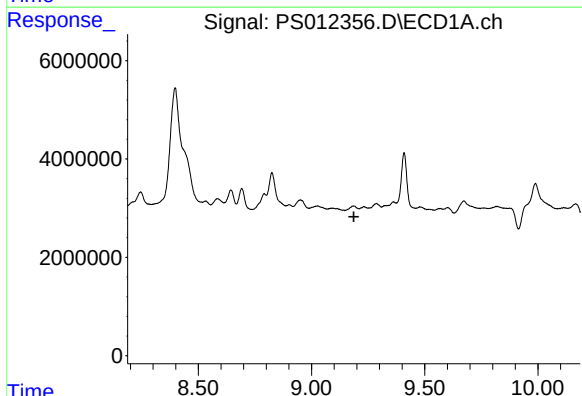


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.187 min
Response: 0
Conc: N.D.

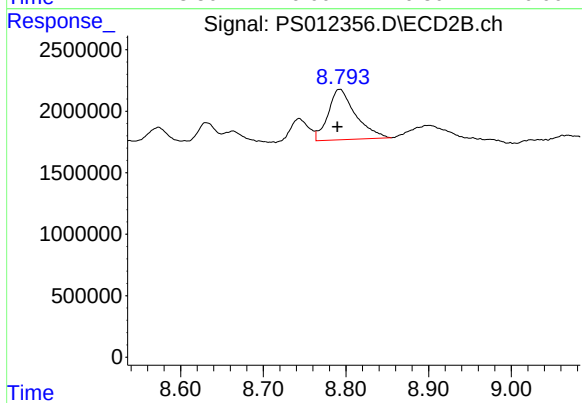

#11 2,4,5-TP (SILVEX)


R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 9423869
Conc: 3.26 ng/ml

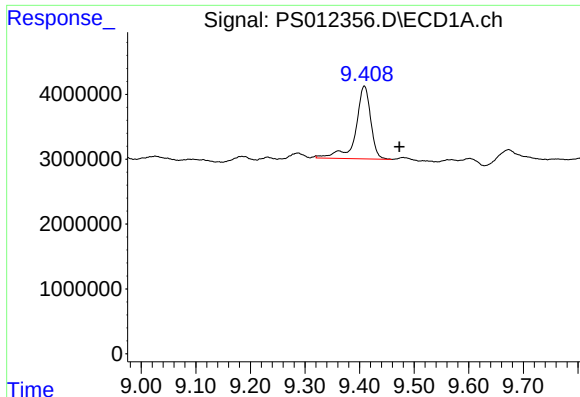

#12 2,4,5-T


R.T.: 9.409 min
Delta R.T.: -0.064 min
Response: 21383974
Conc: 3.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

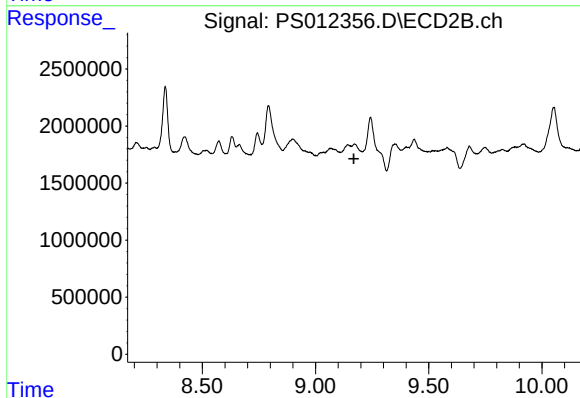


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

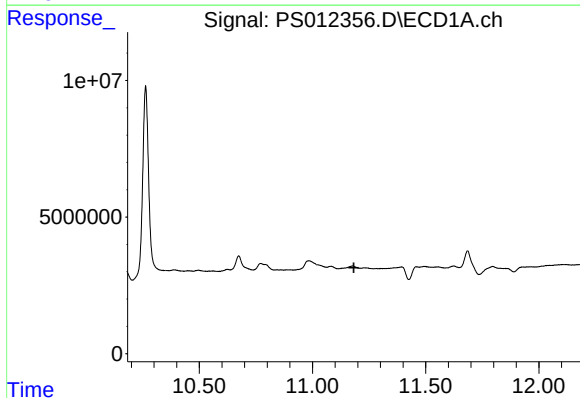


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.183 min
Response: 0
Conc: N.D.

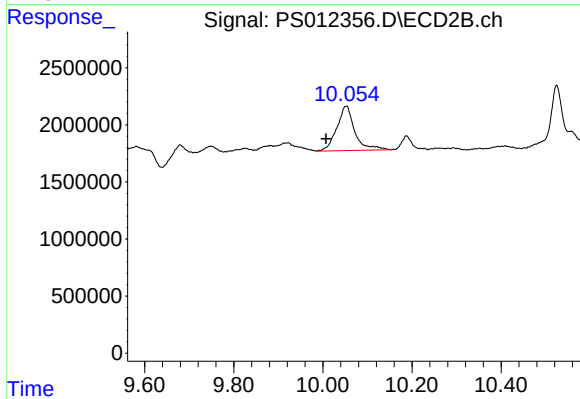

#14 DINOSEB


R.T.: 10.052 min
Delta R.T.: 0.045 min
Response: 10855673
Conc: 5.23 ng/ml

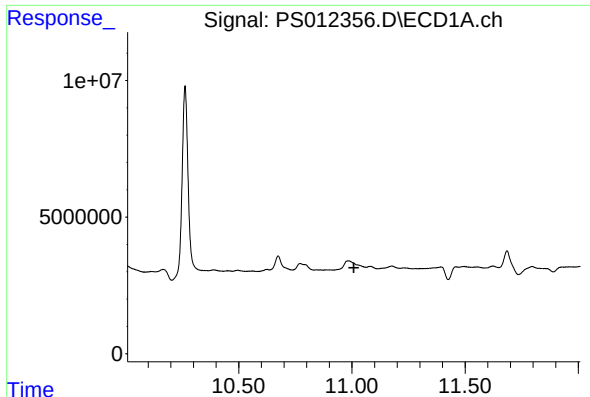

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

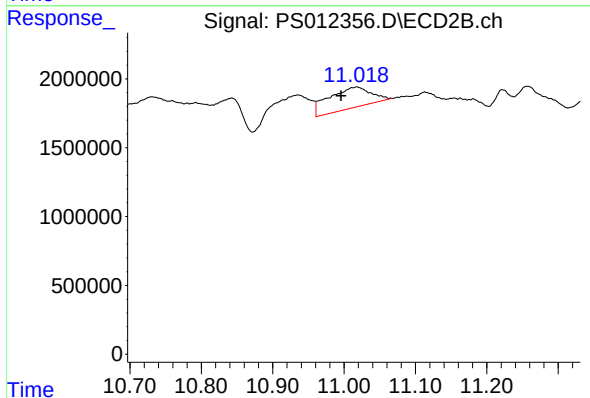


#15 Picloram

R.T.: 11.017 min
Delta R.T.: 0.022 min
Response: 6260749
Conc: 1.48 ng/ml

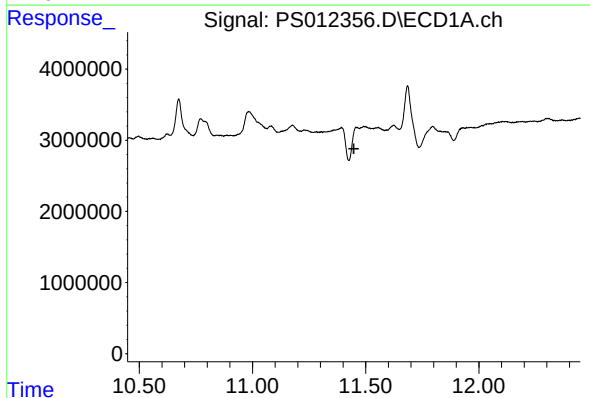

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.448 min
Response: 0
Conc: N.D.

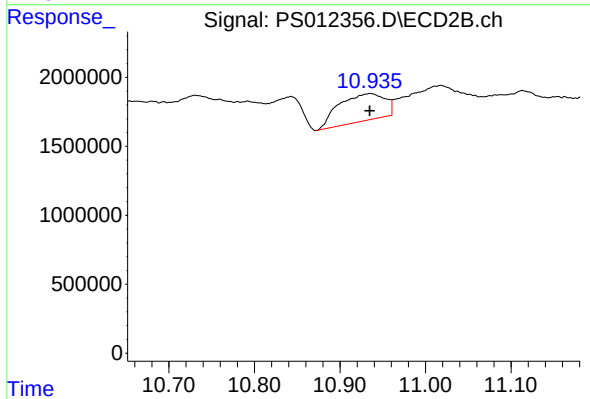

#16 DCPA

R.T.: 10.935 min
Delta R.T.: 0.000 min
Response: 7373703
Conc: 2.03 ng/ml