

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
 Data File : PS012359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2020 22:32
 Operator : DD\AJ
 Sample : L4019-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 05:16:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	443.9E6	247.4E6	409.545	468.832
Target Compounds							
1) T	Dalapon	0.000	2.592	0	7684686	N.D.	11.544
2) T	3,5-DICHL...	0.000	6.094	0	73382621	N.D.	90.708
3) T	4-Nitroph...	7.053	0.000	3600647	0	6.761	N.D. #
5) T	DICAMBA	7.393	7.046	10071445	15225235	2.394	7.059 #
6) T	MCPD	7.569	0.000	5599804	0	1.738	N.D. #
7) T	MCPA	7.699	7.421	109.7E6	3660066	23.470	1.302 #
8) T	DICHLORPROP	0.000	7.737	0	19048399	N.D.	33.666
9) T	2,4-D	8.395	0.000	94788886	0	83.224	N.D. #
10) T	Pentachlo...	8.691	0.000	6932591	0	<MDL	N.D. #
12) T	2,4,5-T	9.410	0.000	25272821	0	4.121	N.D. #
14) T	DINOSEB	0.000	10.052	0	9266759	N.D.	4.462
15) T	Picloram	0.000	10.932	0	4641967	N.D.	1.095
16) T	DCPA	0.000	10.932	0	4641967	N.D.	1.277



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091720\
Data File : PS012359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2020 22:32
Operator : DD\AJ
Sample : L4019-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 05:16:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

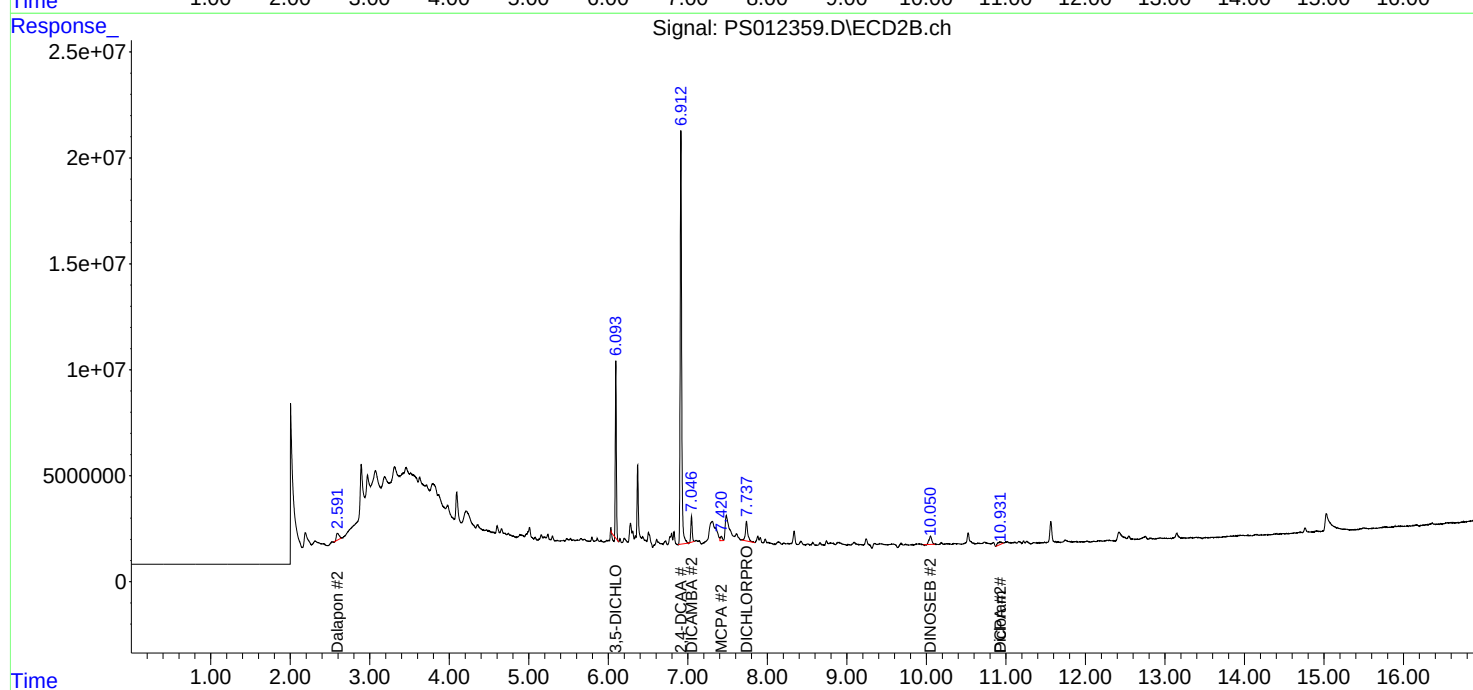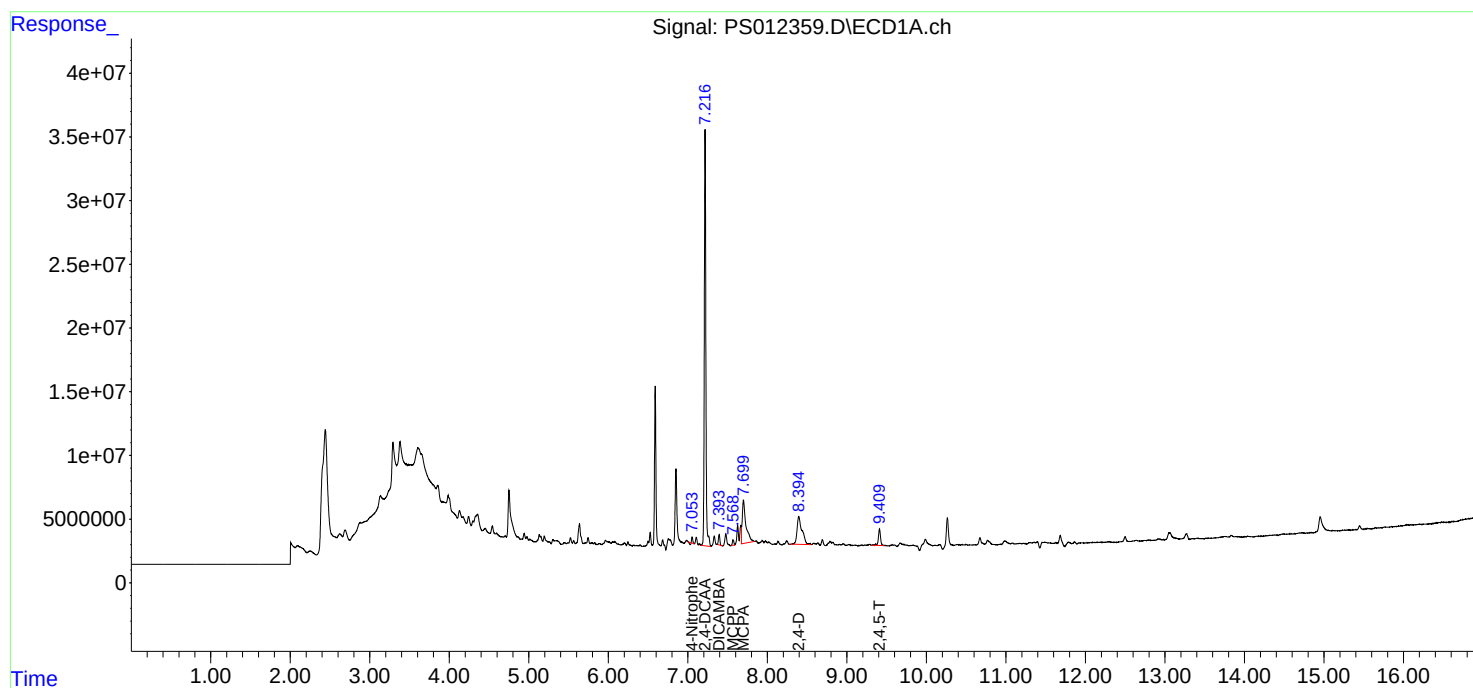


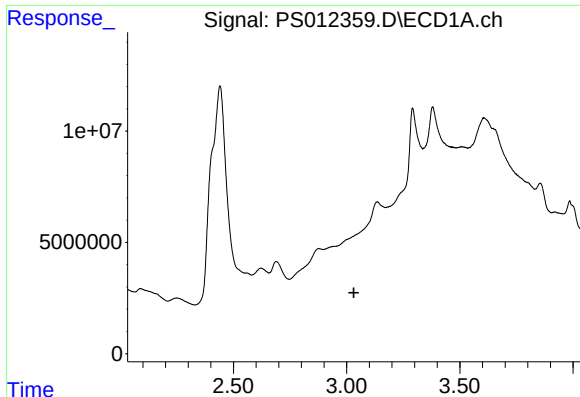

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

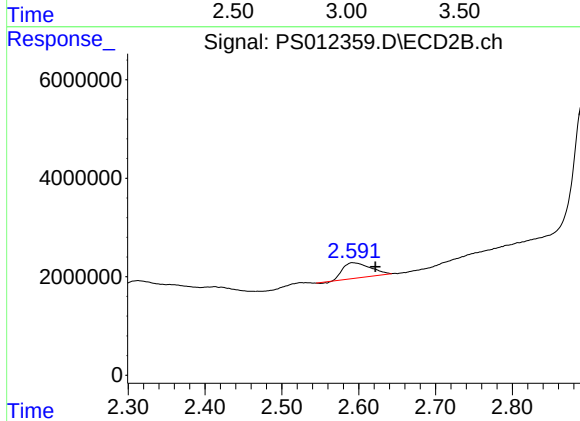


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.029 min
Response: 7684686
Conc: 11.54 ng/ml

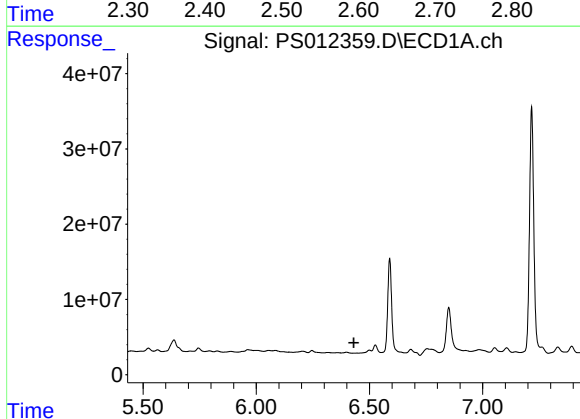


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

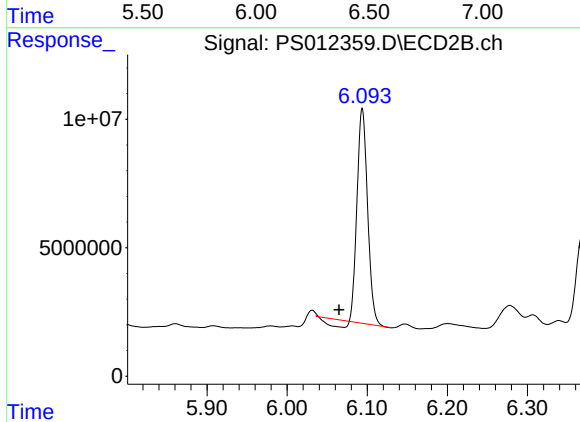

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 73382621
Conc: 90.71 ng/ml

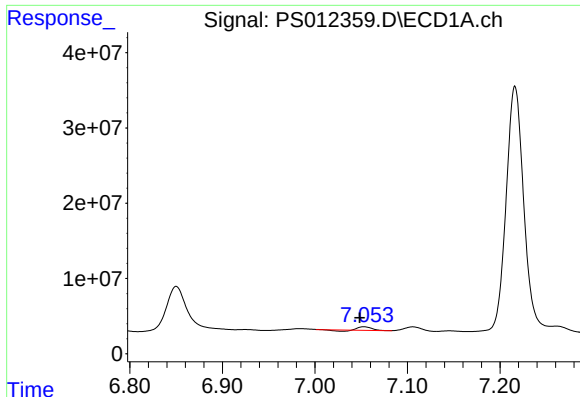

#3 4-Nitrophenol


R.T.: 7.053 min
Delta R.T.: 0.005 min
Response: 3600647
Conc: 6.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

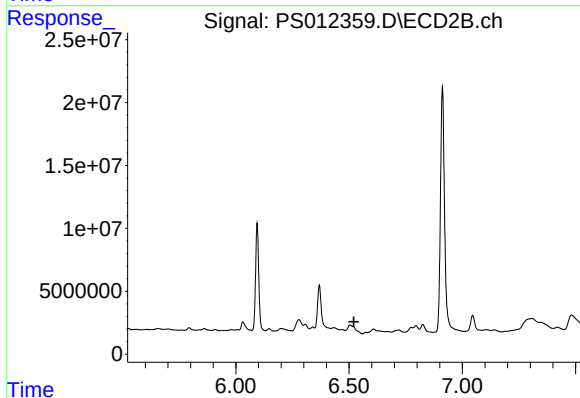


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

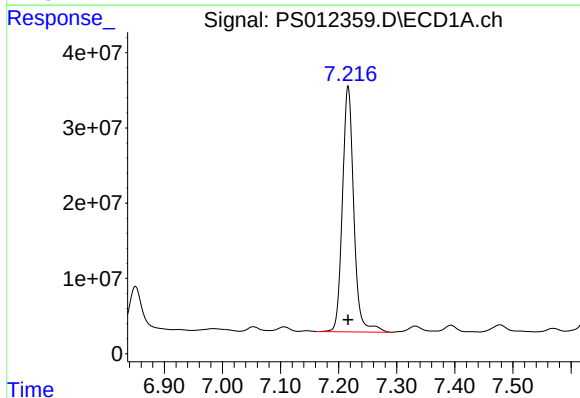


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 443904350
Conc: 409.55 ng/ml

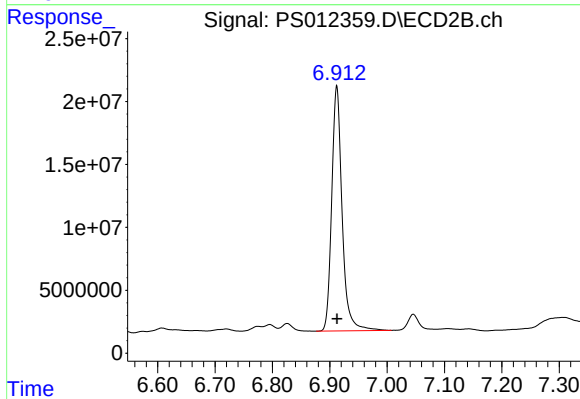

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 247358040
Conc: 468.83 ng/ml

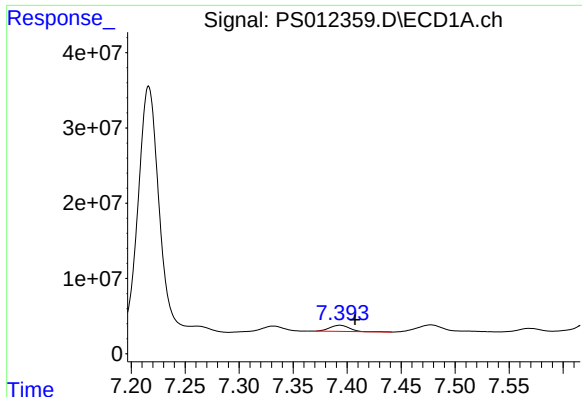

#5 DICAMBA


R.T.: 7.393 min
Delta R.T.: -0.014 min
Response: 10071445
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

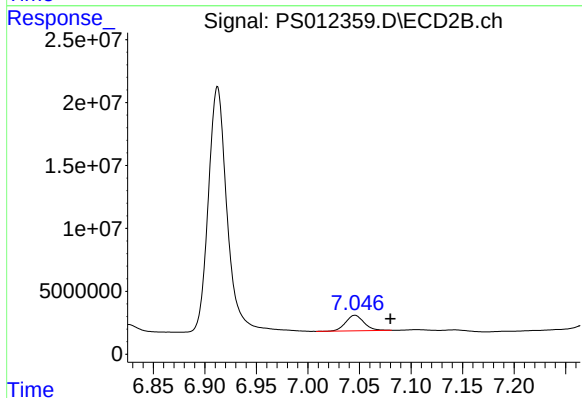


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 15225235
Conc: 7.06 ng/ml

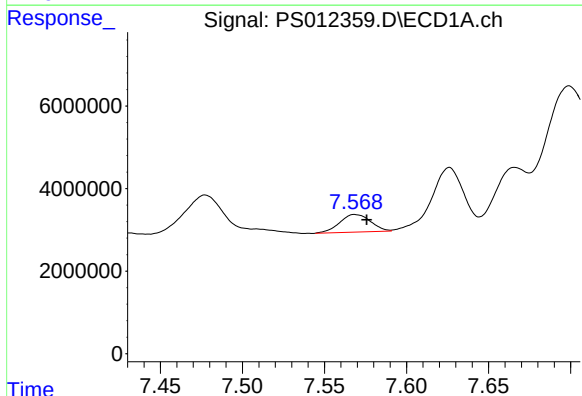


#6 MCP

R.T.: 7.569 min
Delta R.T.: -0.007 min
Response: 5599804
Conc: 1.74 ug/ml

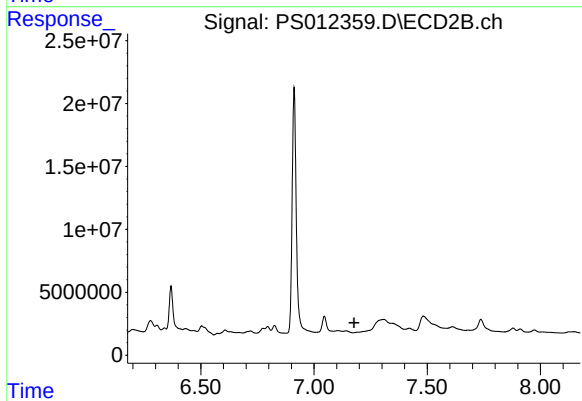

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.177 min
Response: 0
Conc: N.D.

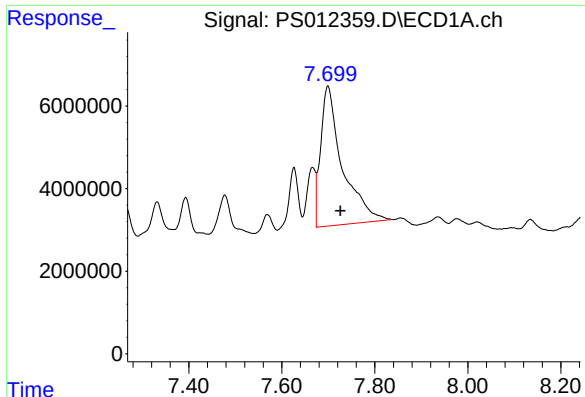

#7 MCPA


R.T.: 7.699 min
Delta R.T.: -0.027 min
Response: 109662213
Conc: 23.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

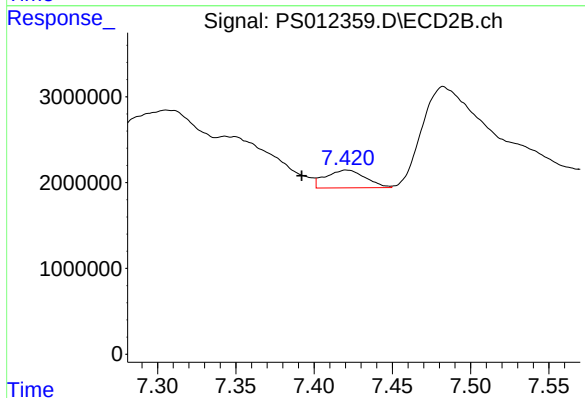


#7 MCPA

R.T.: 7.421 min
Delta R.T.: 0.029 min
Response: 3660066
Conc: 1.30 ug/ml

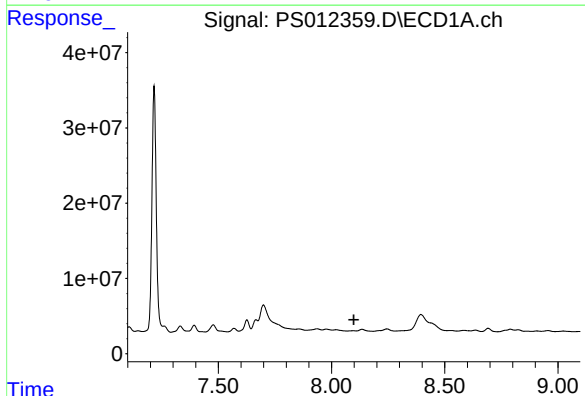


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.099 min
Response: 0
Conc: N.D.

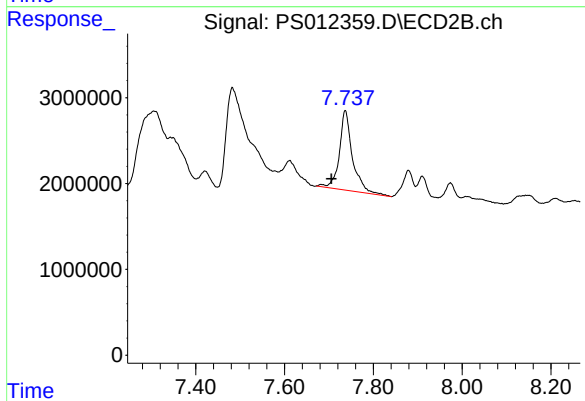

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.031 min
Response: 19048399
Conc: 33.67 ng/ml

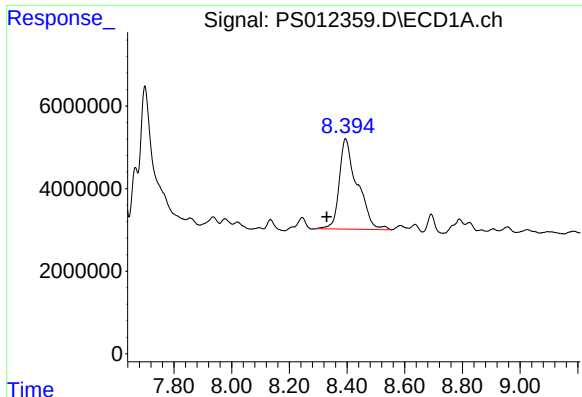

#9 2,4-D


R.T.: 8.395 min
Delta R.T.: 0.065 min
Response: 94788886
Conc: 83.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

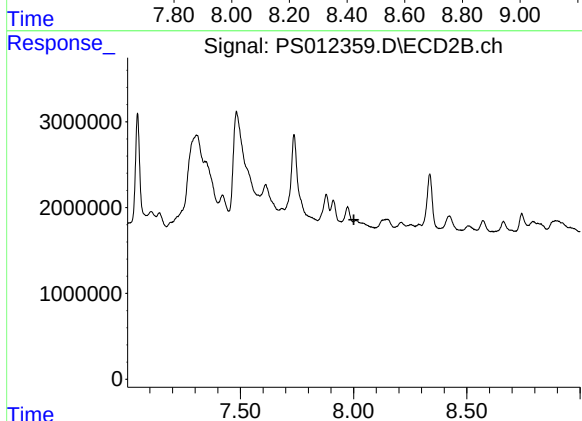


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

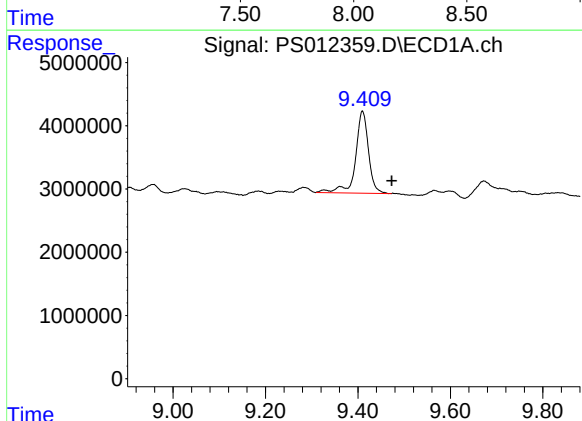


#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.063 min
Response: 25272821
Conc: 4.12 ng/ml

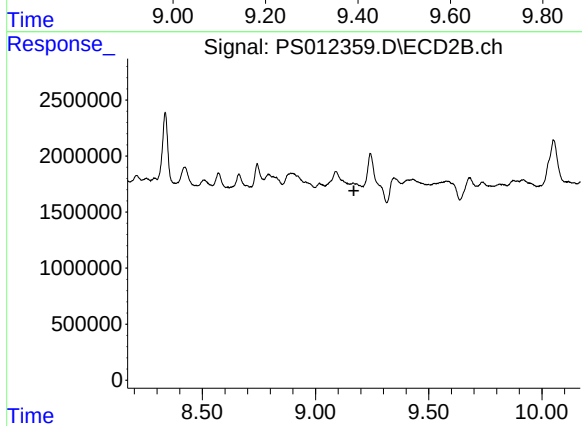

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

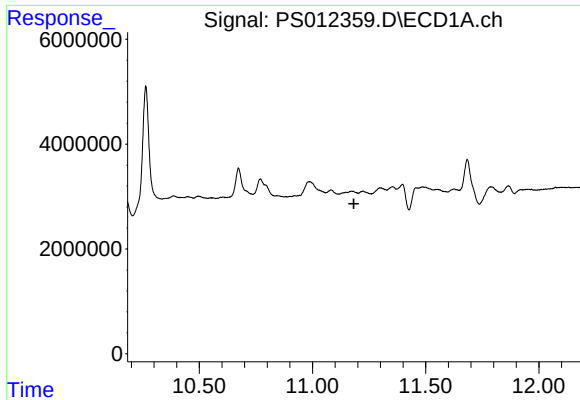

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

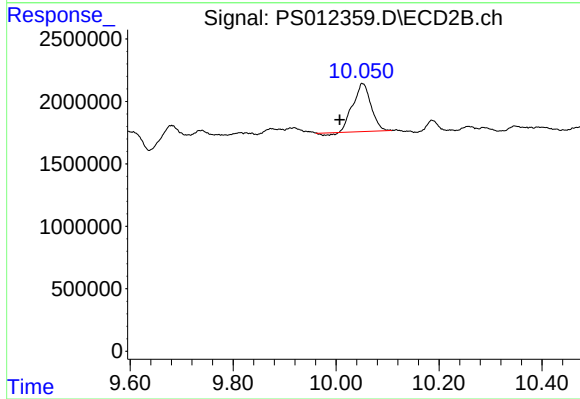


#14 DINOSEB

R.T.: 10.052 min
Delta R.T.: 0.044 min
Response: 9266759
Conc: 4.46 ng/ml

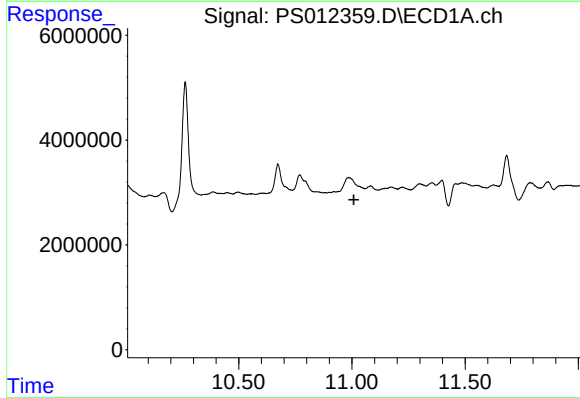


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

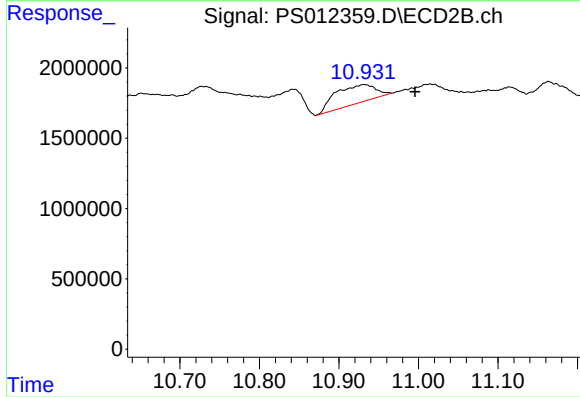

#15 Picloram


R.T.: 10.932 min
Delta R.T.: -0.064 min
Response: 4641967
Conc: 1.09 ng/ml

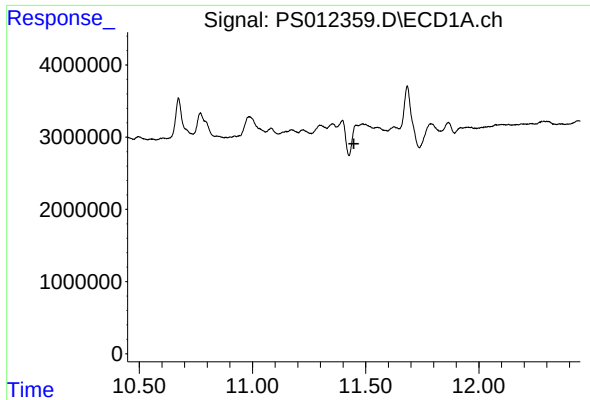

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

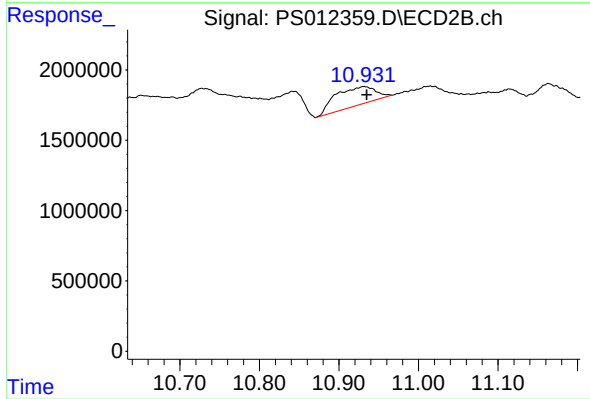

#16 DCPA

R.T.: 10.932 min
Delta R.T.: -0.003 min
Response: 4641967
Conc: 1.28 ng/ml