

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091724\
 Data File : PS027698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2024 09:54
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 13:59:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.091	7.650	705060	827550	<MDL	<MDL	#
Target Compounds								
1) T	Dalapon	2.548	0.000	14490038	0	3.497	N.D.	#
2) T	3,5-DICHL...	0.000	6.649f	0	2009364	N.D.	1.247	
3) T	4-Nitroph...	6.897	0.000	4661233	0	2.753	N.D.	#
5) T	DICAMBA	0.000	7.819	0	2615878	N.D.	<MDL	
6) T	MCP	0.000	7.910	0	804918	N.D.	<MDL	
8) T	DICHLORPROP	8.017f	8.578f	-653522	924996	N.D.	<MDL	
9) T	2,4-D	0.000	8.813f	0	972324	N.D.	<MDL	
10) T	Pentachlo...	8.506	9.361	2533161	462884	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.033	9.708f	3202635	2103983	<MDL	<MDL	#
12) T	2,4,5-T	0.000	10.150	0	4220633	N.D.	<MDL	
13) T	2,4-DB	9.919	0.000	987473	0	<MDL	N.D.	#
15) T	Picloram	10.905	12.193	35648150	5349276	1.906	1.151	#
16) T	DCPA	11.373	12.132	2243805	5014744	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091724\
Data File : PS027698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 09:54
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 13:59:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

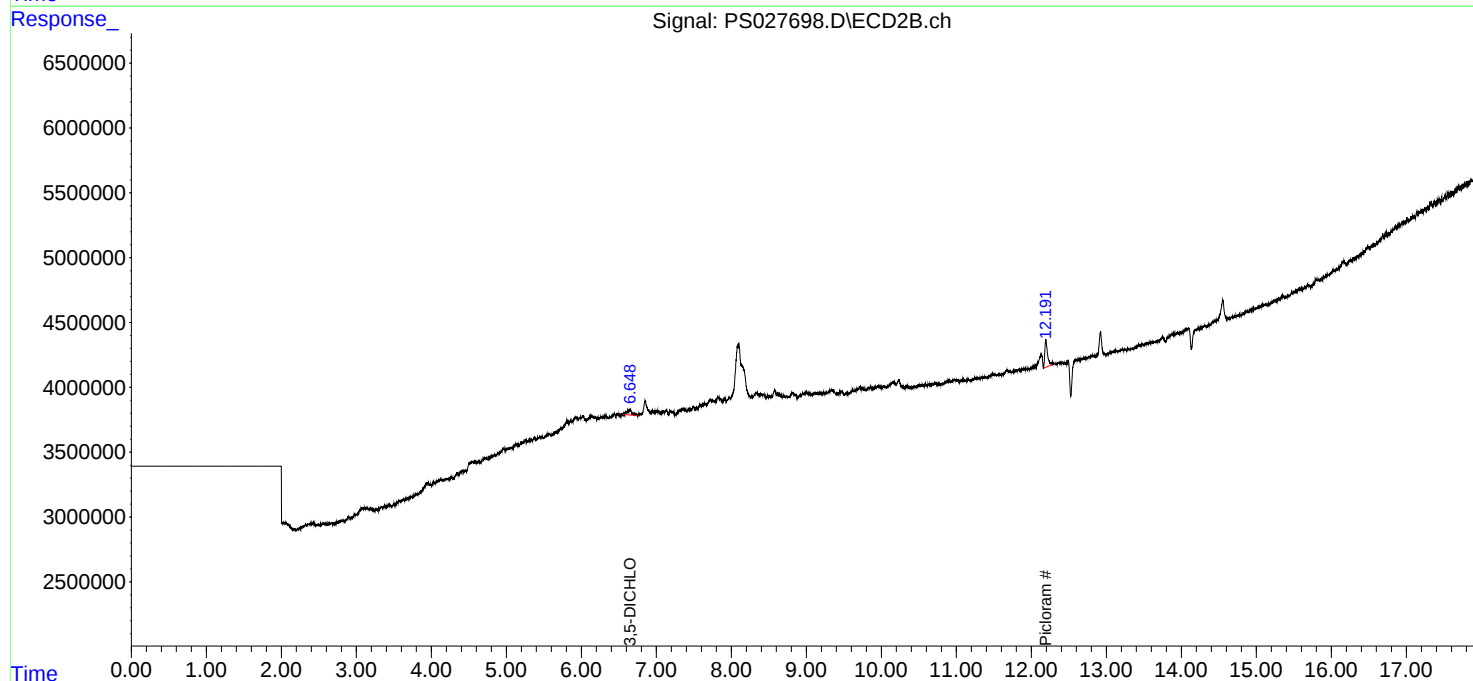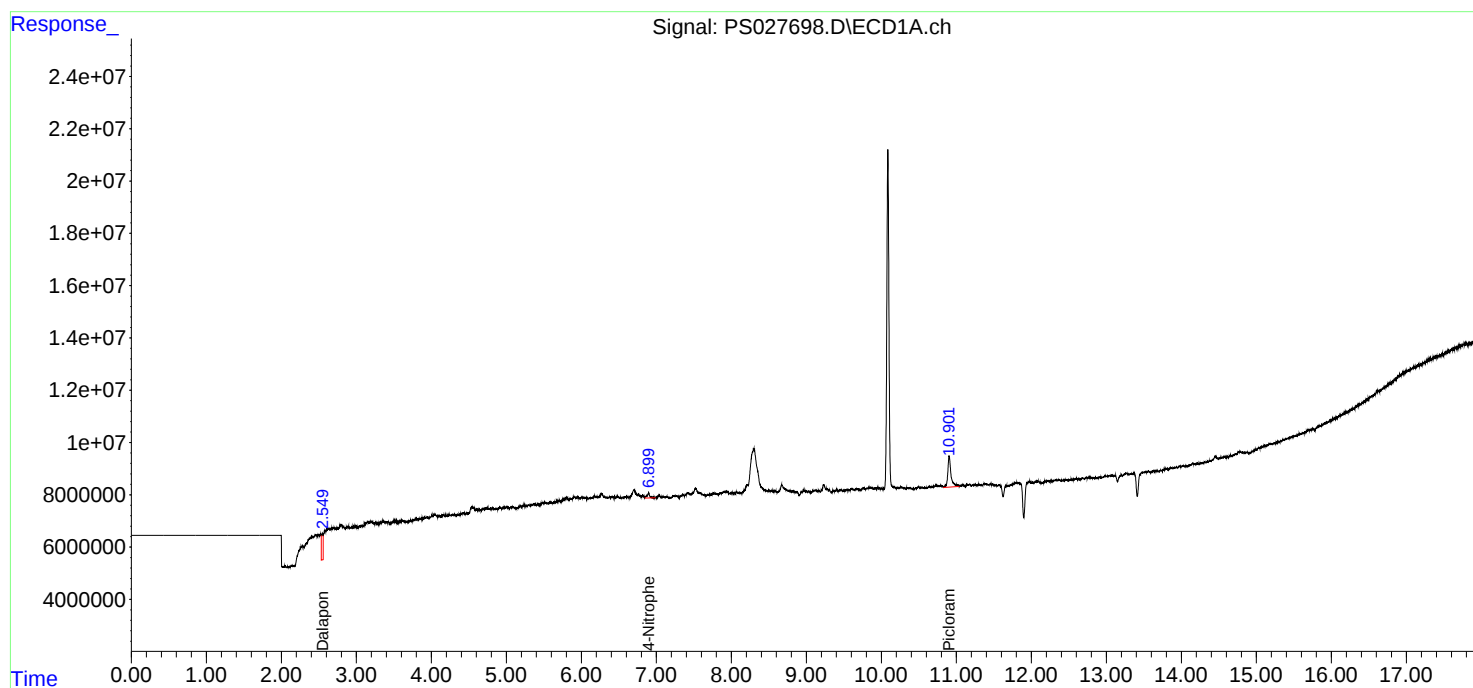


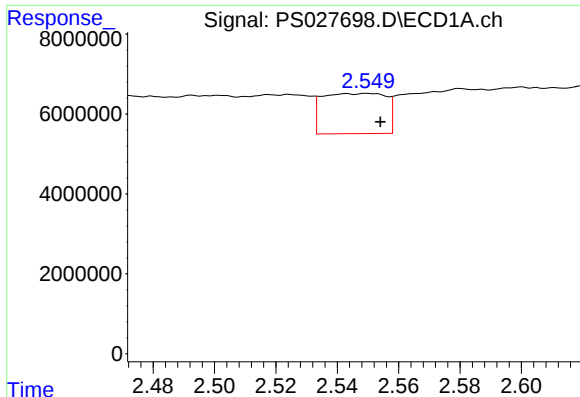

#1 Dalapon


R.T.: 2.548 min
Delta R.T.: -0.006 min
Response: 14490038
Conc: 3.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

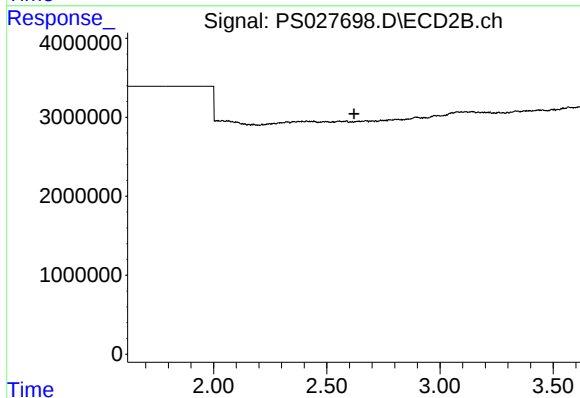


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

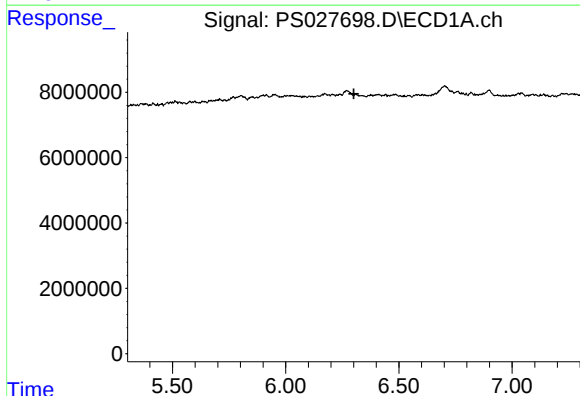


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.301 min
Response: 0
Conc: N.D.

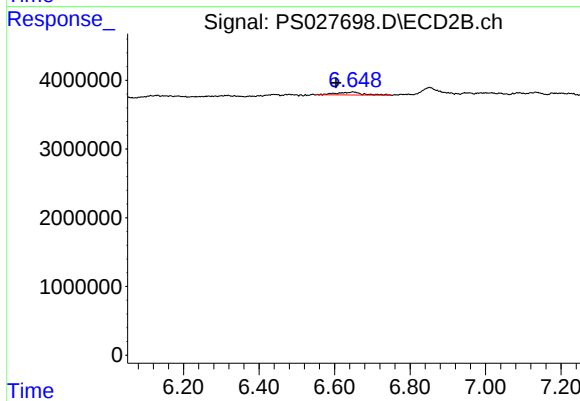

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.649 min
Delta R.T.: 0.045 min
Response: 2009364
Conc: 1.25 ng/ml

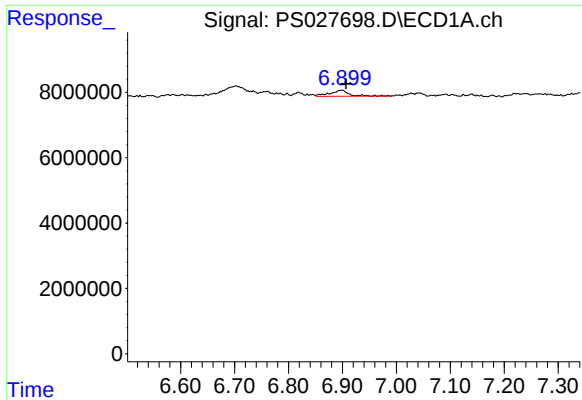

#3 4-Nitrophenol


R.T.: 6.897 min
Delta R.T.: -0.009 min
Response: 4661233
Conc: 2.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

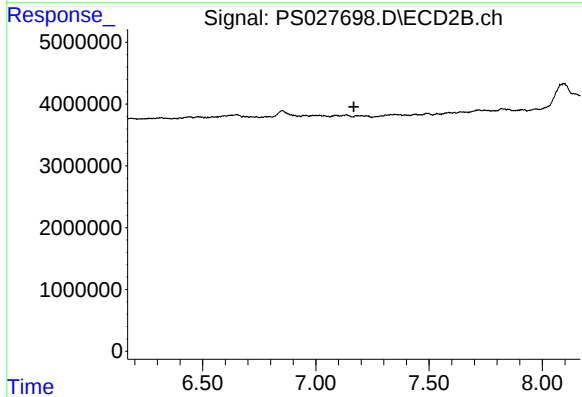


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

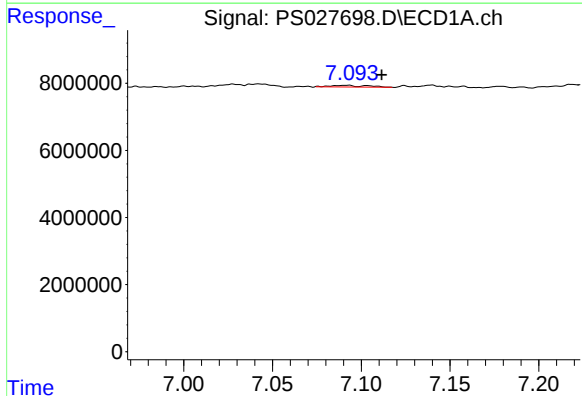


#4 2,4-DCAA

R.T.: 7.091 min
Delta R.T.: -0.020 min
Response: 705060
Conc: N.D.

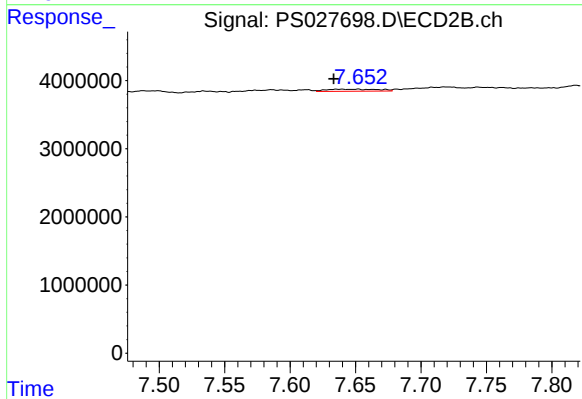

#4 2,4-DCAA


R.T.: 7.650 min
Delta R.T.: 0.017 min
Response: 827550
Conc: N.D.

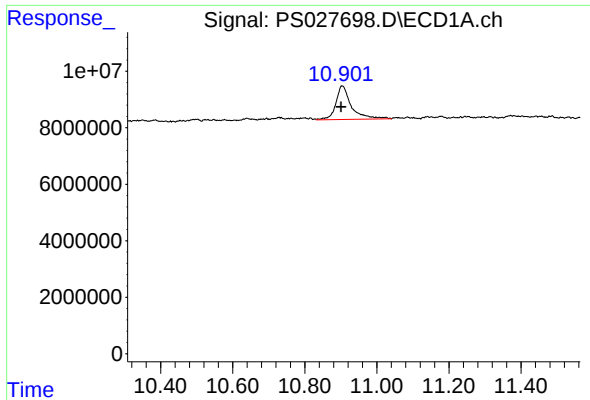

#15 Picloram

R.T.: 10.905 min
Delta R.T.: 0.004 min
Response: 35648150
Conc: 1.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

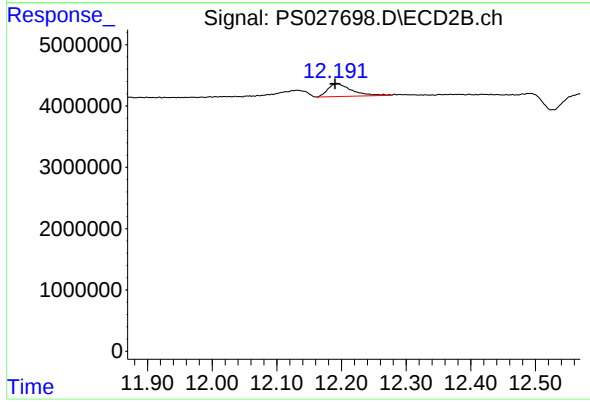

#15 Picloram

R.T.: 12.193 min
Delta R.T.: 0.003 min
Response: 5349276
Conc: 1.15 ng/ml