

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091819\
 Data File : PS006804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2019 14:50
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:04:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.479	5.209	428.8E6	201.9E6	551.928	472.877
Target Compounds							
9) T	2,4-D	6.545	0.000	59887374	0	77.512	N.D. #
15) T	Picloram	9.024	8.985	50666207	19901448	7.511	5.378 #
16) T	DCPA	0.000	8.985	0	19901448	N.D.	6.317



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091819\
Data File : PS006804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2019 14:50
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:04:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

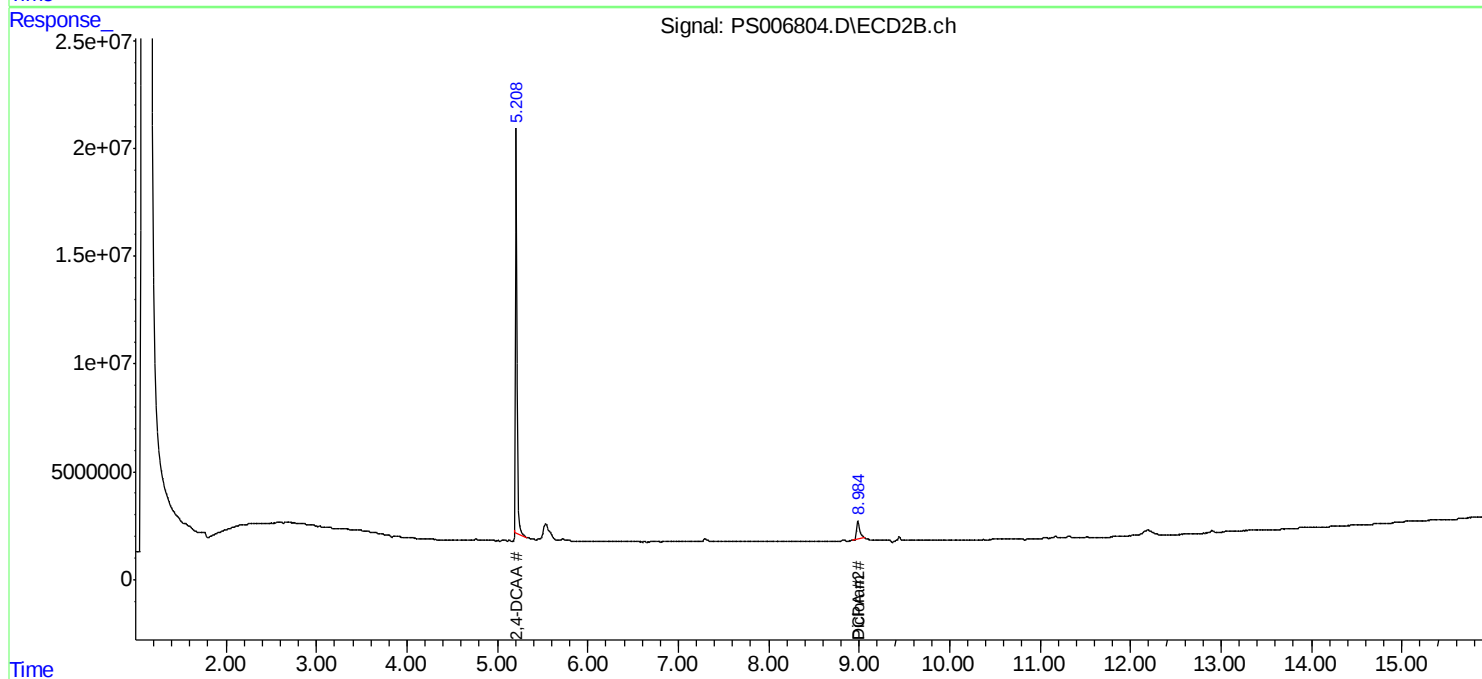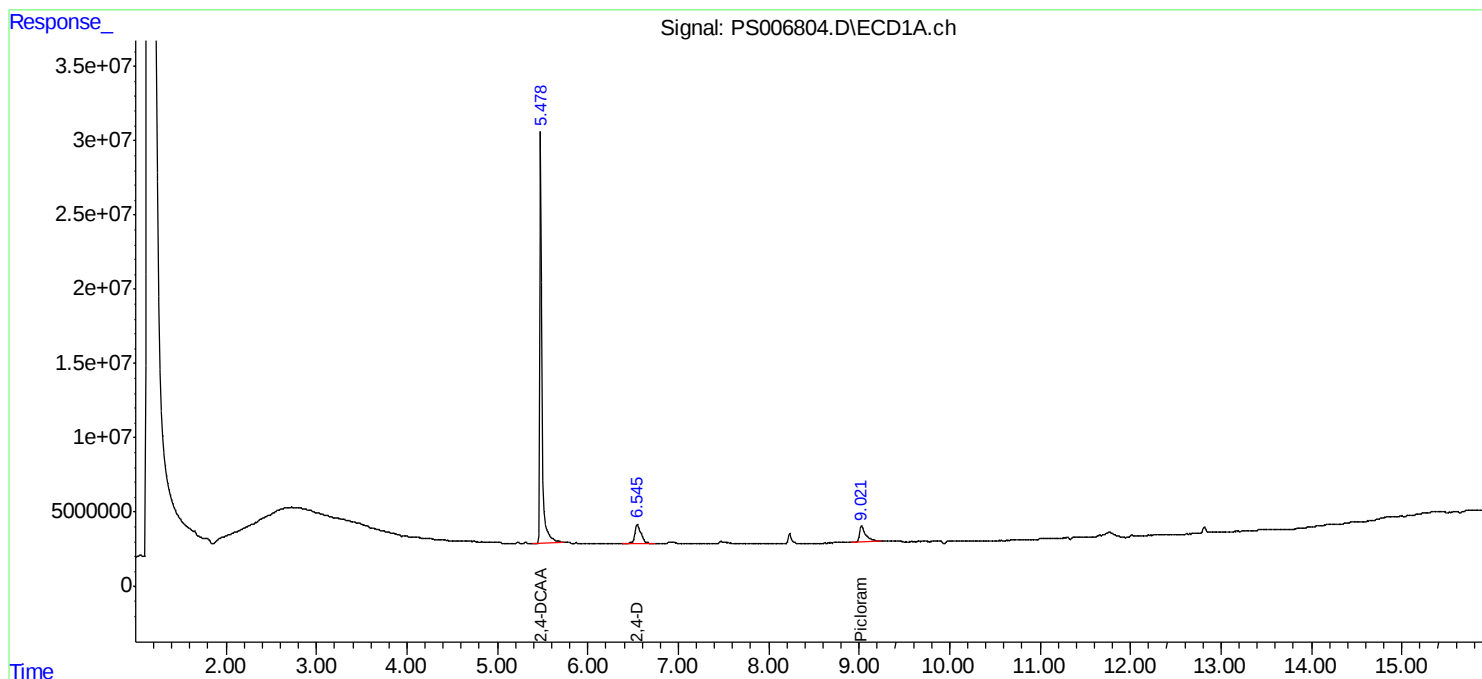


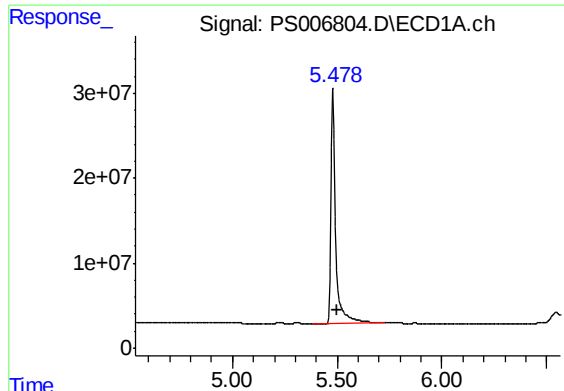

#4 2,4-DCAA


R.T.: 5.479 min
Delta R.T.: -0.021 min
Response: 428784886
Conc: 551.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

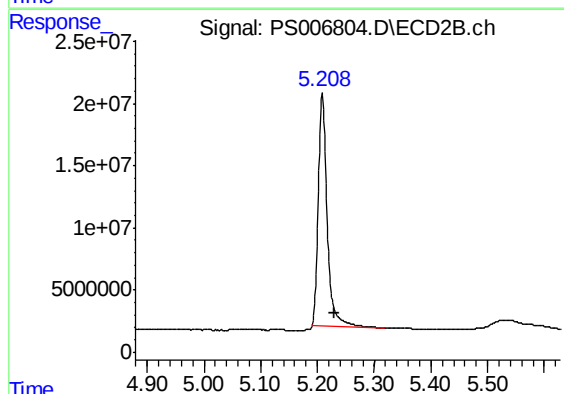


#4 2,4-DCAA

R.T.: 5.209 min
Delta R.T.: -0.021 min
Response: 201919755
Conc: 472.88 ng/ml

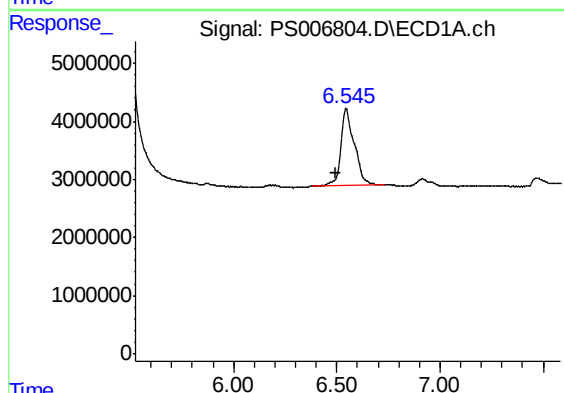


#9 2,4-D

R.T.: 6.545 min
Delta R.T.: 0.048 min
Response: 59887374
Conc: 77.51 ng/ml

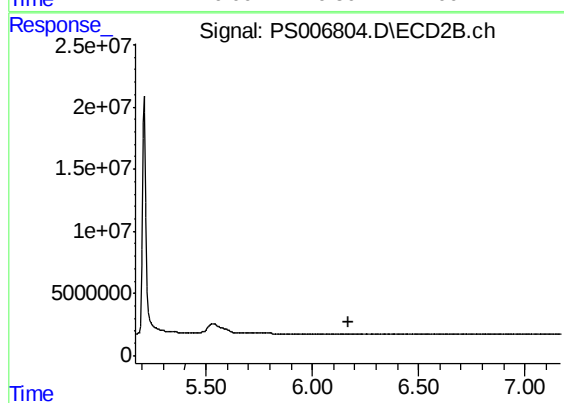

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

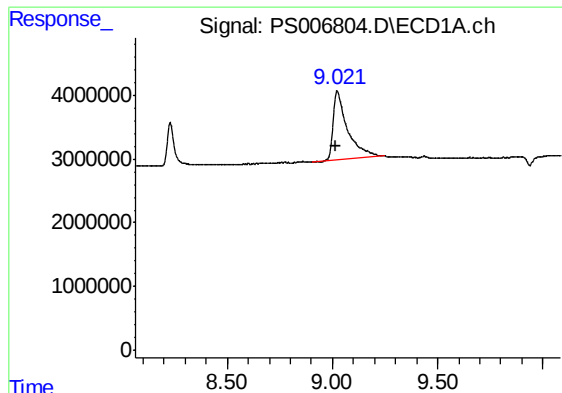

#15 Picloram


R.T.: 9.024 min
Delta R.T.: 0.006 min
Response: 50666207
Conc: 7.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

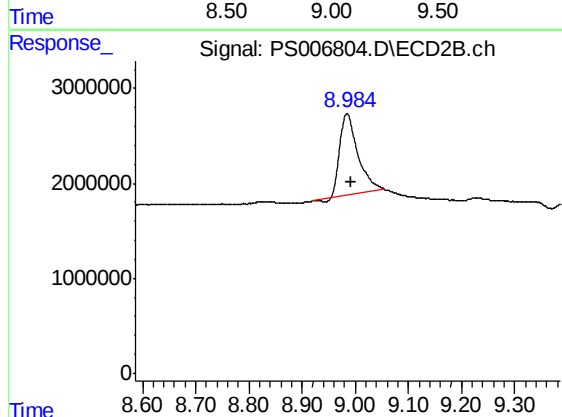


#15 Picloram

R.T.: 8.985 min
Delta R.T.: -0.006 min
Response: 19901448
Conc: 5.38 ng/ml

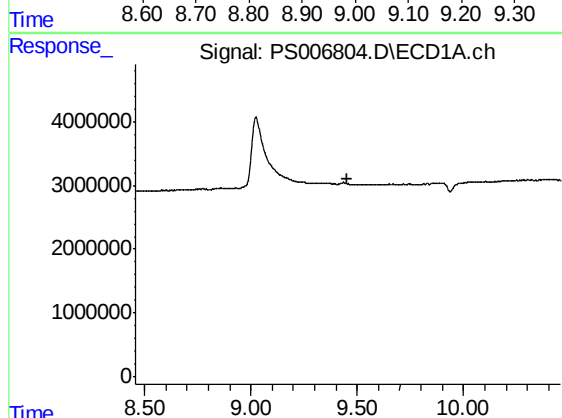

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.456 min
Response: 0
Conc: N.D.

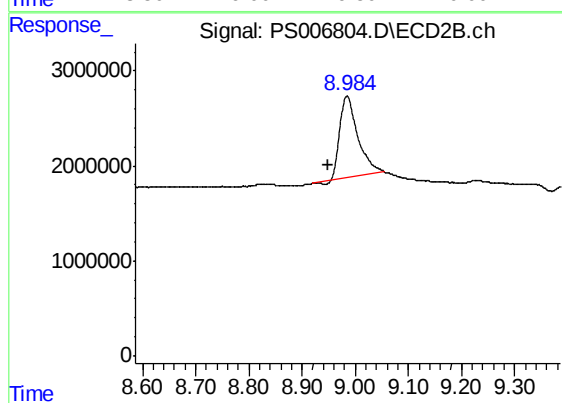

#16 DCPA

R.T.: 8.985 min
Delta R.T.: 0.036 min
Response: 19901448
Conc: 6.32 ng/ml