

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS091819\  
 Data File : PS006808.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Sep 2019 18:02  
 Operator : SM\AJ  
 Sample : PB123207TB  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 PB123207TB

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 19 05:05:43 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS090919.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 10 06:14:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|--------------|-------|-------|----------|----------|---------|---------|
| -----                       |              |       |       |          |          |         |         |
| System Monitoring Compounds |              |       |       |          |          |         |         |
| 4) S                        | 2,4-DCAA     | 5.529 | 5.259 | 344.2E6  | 181.7E6  | 443.065 | 425.506 |
| Target Compounds            |              |       |       |          |          |         |         |
| 7) T                        | MCPA         | 0.000 | 5.585 | 0        | 51280056 | N.D.    | 29.236  |
| 10) T                       | Pentachlo... | 6.786 | 0.000 | 10671872 | 0        | <MDL    | N.D. #  |
| 15) T                       | Picloram     | 9.080 | 0.000 | 27253515 | 0        | 4.040   | N.D. #  |
| -----                       |              |       |       |          |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS091819\  
Data File : PS006808.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Sep 2019 18:02  
Operator : SM\AJ  
Sample : PB123207TB  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
PB123207TB

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 19 05:05:43 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS090919.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 10 06:14:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

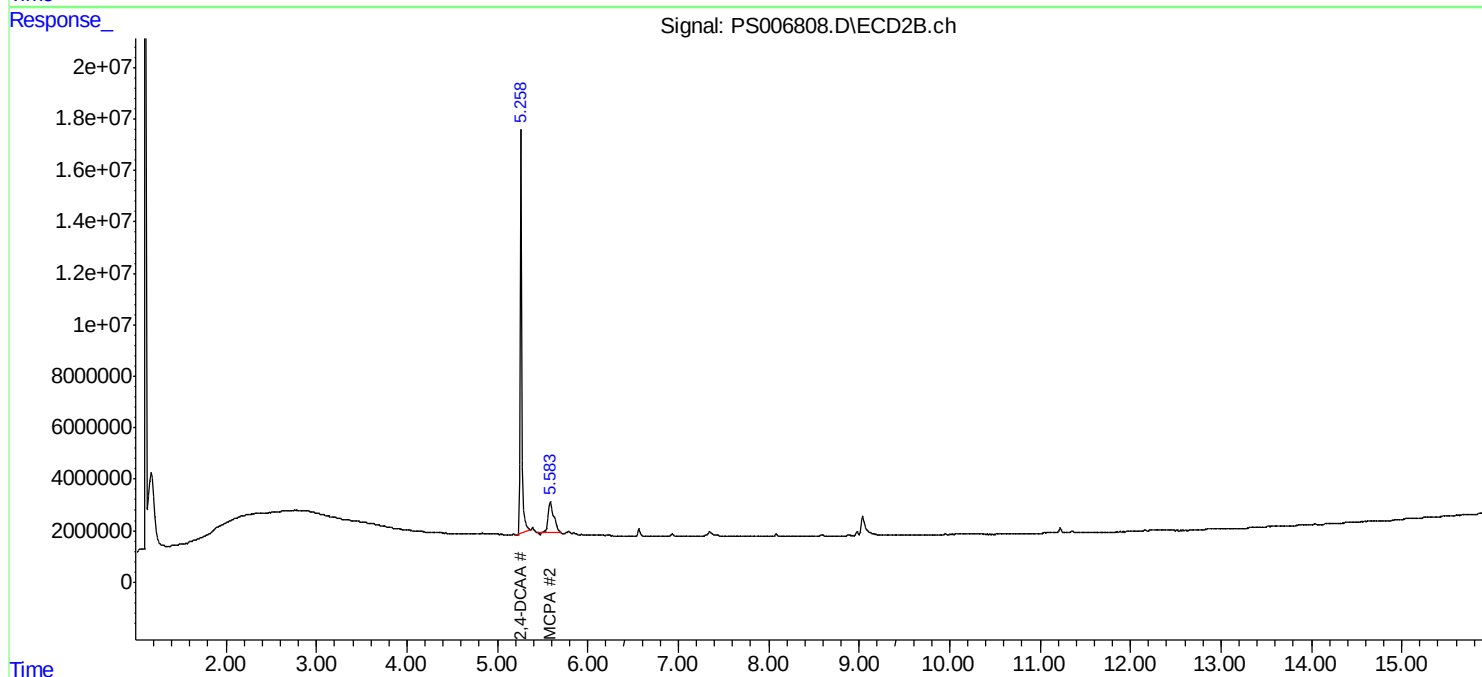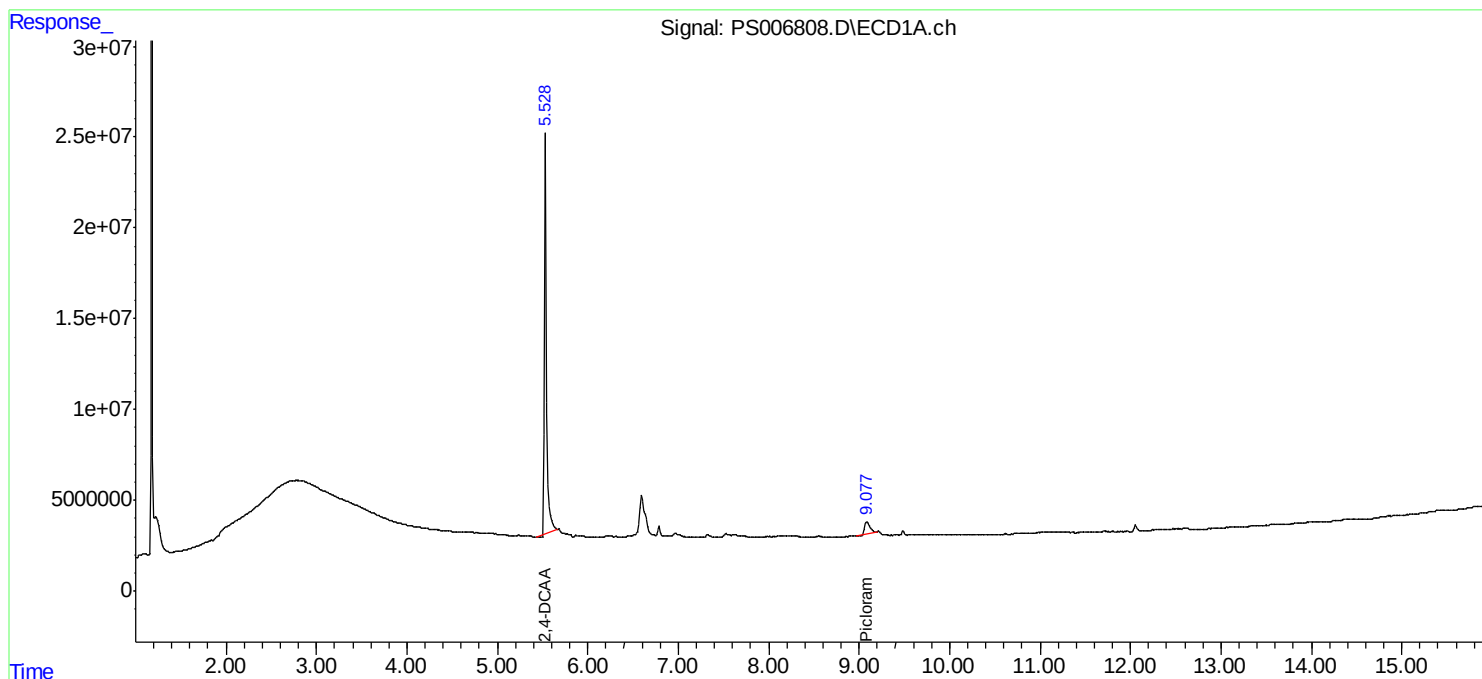


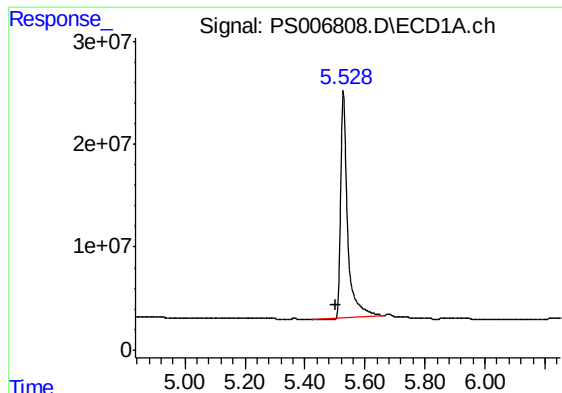

#4 2,4-DCAA


R.T.: 5.529 min  
Delta R.T.: 0.028 min  
Response: 344210564  
Conc: 443.06 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
PB123207TB

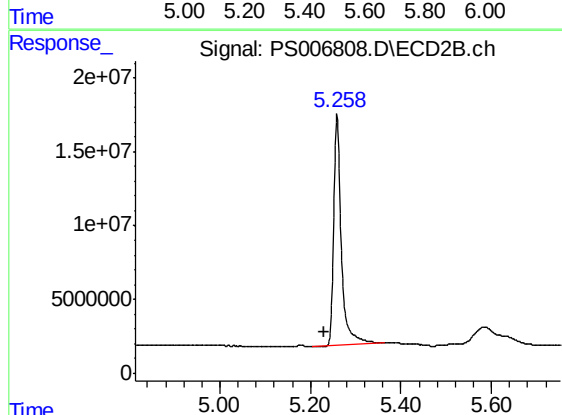


#4 2,4-DCAA

R.T.: 5.259 min  
Delta R.T.: 0.029 min  
Response: 181692188  
Conc: 425.51 ng/ml

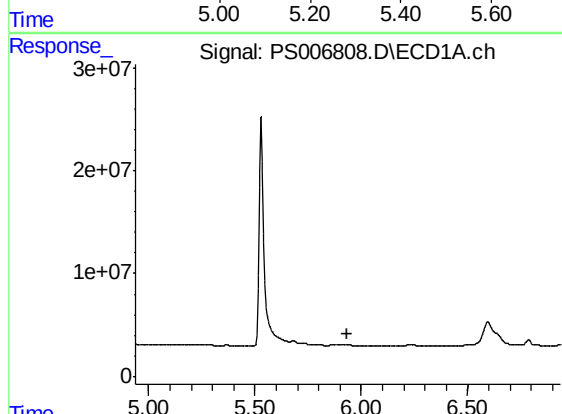


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 5.937 min  
Response: 0  
Conc: N.D.

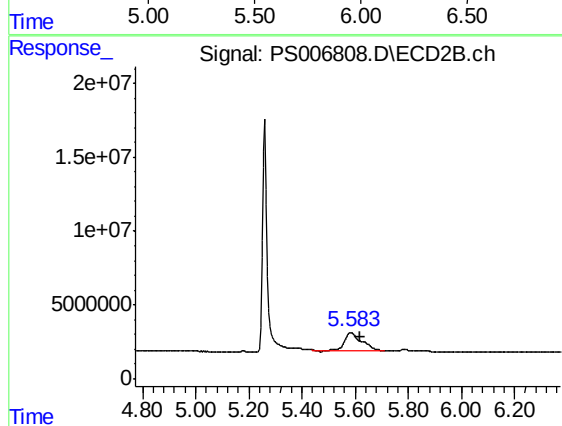

#7 MCPA


R.T.: 5.585 min  
Delta R.T.: -0.035 min  
Response: 51280056  
Conc: 29.24 ug/ml

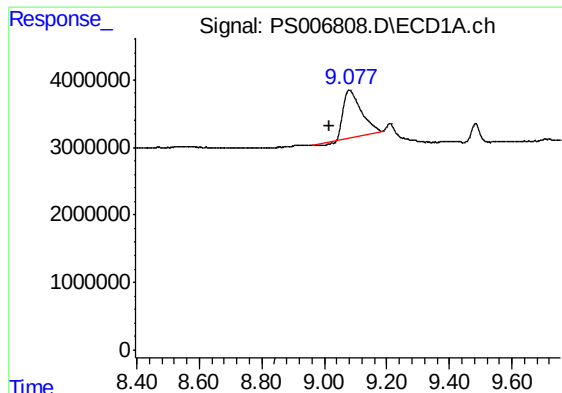

#15 Picloram

R.T.: 9.080 min  
Delta R.T.: 0.063 min  
Response: 27253515  
Conc: 4.04 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
PB123207TB

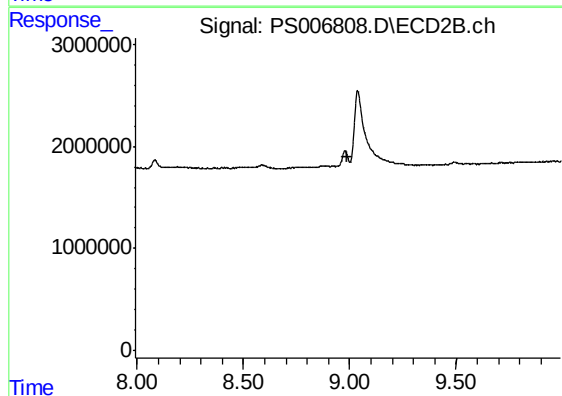

#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 8.991 min  
Response: 0  
Conc: N.D.