

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091819\
 Data File : PS006812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2019 19:30
 Operator : SM\AJ
 Sample : K4668-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-01-091719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:06:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.477	5.208	374.3E6	192.5E6	481.792	450.826
Target Compounds							
1) T	Dalapon	2.110	1.737	58638786	65630036	59.995	128.422 #
2) T	3,5-DICHL...	0.000	4.537	0	26876386	N.D.	49.656
3) T	4-Nitroph...	5.330	0.000	8589265	0	24.204	N.D. #
5) T	DICAMBA	5.690	0.000	8662261	0	3.005	N.D. #
9) T	2,4-D	6.487	0.000	168.9E6	0	218.591	N.D. #
10) T	Pentachlo...	6.732	0.000	44790504	0	4.021	N.D. #
11) T	2,4,5-TP ...	7.335	0.000	23962765	0	5.569	N.D. #
12) T	2,4,5-T	7.544	0.000	28405424	0	6.096	N.D. #
15) T	Picloram	9.004	0.000	14643442	0	2.171	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091819\
Data File : PS006812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2019 19:30
Operator : SM\AJ
Sample : K4668-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-01-091719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:06:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

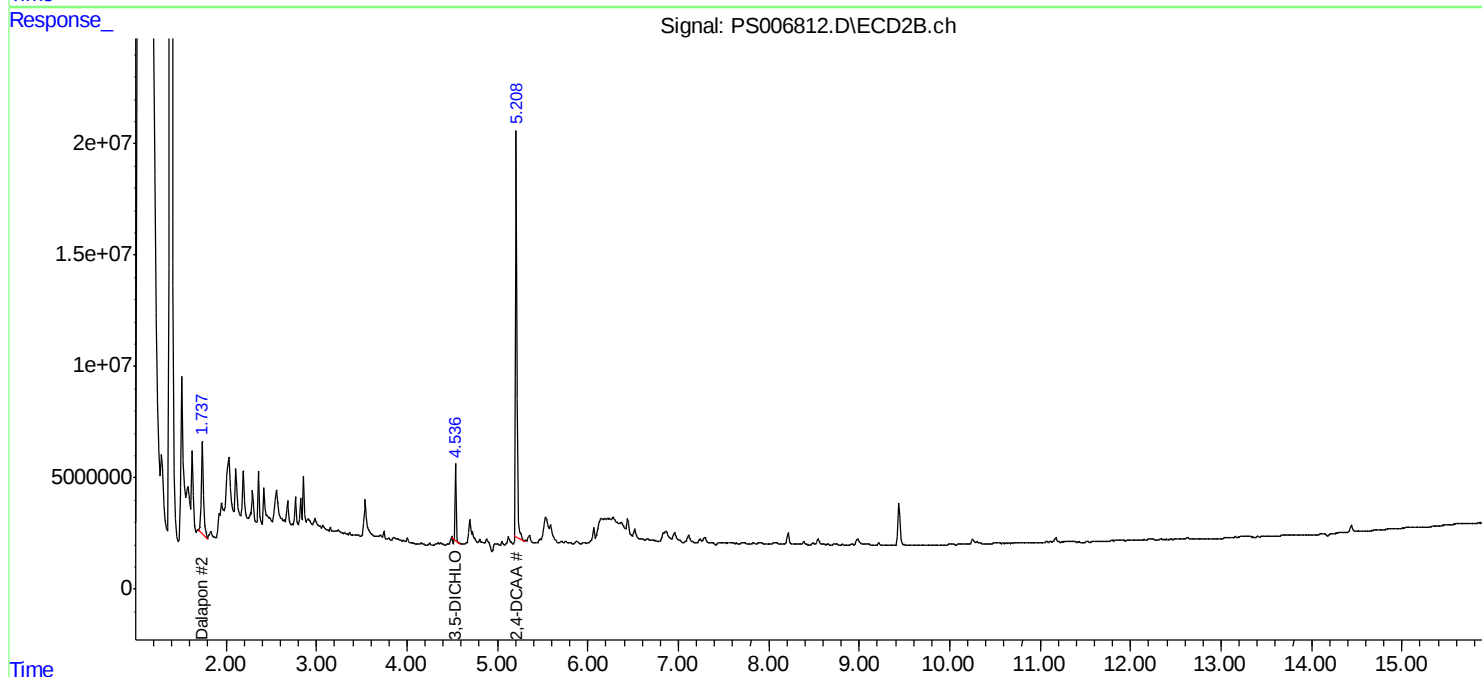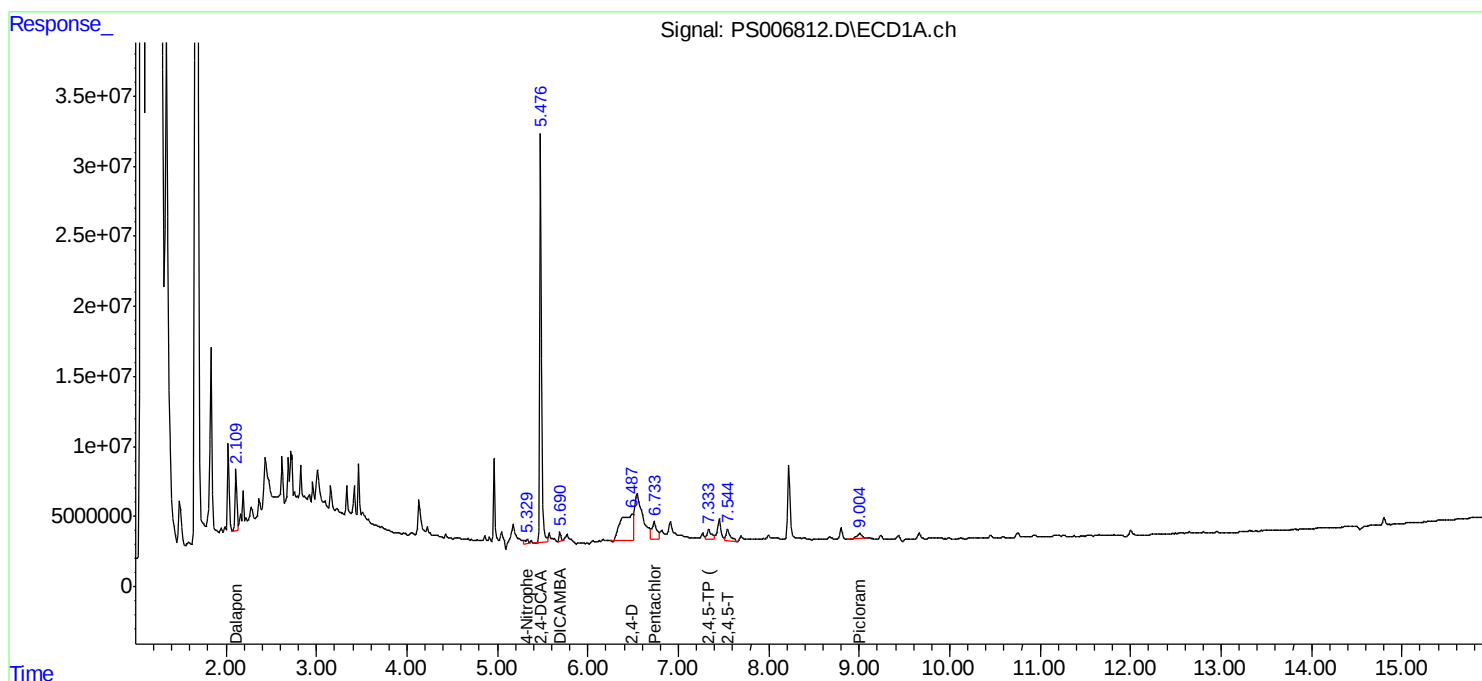


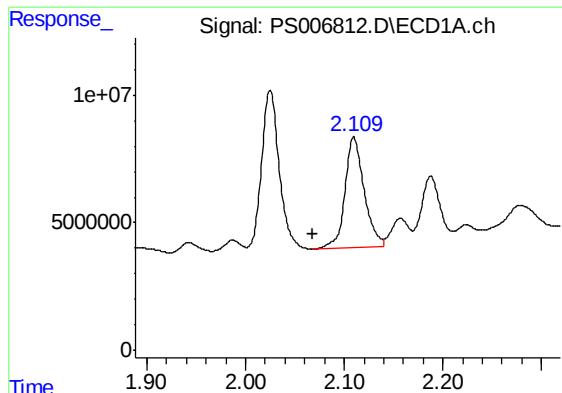

#1 Dalapon


R.T.: 2.110 min
Delta R.T.: 0.042 min
Response: 58638786
Conc: 59.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-091719

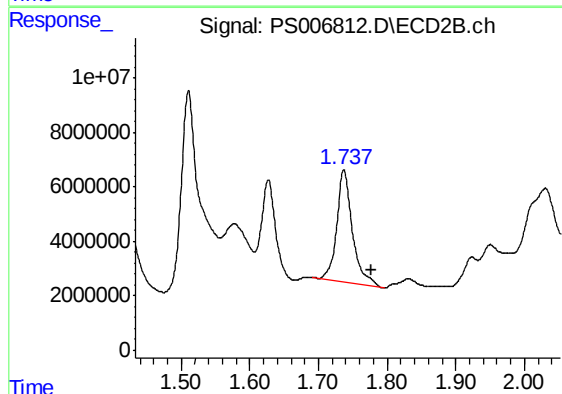


#1 Dalapon

R.T.: 1.737 min
Delta R.T.: -0.040 min
Response: 65630036
Conc: 128.42 ng/ml

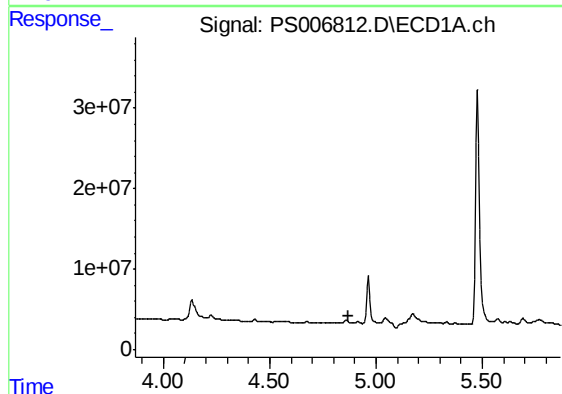


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

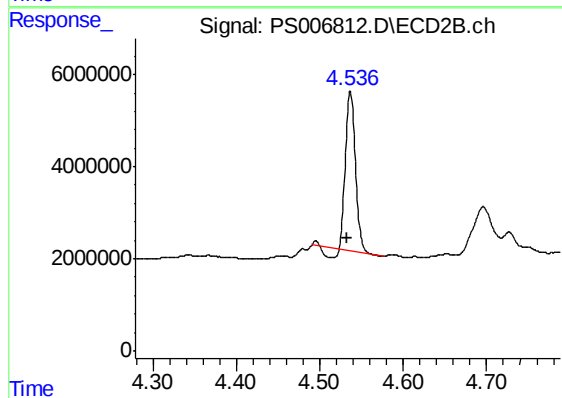

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.537 min
Delta R.T.: 0.003 min
Response: 26876386
Conc: 49.66 ng/ml

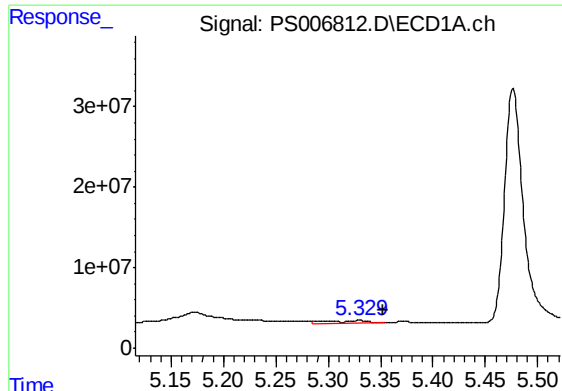

#3 4-Nitrophenol


R.T.: 5.330 min
Delta R.T.: -0.023 min
Response: 8589265
Conc: 24.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-091719

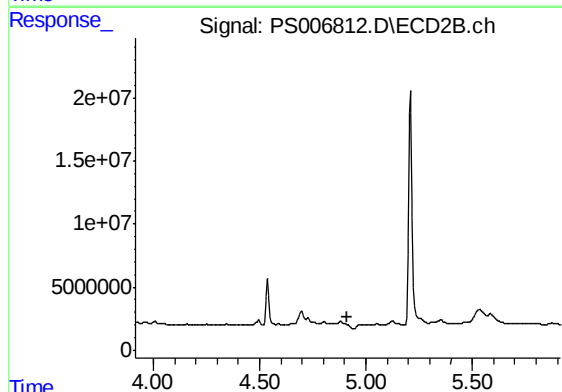


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

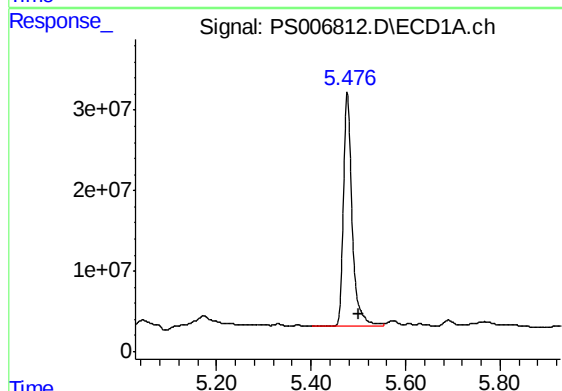


#4 2,4-DCAA

R.T.: 5.477 min
Delta R.T.: -0.024 min
Response: 374297494
Conc: 481.79 ng/ml

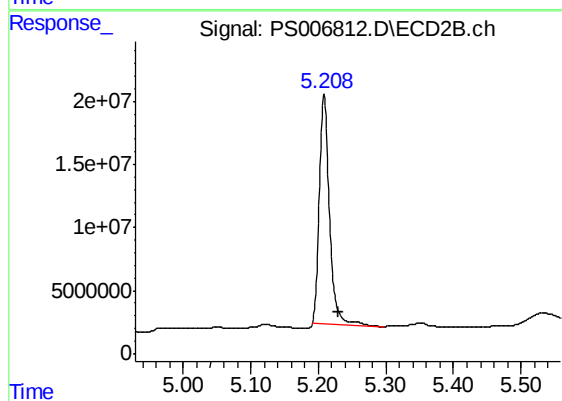

#4 2,4-DCAA


R.T.: 5.208 min
Delta R.T.: -0.022 min
Response: 192503735
Conc: 450.83 ng/ml

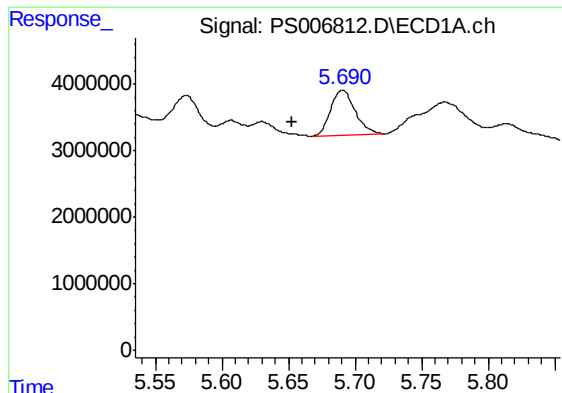

#5 DICAMBA


R.T.: 5.690 min
Delta R.T.: 0.037 min
Response: 8662261
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-091719

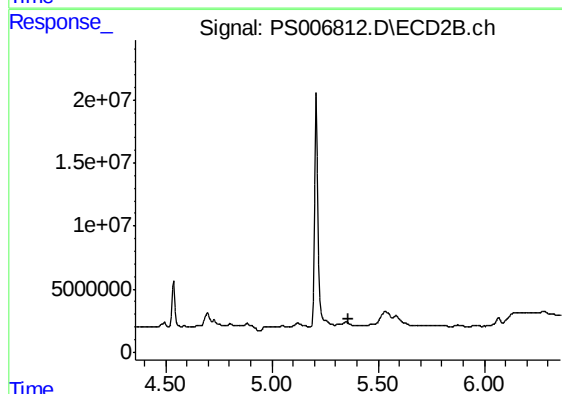


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

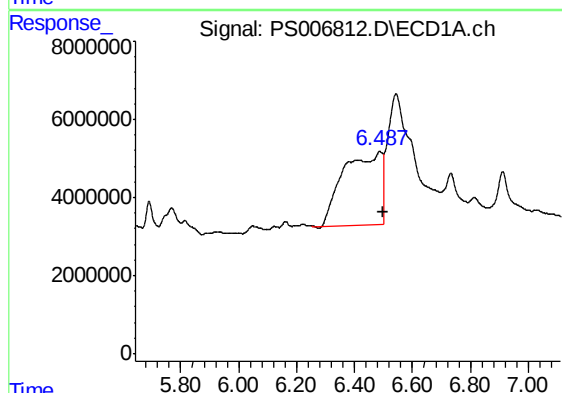


#9 2,4-D

R.T.: 6.487 min
Delta R.T.: -0.010 min
Response: 168888302
Conc: 218.59 ng/ml

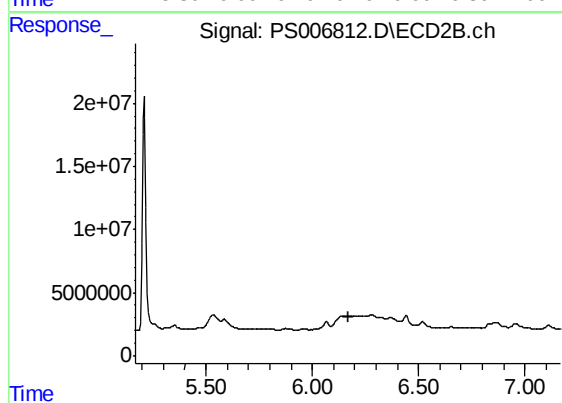

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

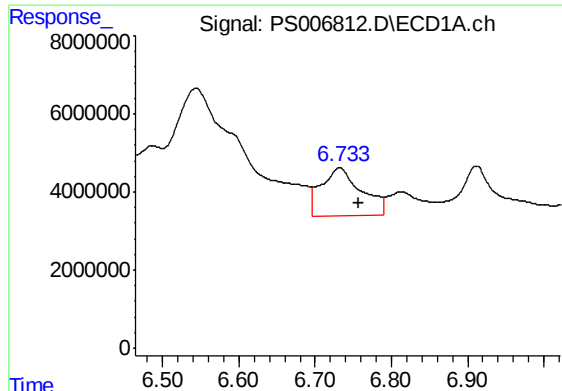

#10 Pentachlorophenol


R.T.: 6.732 min
Delta R.T.: -0.025 min
Response: 44790504
Conc: 4.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-091719

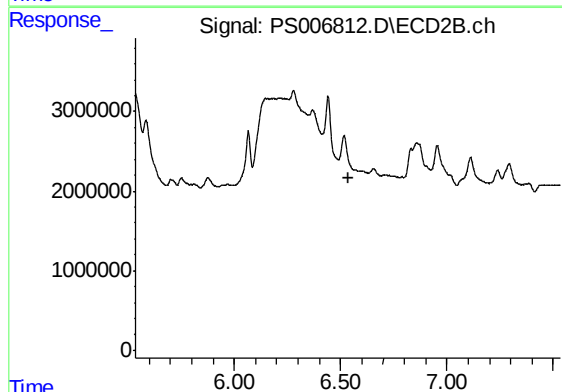


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.535 min
Response: 0
Conc: N.D.

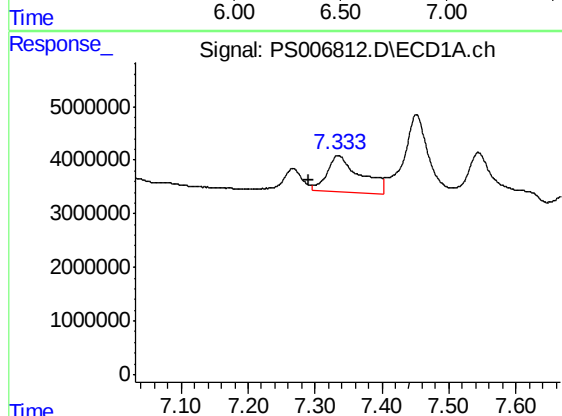


#11 2,4,5-TP (SILVEX)

R.T.: 7.335 min
Delta R.T.: 0.043 min
Response: 23962765
Conc: 5.57 ng/ml

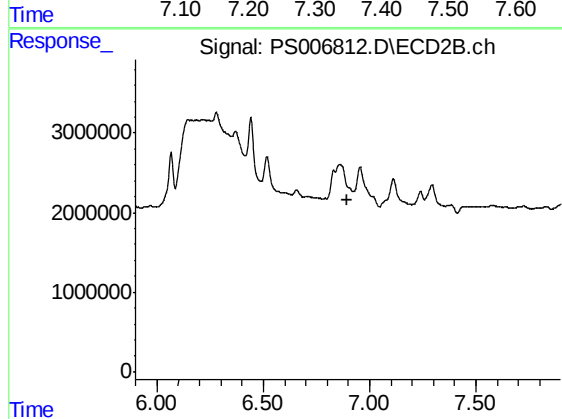

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 6.898 min
Response: 0
Conc: N.D.

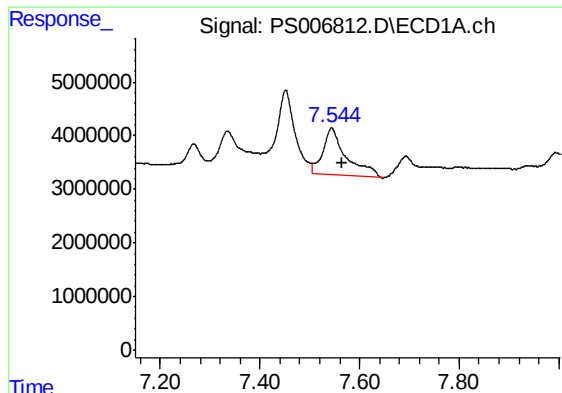

#12 2,4,5-T


R.T.: 7.544 min
Delta R.T.: -0.021 min
Response: 28405424
Conc: 6.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-091719

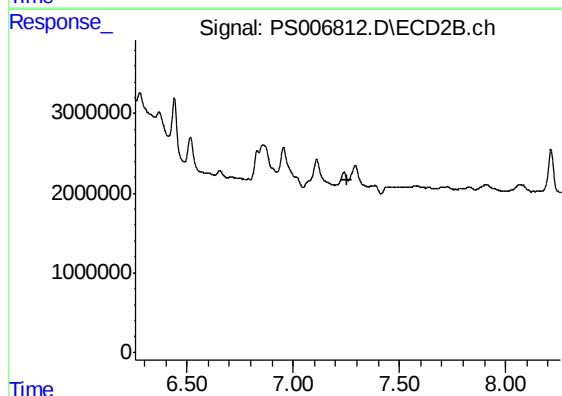


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.258 min
Response: 0
Conc: N.D.

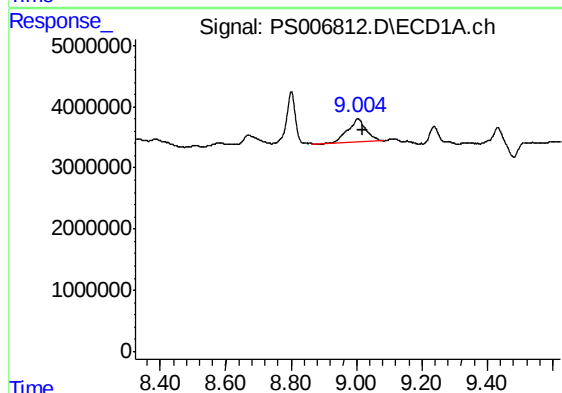

#15 Picloram

R.T.: 9.004 min
Delta R.T.: -0.013 min
Response: 14643442
Conc: 2.17 ng/ml

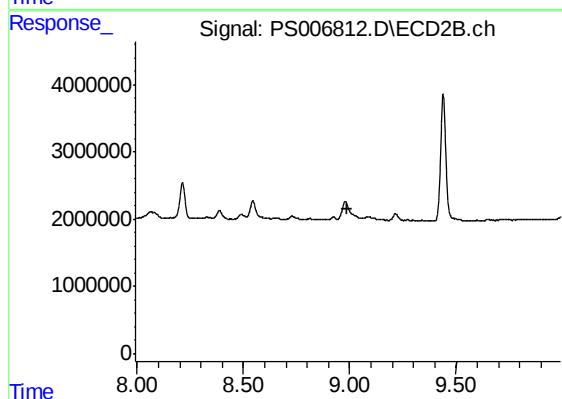

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.