

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091819\
 Data File : PS006814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2019 20:14
 Operator : SM\AJ
 Sample : K4931-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 290-371

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:07:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.497	5.228	390.7E6	216.4E6	502.899	506.875
Target Compounds							
1) T	Dalapon	2.045	1.757	67574217	58740660	69.137	114.941 #
2) T	3,5-DICHL...	0.000	4.557	0	30504926	N.D.	56.360
5) T	DICAMBA	5.710	0.000	772695	0	<MDL	N.D. #
7) T	MCPA	0.000	5.556	0	14846619	N.D.	8.464
9) T	2,4-D	6.566	0.000	53363578	0	69.068	N.D. #
15) T	Picloram	9.018	0.000	19021076	0	2.820	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091819\
Data File : PS006814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2019 20:14
Operator : SM\AJ
Sample : K4931-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
290-371

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:07:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

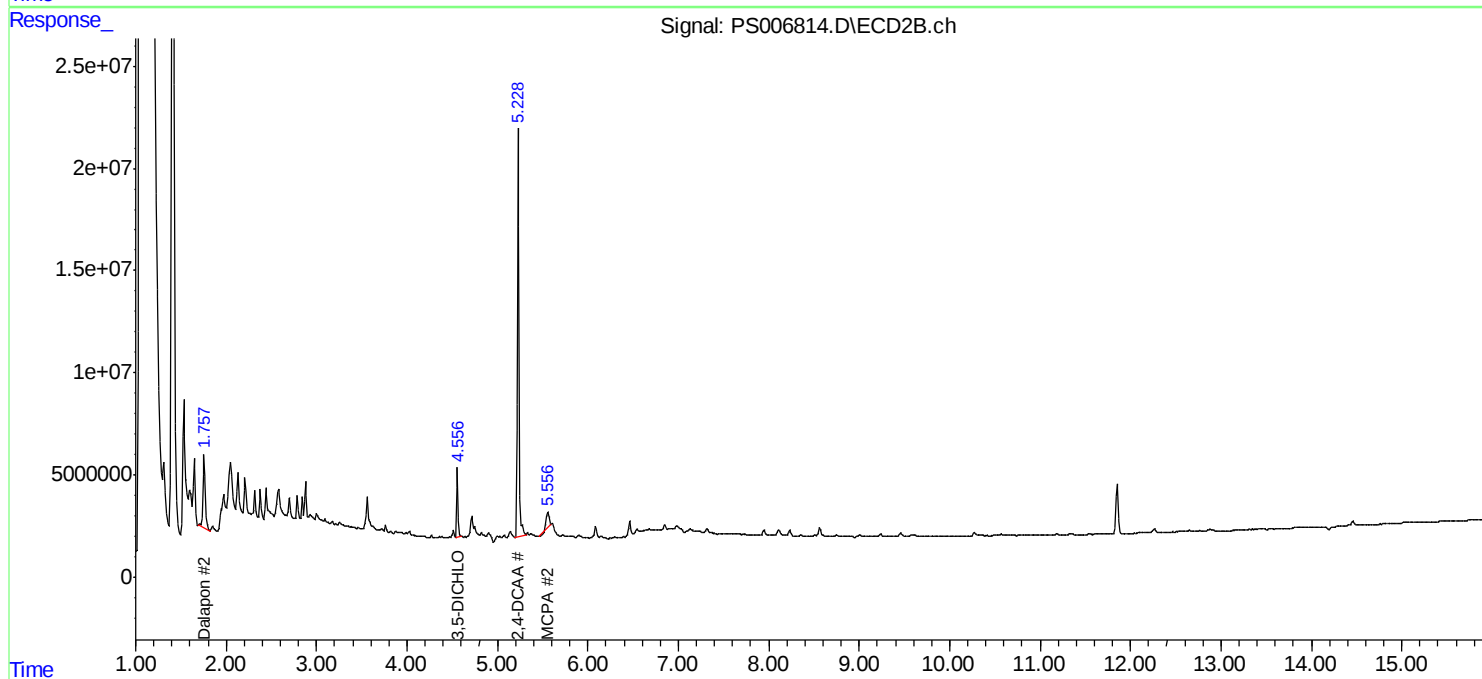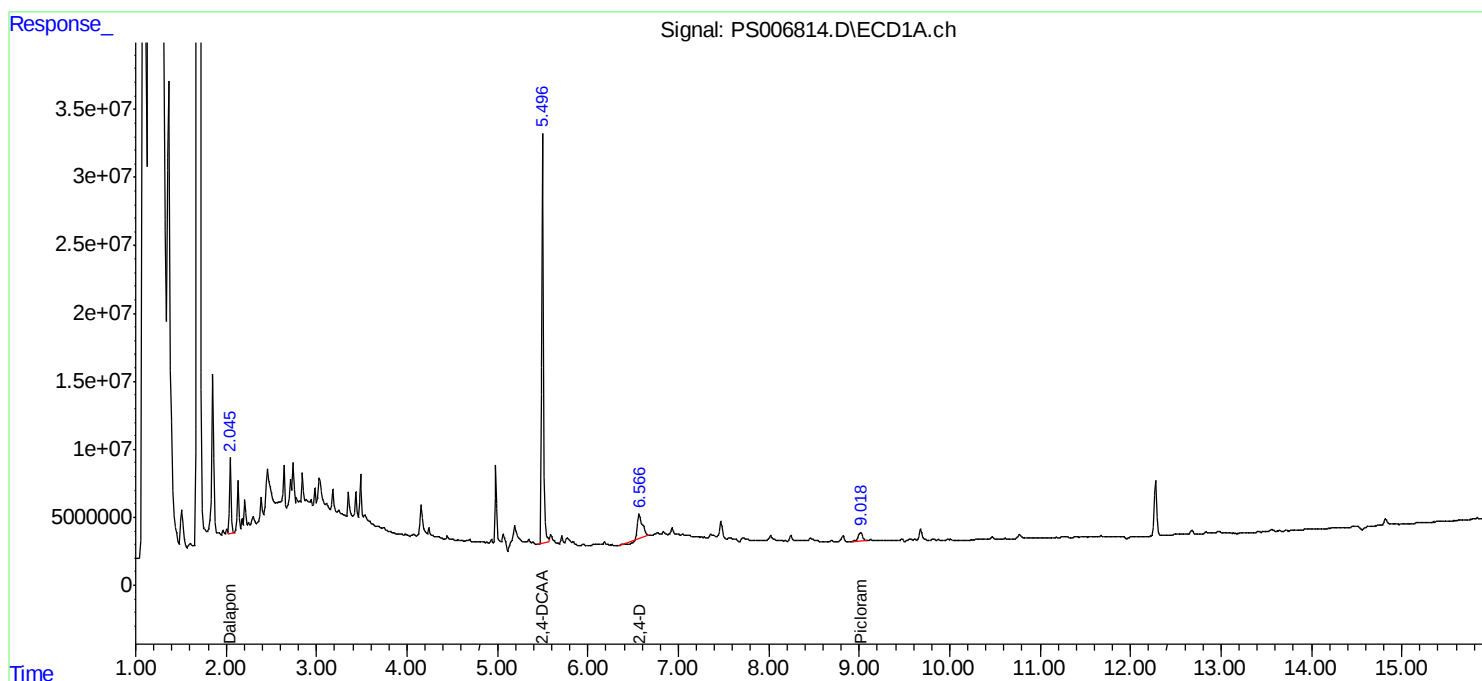


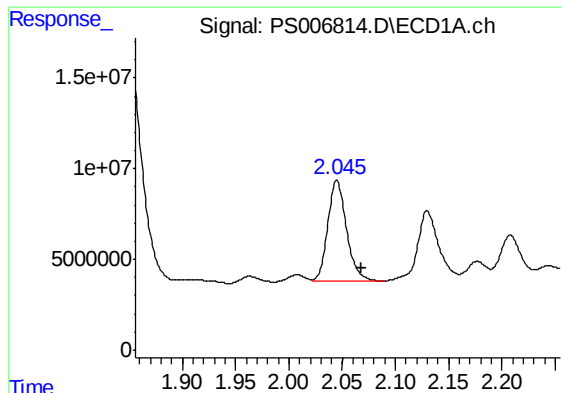

#1 Dalapon


R.T.: 2.045 min
Delta R.T.: -0.023 min
Response: 67574217
Conc: 69.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
290-371

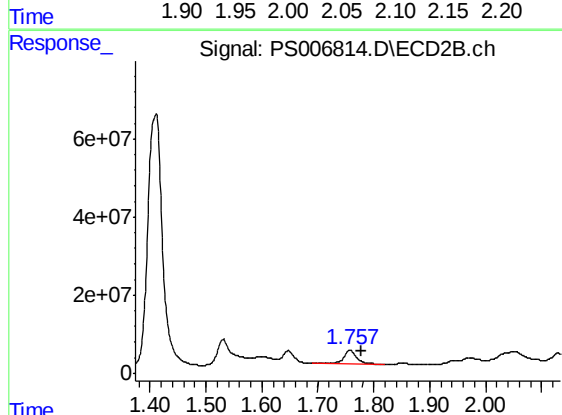


#1 Dalapon

R.T.: 1.757 min
Delta R.T.: -0.020 min
Response: 58740660
Conc: 114.94 ng/ml

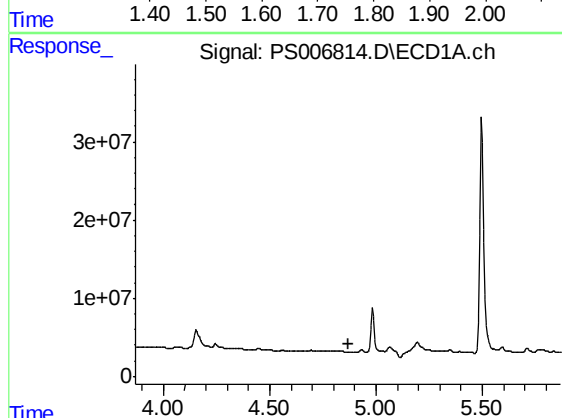


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

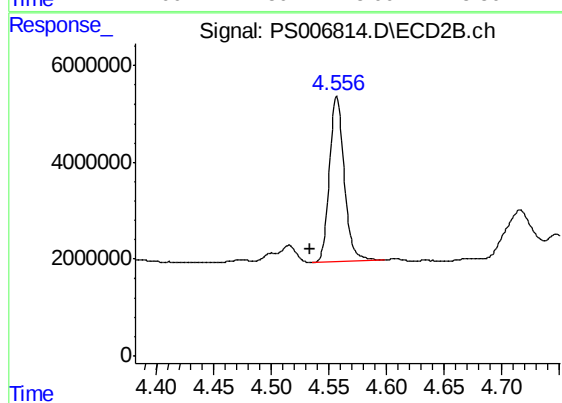

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.557 min
Delta R.T.: 0.023 min
Response: 30504926
Conc: 56.36 ng/ml

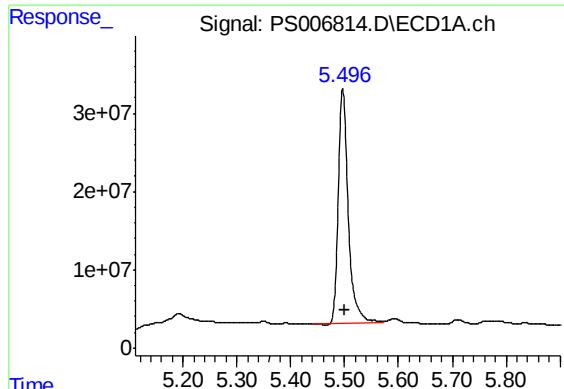

#4 2,4-DCAA


R.T.: 5.497 min
Delta R.T.: -0.004 min
Response: 390694812
Conc: 502.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
290-371

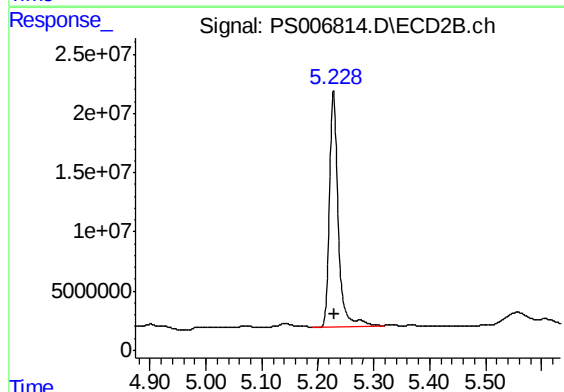


#4 2,4-DCAA

R.T.: 5.228 min
Delta R.T.: -0.002 min
Response: 216436977
Conc: 506.88 ng/ml

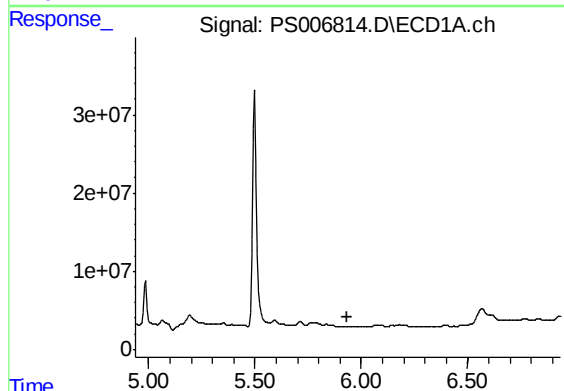


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.937 min
Response: 0
Conc: N.D.

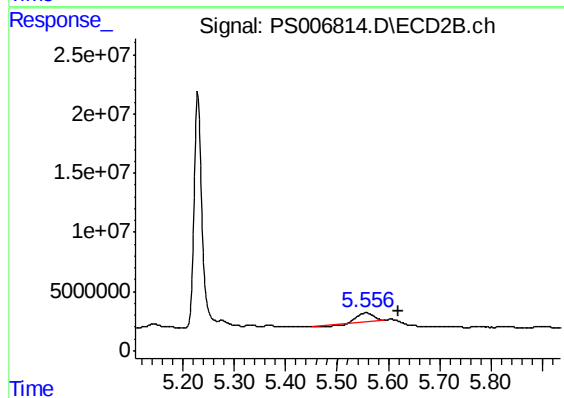

#7 MCPA


R.T.: 5.556 min
Delta R.T.: -0.063 min
Response: 14846619
Conc: 8.46 ug/ml

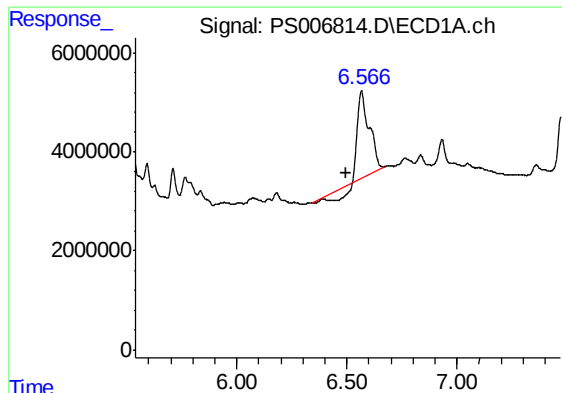

#9 2,4-D


R.T.: 6.566 min
Delta R.T.: 0.069 min
Response: 53363578
Conc: 69.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
290-371

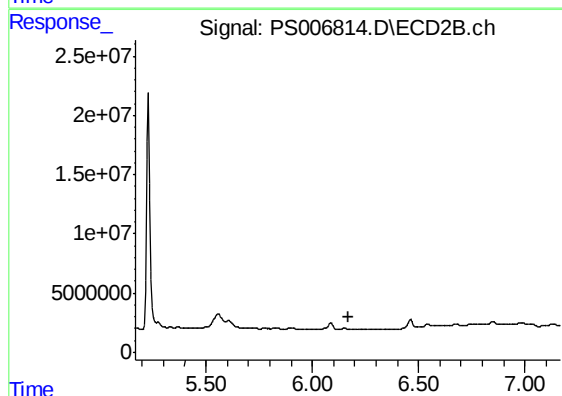


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

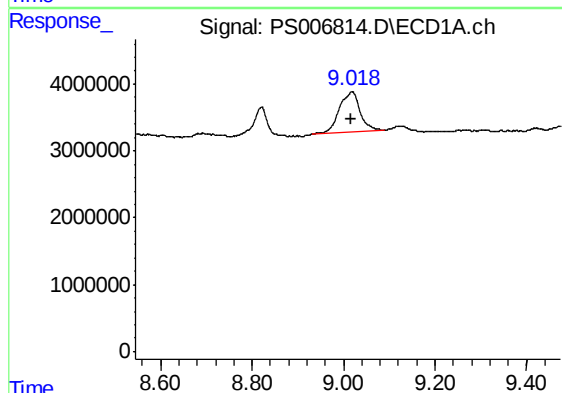

#15 Picloram

R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 19021076
Conc: 2.82 ng/ml

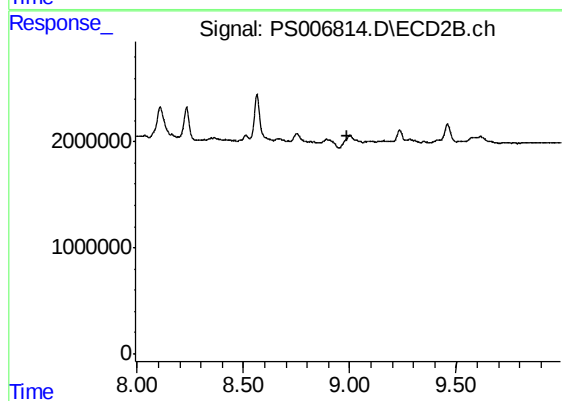

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.