

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091820\
 Data File : PS012374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2020 15:25
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:48:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	0.000	29970080	0	27.650	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.472	0.000	1585.0E6	0	1081.008	N.D. #
7) T	MCPA	7.674	0.000	16796447	0	3.595	N.D. #
8) T	DICHLORPROP	0.000	7.738	0	9299673	N.D.	16.436
9) T	2,4-D	8.352	7.946	22632545	9381384	19.871	12.897 #
10) T	Pentachlo...	8.644	8.428	9640558	4550774	<MDL	<MDL #
11) T	2,4,5-TP ...	9.194	8.792	7138375	5479980	1.213	1.893 #
12) T	2,4,5-T	9.488	9.178	14526956	6265258	2.369	2.175
14) T	DINOSEB	0.000	10.007	0	3170400	N.D.	1.527
15) T	Picloram	11.019	10.999	438.6E6	355.3E6	59.572	83.818 #
16) T	DCPA	11.454	10.935	14287692	20358458	1.931	5.601 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091820\
Data File : PS012374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2020 15:25
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:48:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

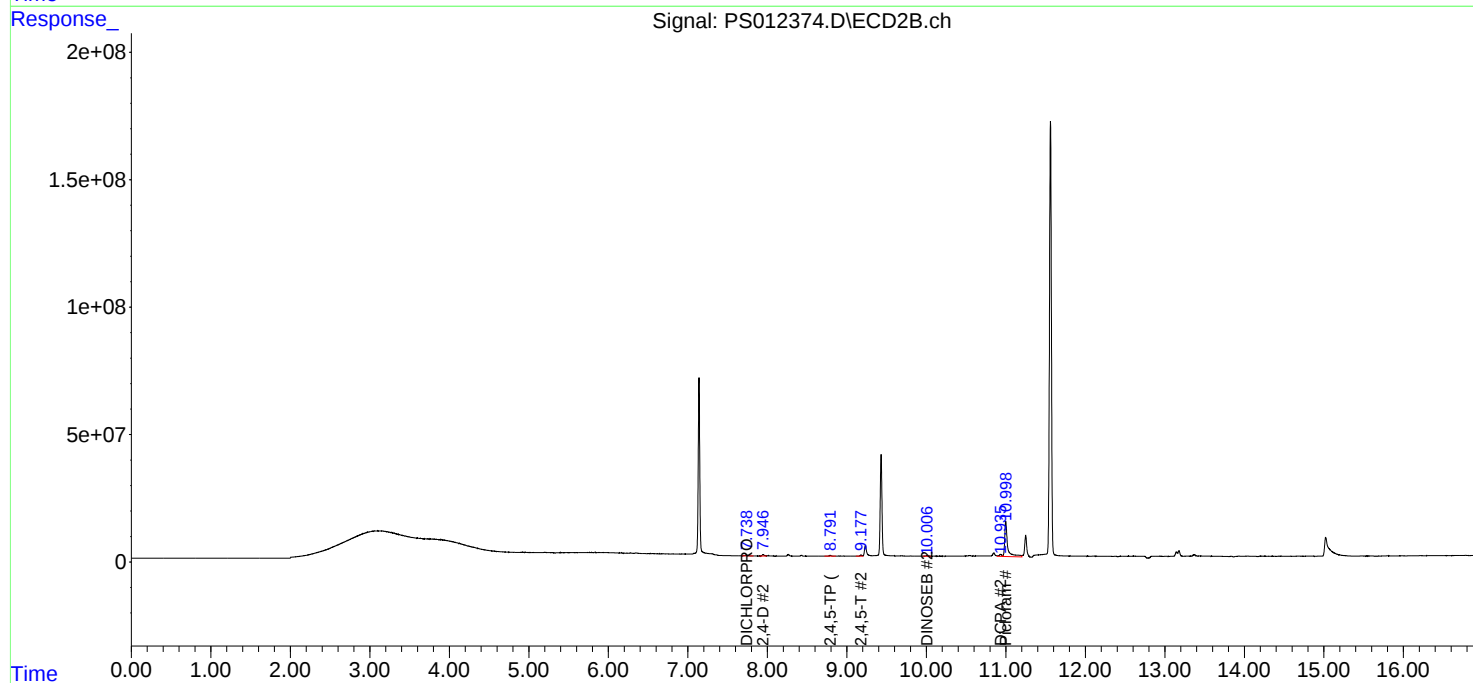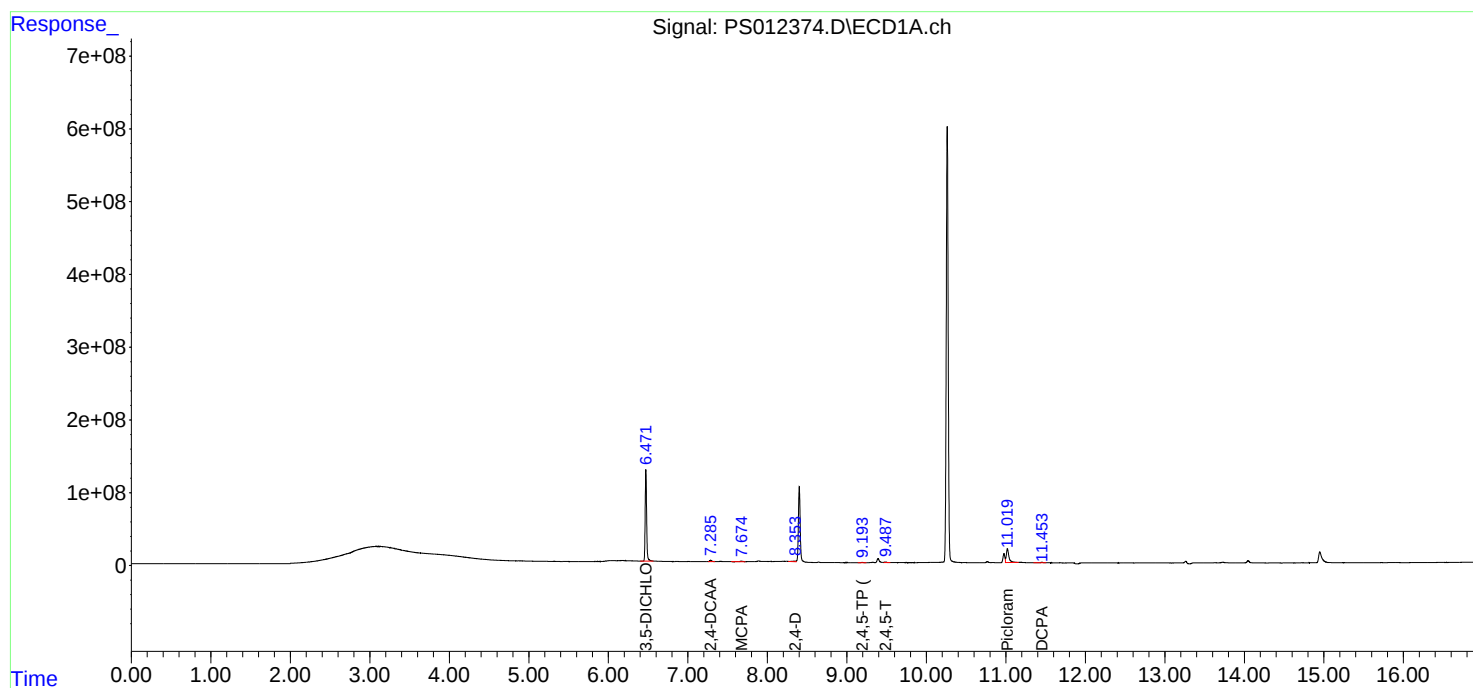


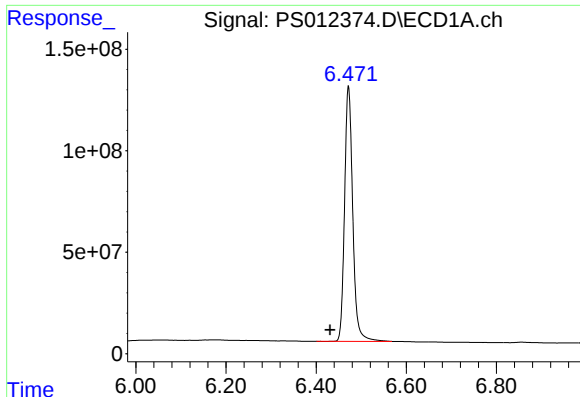

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.472 min
Delta R.T.: 0.040 min
Response: 1584979450
Conc: 1081.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

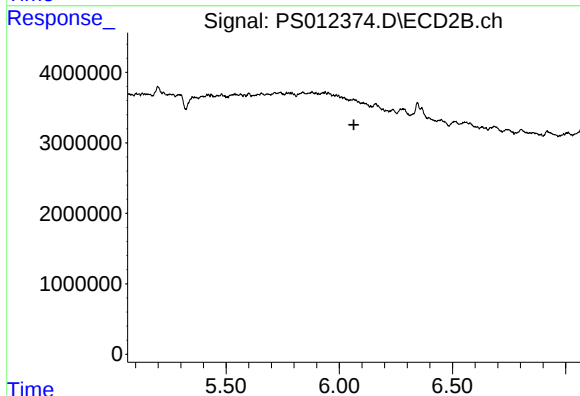


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.065 min
Response: 0
Conc: N.D.

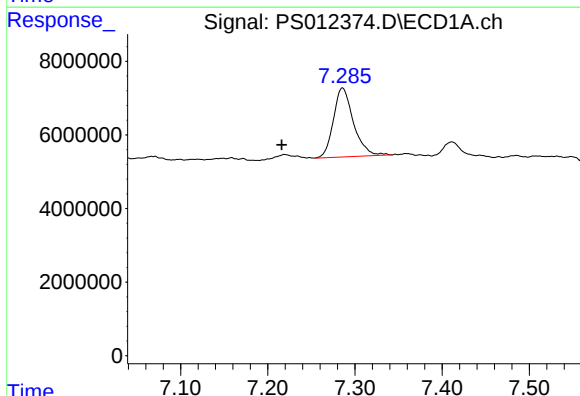


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.070 min
Response: 29970080
Conc: 27.65 ng/ml

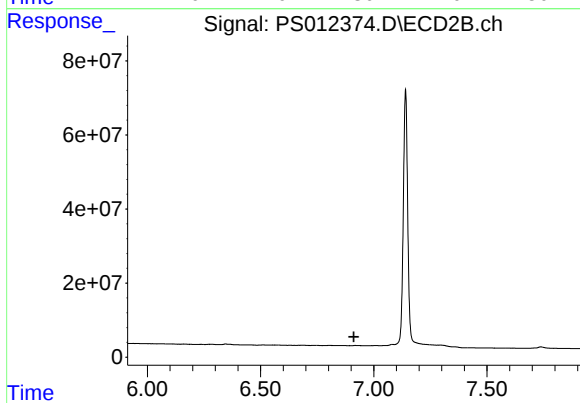

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

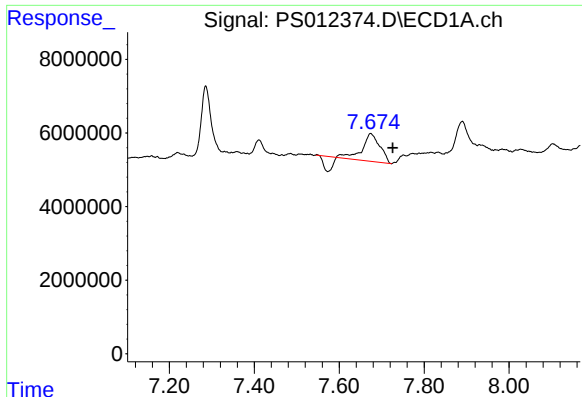

#7 MCPA


R.T.: 7.674 min
Delta R.T.: -0.052 min
Response: 16796447
Conc: 3.59 ug/ml

Instrument :
ECD_S
ClientSampleId :

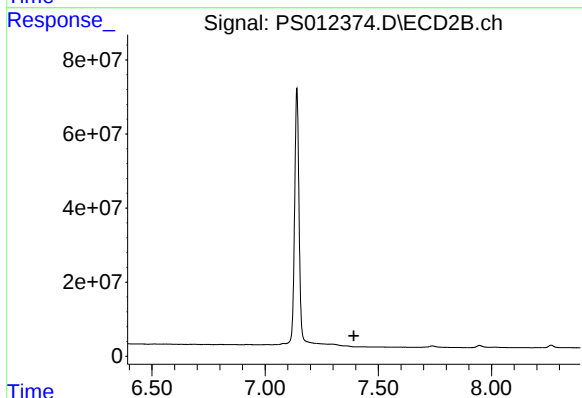


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

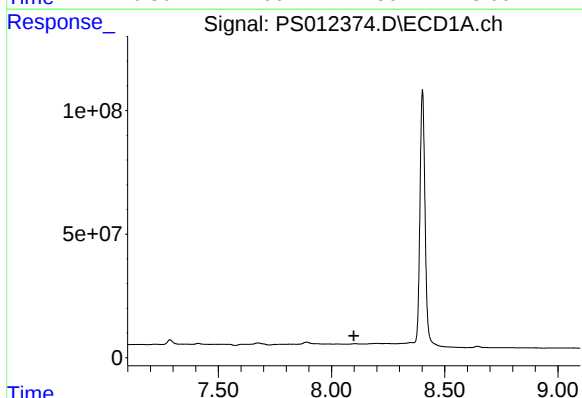


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.099 min
Response: 0
Conc: N.D.

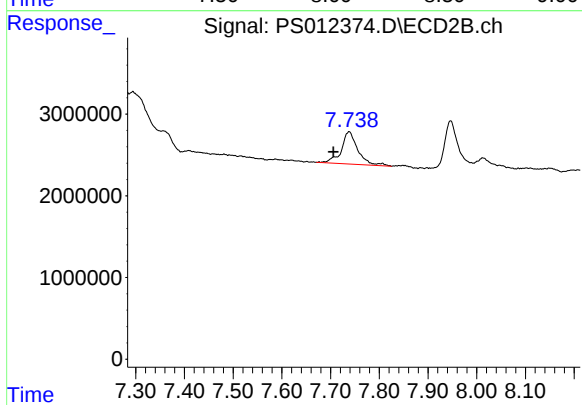

#8 DICHLORPROP


R.T.: 7.738 min
Delta R.T.: 0.032 min
Response: 9299673
Conc: 16.44 ng/ml

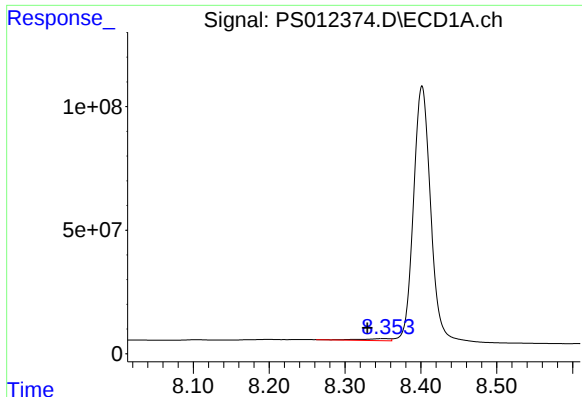

#9 2,4-D


R.T.: 8.352 min
Delta R.T.: 0.022 min
Response: 22632545
Conc: 19.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

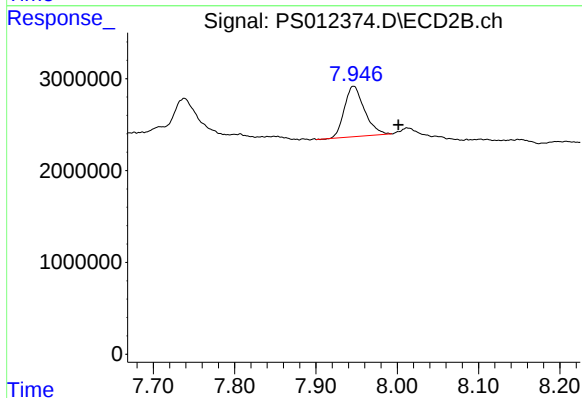


#9 2,4-D

R.T.: 7.946 min
Delta R.T.: -0.055 min
Response: 9381384
Conc: 12.90 ng/ml

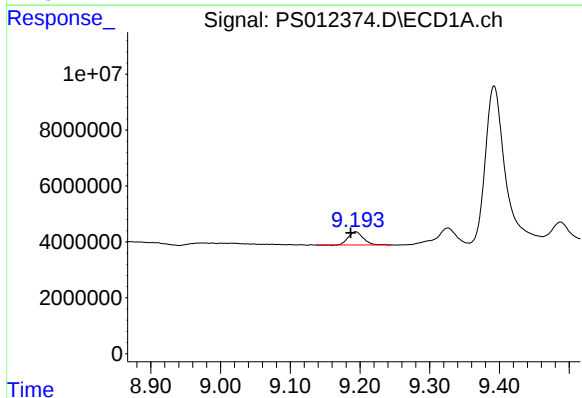


#11 2,4,5-TP (SILVEX)

R.T.: 9.194 min
Delta R.T.: 0.007 min
Response: 7138375
Conc: 1.21 ng/ml

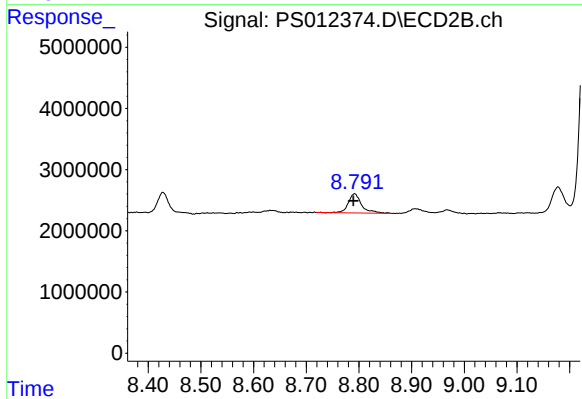

#11 2,4,5-TP (SILVEX)


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 5479980
Conc: 1.89 ng/ml

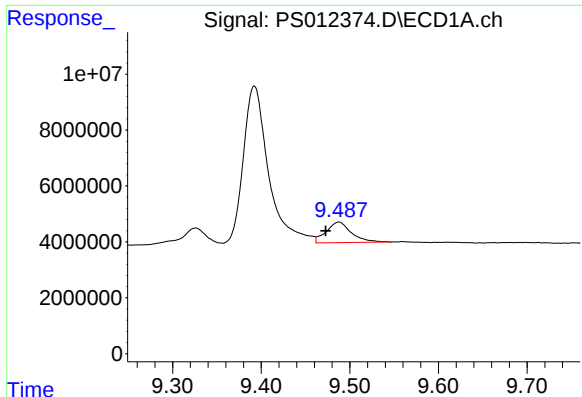

#12 2,4,5-T


R.T.: 9.488 min
Delta R.T.: 0.015 min
Response: 14526956
Conc: 2.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

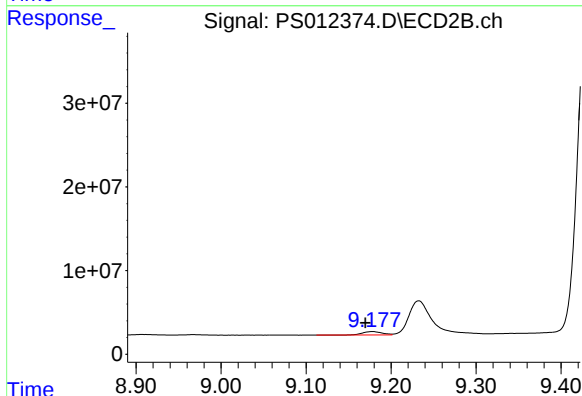


#12 2,4,5-T

R.T.: 9.178 min
Delta R.T.: 0.008 min
Response: 6265258
Conc: 2.18 ng/ml

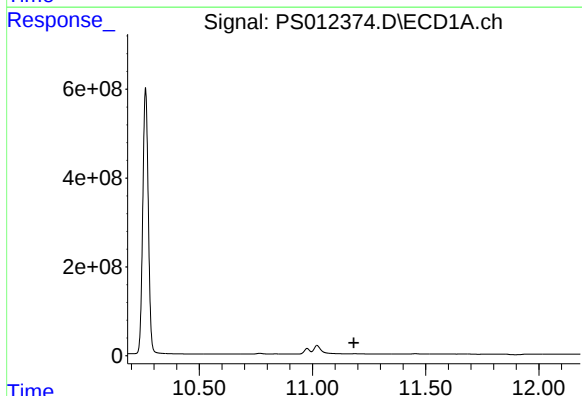


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.183 min
Response: 0
Conc: N.D.

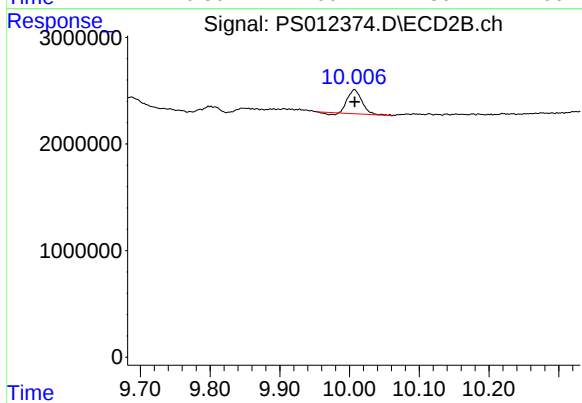

#14 DINOSEB


R.T.: 10.007 min
Delta R.T.: 0.000 min
Response: 3170400
Conc: 1.53 ng/ml

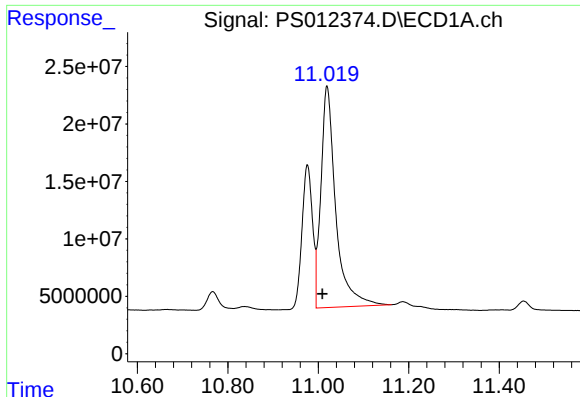

#15 Picloram


R.T.: 11.019 min
Delta R.T.: 0.010 min
Response: 438627728
Conc: 59.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

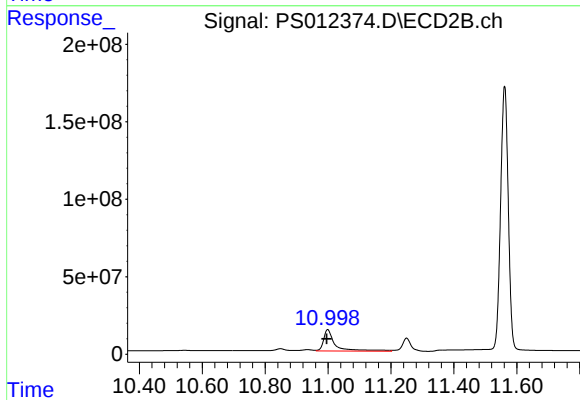


#15 Picloram

R.T.: 10.999 min
Delta R.T.: 0.003 min
Response: 355337624
Conc: 83.82 ng/ml

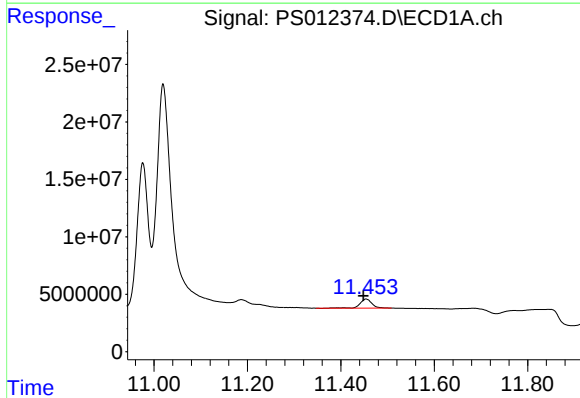

#16 DCPA

R.T.: 11.454 min
Delta R.T.: 0.006 min
Response: 14287692
Conc: 1.93 ng/ml

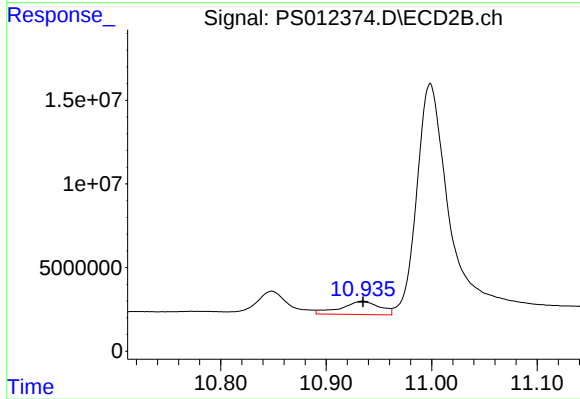

#16 DCPA

R.T.: 10.935 min
Delta R.T.: 0.000 min
Response: 20358458
Conc: 5.60 ng/ml