

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091820\
 Data File : PS012375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2020 15:47
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:48:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	462.7E6	259.5E6	426.885	491.785
Target Compounds							
9) T	2,4-D	8.395	0.000	73465856	0	64.503	N.D. #
12) T	2,4,5-T	9.423	0.000	47701532	0	7.778	N.D. #
15) T	Picloram	11.050	11.027	225.7E6	186.4E6	30.655	43.968 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091820\
Data File : PS012375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2020 15:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:48:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

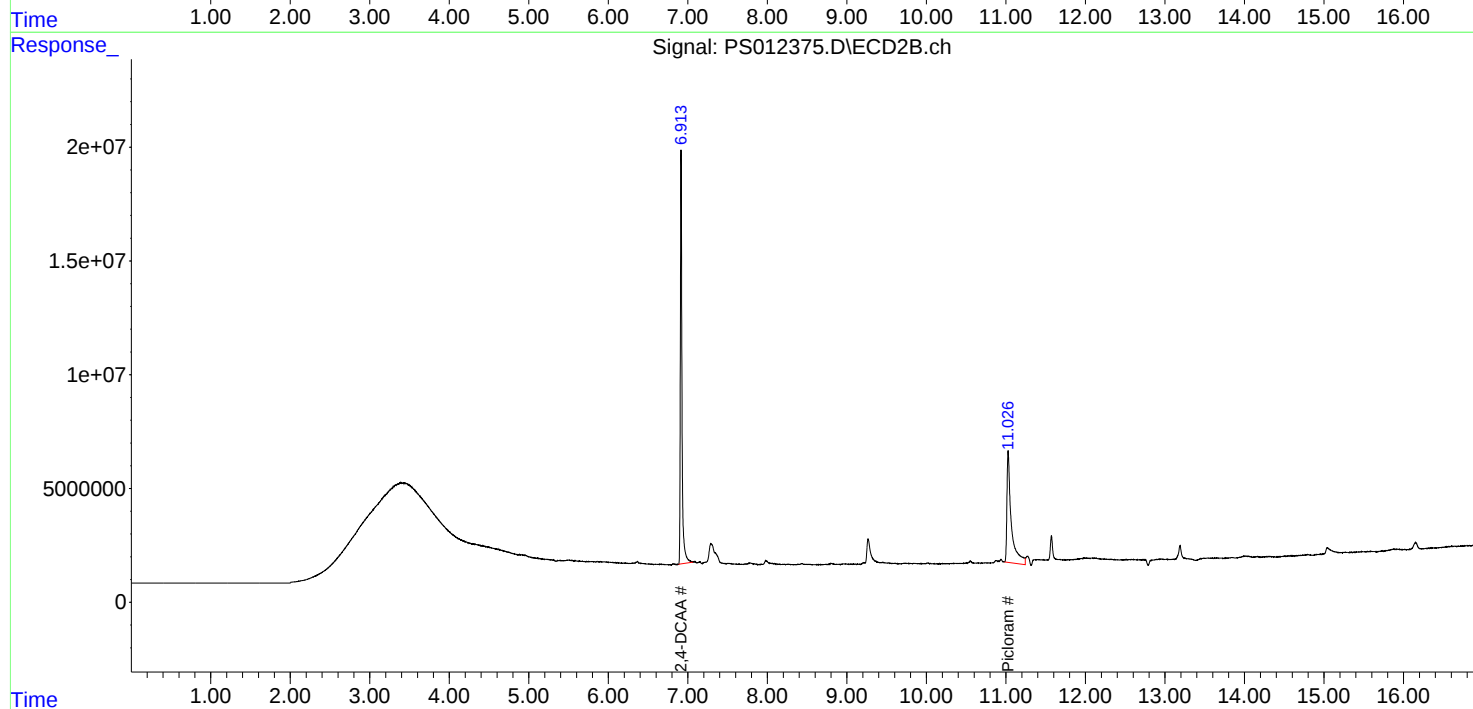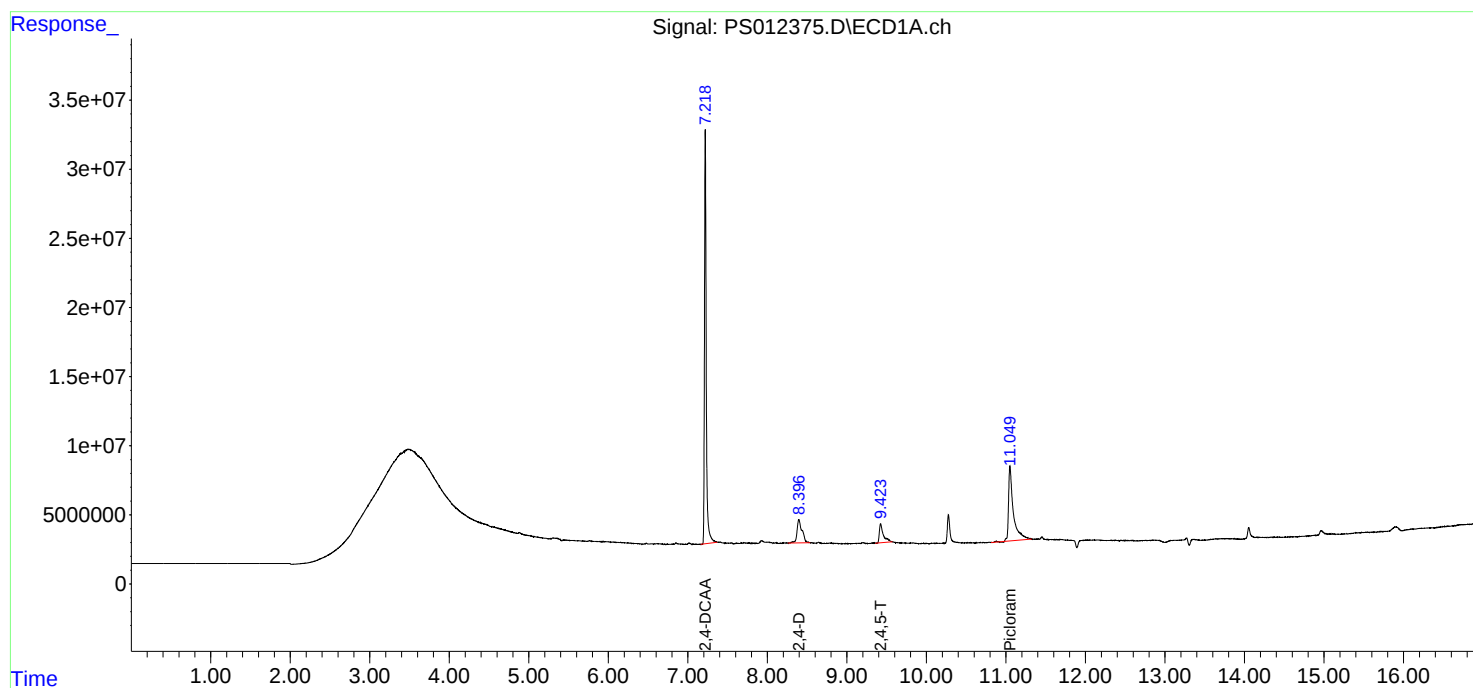


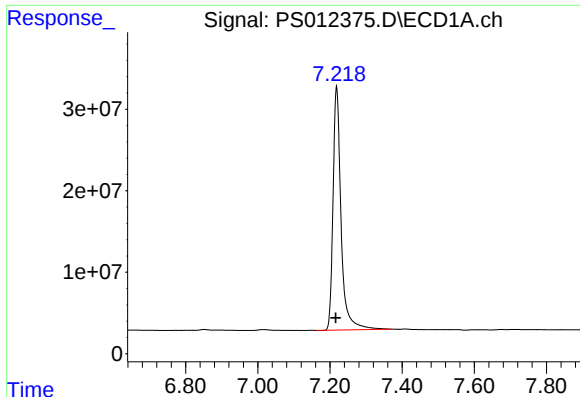

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: 0.002 min
Response: 462698665
Conc: 426.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

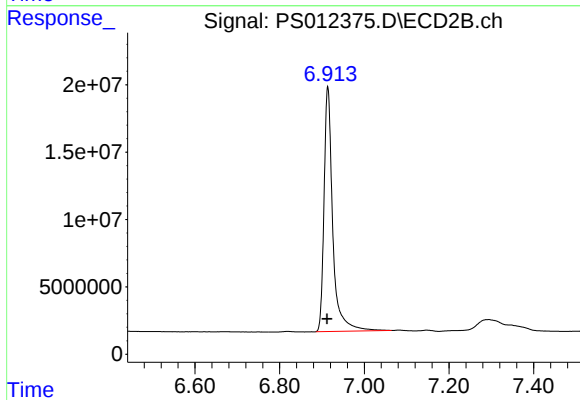


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.001 min
Response: 259468452
Conc: 491.79 ng/ml

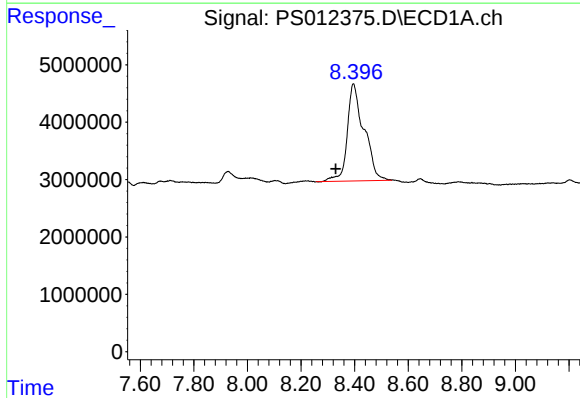


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.066 min
Response: 73465856
Conc: 64.50 ng/ml

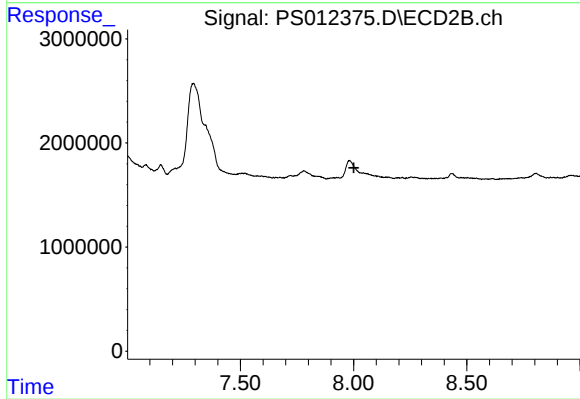

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

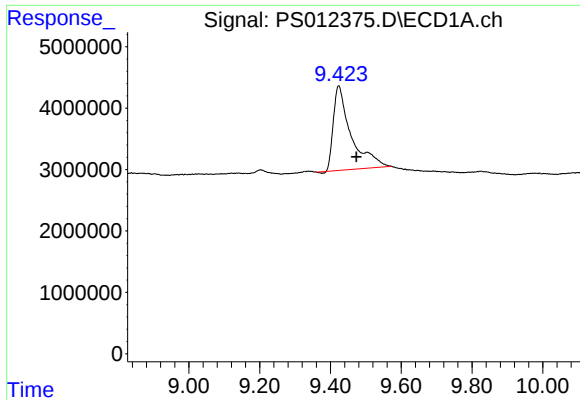

#12 2,4,5-T


R.T.: 9.423 min
Delta R.T.: -0.050 min
Response: 47701532
Conc: 7.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

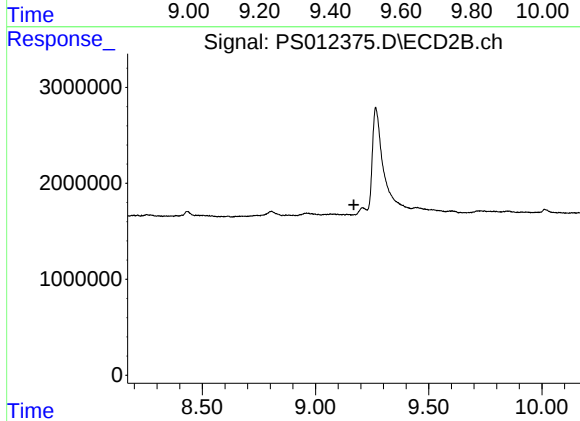


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

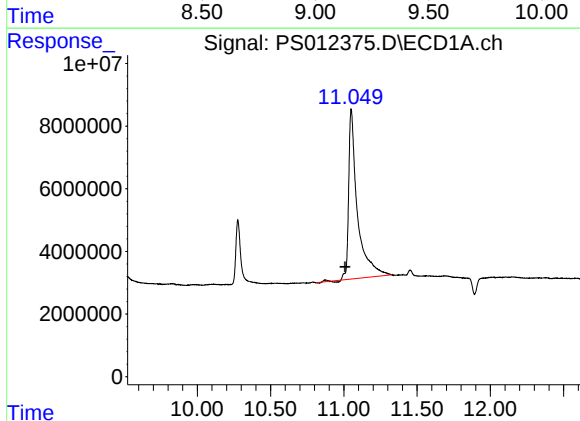

#15 Picloram

R.T.: 11.050 min
Delta R.T.: 0.041 min
Response: 225712087
Conc: 30.65 ng/ml

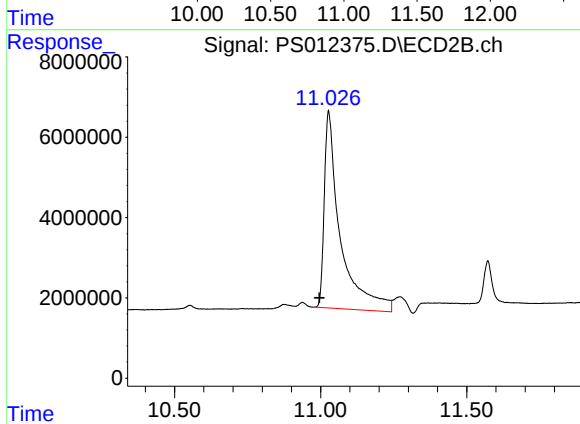

#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.031 min
Response: 186396523
Conc: 43.97 ng/ml