

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091824\
 Data File : PS027713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 09:48
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:03:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.125	0.000	920469	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.556	0.000	9704784	0	2.342	N.D. #
2) T	3,5-DICHL...	0.000	6.639f	0	1462269	N.D.	<MDL
3) T	4-Nitroph...	6.897	7.135f	10596586	614074	6.259	<MDL #
5) T	DICAMBA	0.000	7.823	0	2361842	N.D.	<MDL
6) T	MCP	0.000	7.916	0	422845	N.D.	<MDL
8) T	DICHLORPROP	0.000	8.576f	0	2480830	N.D.	2.221
10) T	Pentachlo...	8.508	0.000	7305538	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.030f	9.754	4170362	2086646	<MDL	<MDL #
12) T	2,4,5-T	9.370f	10.149	751986	3890878	<MDL	<MDL #
13) T	2,4-DB	9.889	0.000	1918032	0	<MDL	N.D. #
15) T	Picloram	10.903	12.191	32334250	5864651	1.728	1.262 #
16) T	DCPA	11.376	12.130	2845846	4503418	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091824\
Data File : PS027713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 09:48
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:03:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

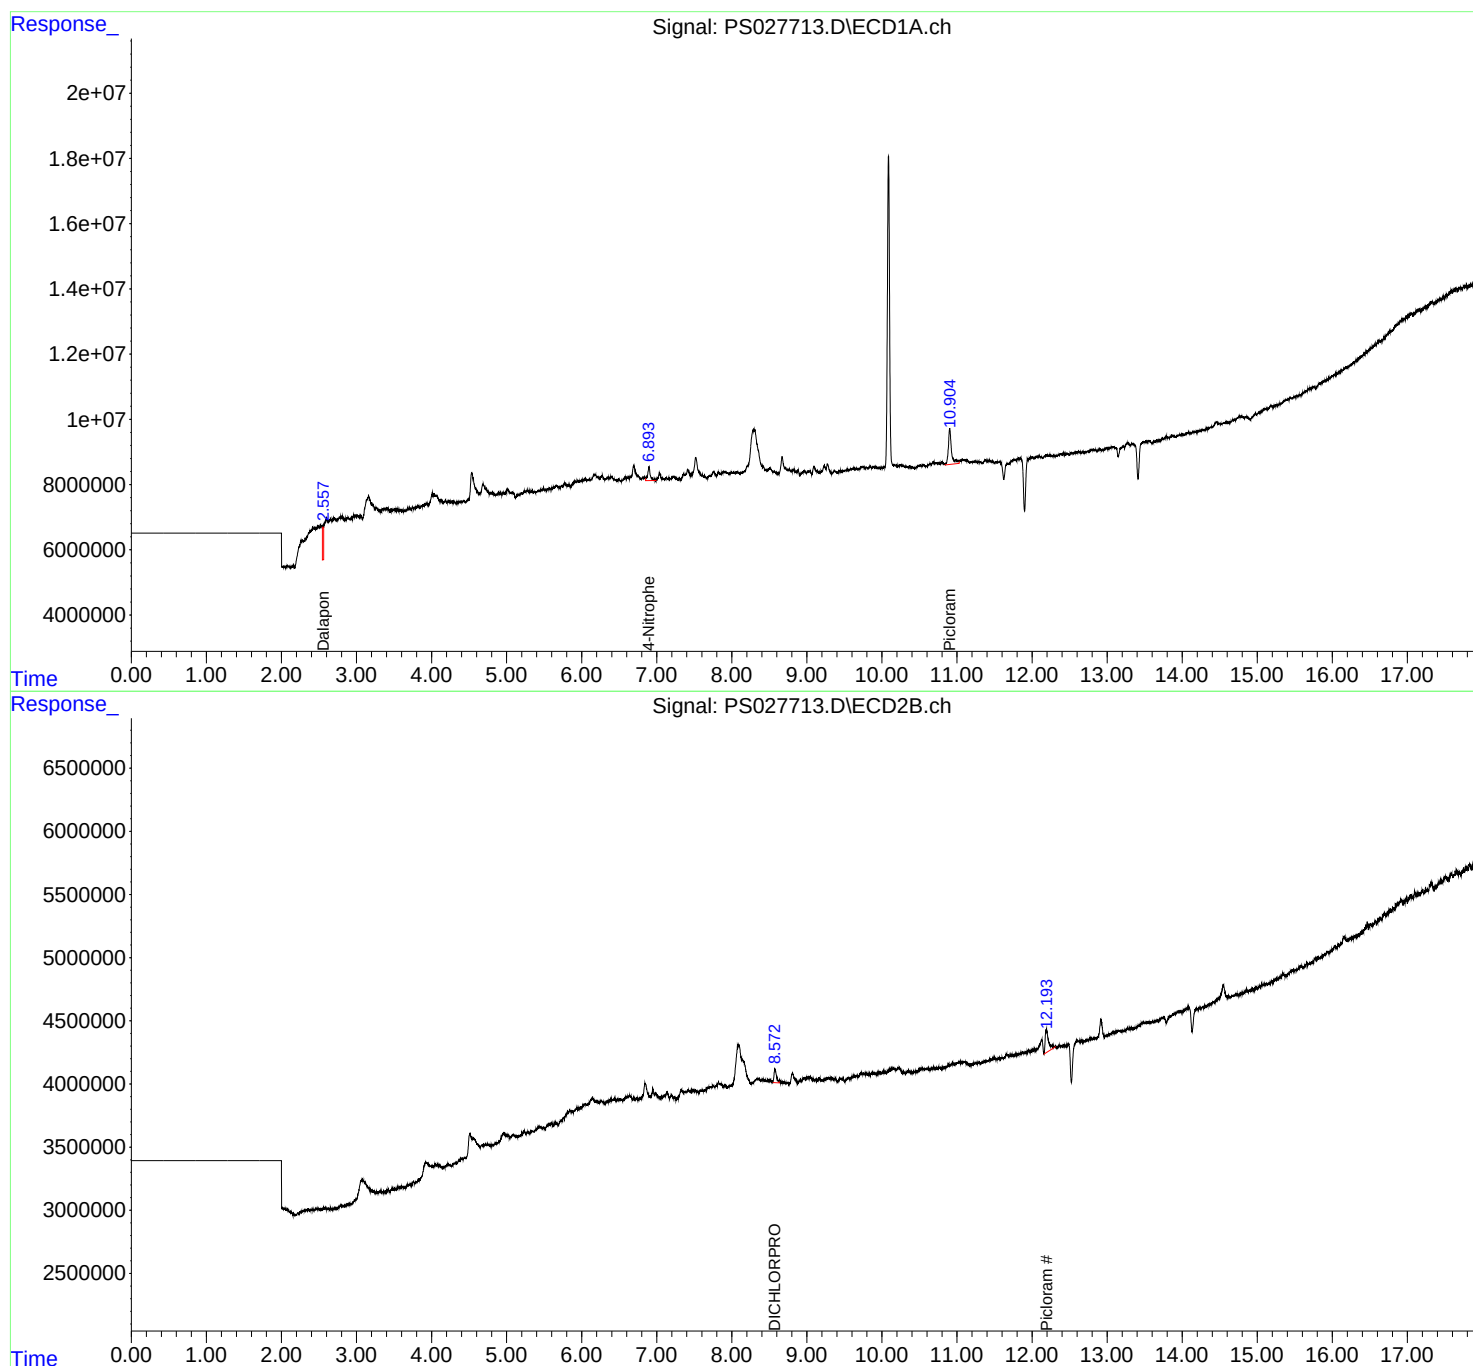


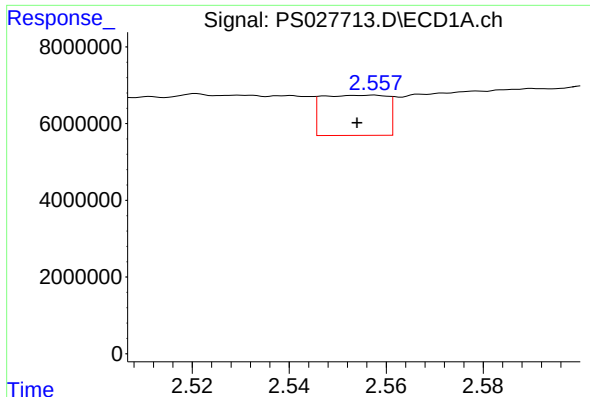

#1 Dalapon


R.T.: 2.556 min
Delta R.T.: 0.002 min
Response: 9704784
Conc: 2.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

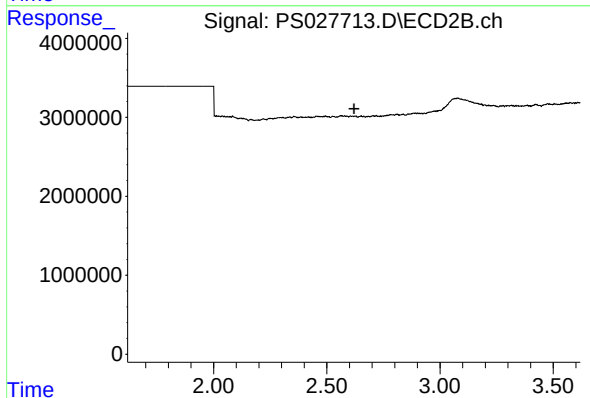


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

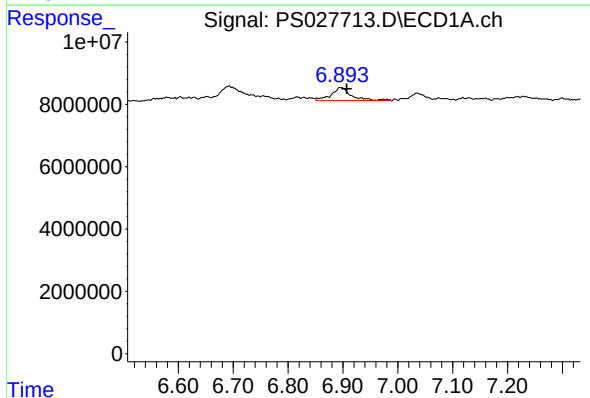


#3 4-Nitrophenol

R.T.: 6.897 min
Delta R.T.: -0.010 min
Response: 10596586
Conc: 6.26 ng/ml

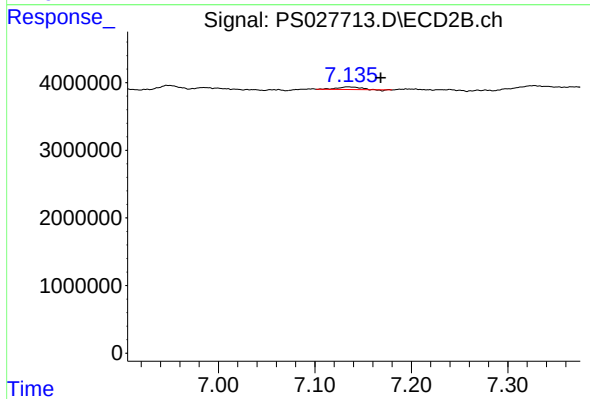

#3 4-Nitrophenol


R.T.: 7.135 min
Delta R.T.: -0.033 min
Response: 614074
Conc: N.D.

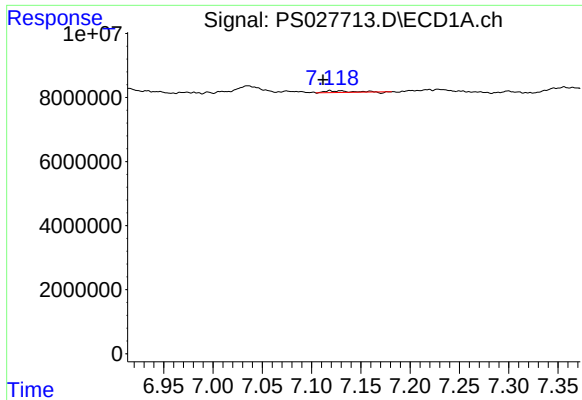

#4 2,4-DCAA


R.T.: 7.125 min
Delta R.T.: 0.013 min
Response: 920469
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

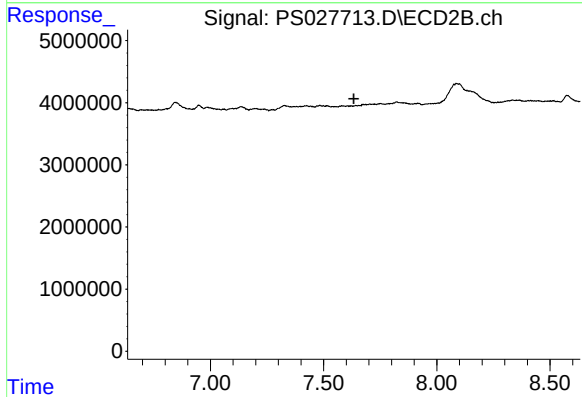


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.633 min
Response: 0
Conc: N.D.

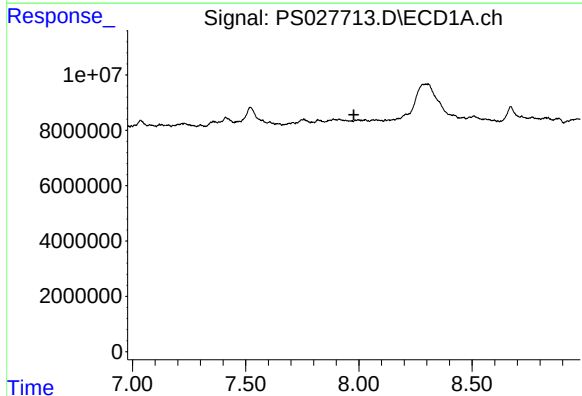


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.978 min
Response: 0
Conc: N.D.

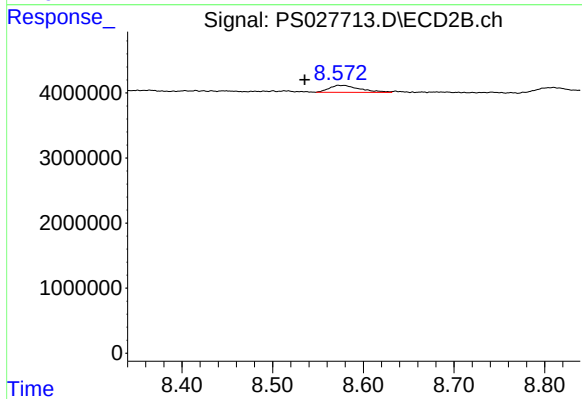

#8 DICHLORPROP


R.T.: 8.576 min
Delta R.T.: 0.040 min
Response: 2480830
Conc: 2.22 ng/ml

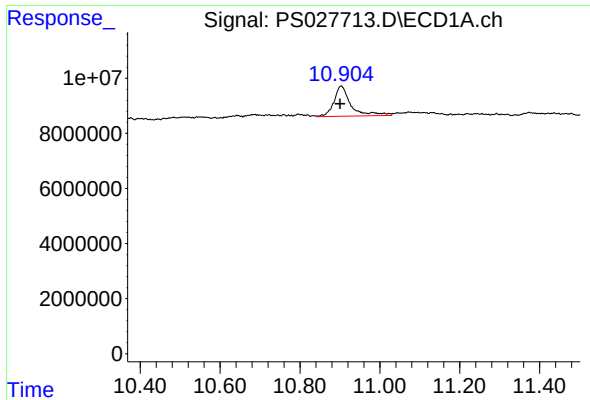

#15 Picloram

R.T.: 10.903 min
Delta R.T.: 0.003 min
Response: 32334250
Conc: 1.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

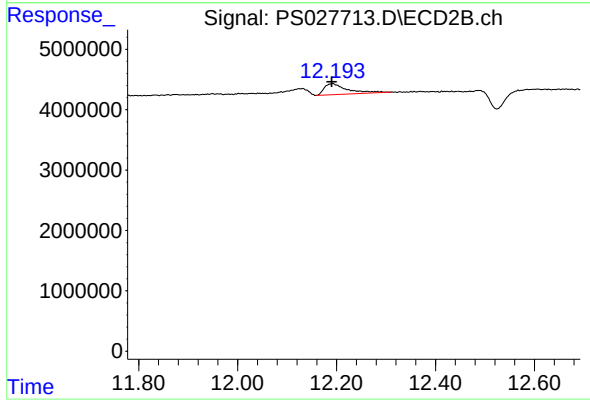

#15 Picloram

R.T.: 12.191 min
Delta R.T.: 0.001 min
Response: 5864651
Conc: 1.26 ng/ml