

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091824\
 Data File : PS027714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 13:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:04:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.111	7.628	1290.7E6	548.0E6	518.851	552.983
Target Compounds							
1) T	Dalapon	2.528f	0.000	30587829	0	7.383	N.D. #
2) T	3,5-DICHL...	6.323	0.000	90705	0	<MDL	N.D. #
3) T	4-Nitroph...	6.909	7.140f	425054	1449620	<MDL	2.022 #
5) T	DICAMBA	0.000	7.818	0	23411417	N.D.	5.313
6) T	MCPD	0.000	7.962f	0	12566252	N.D.	3.828
7) T	MCPA	7.637	0.000	2215523	0	<MDL	N.D. #
8) T	DICHLORPROP	7.960	8.517	2652299	415590	1.001	<MDL #
9) T	2,4-D	8.210	0.000	14083088	0	4.594	N.D. #
10) T	Pentachlo...	8.498	0.000	5456389	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.017f	0.000	3559070	0	<MDL	N.D. #
12) T	2,4,5-T	9.348	10.167	1790291	1167000	<MDL	<MDL #
13) T	2,4-DB	9.912	0.000	1106087	0	<MDL	N.D. #
14) T	DINOSEB	11.080	0.000	2840100	0	<MDL	N.D. #
15) T	Picloram	10.906	12.187	33199696	4802530	1.775	1.033 #
16) T	DCPA	11.376	12.187f	6092287	4802530	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091824\
Data File : PS027714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 13:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:04:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

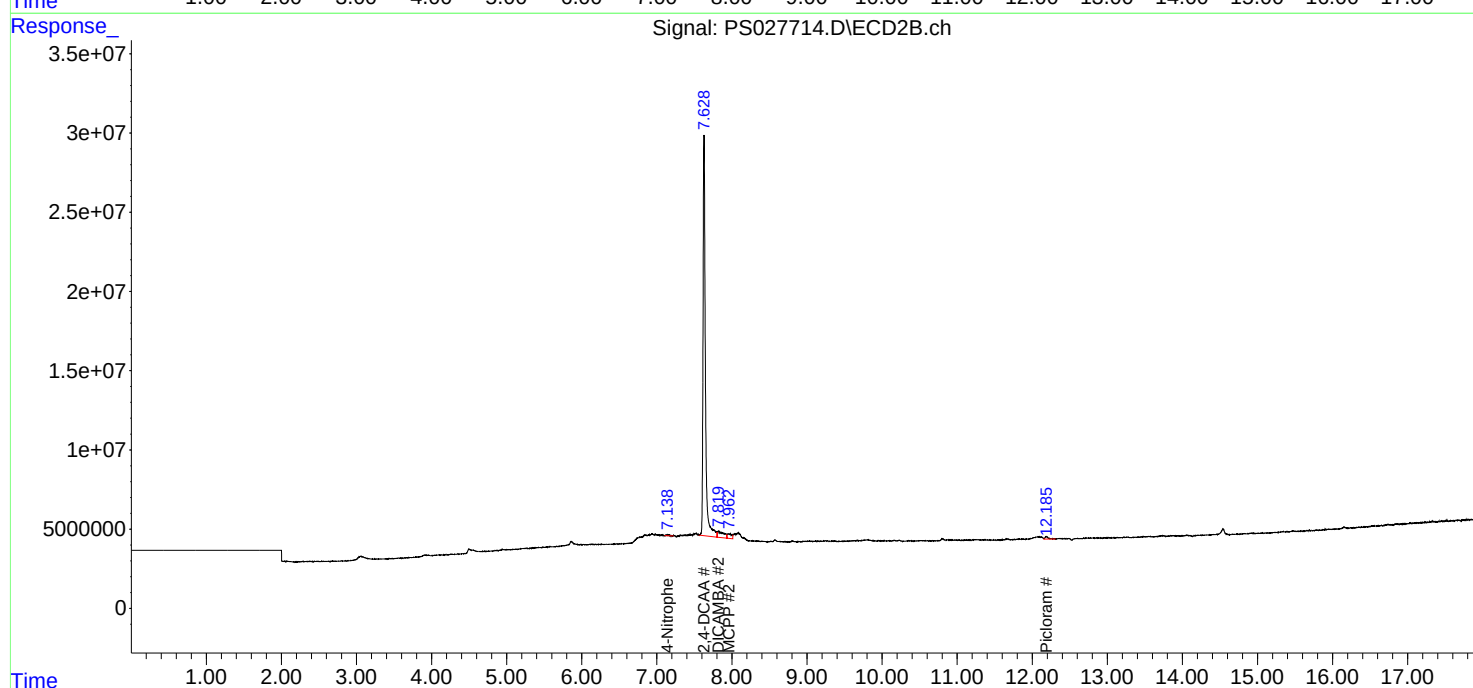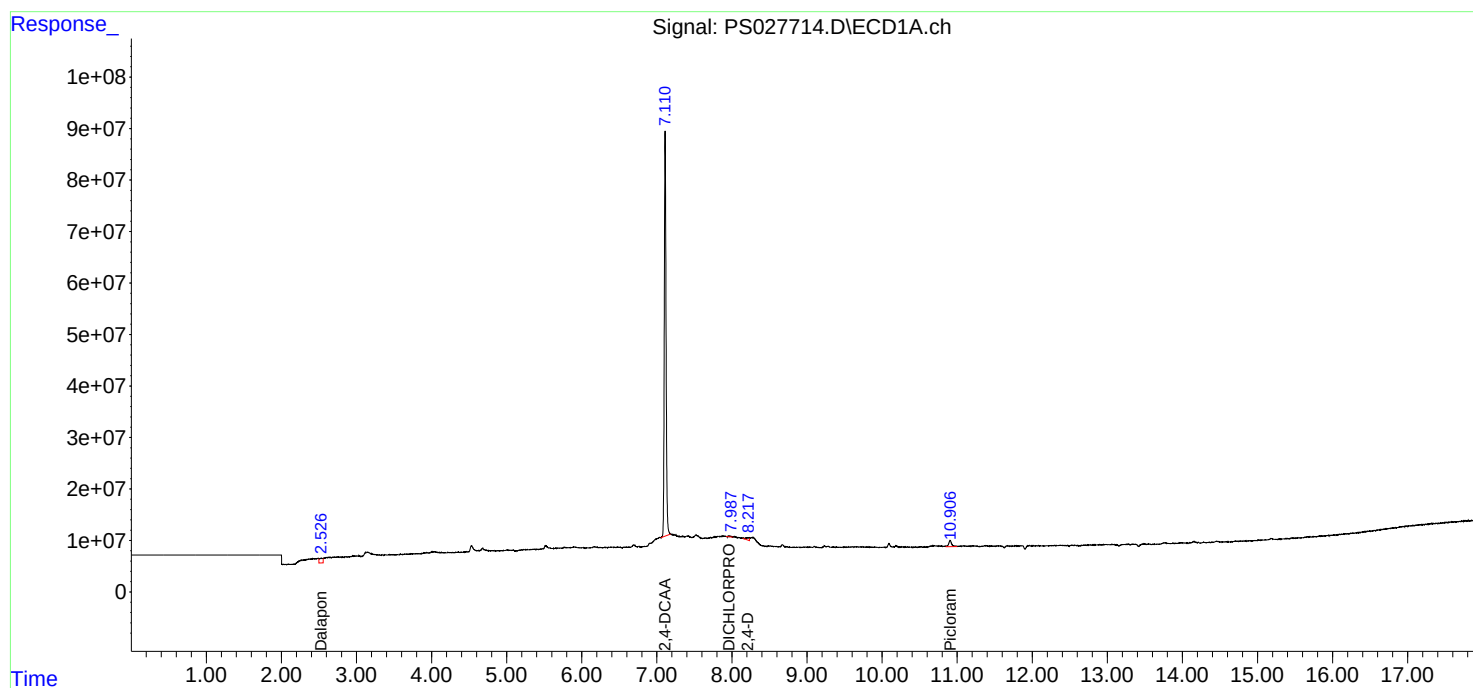


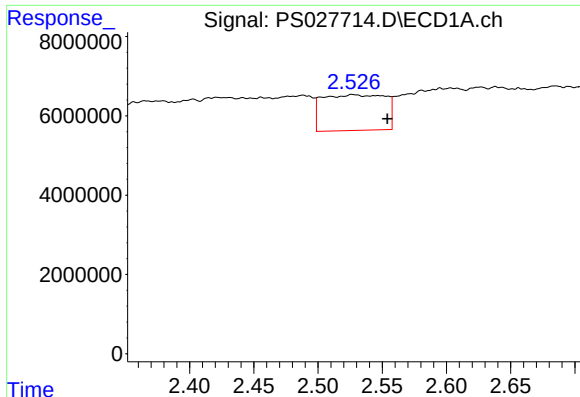

#1 Dalapon


R.T.: 2.528 min
Delta R.T.: -0.026 min
Response: 30587829
Conc: 7.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

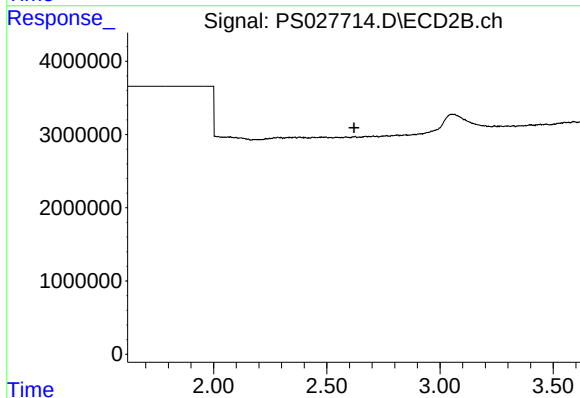


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

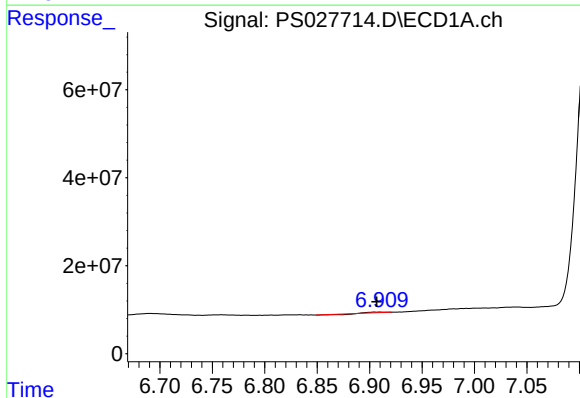


#3 4-Nitrophenol

R.T.: 6.909 min
Delta R.T.: 0.002 min
Response: 425054
Conc: N.D.

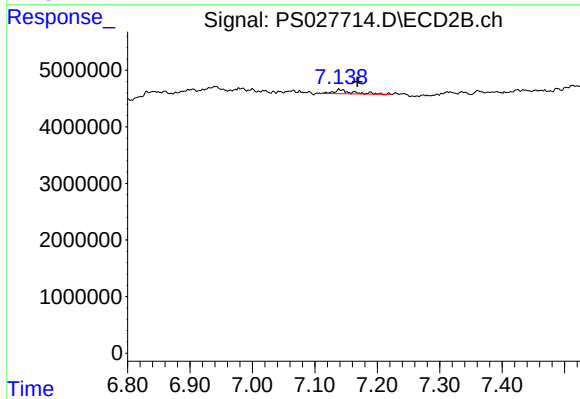

#3 4-Nitrophenol


R.T.: 7.140 min
Delta R.T.: -0.028 min
Response: 1449620
Conc: 2.02 ng/ml

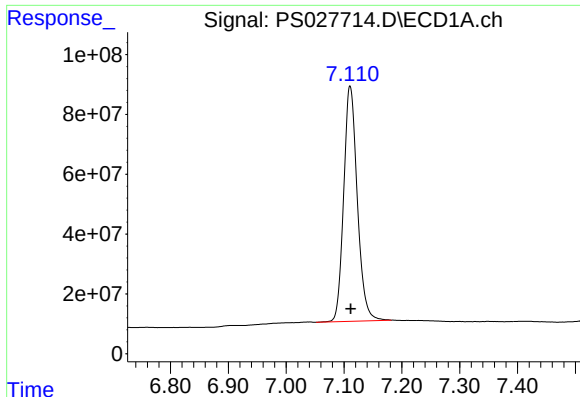

#4 2,4-DCAA


R.T.: 7.111 min
Delta R.T.: 0.000 min
Response: 1290696252
Conc: 518.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

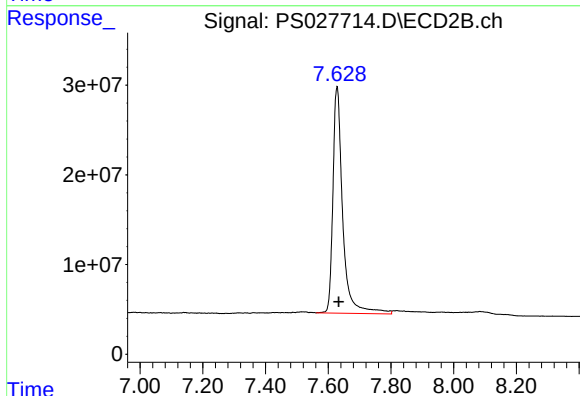


#4 2,4-DCAA

R.T.: 7.628 min
Delta R.T.: -0.006 min
Response: 548024832
Conc: 552.98 ng/ml

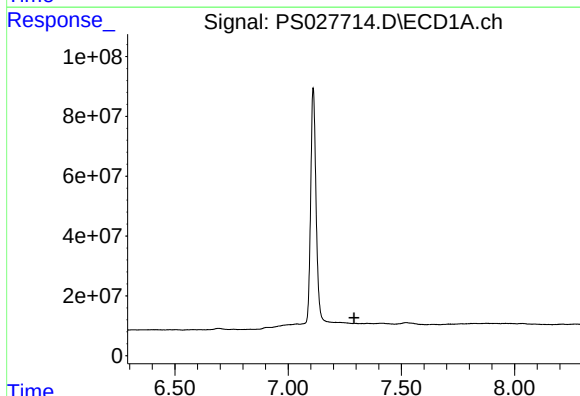


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.291 min
Response: 0
Conc: N.D.

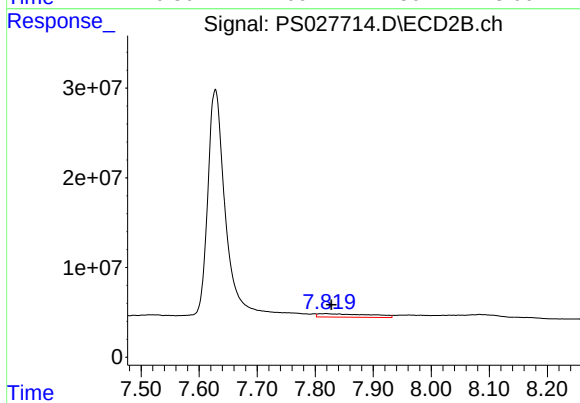

#5 DICAMBA


R.T.: 7.818 min
Delta R.T.: -0.010 min
Response: 23411417
Conc: 5.31 ng/ml

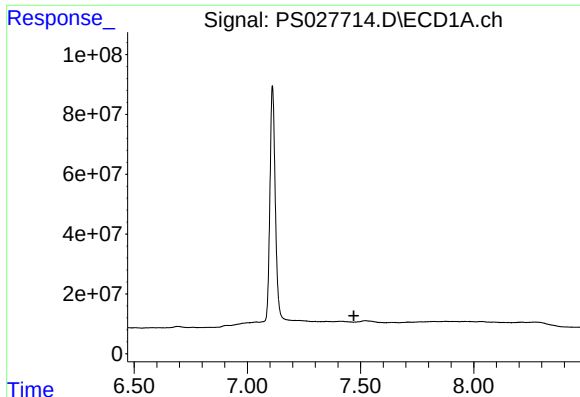

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

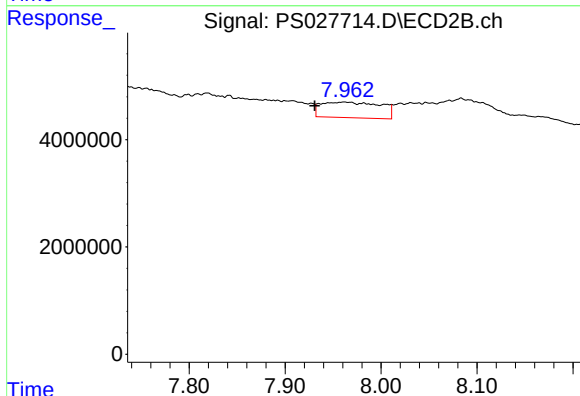


#6 MCP

R.T.: 7.962 min
Delta R.T.: 0.031 min
Response: 12566252
Conc: 3.83 ug/ml

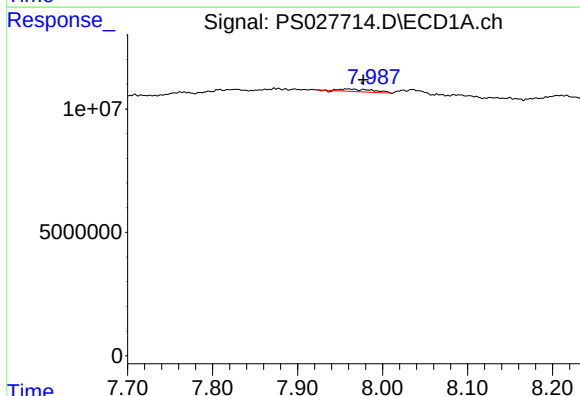


#8 DICHLORPROP

R.T.: 7.960 min
Delta R.T.: -0.018 min
Response: 2652299
Conc: 1.00 ng/ml

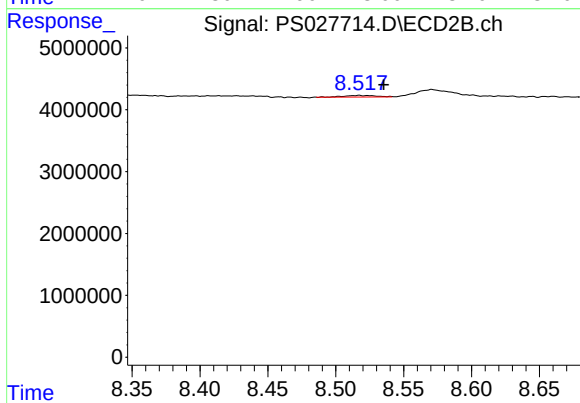

#8 DICHLORPROP


R.T.: 8.517 min
Delta R.T.: -0.018 min
Response: 415590
Conc: N.D.

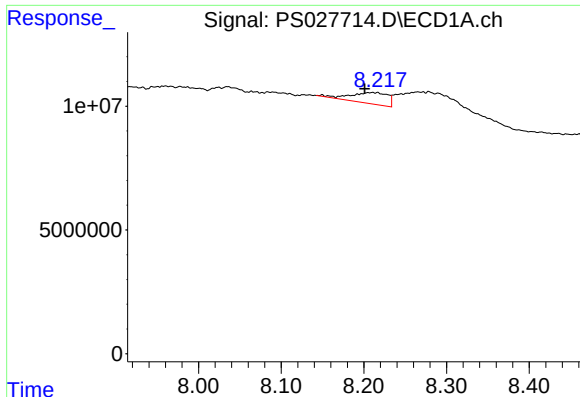

#9 2,4-D


R.T.: 8.210 min
Delta R.T.: 0.009 min
Response: 14083088
Conc: 4.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

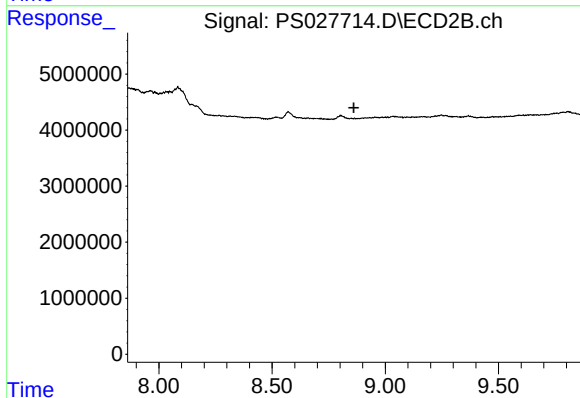


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.861 min
Response: 0
Conc: N.D.

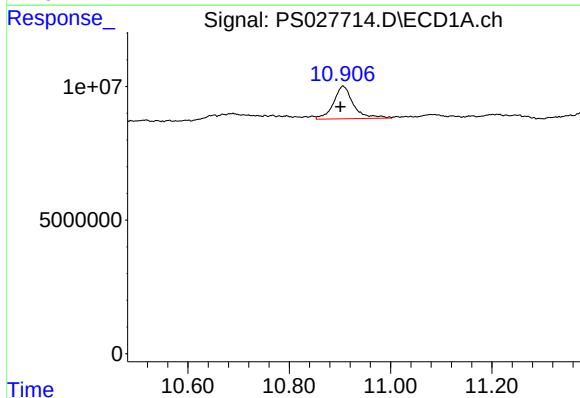

#15 Picloram

R.T.: 10.906 min
Delta R.T.: 0.005 min
Response: 33199696
Conc: 1.77 ng/ml

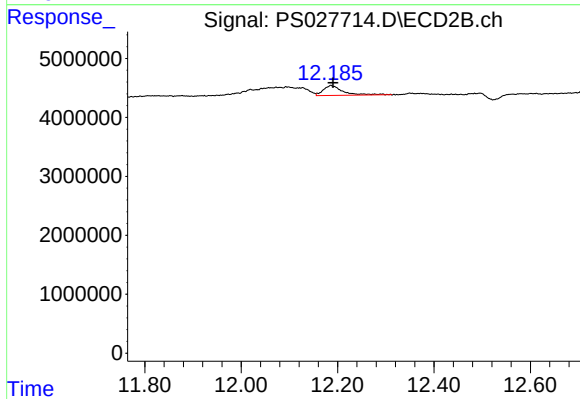

#15 Picloram

R.T.: 12.187 min
Delta R.T.: -0.003 min
Response: 4802530
Conc: 1.03 ng/ml