

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091922\
 Data File : PS020582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 09:08
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 06:32:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.760	1658.0E6	445.3E6	481.756	522.826
Target Compounds							
1) T	Dalapon	3.039	0.000	976140	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.460f	0.000	870908	0	<MDL	N.D. #
7) T	MCPA	7.638	0.000	547329	0	<MDL	N.D. #
9) T	2,4-D	8.359f	0.000	86745631	0	18.663	N.D. #
10) T	Pentachlo...	8.535f	0.000	1085598	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.155	0.000	820719	0	<MDL	N.D. #
12) T	2,4,5-T	9.438	0.000	16079965	0	<MDL	N.D. #
13) T	2,4-DB	9.948	0.000	168953	0	<MDL	N.D. #
14) T	DINOSEB	11.066f	0.000	94783347	0	5.161	N.D. #
15) T	Picloram	10.926f	10.877f	796383	15847917	<MDL	1.968 #
16) T	DCPA	11.399	0.000	2808137	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091922\
Data File : PS020582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 09:08
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 06:32:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

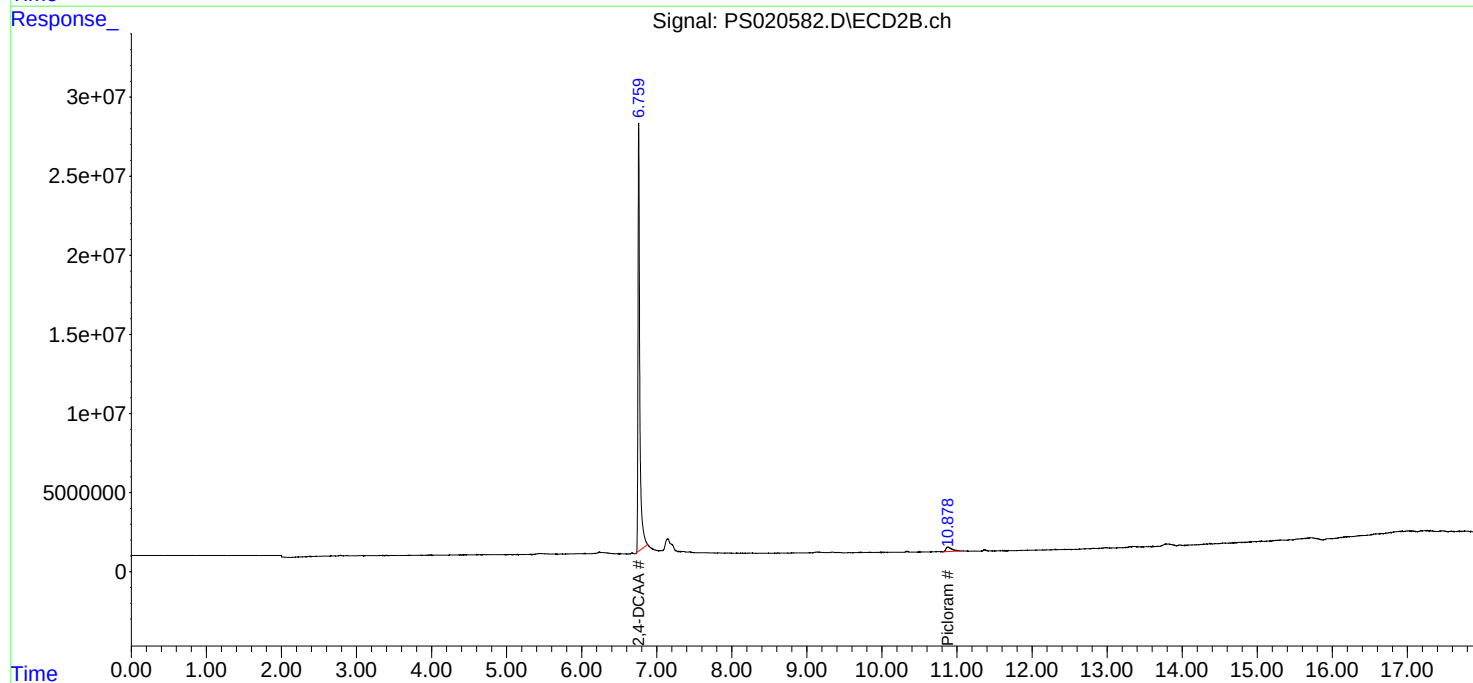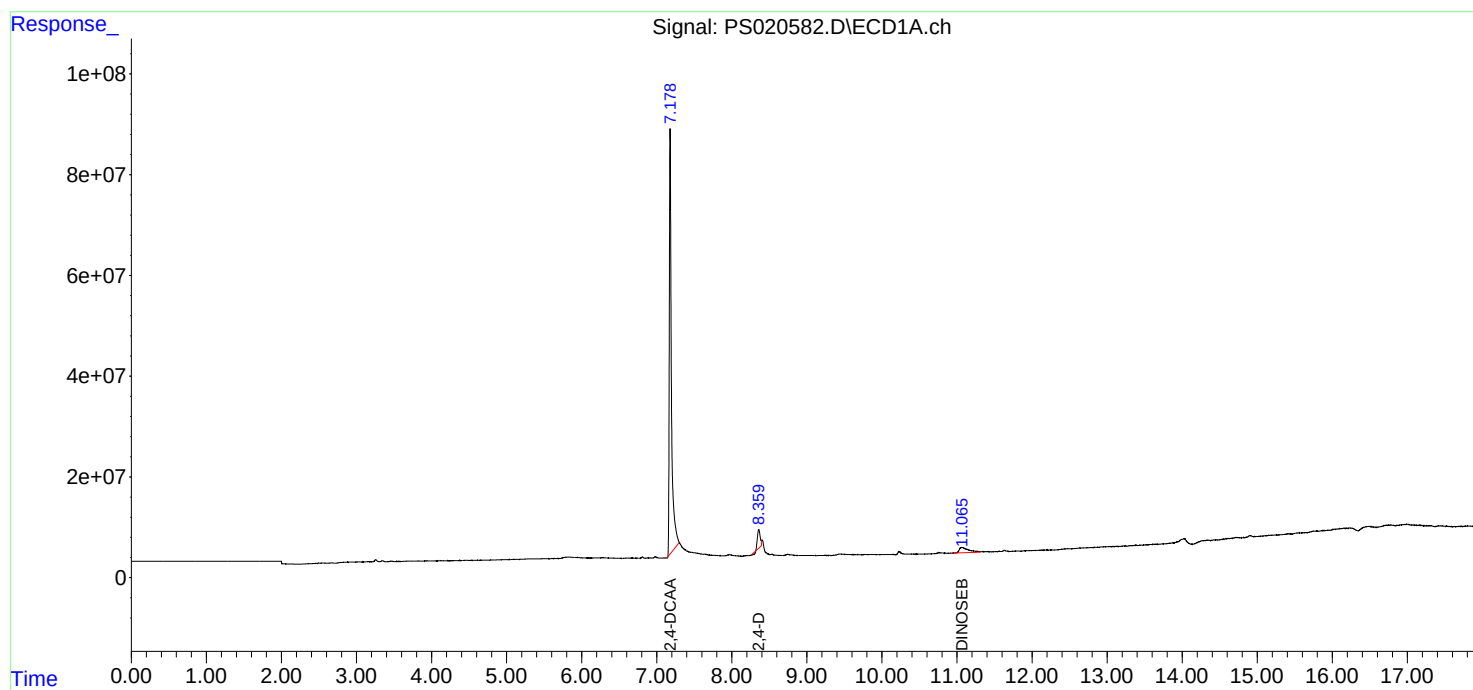


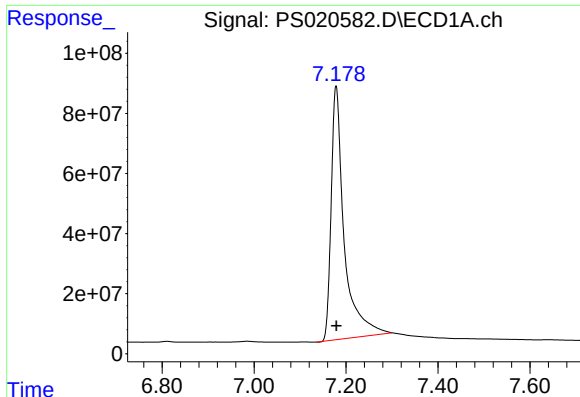

#4 2,4-DCAA


R.T.: 7.179 min
Delta R.T.: 0.000 min
Response: 1657955463
Conc: 481.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

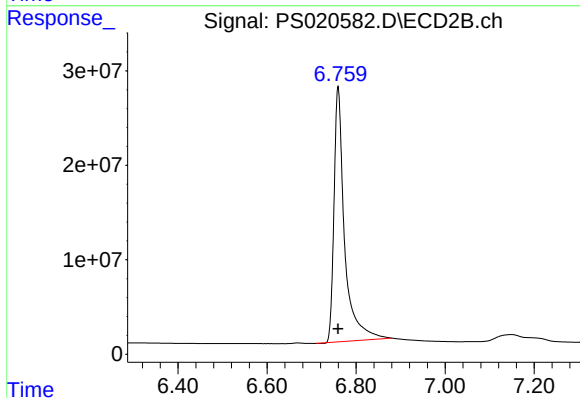


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 445288418
Conc: 522.83 ng/ml

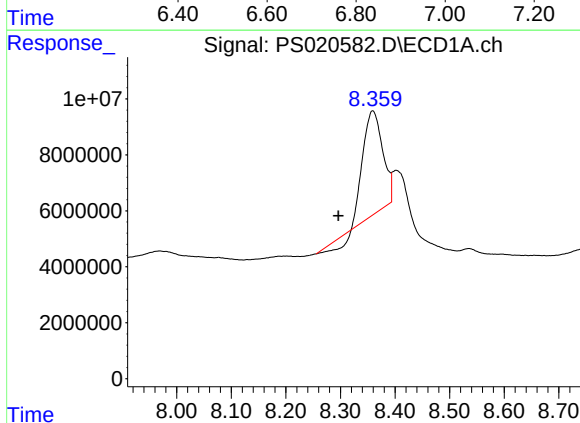


#9 2,4-D

R.T.: 8.359 min
Delta R.T.: 0.063 min
Response: 86745631
Conc: 18.66 ng/ml

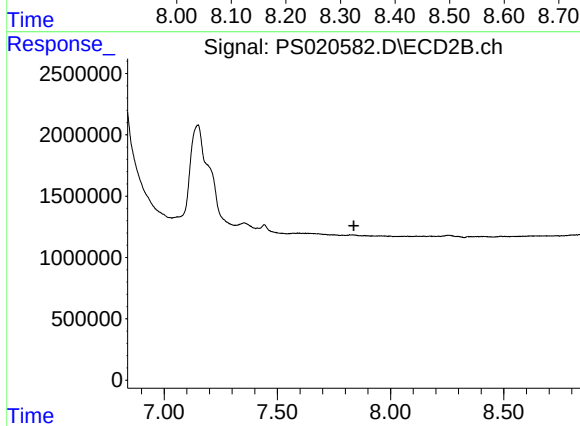

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

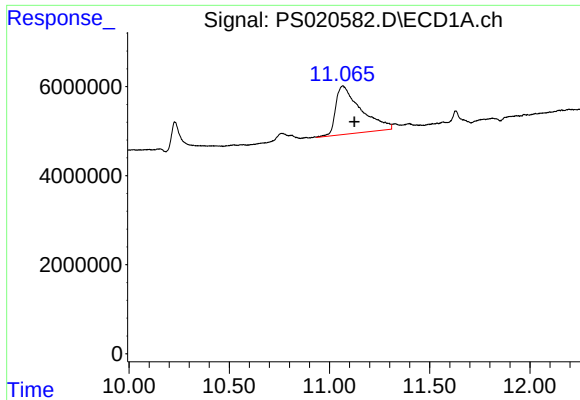

#14 DINoseb


R.T.: 11.066 min
Delta R.T.: -0.059 min
Response: 94783347
Conc: 5.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

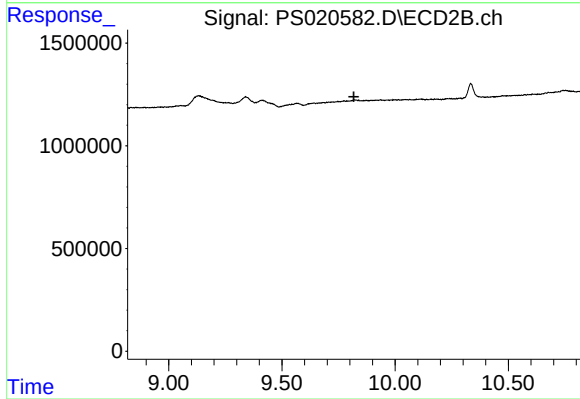


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

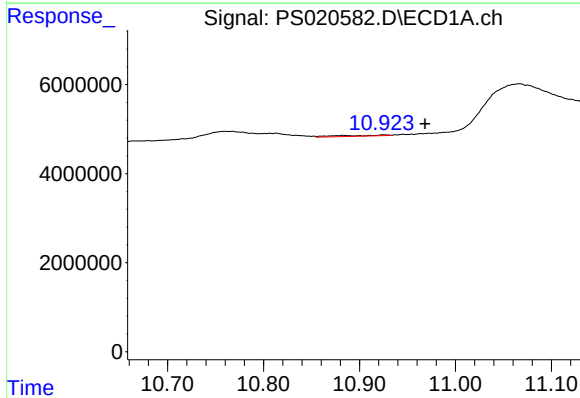

#15 Picloram

R.T.: 10.926 min
Delta R.T.: -0.042 min
Response: 796383
Conc: N.D.

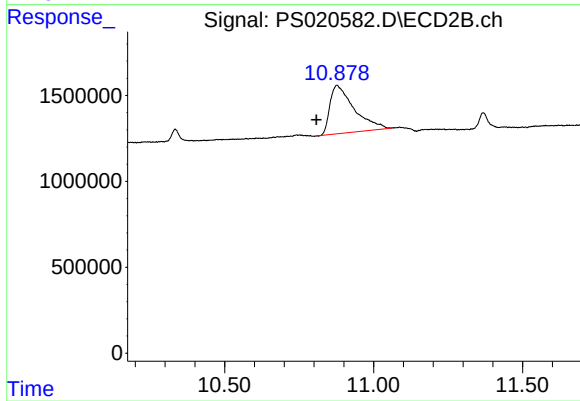

#15 Picloram

R.T.: 10.877 min
Delta R.T.: 0.069 min
Response: 15847917
Conc: 1.97 ng/ml