

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091922\
 Data File : PS020606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 00:51
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 06:45:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.178	6.760	1776.0E6	487.0E6	516.048	571.851
Target Compounds							
1) T	Dalapon	3.015	0.000	536577	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.449f	0.000	3210548	0	<MDL	N.D. #
7) T	MCPA	7.641	7.192	-26437	24304950	N.D.	5.629
9) T	2,4-D	8.355f	0.000	273.4E6	0	58.817	N.D. #
10) T	Pentachlo...	8.533f	0.000	475354	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.101f	0.000	7698884	0	<MDL	N.D. #
12) T	2,4,5-T	9.426	0.000	16889928	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.569f	0	1301449	N.D.	1.819
14) T	DINOSEB	11.122	0.000	10543520	0	<MDL	N.D. #
15) T	Picloram	10.961	10.796	10898700	314108	<MDL	<MDL #
16) T	DCPA	11.402	10.742	3244693	602080	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091922\
Data File : PS020606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 00:51
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 06:45:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

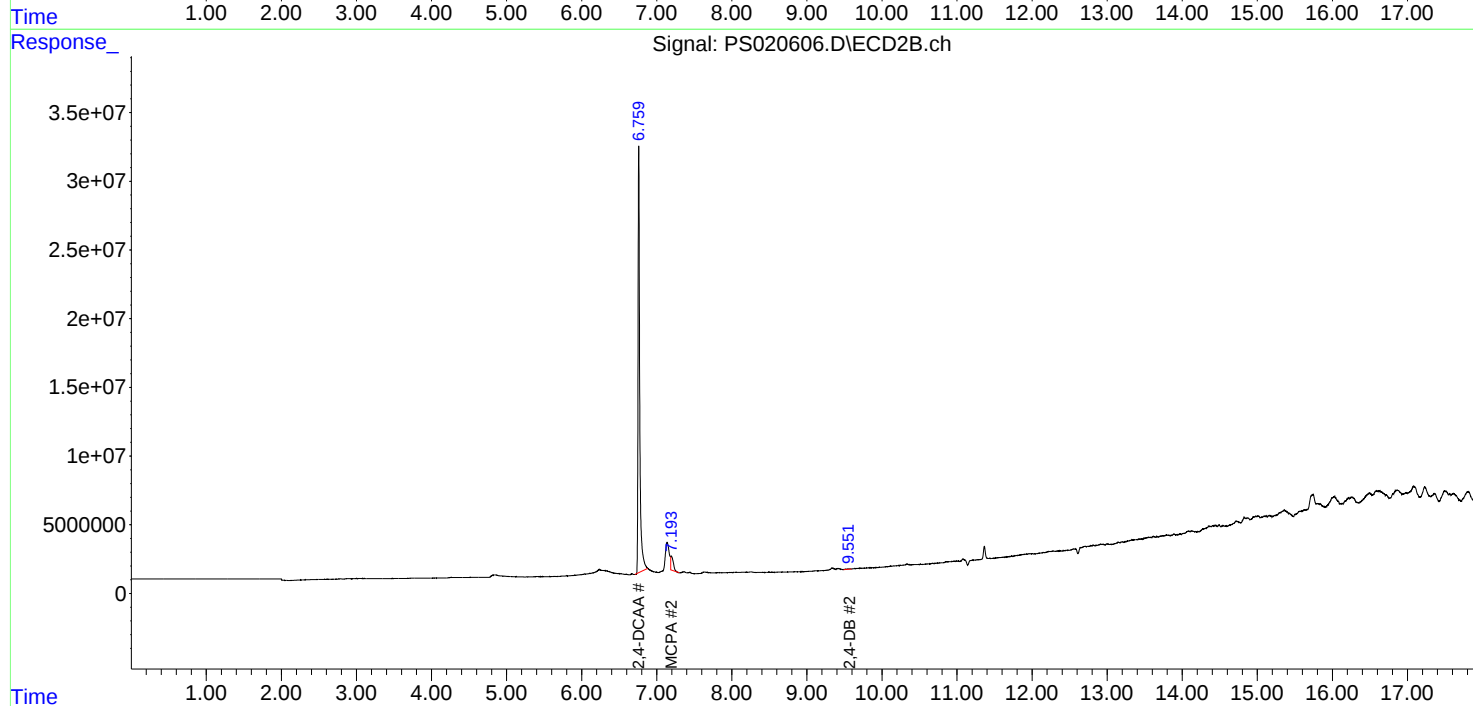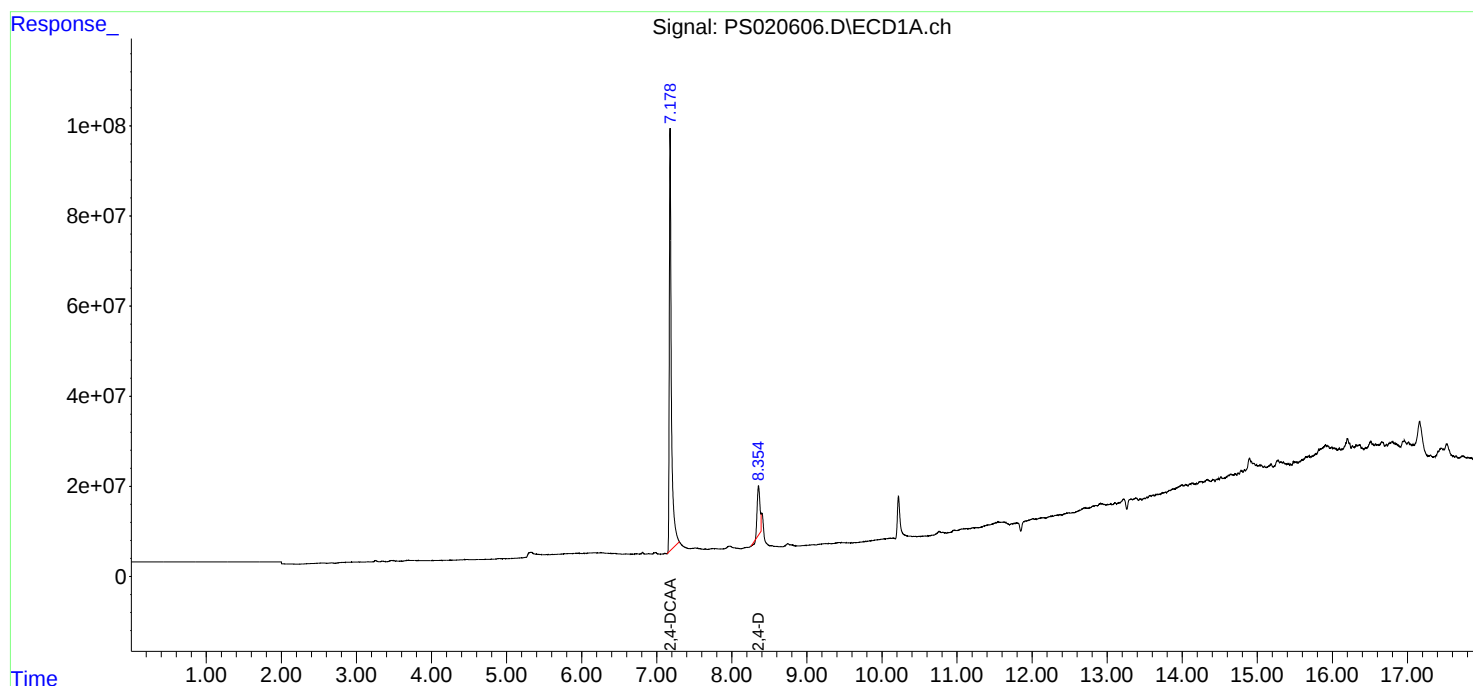


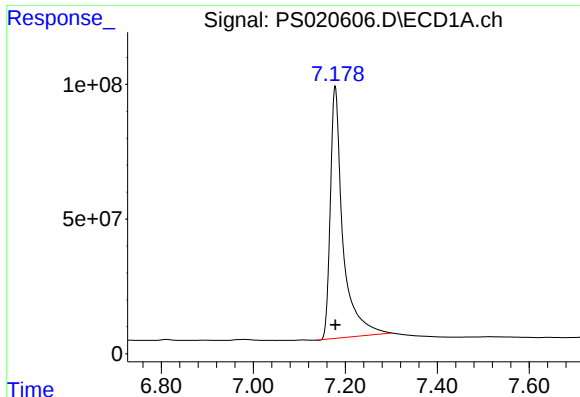

#4 2,4-DCAA


R.T.: 7.178 min
Delta R.T.: 0.000 min
Response: 1775971784
Conc: 516.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

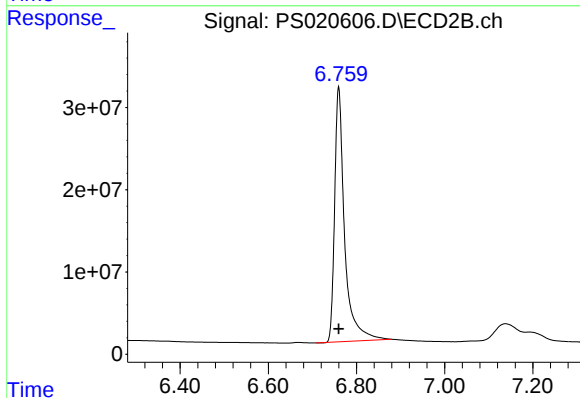


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 487043062
Conc: 571.85 ng/ml

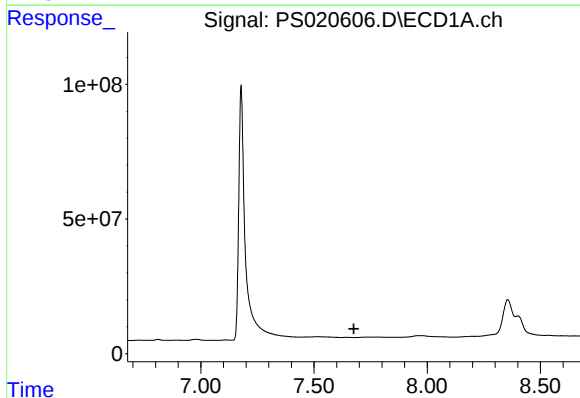


#7 MCPA

R.T.: 7.641 min
Delta R.T.: -0.035 min
Response: -26437
Conc: N.D.

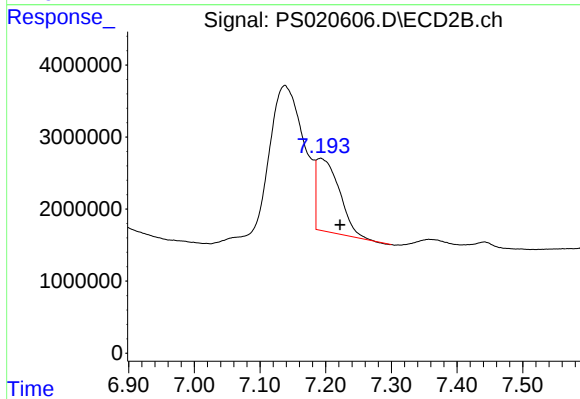

#7 MCPA


R.T.: 7.192 min
Delta R.T.: -0.030 min
Response: 24304950
Conc: 5.63 ug/ml

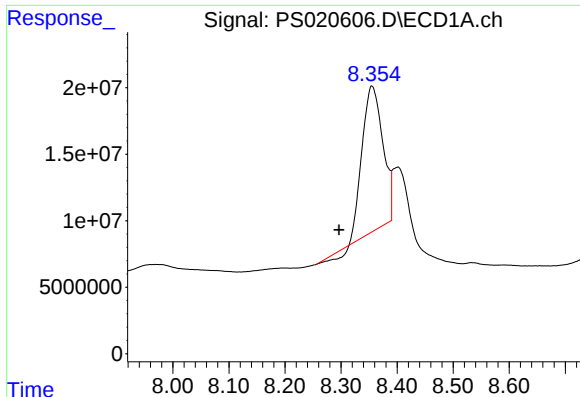

#9 2,4-D


R.T.: 8.355 min
Delta R.T.: 0.059 min
Response: 273384986
Conc: 58.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

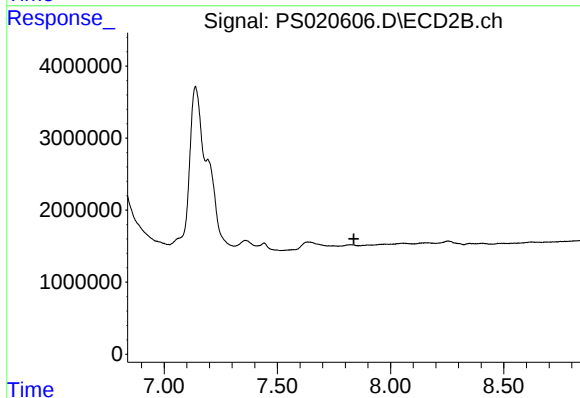


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

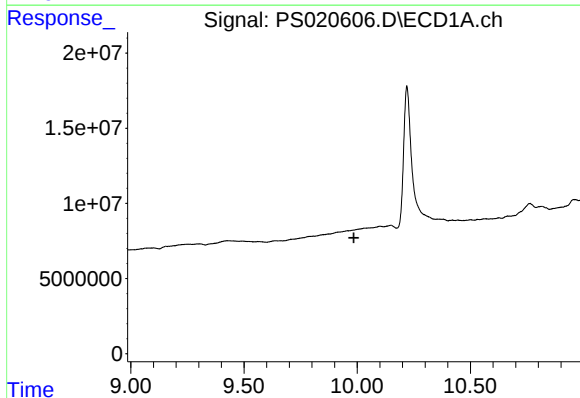

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.985 min
Response: 0
Conc: N.D.

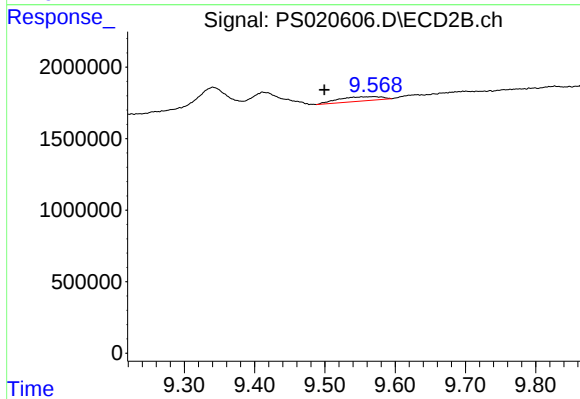

#13 2,4-DB

R.T.: 9.569 min
Delta R.T.: 0.070 min
Response: 1301449
Conc: 1.82 ng/ml