

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091922\
 Data File : PS020613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 05:44
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 06:50:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.760	1725.8E6	485.1E6	501.474	569.520
Target Compounds							
1) T	Dalapon	2.980	0.000	153187	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.456f	0.000	2659207	0	<MDL	N.D. #
3) T	4-Nitroph...	6.986f	0.000	199771	0	127.206	N.D. #
6) T	MCP	7.475f	0.000	116185	0	<MDL	N.D. #
7) T	MCPA	7.646	0.000	2562837	0	<MDL	N.D. #
9) T	2,4-D	8.356f	0.000	257.3E6	0	55.358	N.D. #
10) T	Pentachlo...	8.596	0.000	1403728	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.099f	0.000	9155377	0	<MDL	N.D. #
14) T	DINOSEB	11.130	0.000	5050622	0	<MDL	N.D. #
15) T	Picloram	10.980	0.000	11768167	0	<MDL	N.D. #
16) T	DCPA	11.459f	10.677f	7826503	560572	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091922\
Data File : PS020613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 05:44
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 06:50:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

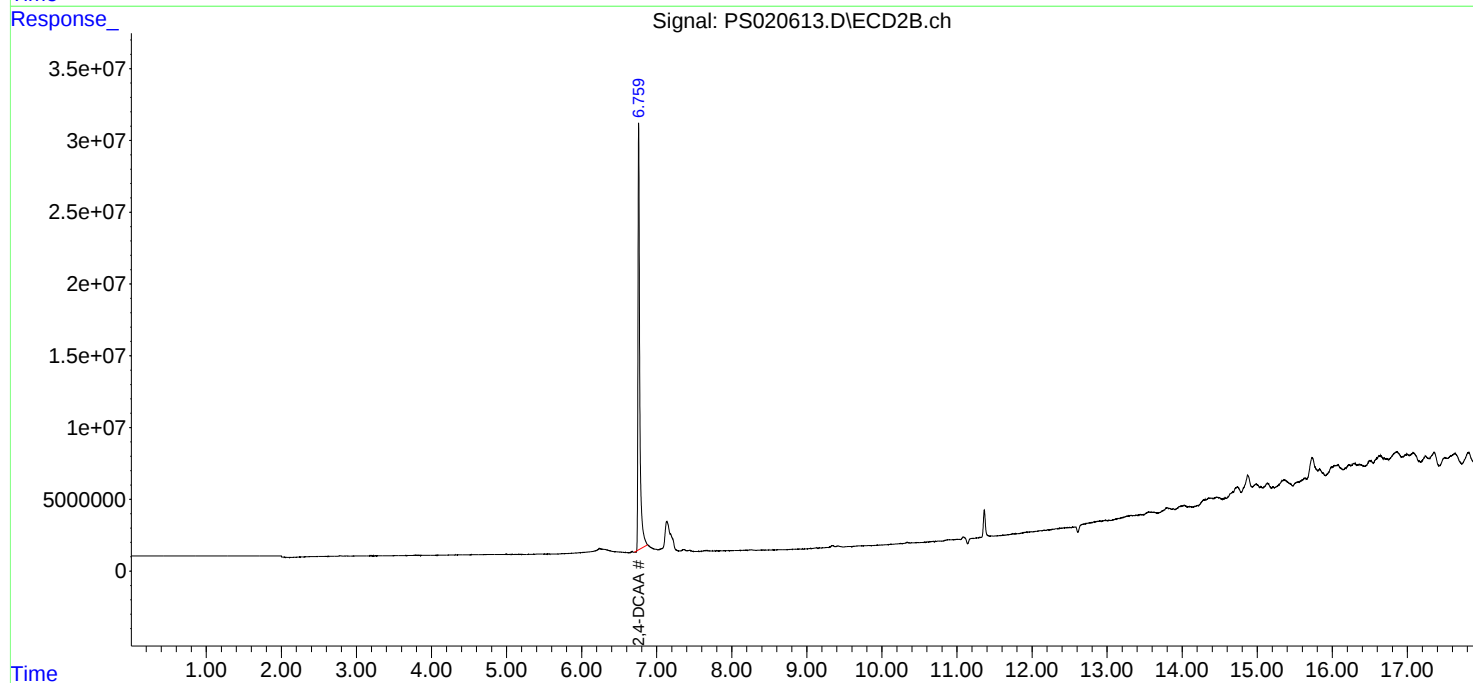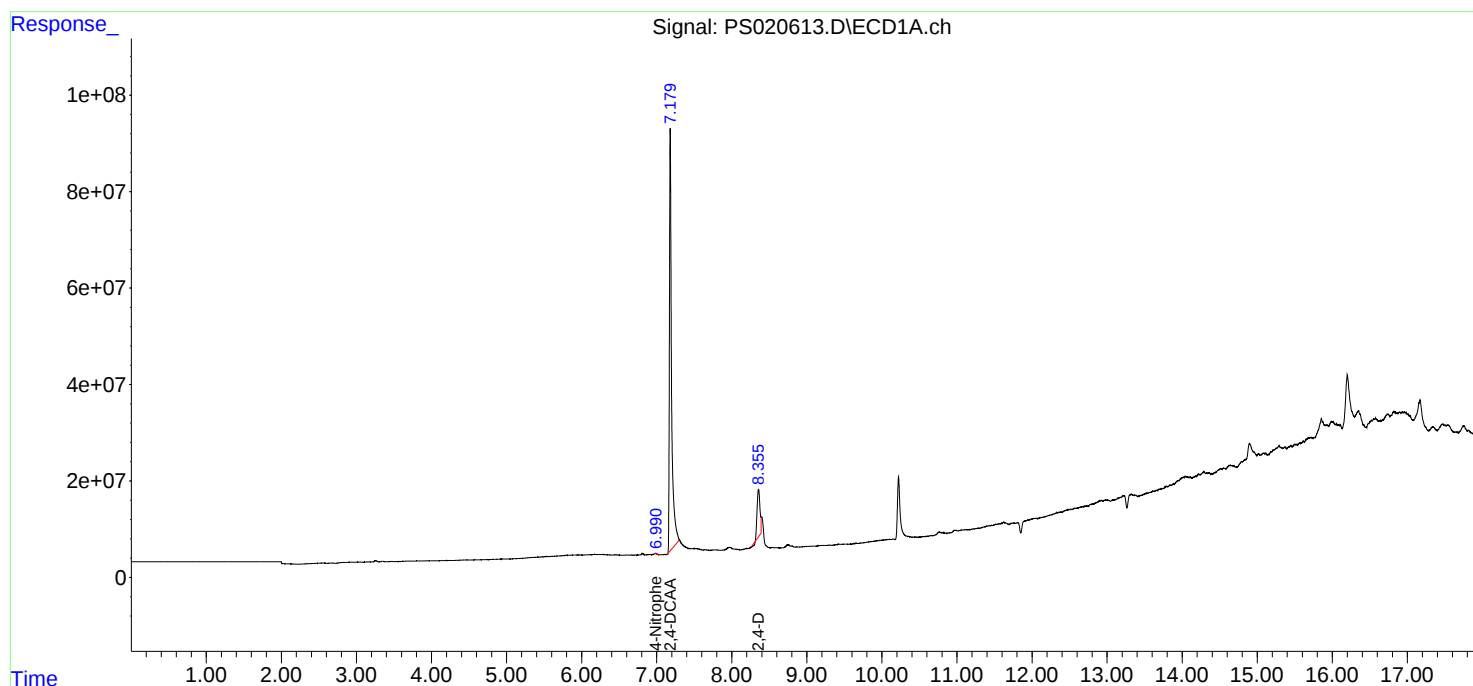


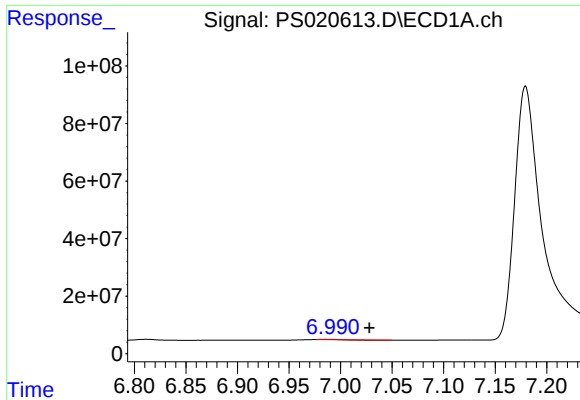

#3 4-Nitrophenol


R.T.: 6.986 min
Delta R.T.: -0.042 min
Response: 199771
Conc: 127.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

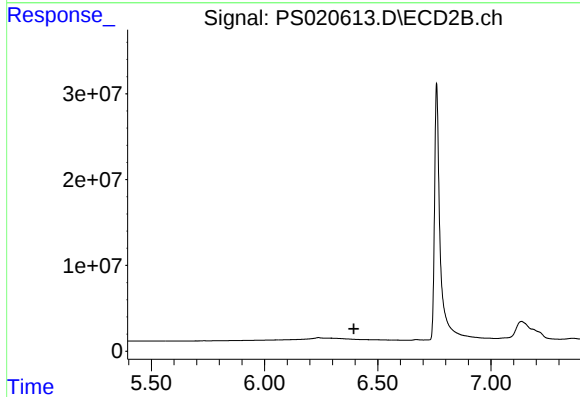


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

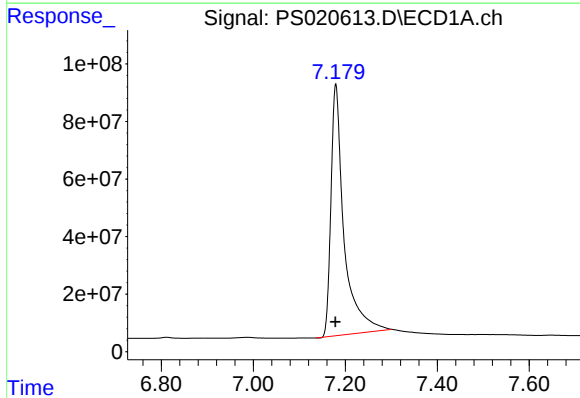


#4 2,4-DCAA

R.T.: 7.179 min
Delta R.T.: 0.000 min
Response: 1725814316
Conc: 501.47 ng/ml

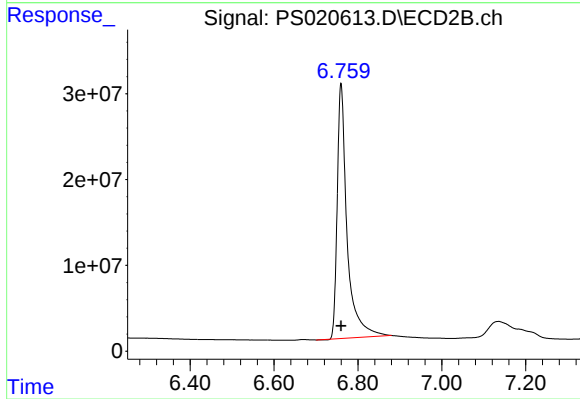

#4 2,4-DCAA


R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 485057279
Conc: 569.52 ng/ml

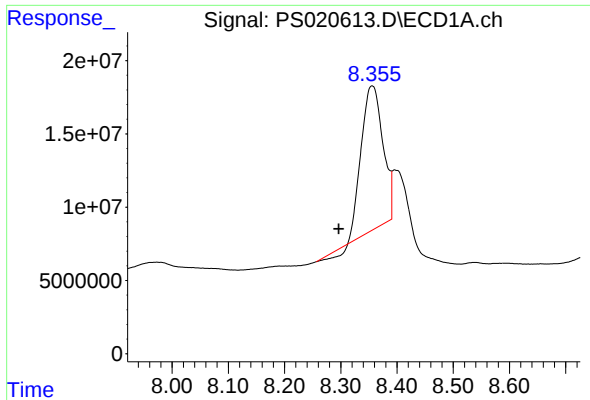

#9 2,4-D

R.T.: 8.356 min
Delta R.T.: 0.059 min
Response: 257308028
Conc: 55.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

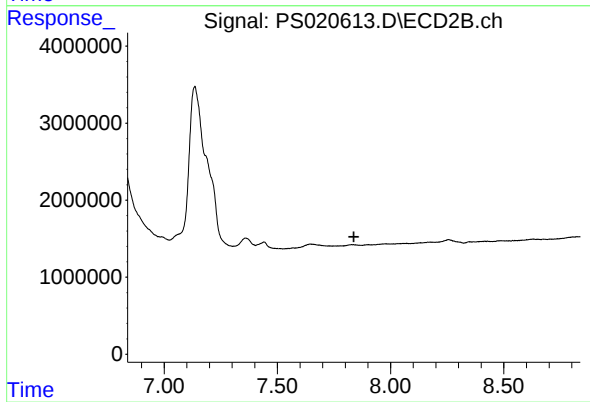

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.