

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091925\
 Data File : PS031778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2025 11:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 00:36:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.747	1779.9E6	489.3E6	494.195	538.356
Target Compounds							
1) T	Dalapon	0.000	2.658f	0	57639923	N.D.	20.457
2) T	3,5-DICHL...	6.448	0.000	7328479	0	1.374	N.D. #
3) T	4-Nitroph...	7.076	0.000	5522374	0	5.006	N.D. #
7) T	MCPA	7.756f	0.000	15494559	0	1.395	N.D. #
8) T	DICHLORPROP	8.193	0.000	968436	0	<MDL	N.D. #
10) T	Pentachlo...	8.708	9.513	8865411	8592644	<MDL	<MDL #
11) T	2,4,5-TP ...	9.290	9.908	5357655	3799054	<MDL	<MDL #
12) T	2,4,5-T	9.625f	0.000	4463326	0	<MDL	N.D. #
13) T	2,4-DB	10.152	10.878	2345296	3154808	1.005	2.948 #
14) T	DINOSEB	11.361	0.000	3021894	0	<MDL	N.D. #
15) T	Picloram	11.194	0.000	3151969	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091925\
Data File : PS031778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2025 11:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 00:36:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

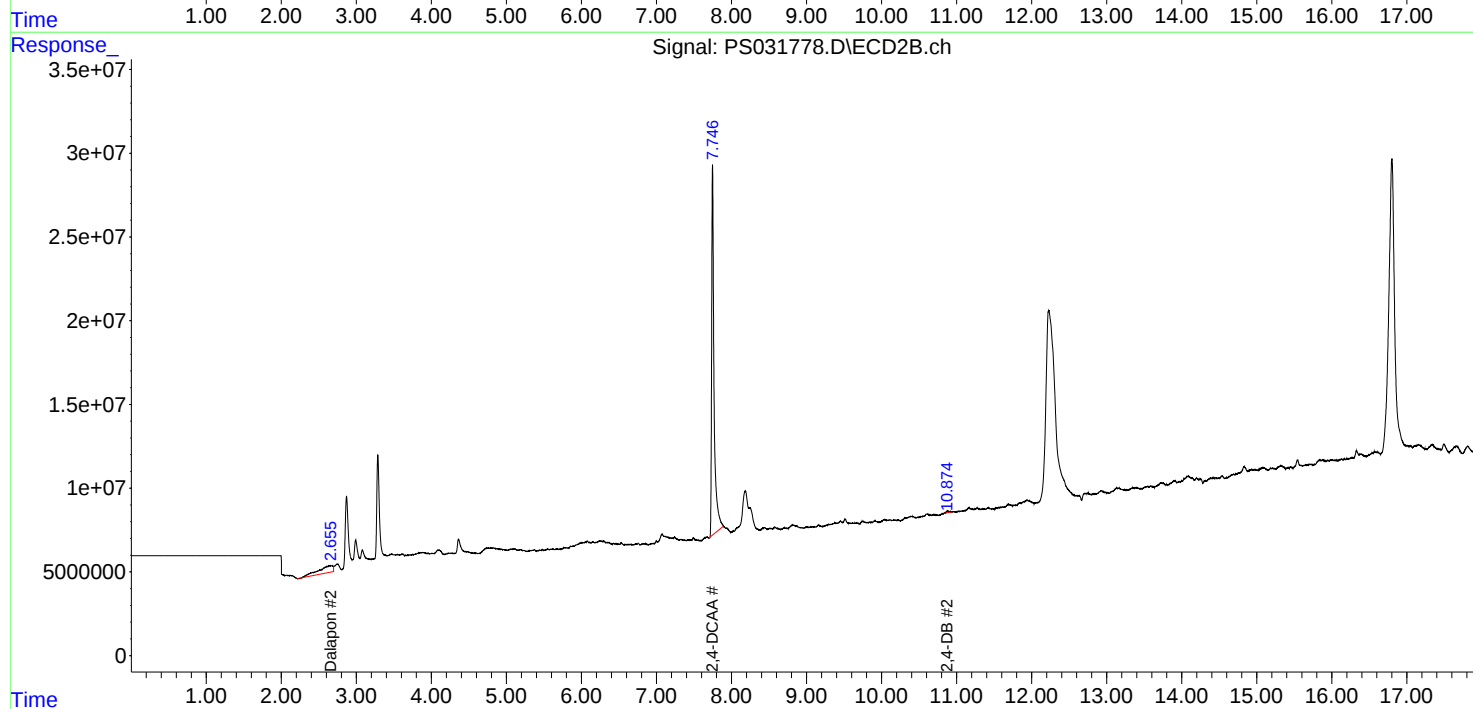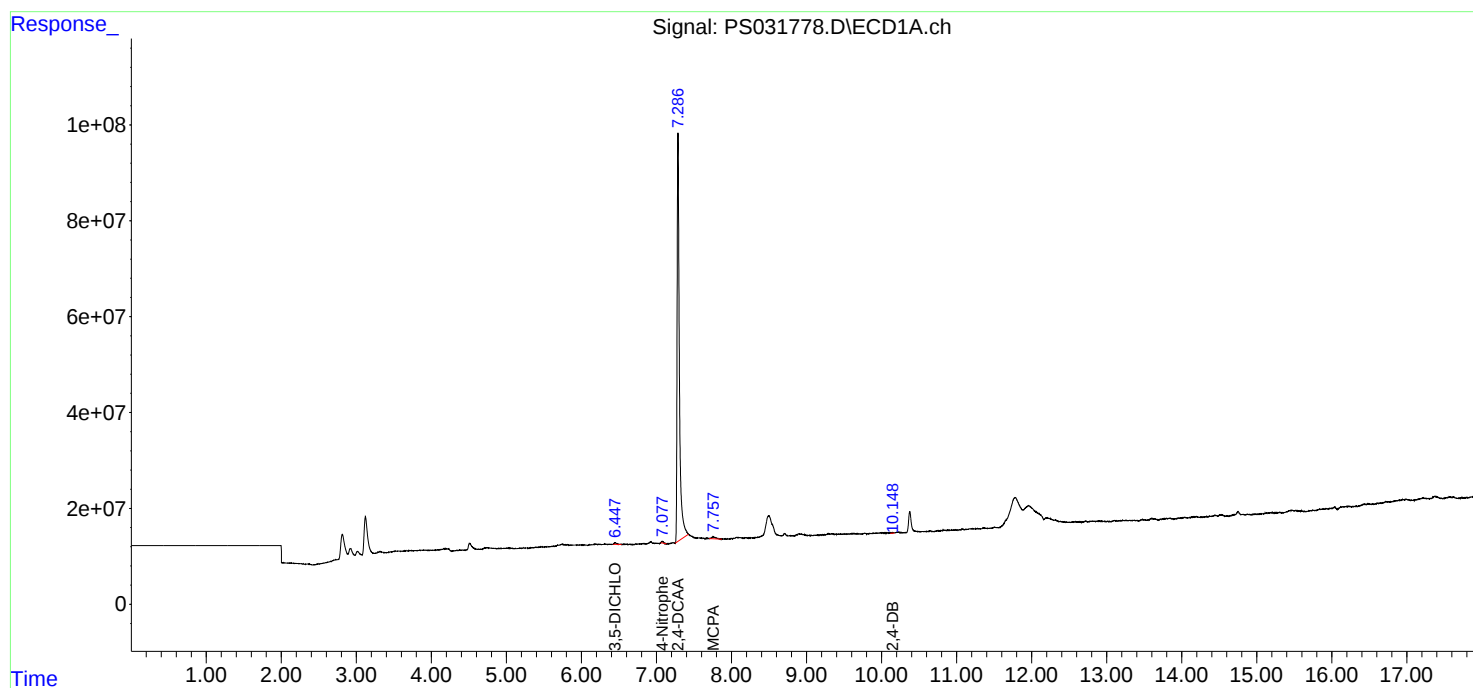


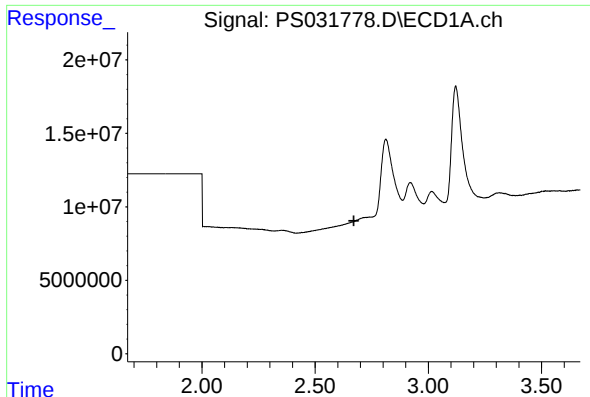

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

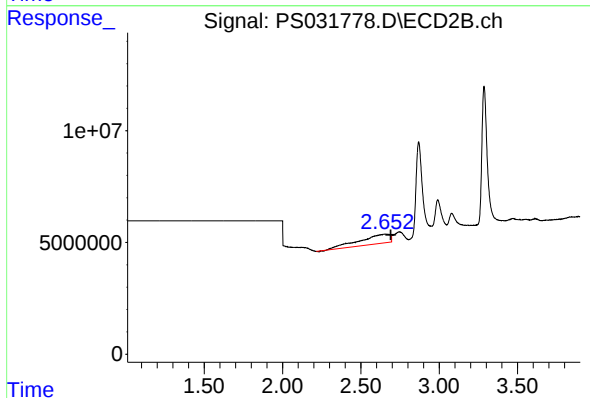


#1 Dalapon

R.T.: 2.658 min
Delta R.T.: -0.034 min
Response: 57639923
Conc: 20.46 ng/ml

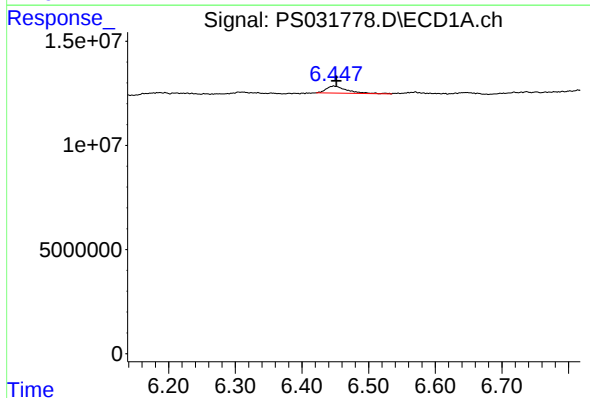


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.448 min
Delta R.T.: -0.004 min
Response: 7328479
Conc: 1.37 ng/ml

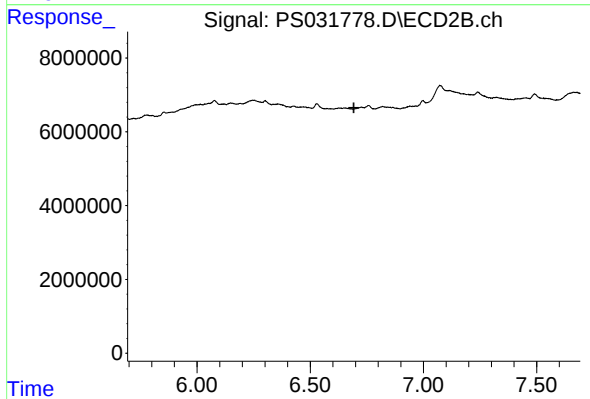

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

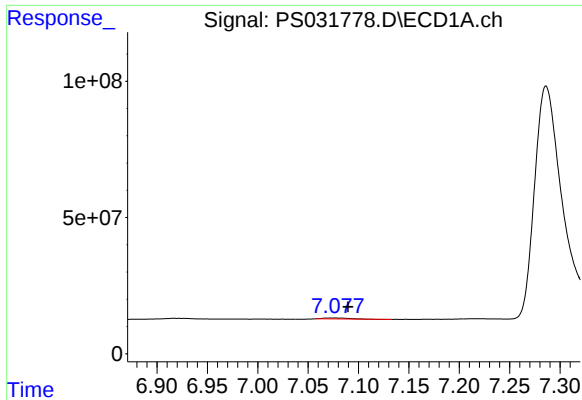

#3 4-Nitrophenol


R.T.: 7.076 min
Delta R.T.: -0.013 min
Response: 5522374
Conc: 5.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

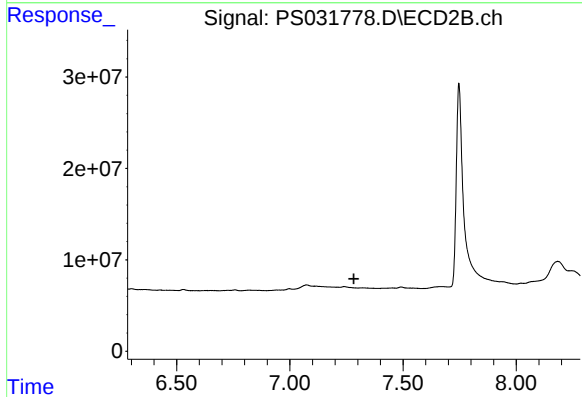


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

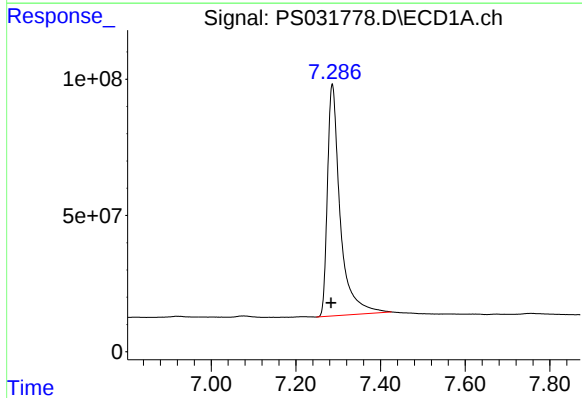


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.003 min
Response: 1779855833
Conc: 494.19 ng/ml

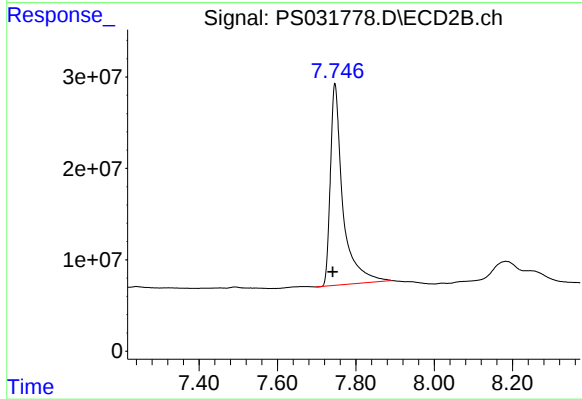

#4 2,4-DCAA


R.T.: 7.747 min
Delta R.T.: 0.006 min
Response: 489311429
Conc: 538.36 ng/ml

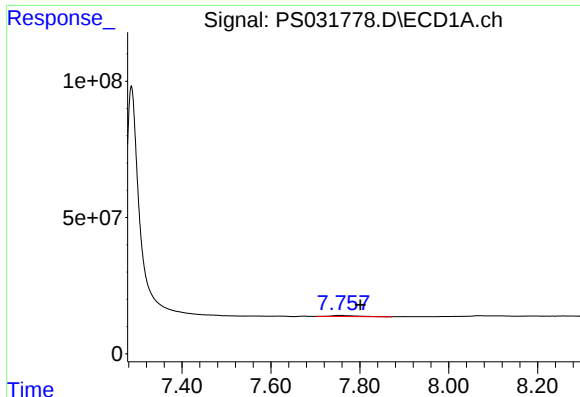

#7 MCPA


R.T.: 7.756 min
Delta R.T.: -0.046 min
Response: 15494559
Conc: 1.39 ug/ml

Instrument :
ECD_S
ClientSampleId :

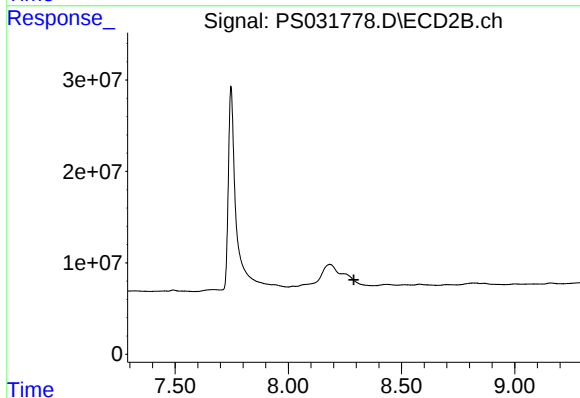


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.290 min
Response: 0
Conc: N.D.

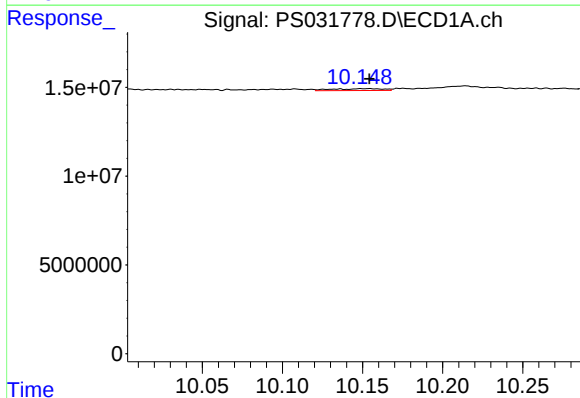

#13 2,4-DB

R.T.: 10.152 min
Delta R.T.: -0.002 min
Response: 2345296
Conc: 1.01 ng/ml

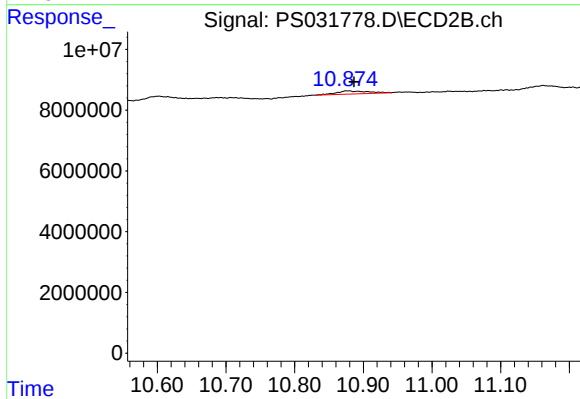

#13 2,4-DB

R.T.: 10.878 min
Delta R.T.: -0.009 min
Response: 3154808
Conc: 2.95 ng/ml