

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092018\
 Data File : PS001788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2018 10:47
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:28:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.437	0	779272	N.D. 2.638 #
5) T	DICAMBA	11.807	0.000	950840	0	1.097 N.D. #
8) T	DICHLORPROP	12.987	0.000	1966488	0	8.474 N.D. #
15) T	Picloram	17.013	0.000	4256681	0	2.445 N.D. #
16) T	DCPA	0.000	16.925	0	3315031	N.D. 1.797 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092018\
Data File : PS001788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2018 10:47
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:28:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

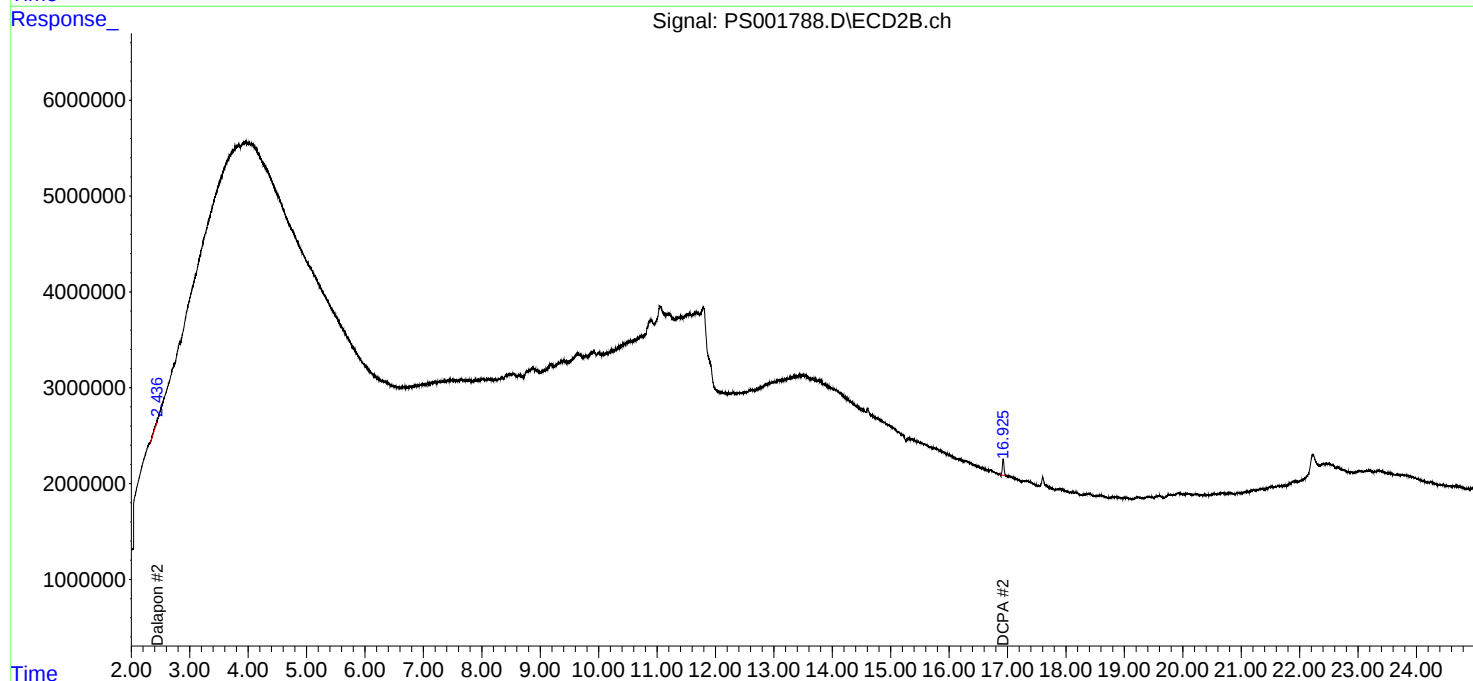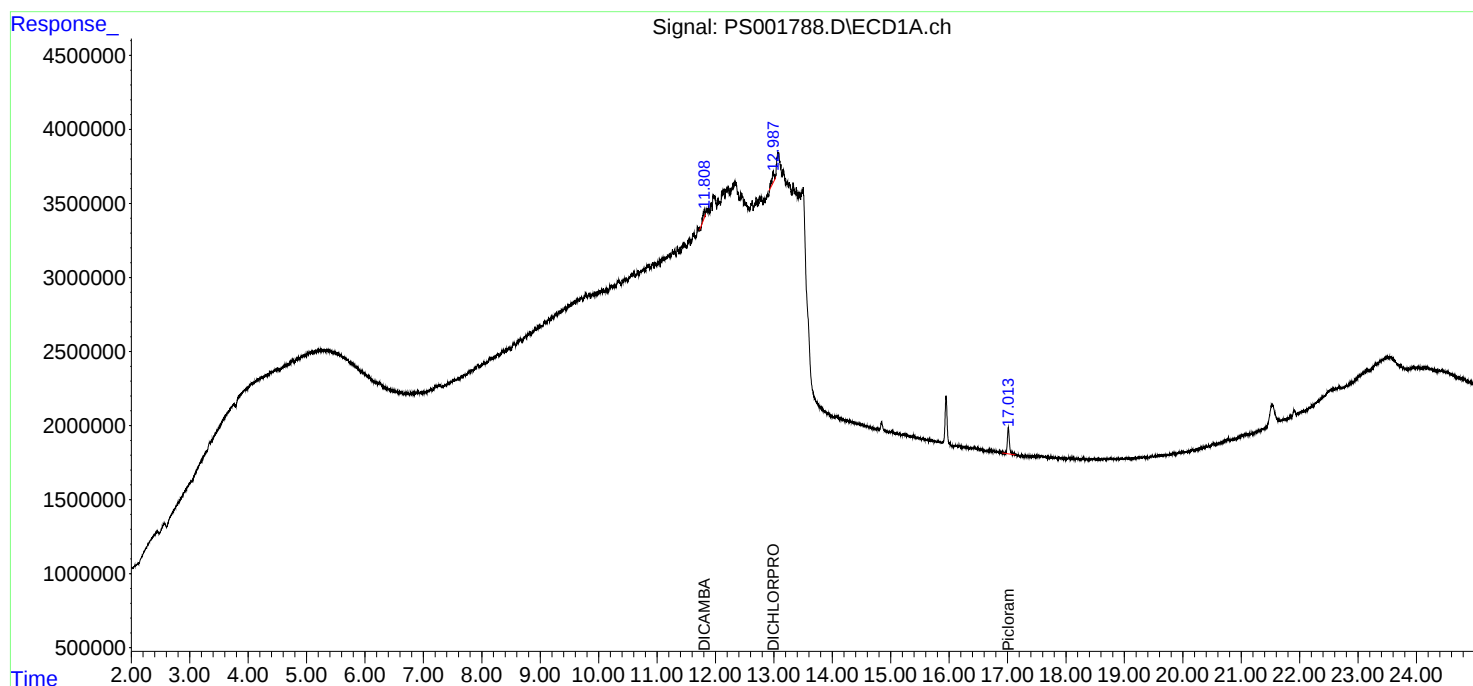


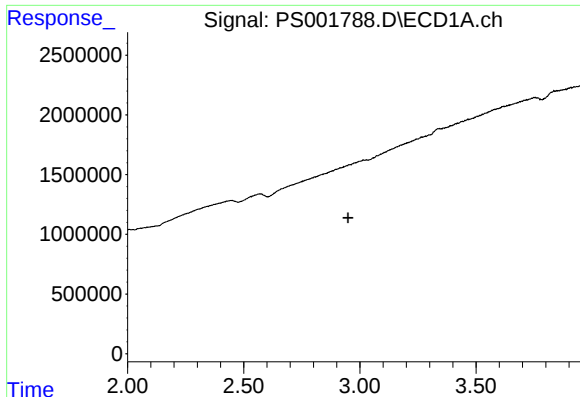

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

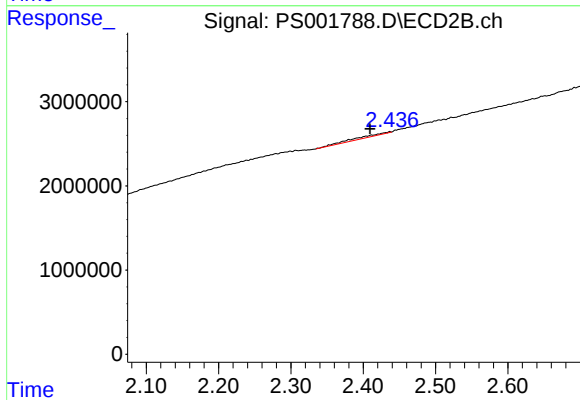


#1 Dalapon

R.T.: 2.437 min
Delta R.T.: 0.027 min
Response: 779272
Conc: 2.64 ng/ml

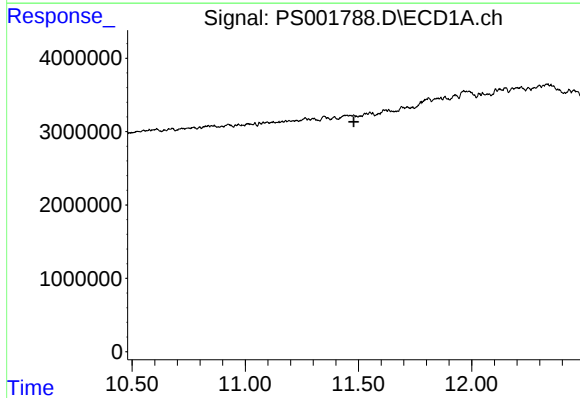


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.480 min
Response: 0
Conc: N.D.

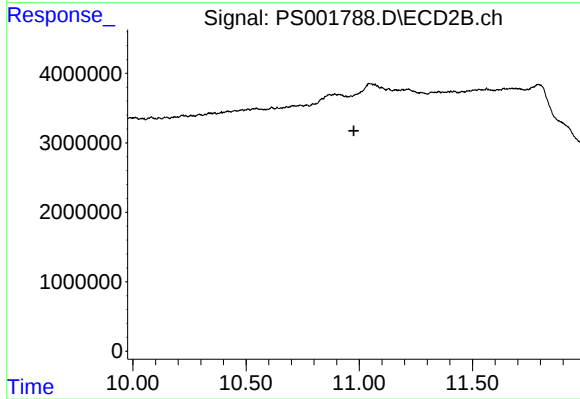

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.976 min
Response: 0
Conc: N.D.

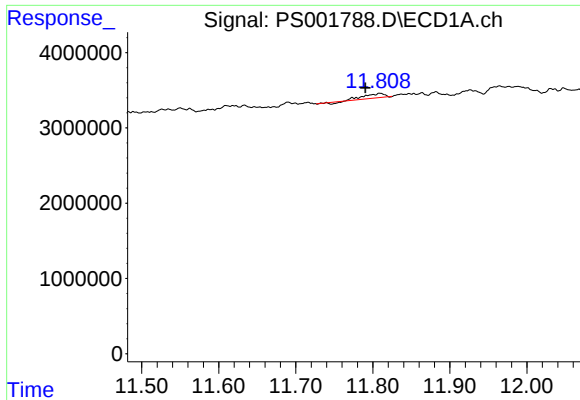

#5 DICAMBA


R.T.: 11.807 min
Delta R.T.: 0.017 min
Response: 950840
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

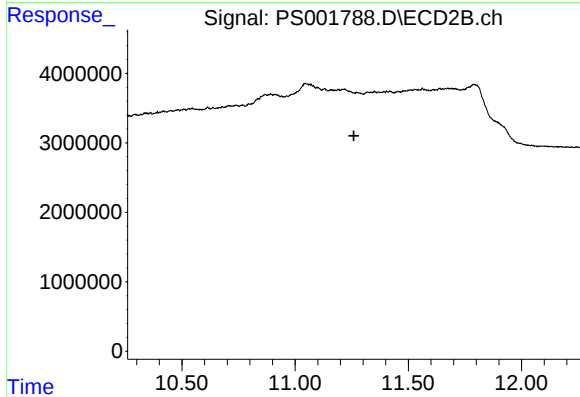


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.260 min
Response: 0
Conc: N.D.

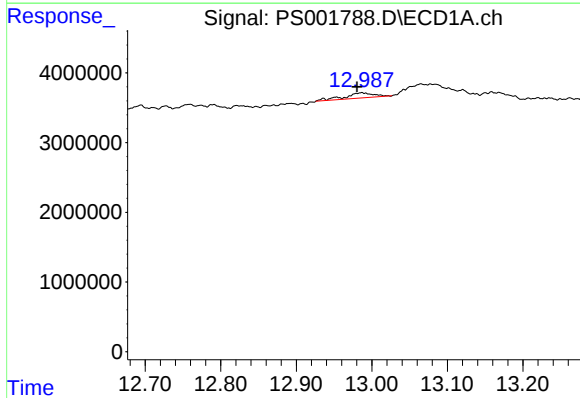


#8 DICHLORPROP

R.T.: 12.987 min
Delta R.T.: 0.007 min
Response: 1966488
Conc: 8.47 ng/ml

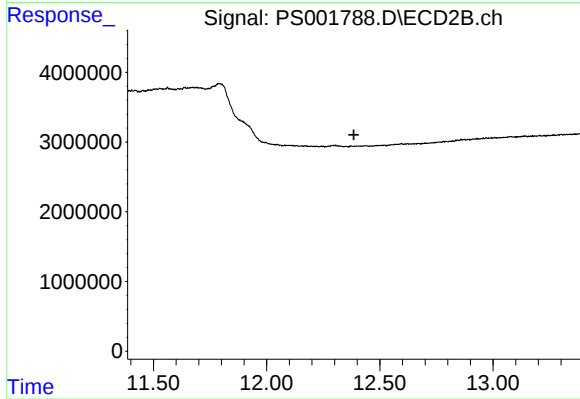

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.386 min
Response: 0
Conc: N.D.

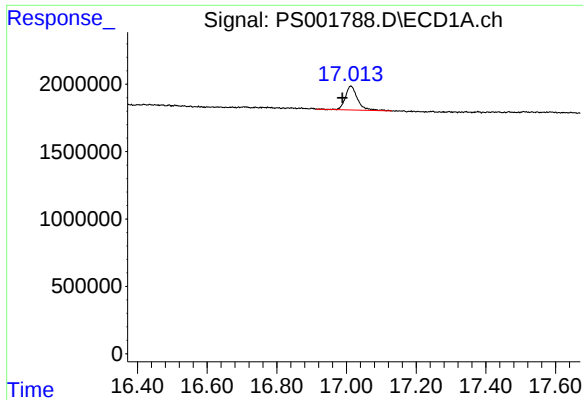

#15 Picloram


R.T.: 17.013 min
Delta R.T.: 0.024 min
Response: 4256681
Conc: 2.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

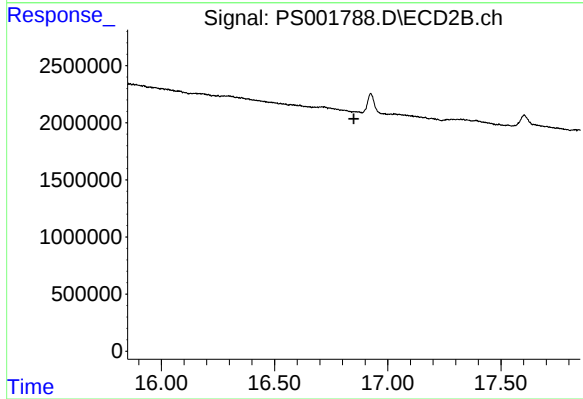


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.850 min
Response: 0
Conc: N.D.

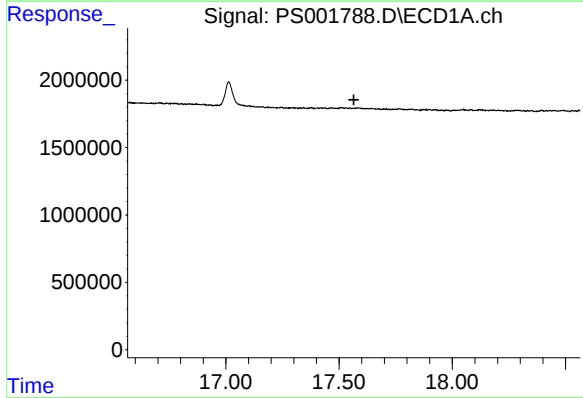

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

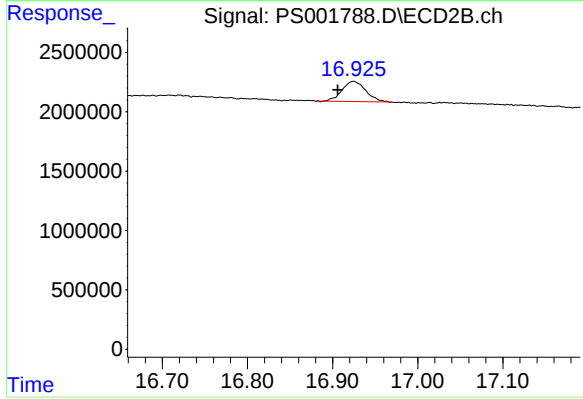

#16 DCPA

R.T.: 16.925 min
Delta R.T.: 0.019 min
Response: 3315031
Conc: 1.80 ng/ml