

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092018\  
 Data File : PS001794.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Sep 2018 18:16  
 Operator : EI\SJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 21 01:30:28 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS091718.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 18 03:01:16 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1   | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|--------|--------|---------|---------|---------|---------|
| -----                       |          |        |        |         |         |         |         |
| System Monitoring Compounds |          |        |        |         |         |         |         |
| 4) S                        | 2,4-DCAA | 11.474 | 10.973 | 112.1E6 | 110.0E6 | 499.841 | 433.140 |
| Target Compounds            |          |        |        |         |         |         |         |
| 15) T                       | Picloram | 16.992 | 16.905 | 3272001 | 3303623 | 1.879   | 1.942   |
| 16) T                       | DCPA     | 0.000  | 16.905 | 0       | 3303623 | N.D.    | 1.791 # |
| -----                       |          |        |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092018\  
Data File : PS001794.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Sep 2018 18:16  
Operator : EI\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 21 01:30:28 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS091718.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 18 03:01:16 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

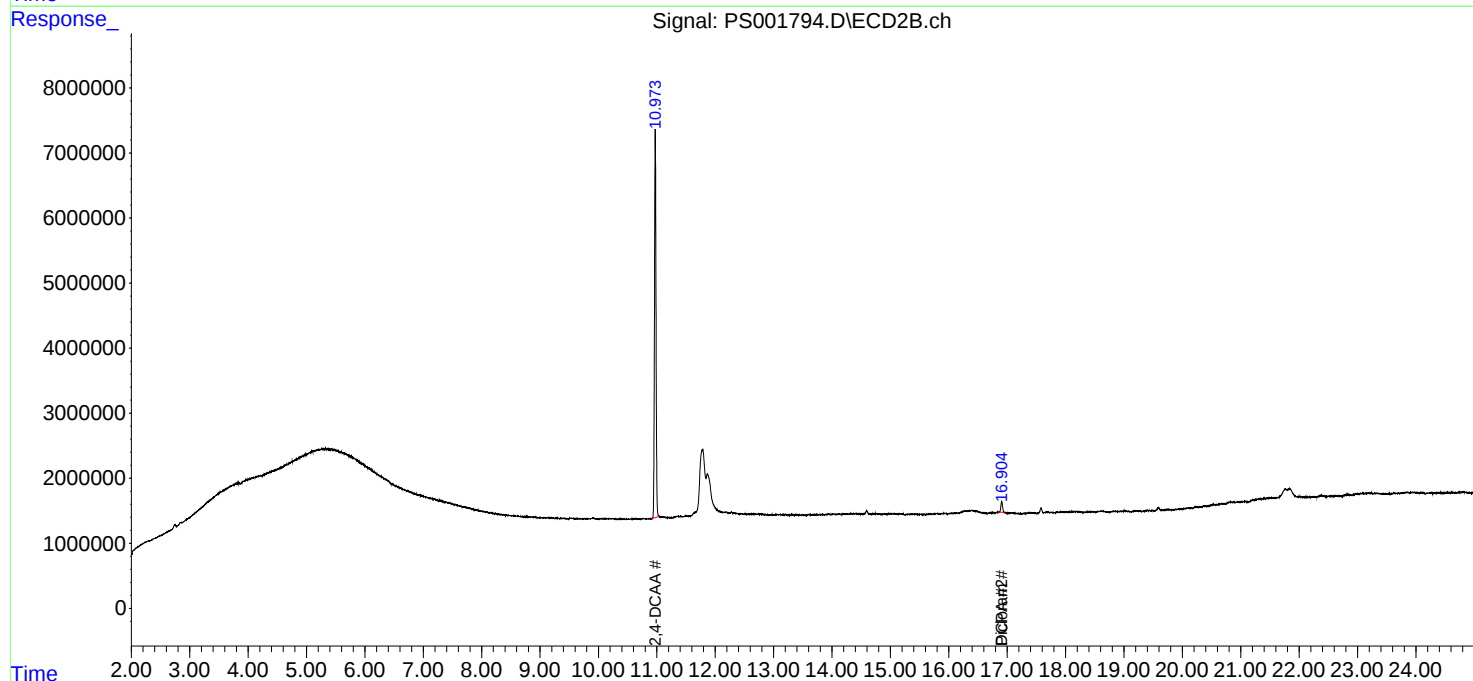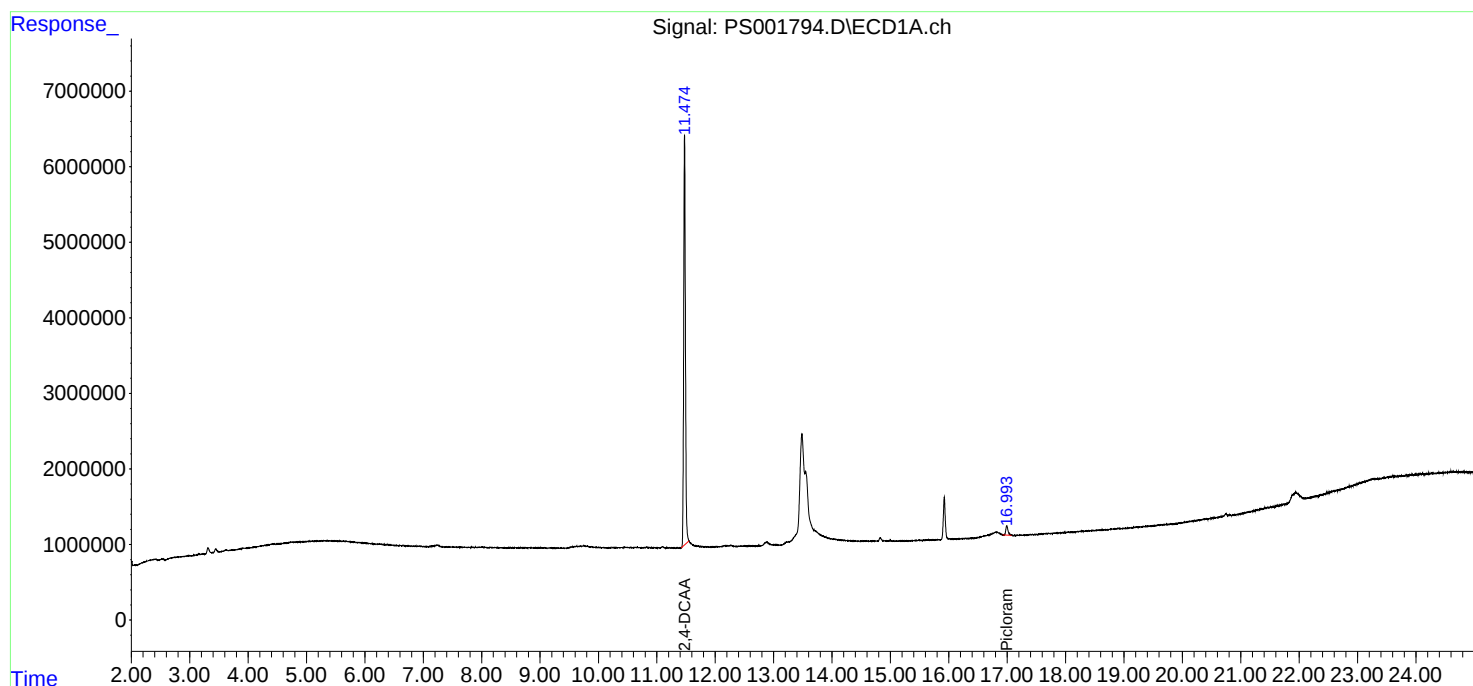


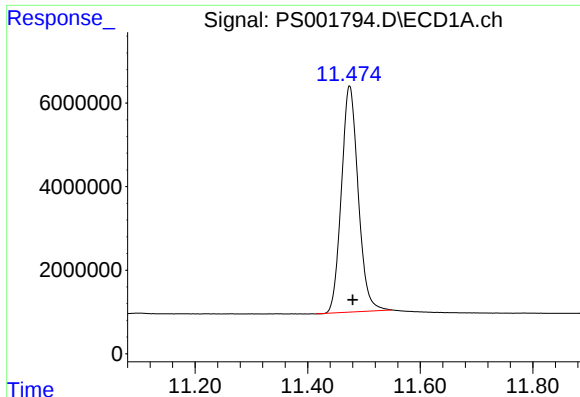

#4 2,4-DCAA


R.T.: 11.474 min  
Delta R.T.: -0.005 min  
Response: 112122218  
Conc: 499.84 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

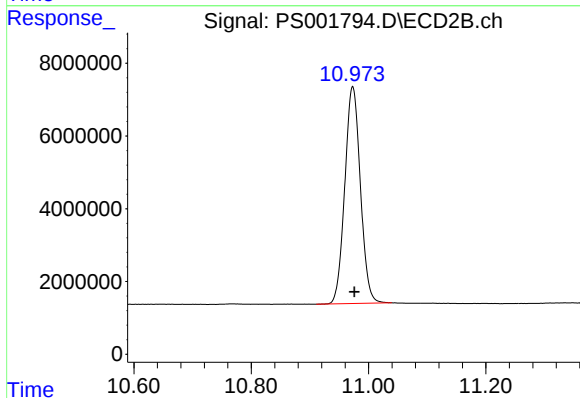


#4 2,4-DCAA

R.T.: 10.973 min  
Delta R.T.: -0.003 min  
Response: 110024807  
Conc: 433.14 ng/ml

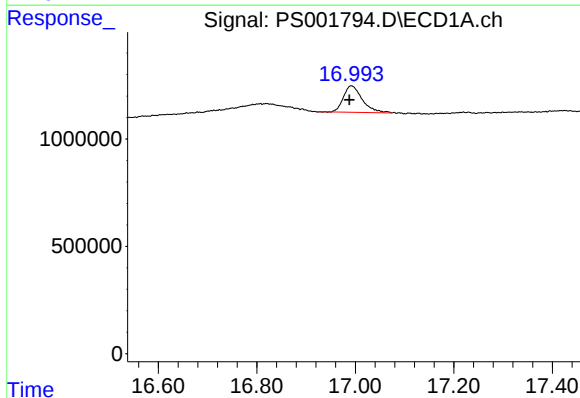


#15 Picloram

R.T.: 16.992 min  
Delta R.T.: 0.003 min  
Response: 3272001  
Conc: 1.88 ng/ml

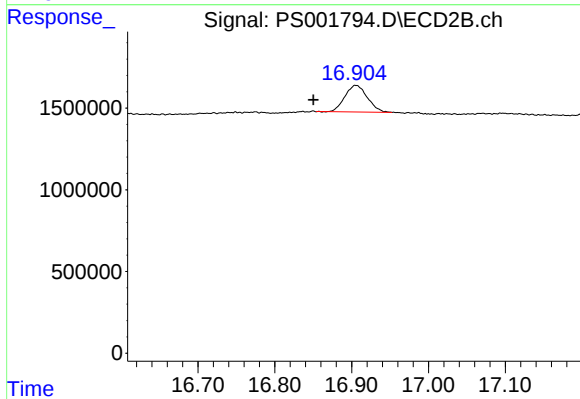

#15 Picloram


R.T.: 16.905 min  
Delta R.T.: 0.055 min  
Response: 3303623  
Conc: 1.94 ng/ml

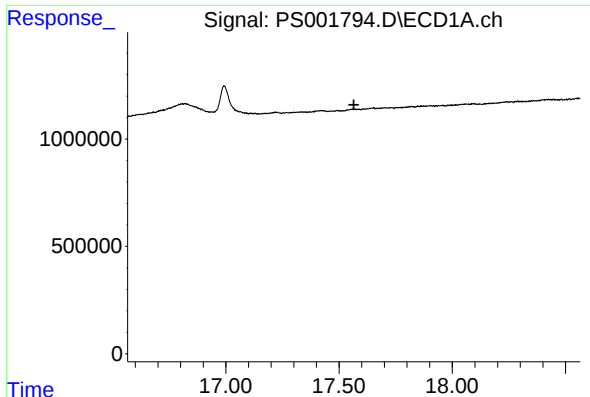

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.565 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

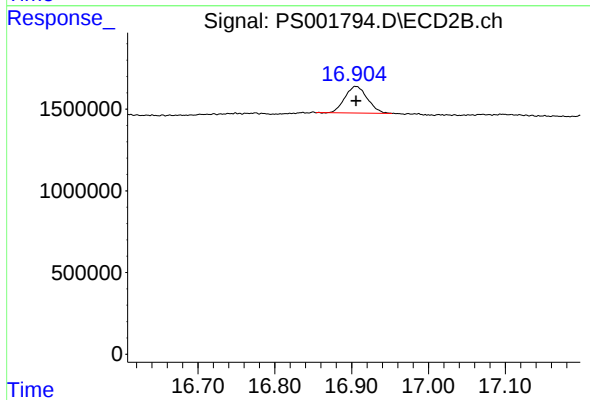

#16 DCPA

R.T.: 16.905 min  
Delta R.T.: 0.000 min  
Response: 3303623  
Conc: 1.79 ng/ml