

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092019\
 Data File : PS006863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2019 19:46
 Operator : SM\AJ
 Sample : K4662-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 23:55:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.483	5.214	367.5E6	213.6E6	402.146	464.559
Target Compounds							
1) T	Dalapon	2.118	1.744	46823217	35017146	43.825	65.690 #
2) T	3,5-DICHL...	4.917	4.542	14762576	39027971	13.572	67.891 #
3) T	4-Nitroph...	5.379	0.000	4897131	0	12.843	N.D. #
5) T	DICAMBA	5.695	0.000	9304242	0	2.880	N.D. #
9) T	2,4-D	6.548	0.000	72119111	0	88.002	N.D. #
10) T	Pentachlo...	6.740	6.519	39699169	25022781	3.331	3.977
15) T	Picloram	8.987	0.000	14545775	0	2.169	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092019\
Data File : PS006863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2019 19:46
Operator : SM\AJ
Sample : K4662-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 23:55:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

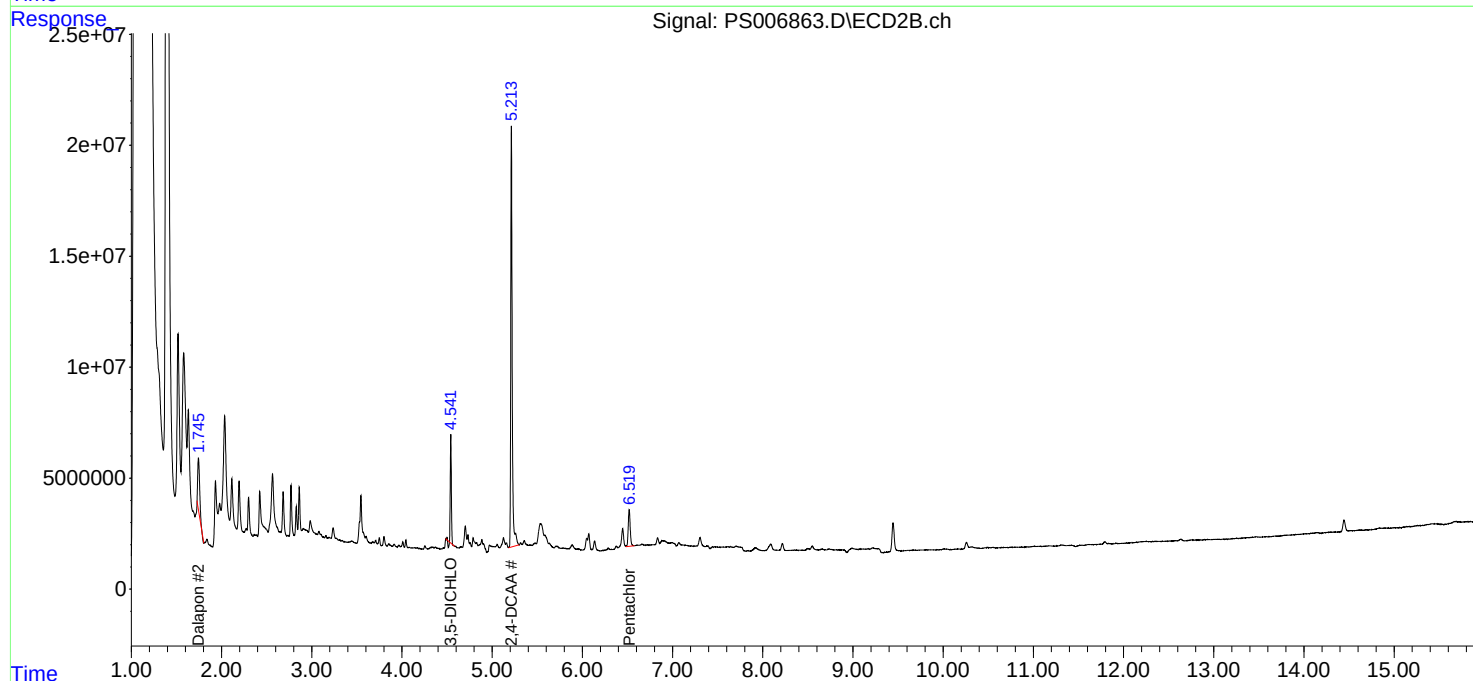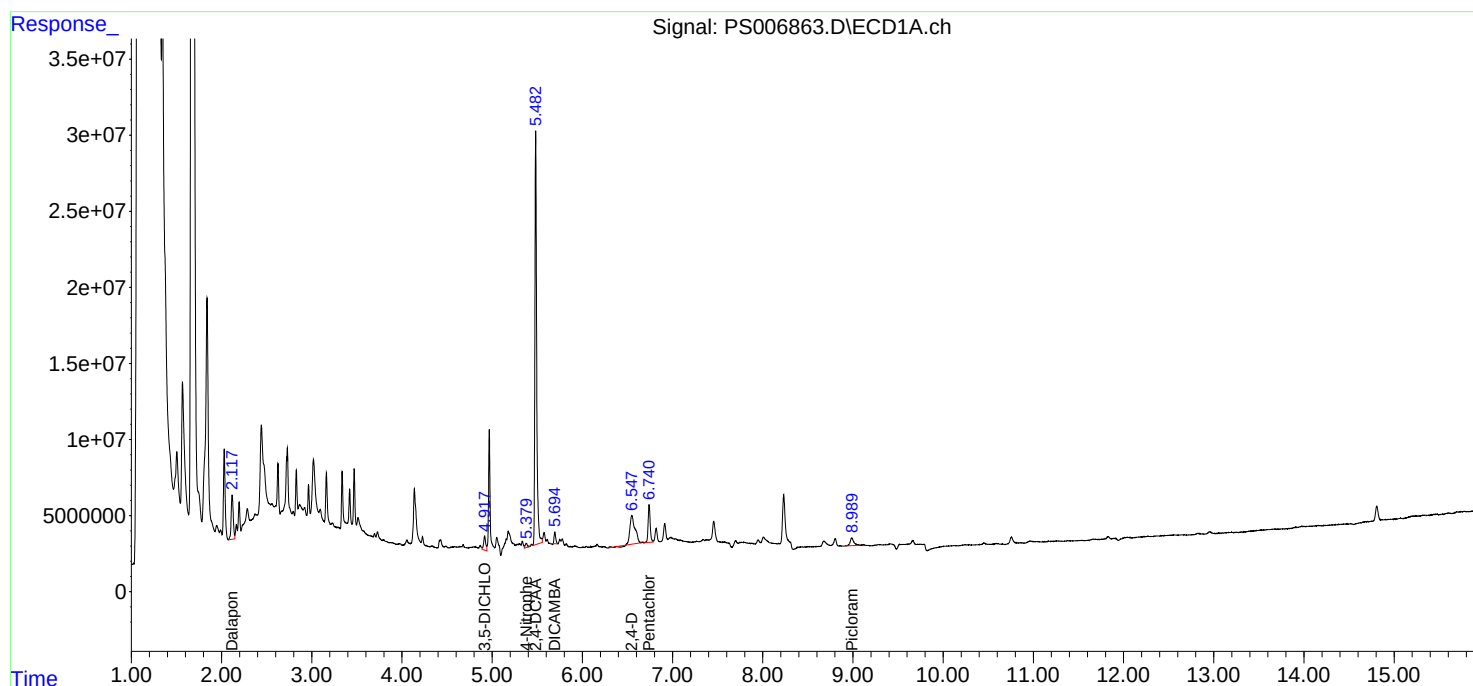


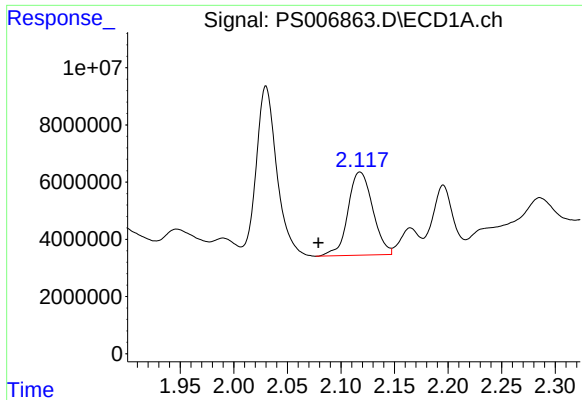

#1 Dalapon


R.T.: 2.118 min
Delta R.T.: 0.039 min
Response: 46823217
Conc: 43.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

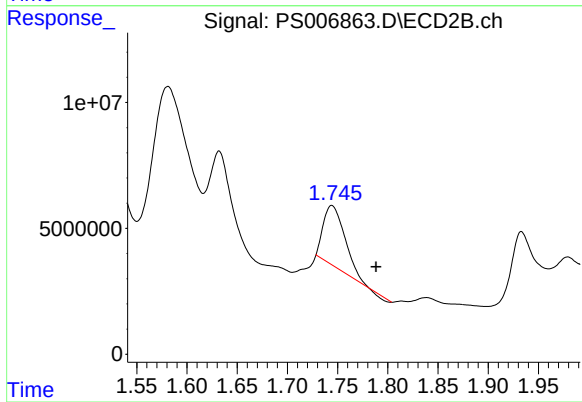


#1 Dalapon

R.T.: 1.744 min
Delta R.T.: -0.044 min
Response: 35017146
Conc: 65.69 ng/ml

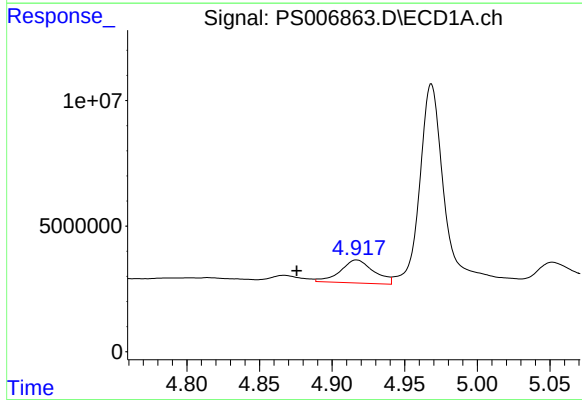


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.917 min
Delta R.T.: 0.041 min
Response: 14762576
Conc: 13.57 ng/ml

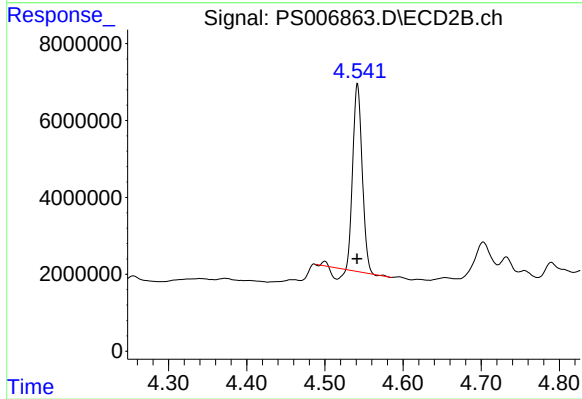

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.542 min
Delta R.T.: 0.000 min
Response: 39027971
Conc: 67.89 ng/ml

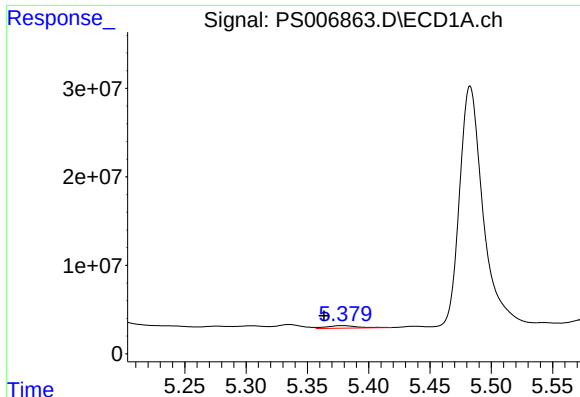

#3 4-Nitrophenol


R.T.: 5.379 min
Delta R.T.: 0.015 min
Response: 4897131
Conc: 12.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

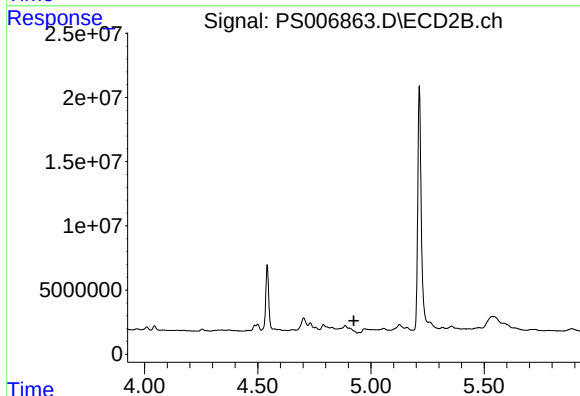


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

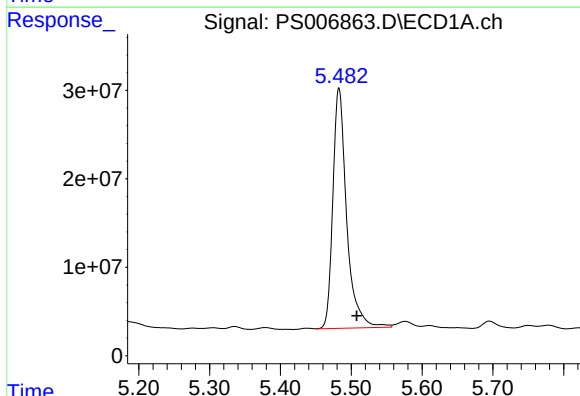


#4 2,4-DCAA

R.T.: 5.483 min
Delta R.T.: -0.025 min
Response: 367486546
Conc: 402.15 ng/ml

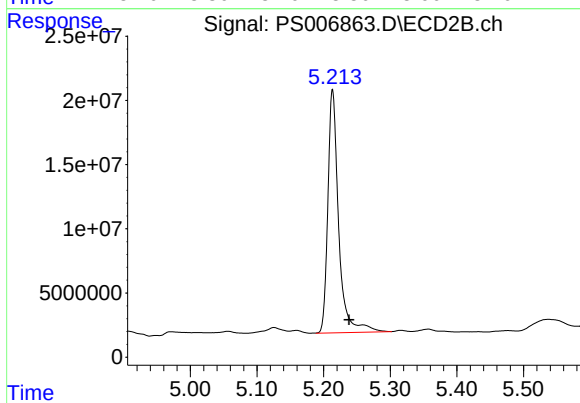

#4 2,4-DCAA


R.T.: 5.214 min
Delta R.T.: -0.024 min
Response: 213623599
Conc: 464.56 ng/ml

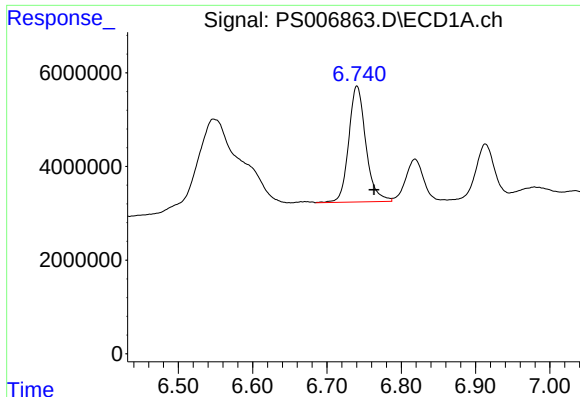

#10 Pentachlorophenol


R.T.: 6.740 min
Delta R.T.: -0.023 min
Response: 39699169
Conc: 3.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

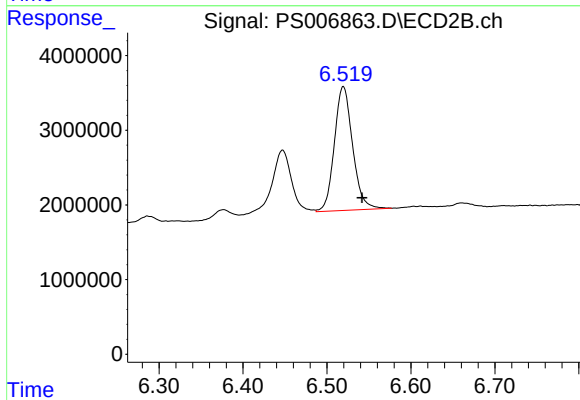


#10 Pentachlorophenol

R.T.: 6.519 min
Delta R.T.: -0.022 min
Response: 25022781
Conc: 3.98 ng/ml

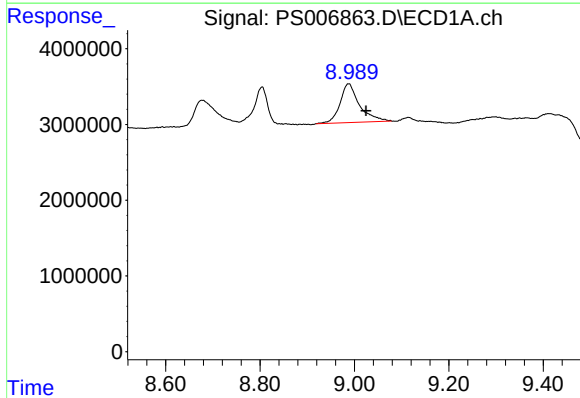

#15 Picloram

R.T.: 8.987 min
Delta R.T.: -0.037 min
Response: 14545775
Conc: 2.17 ng/ml

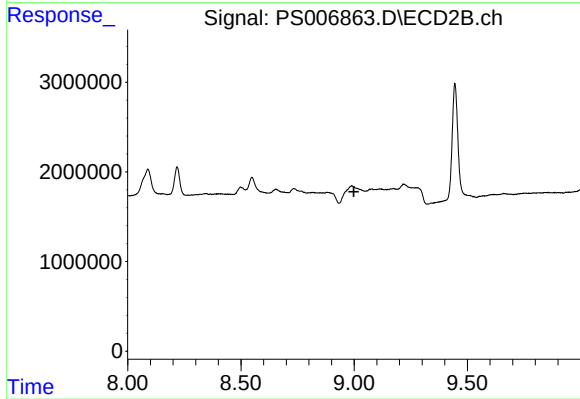

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.999 min
Response: 0
Conc: N.D.