

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092021\
 Data File : PS016842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 18:27
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:37:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:35:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.170	6.759	1159.9E6	449.3E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.999	2.502	1664.9E6	504.6E6	682.500	682.500
2) T	3,5-DICHL...	6.391	5.951	1509.1E6	635.3E6	697.500	697.500
3) T	4-Nitroph...	6.999	6.381	603.5E6	219.1E6	682.500	682.500
5) T	DICAMBA	7.360	6.921	4216.4E6	1859.9E6	705.000	705.000
6) T	MCPD	7.529	7.018	319.6E6	149.8E6	70.500	70.500
7) T	MCPA	7.678	7.229	443.0E6	214.9E6	69.750	69.750
8) T	DICHLORPROP	8.050	7.539	1055.2E6	468.7E6	705.000	705.000
9) T	2,4-D	8.278	7.829	1260.7E6	551.7E6	705.000	705.000
10) T	Pentachlo...	8.585	8.255	14668.8E6	6000.6E6	712.500	712.500
11) T	2,4,5-TP ...	9.134	8.614	5824.3E6	2575.0E6	712.500	712.500
12) T	2,4,5-T	9.418	8.991	6014.3E6	2413.6E6	712.500	712.500
13) T	2,4-DB	9.968	9.496	1215.9E6	303.9E6	712.500	712.500
14) T	DINOSEB	11.121	9.822	4372.5E6	1791.7E6	705.000	705.000
15) T	Picloram	10.943	10.801	8788.7E6	3201.6E6	712.500	712.500
16) T	DCPA	11.389	10.752	7526.2E6	3233.2E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092021\
Data File : PS016842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 18:27
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:37:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:35:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

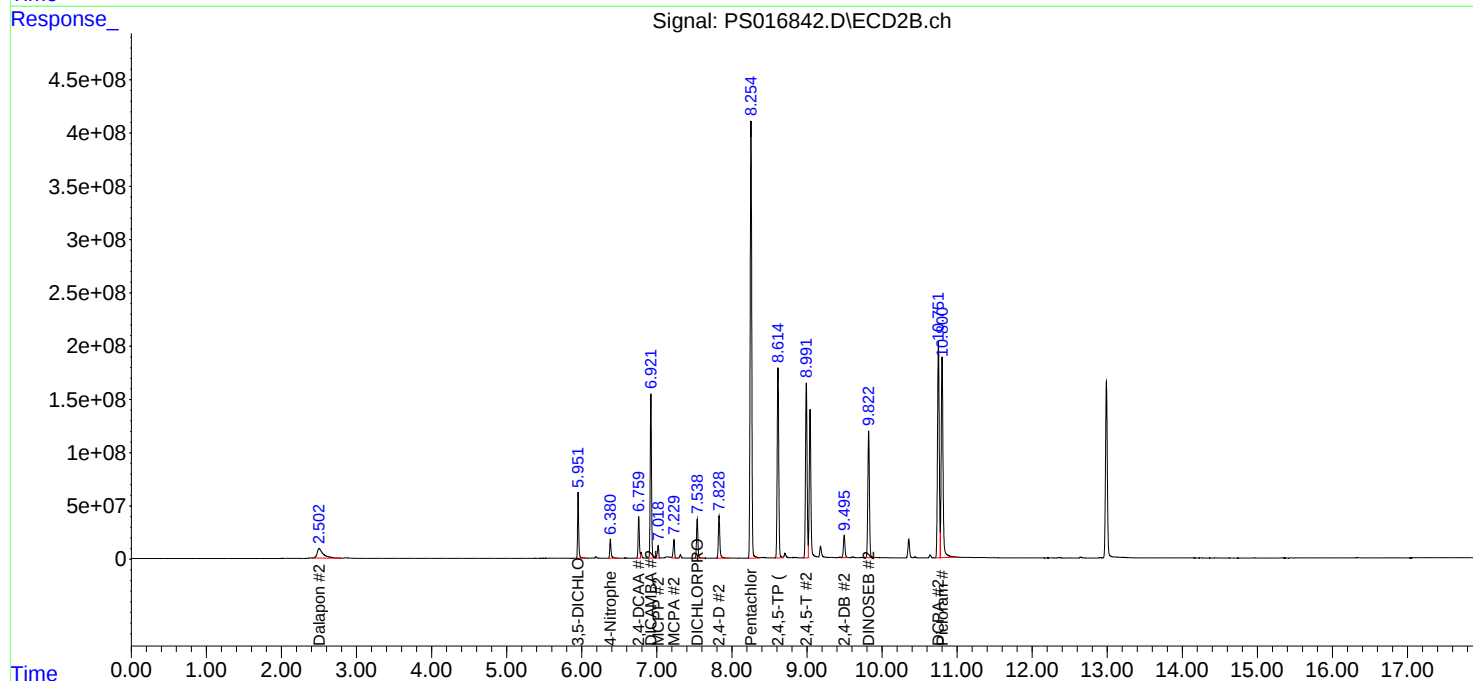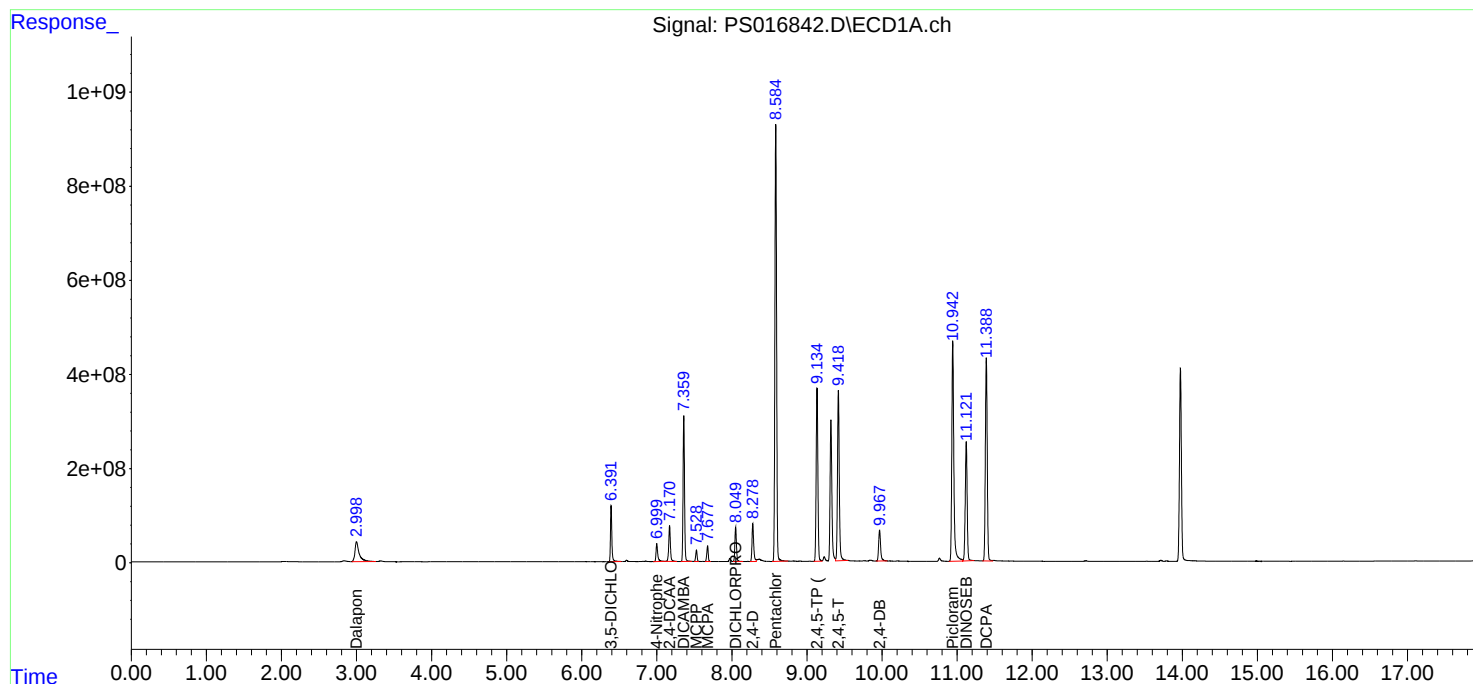


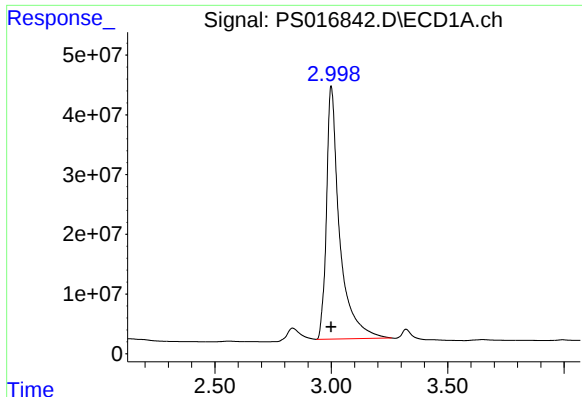

#1 Dalapon


R.T.: 2.999 min
Delta R.T.: 0.000 min
Response: 1664904857
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

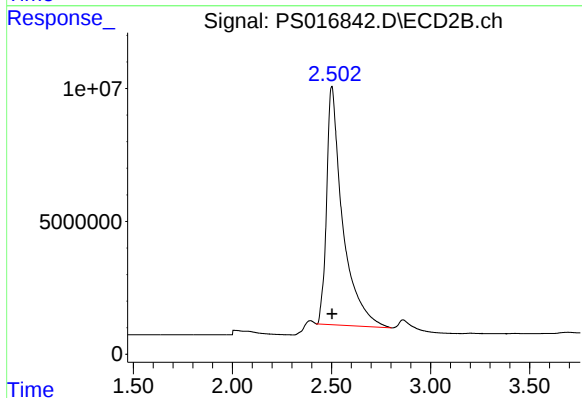


#1 Dalapon

R.T.: 2.502 min
Delta R.T.: 0.000 min
Response: 504647399
Conc: 682.50 ng/ml

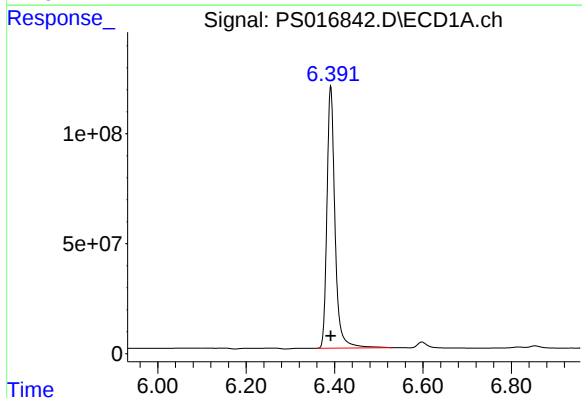


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.391 min
Delta R.T.: 0.000 min
Response: 1509125914
Conc: 697.50 ng/ml

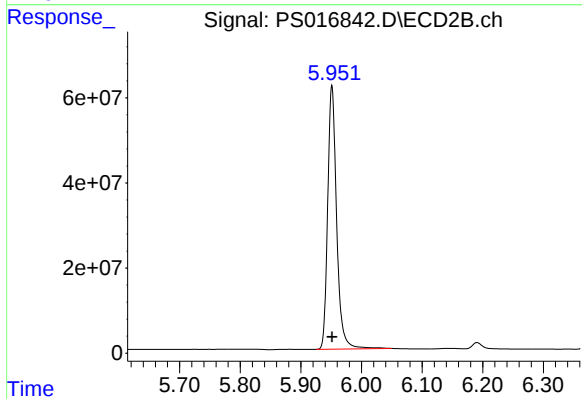

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 635332372
Conc: 697.50 ng/ml

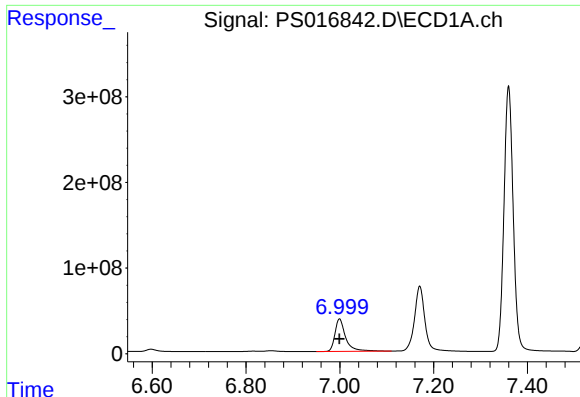

#3 4-Nitrophenol


R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 603540984
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

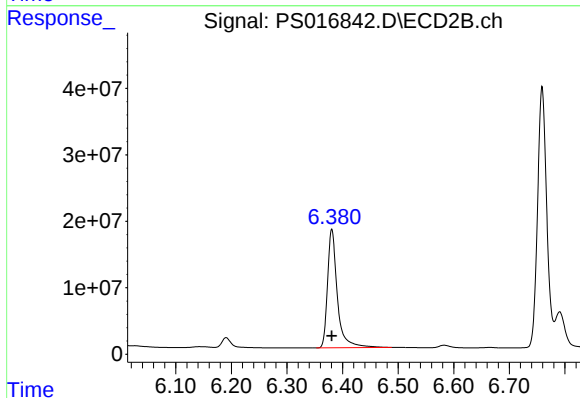


#3 4-Nitrophenol

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 219145946
Conc: 682.50 ng/ml

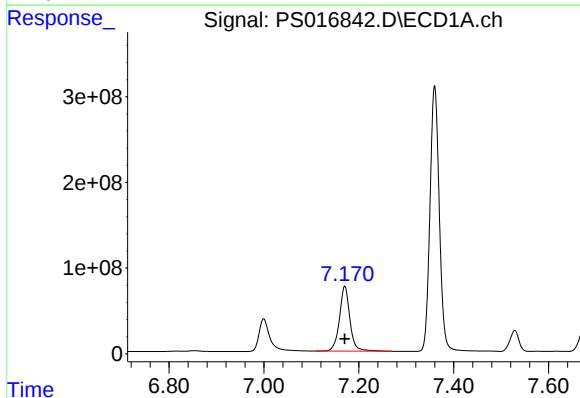


#4 2,4-DCAA

R.T.: 7.170 min
Delta R.T.: 0.000 min
Response: 1159886613
Conc: 750.00 ng/ml

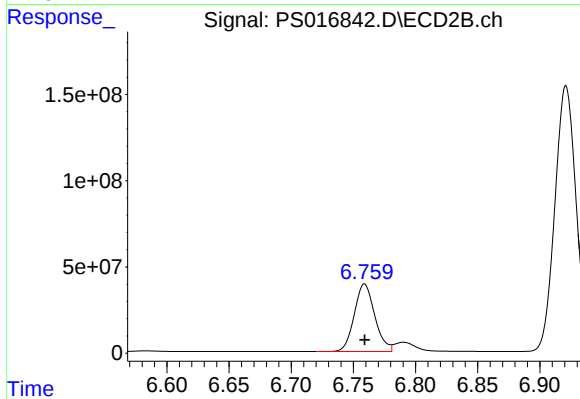

#4 2,4-DCAA


R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 449300730
Conc: 750.00 ng/ml

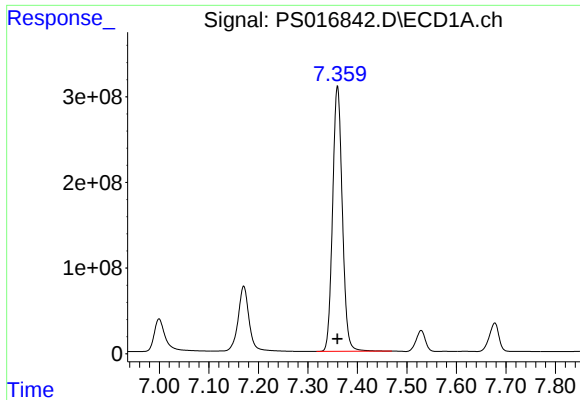

#5 DICAMBA


R.T.: 7.360 min
Delta R.T.: 0.000 min
Response: 4216411648
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

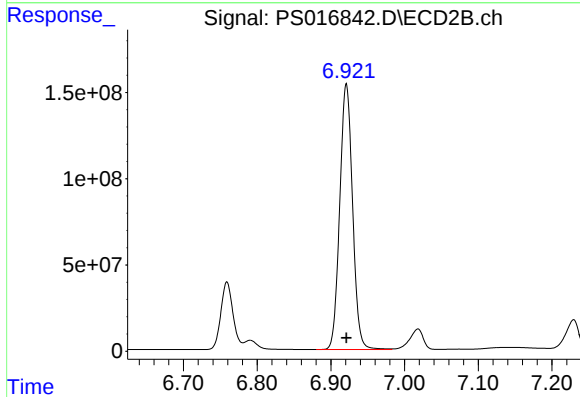


#5 DICAMBA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 1859945811
Conc: 705.00 ng/ml

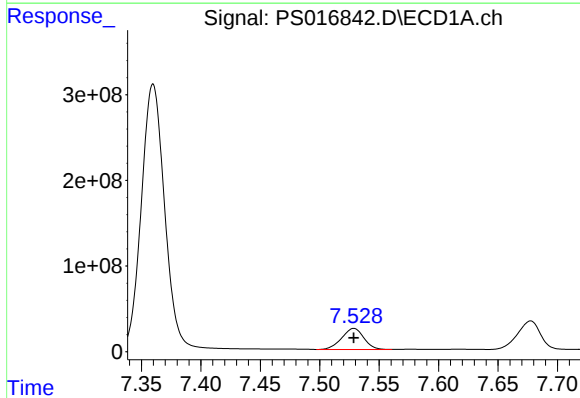


#6 MCP

R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 319620234
Conc: 70.50 ug/ml

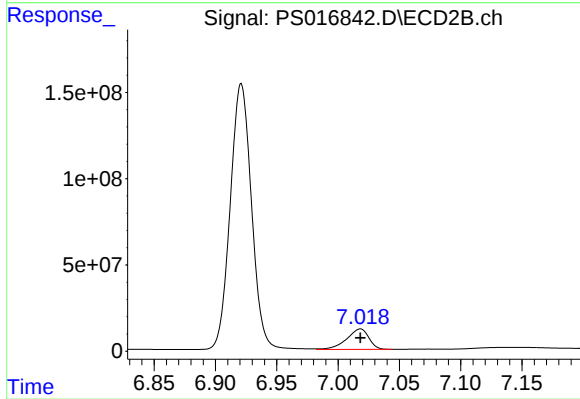

#6 MCP


R.T.: 7.018 min
Delta R.T.: 0.000 min
Response: 149762069
Conc: 70.50 ug/ml

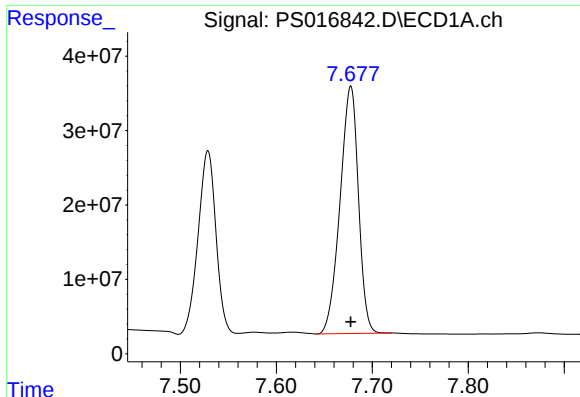

#7 MCPA


R.T.: 7.678 min
Delta R.T.: 0.000 min
Response: 443040295
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

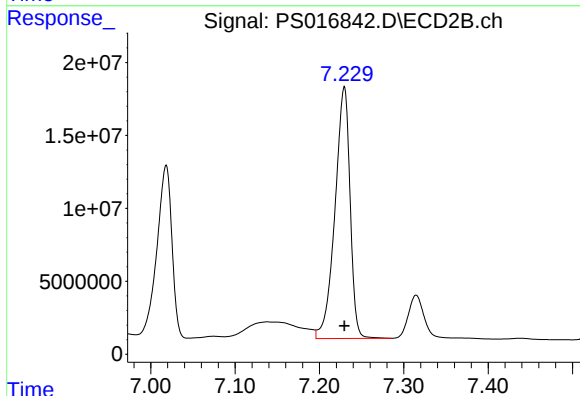


#7 MCPA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 214947453
Conc: 69.75 ug/ml

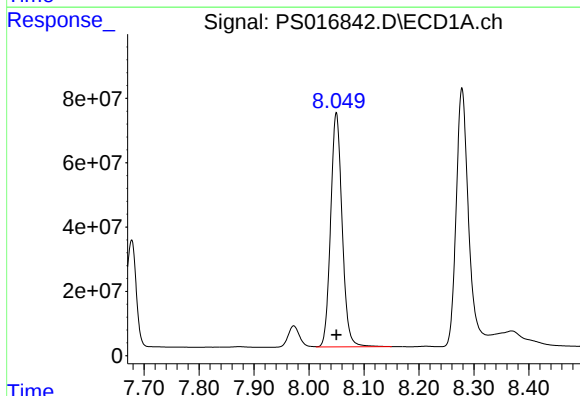


#8 DICHLORPROP

R.T.: 8.050 min
Delta R.T.: 0.000 min
Response: 1055248813
Conc: 705.00 ng/ml

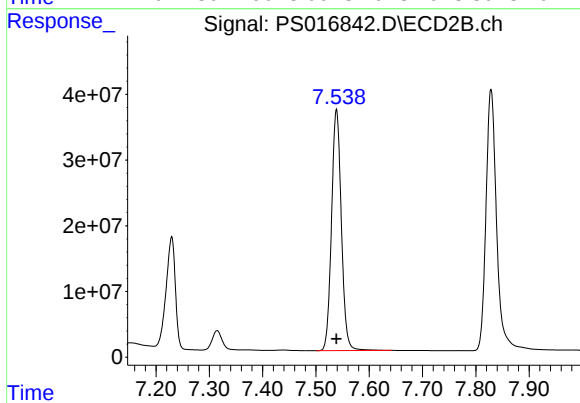

#8 DICHLORPROP


R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 468735546
Conc: 705.00 ng/ml

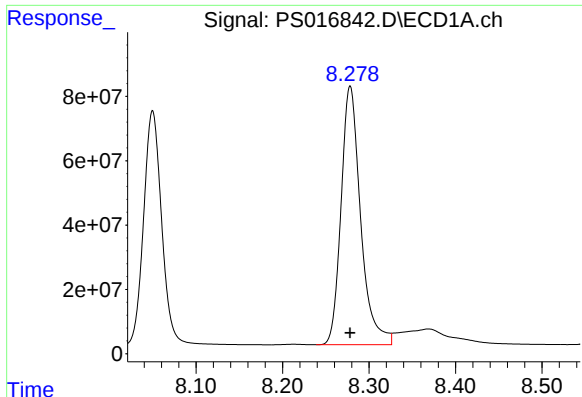

#9 2,4-D


R.T.: 8.278 min
Delta R.T.: 0.000 min
Response: 1260729615
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

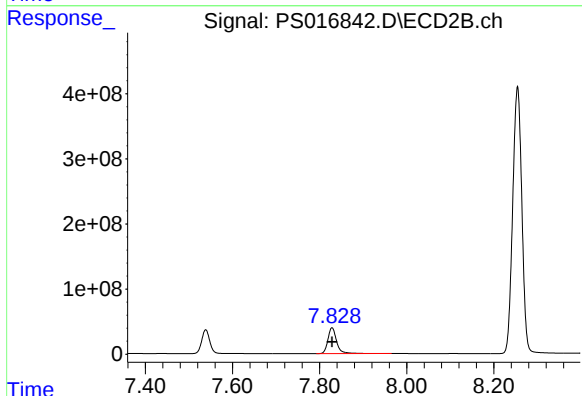


#9 2,4-D

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 551665091
Conc: 705.00 ng/ml

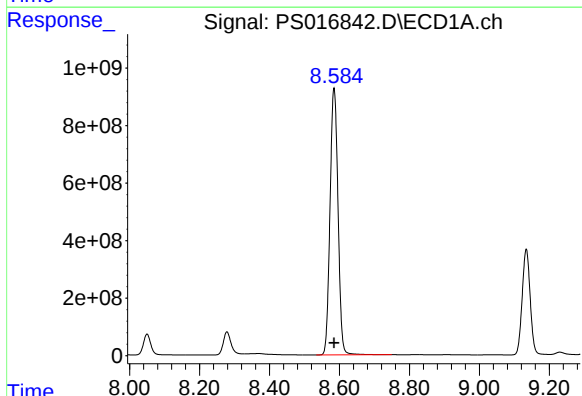


#10 Pentachlorophenol

R.T.: 8.585 min
Delta R.T.: 0.000 min
Response: 14668768086
Conc: 712.50 ng/ml

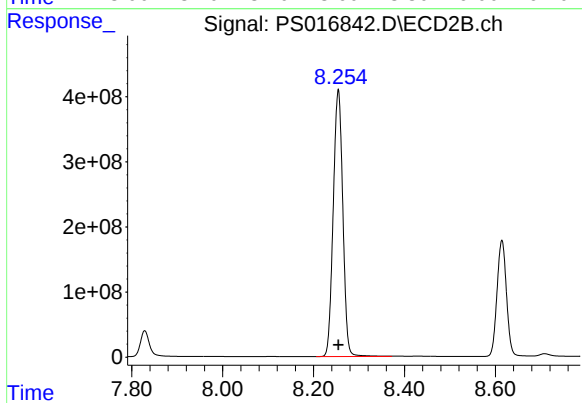

#10 Pentachlorophenol


R.T.: 8.255 min
Delta R.T.: 0.000 min
Response: 6000627849
Conc: 712.50 ng/ml

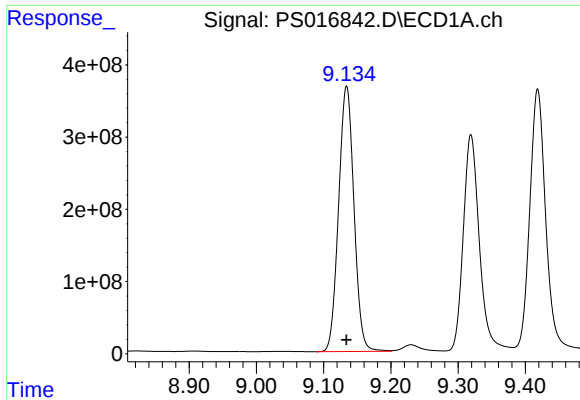

#11 2,4,5-TP (SILVEX)


R.T.: 9.134 min
Delta R.T.: 0.000 min
Response: 5824303302
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

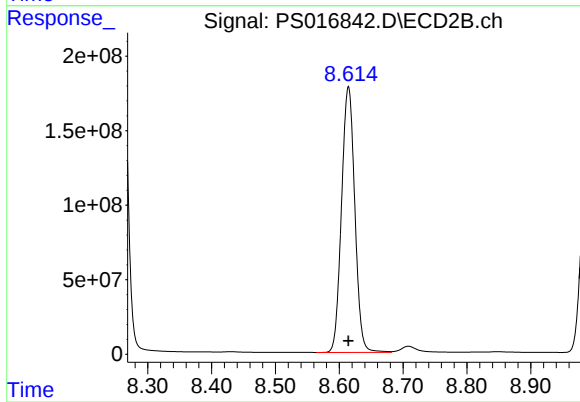


#11 2,4,5-TP (SILVEX)

R.T.: 8.614 min
Delta R.T.: 0.000 min
Response: 2575025851
Conc: 712.50 ng/ml

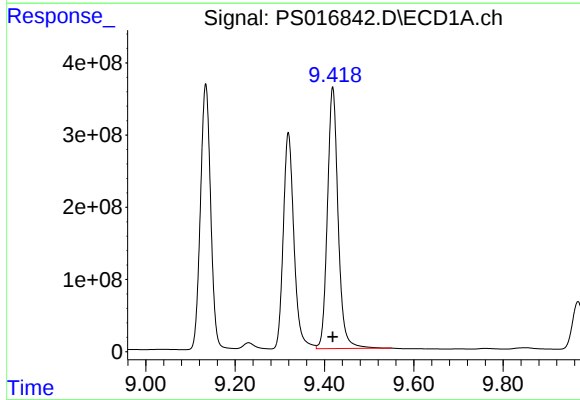


#12 2,4,5-T

R.T.: 9.418 min
Delta R.T.: 0.000 min
Response: 6014291795
Conc: 712.50 ng/ml

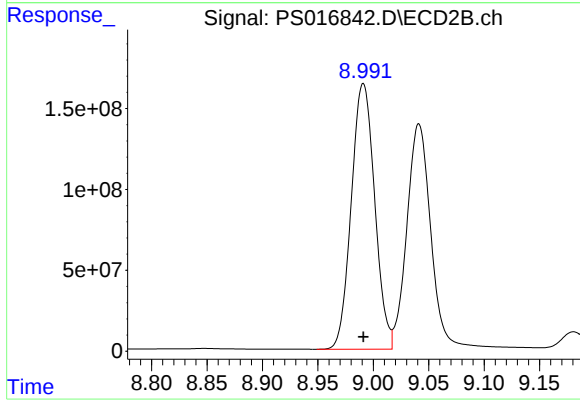

#12 2,4,5-T


R.T.: 8.991 min
Delta R.T.: 0.000 min
Response: 2413617530
Conc: 712.50 ng/ml

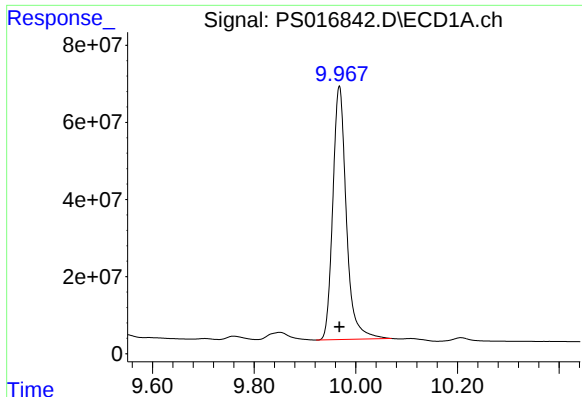

#13 2,4-DB


R.T.: 9.968 min
Delta R.T.: 0.000 min
Response: 1215892544
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

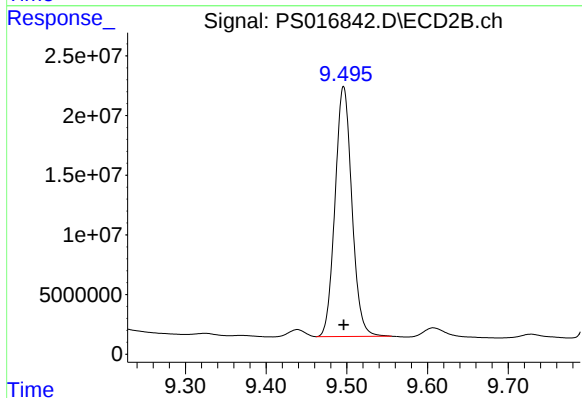


#13 2,4-DB

R.T.: 9.496 min
Delta R.T.: 0.000 min
Response: 303908123
Conc: 712.50 ng/ml

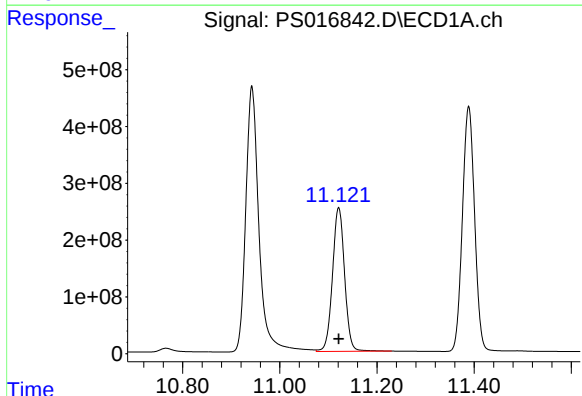


#14 DINOSEB

R.T.: 11.121 min
Delta R.T.: 0.000 min
Response: 4372451198
Conc: 705.00 ng/ml

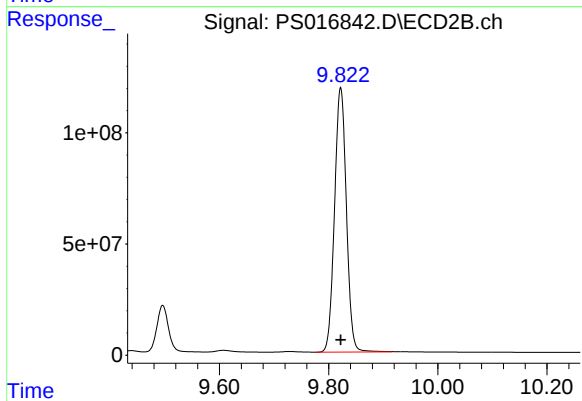

#14 DINOSEB


R.T.: 9.822 min
Delta R.T.: 0.000 min
Response: 1791691087
Conc: 705.00 ng/ml

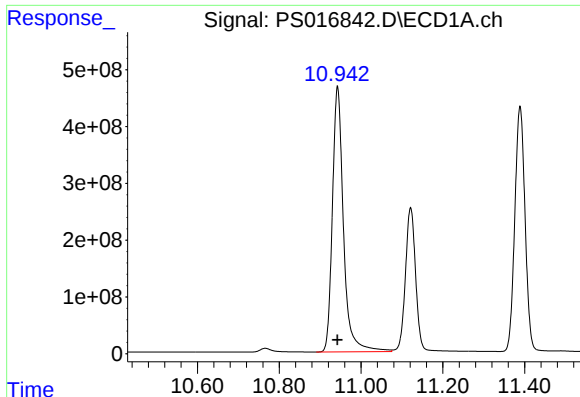

#15 Picloram


R.T.: 10.943 min
Delta R.T.: 0.000 min
Response: 8788678427
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

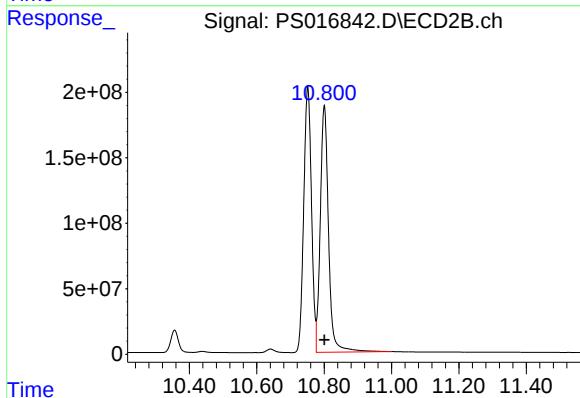


#15 Picloram

R.T.: 10.801 min
Delta R.T.: 0.000 min
Response: 3201582615
Conc: 712.50 ng/ml

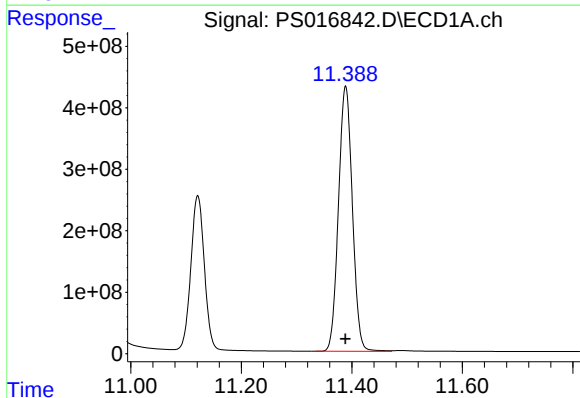

#16 DCPA

R.T.: 11.389 min
Delta R.T.: 0.000 min
Response: 7526237948
Conc: 720.00 ng/ml

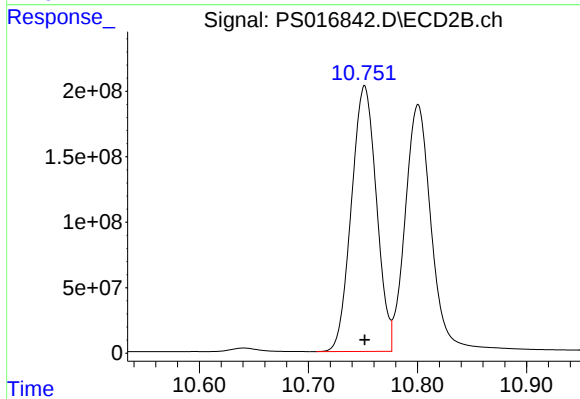

#16 DCPA

R.T.: 10.752 min
Delta R.T.: 0.000 min
Response: 3233168058
Conc: 720.00 ng/ml