

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092021\  
 Data File : PS016846.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Sep 2021 20:27  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 21 02:13:17 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS092021.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 21 01:52:13 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1    | RT#2    | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|----------|---------|---------|----------|----------|---------|---------|
| -----                       |          |         |         |          |          |         |         |
| System Monitoring Compounds |          |         |         |          |          |         |         |
| 4) S                        | 2,4-DCAA | 7.171   | 6.758   | 614.7E6  | 266.6E6  | 403.478 | 454.726 |
| Target Compounds            |          |         |         |          |          |         |         |
| 12) T                       | 2,4,5-T  | 9.369f  | 0.000   | 8656434  | 0        | 1.049   | N.D. #  |
| 15) T                       | Picloram | 10.988f | 10.819  | 41285498 | 15534646 | 3.469   | 3.621   |
| 16) T                       | DCPA     | 0.000   | 10.819f | 0        | 15534646 | N.D.    | 3.564   |
| -----                       |          |         |         |          |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092021\  
Data File : PS016846.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Sep 2021 20:27  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 21 02:13:17 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS092021.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 21 01:52:13 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

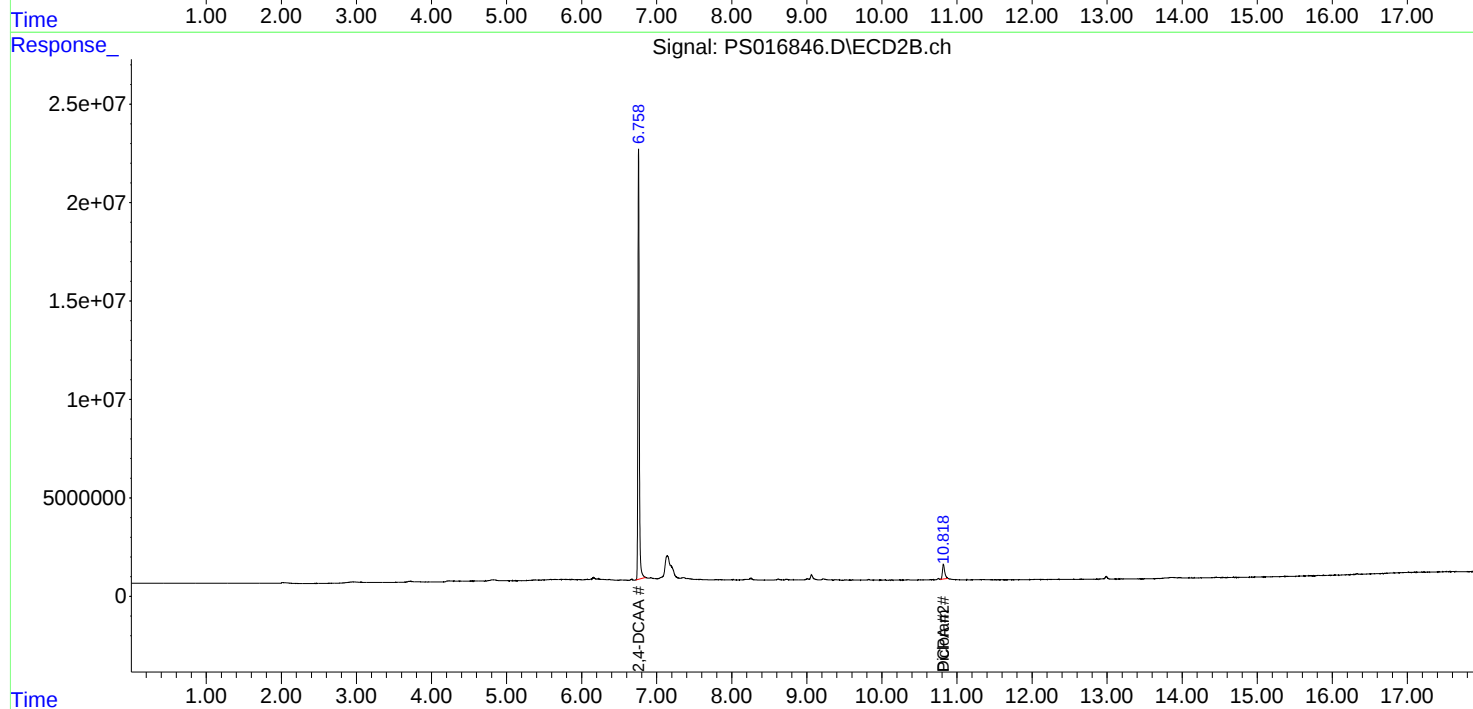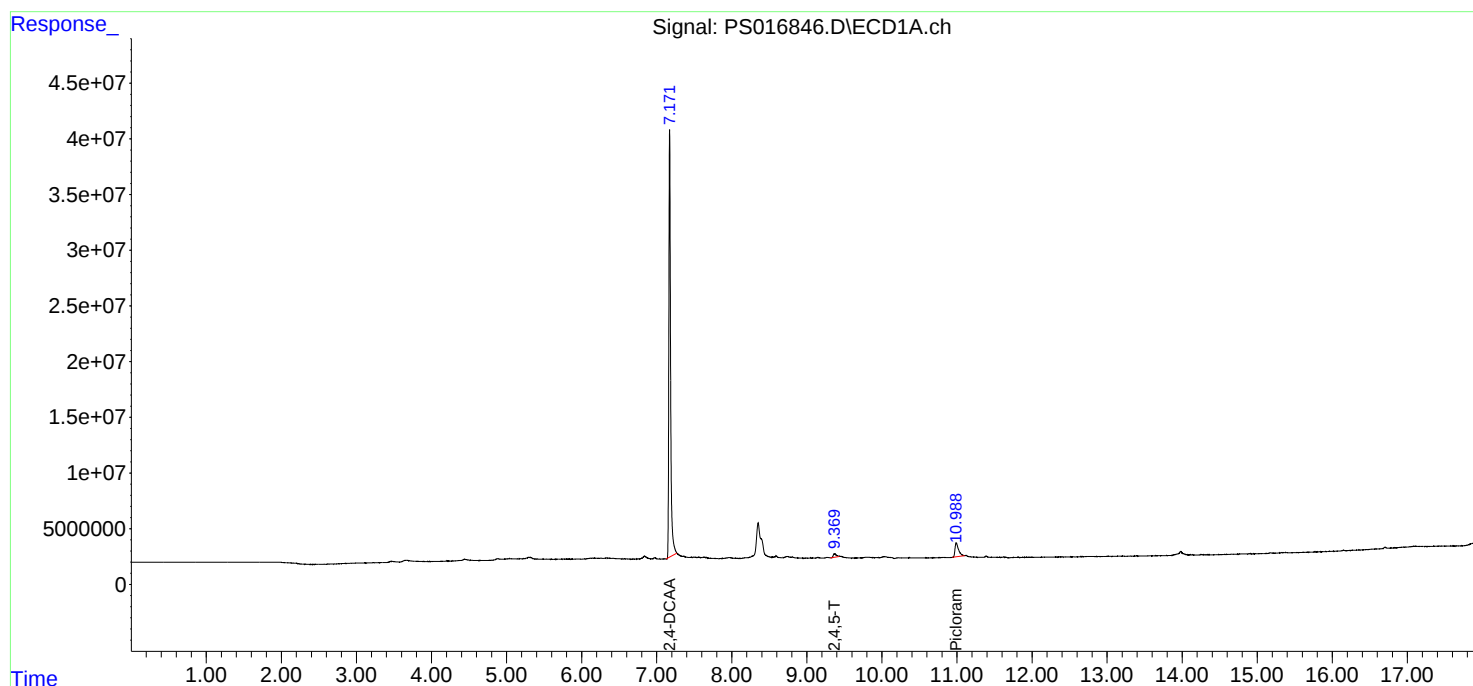


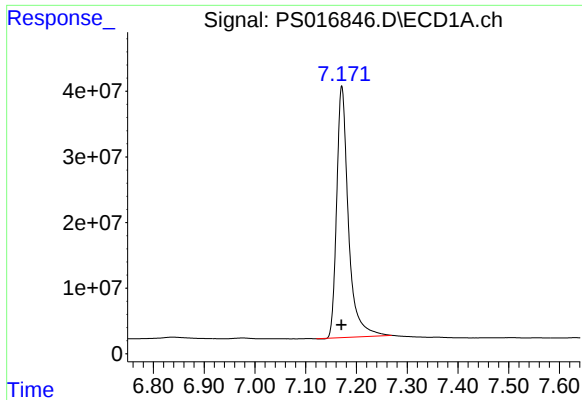

#4 2,4-DCAA


R.T.: 7.171 min  
Delta R.T.: 0.000 min  
Response: 614718073  
Conc: 403.48 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

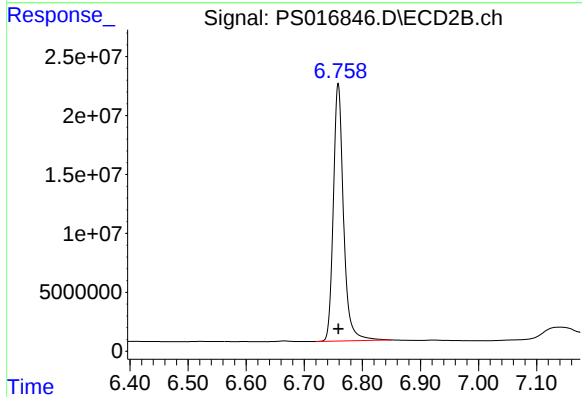


#4 2,4-DCAA

R.T.: 6.758 min  
Delta R.T.: 0.000 min  
Response: 266634516  
Conc: 454.73 ng/ml

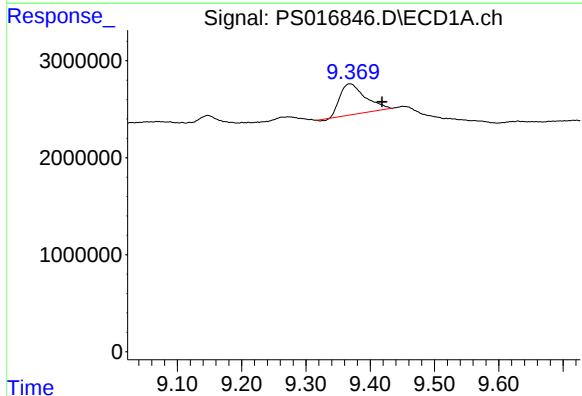


#12 2,4,5-T

R.T.: 9.369 min  
Delta R.T.: -0.049 min  
Response: 8656434  
Conc: 1.05 ng/ml

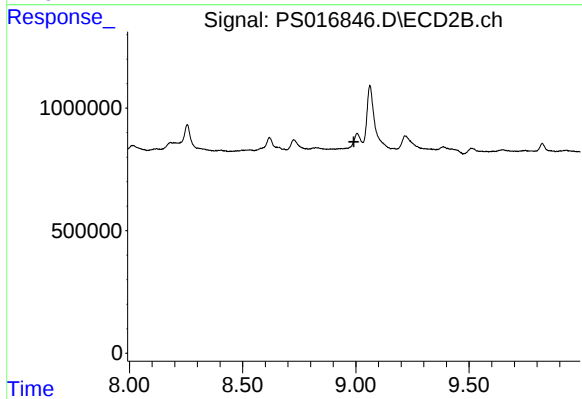

#12 2,4,5-T


R.T.: 0.000 min  
Exp R.T.: 8.991 min  
Response: 0  
Conc: N.D.

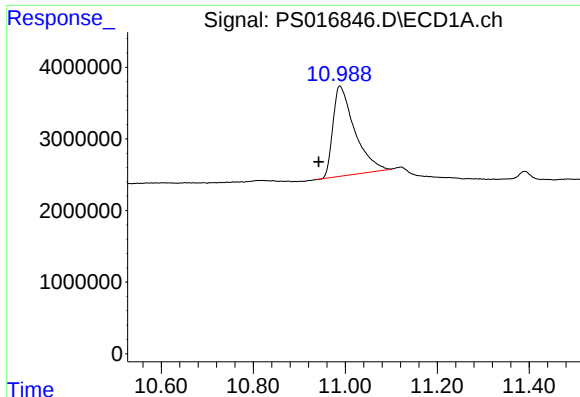

#15 Picloram


R.T.: 10.988 min  
Delta R.T.: 0.045 min  
Response: 41285498  
Conc: 3.47 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

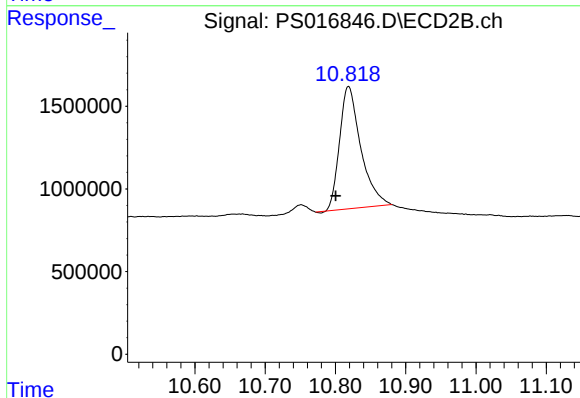


#15 Picloram

R.T.: 10.819 min  
Delta R.T.: 0.018 min  
Response: 15534646  
Conc: 3.62 ng/ml

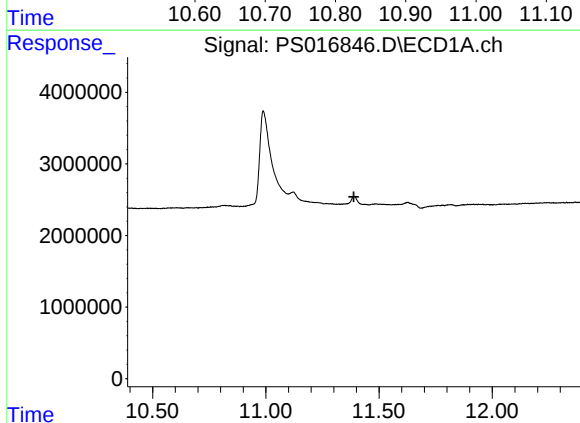

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 11.389 min  
Response: 0  
Conc: N.D.

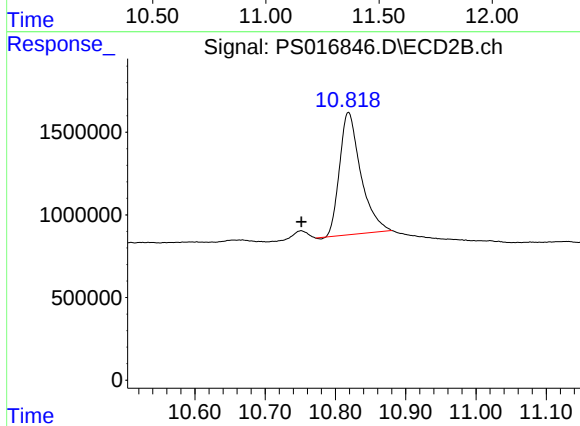

#16 DCPA

R.T.: 10.819 min  
Delta R.T.: 0.067 min  
Response: 15534646  
Conc: 3.56 ng/ml