

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092021\  
 Data File : PS016850.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Sep 2021 22:04  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 21 02:14:03 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS092021.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 21 01:52:13 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1    | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|---------|-------|----------|---------|---------|---------|
| -----                       |          |         |       |          |         |         |         |
| System Monitoring Compounds |          |         |       |          |         |         |         |
| 4) S                        | 2,4-DCAA | 7.171   | 6.757 | 612.0E6  | 266.8E6 | 401.704 | 454.965 |
|                             |          |         |       |          |         |         |         |
| Target Compounds            |          |         |       |          |         |         |         |
| 15) T                       | Picloram | 11.001f | 0.000 | 10673745 | 0       | <MDL    | N.D. #  |
| -----                       |          |         |       |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092021\  
Data File : PS016850.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Sep 2021 22:04  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 21 02:14:03 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS092021.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 21 01:52:13 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

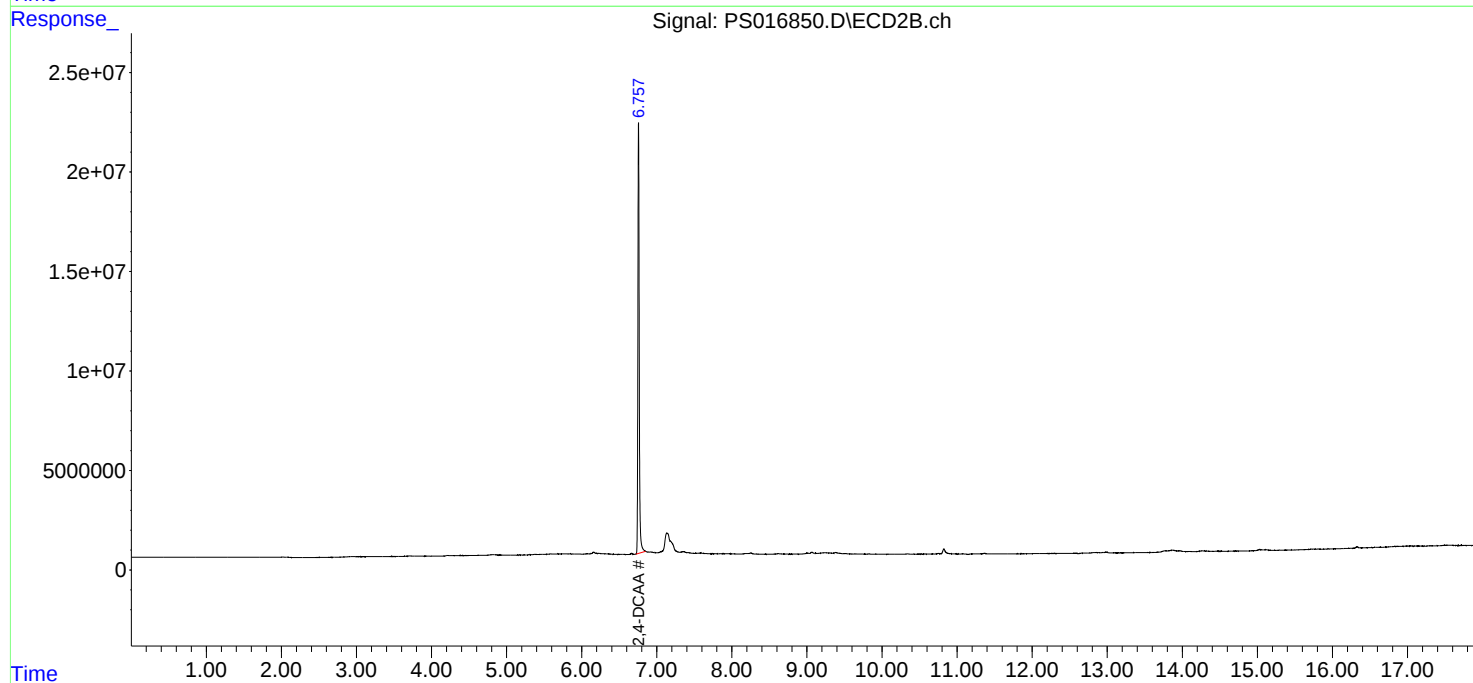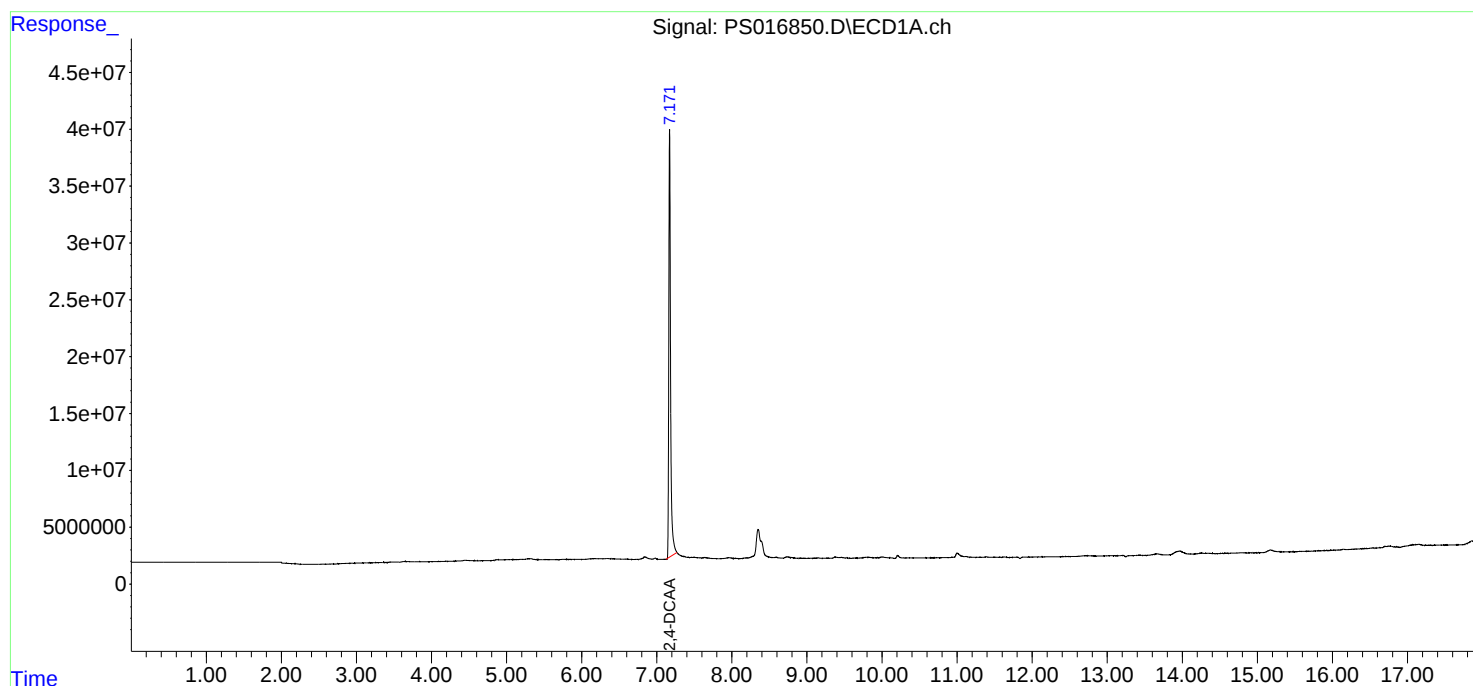


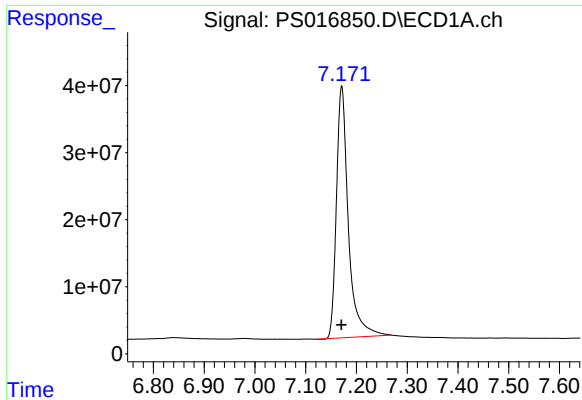

#4 2,4-DCAA

R.T.: 7.171 min  
Delta R.T.: 0.000 min  
Response: 612016054  
Conc: 401.70 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

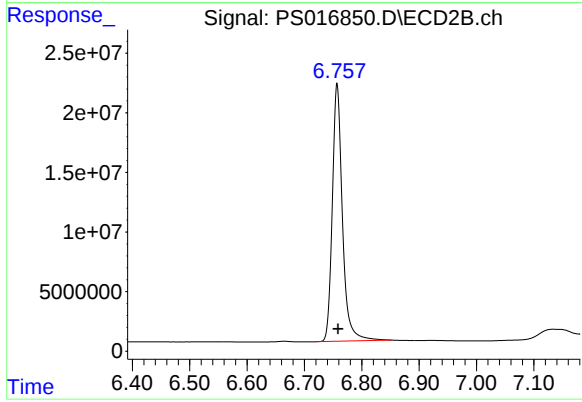

#4 2,4-DCAA

R.T.: 6.757 min  
Delta R.T.: -0.002 min  
Response: 266774375  
Conc: 454.96 ng/ml