

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092022\
 Data File : PS020616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 09:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 12:10:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.180	6.761	1755.2E6	484.5E6	510.001	568.847
Target Compounds							
1) T	Dalapon	3.034	0.000	988914	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.452f	0.000	9975835	0	2.001	N.D. #
3) T	4-Nitroph...	6.985f	0.000	-1280105	0	126.437	N.D. #
7) T	MCPA	7.646	0.000	852479	0	<MDL	N.D. #
9) T	2,4-D	8.357f	0.000	248.2E6	0	53.408	N.D. #
10) T	Pentachlo...	8.596	8.258	1283324	1841765	<MDL	<MDL #
11) T	2,4,5-TP ...	9.162	0.000	6449560	0	<MDL	N.D. #
12) T	2,4,5-T	9.441	0.000	38434279	0	1.736	N.D. #
13) T	2,4-DB	9.947	0.000	623540	0	<MDL	N.D. #
14) T	DINOSEB	11.060f	0.000	157.7E6	0	8.590	N.D. #
15) T	Picloram	10.960	10.871f	57419805	26000390	1.908	3.229 #
16) T	DCPA	11.396	0.000	7360422	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092022\
Data File : PS020616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 09:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 12:10:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

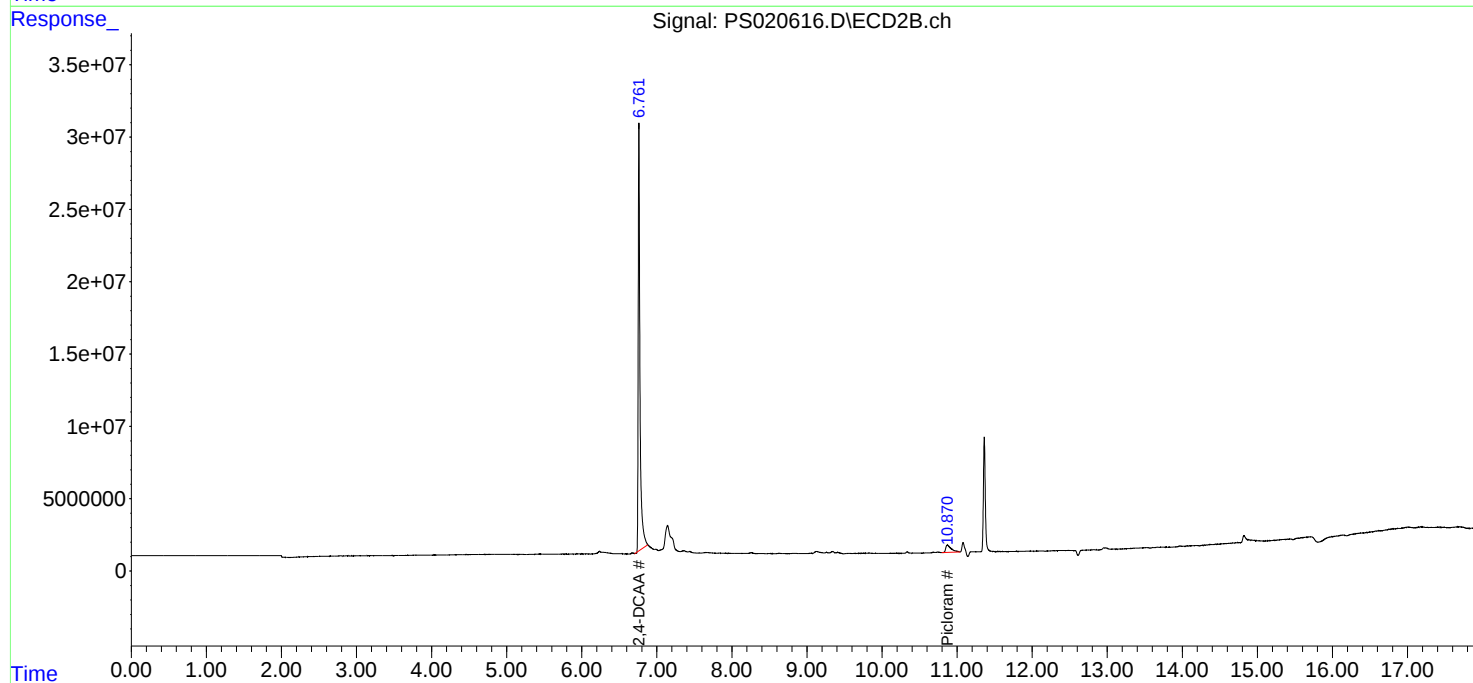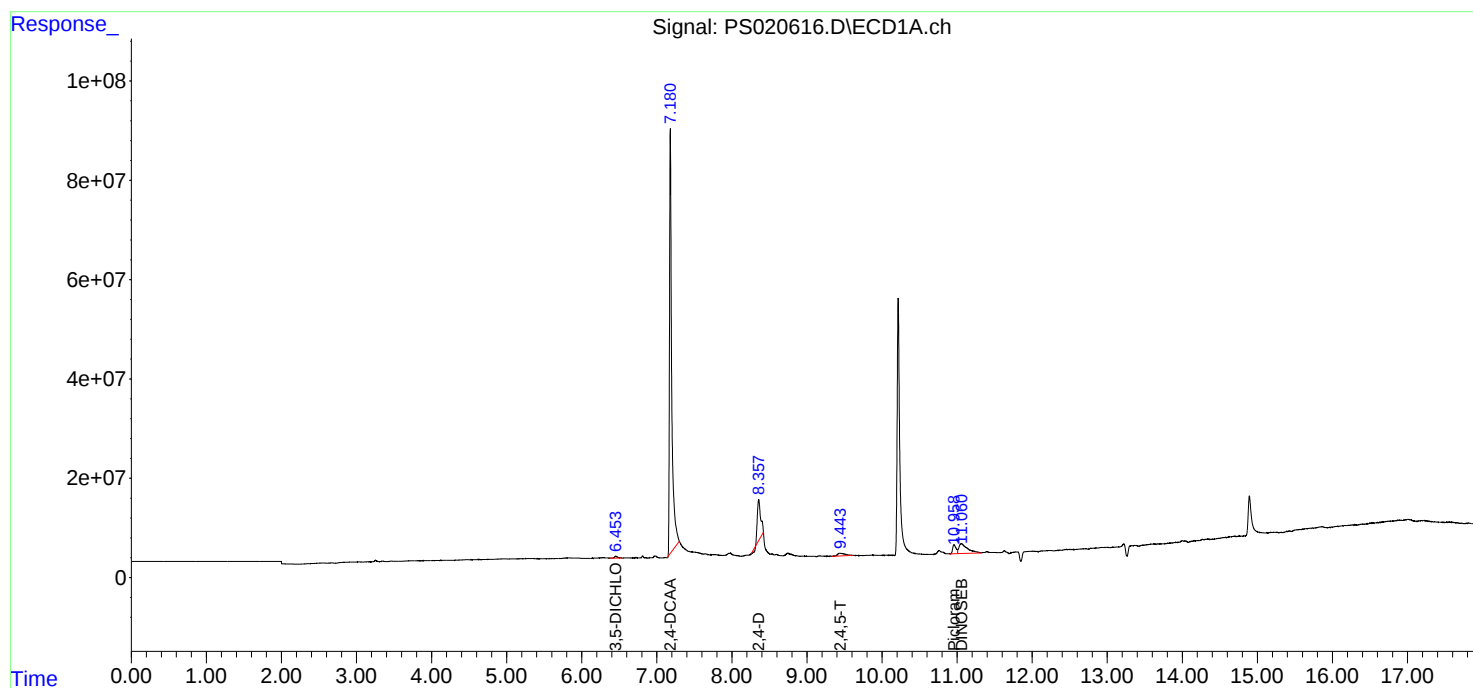


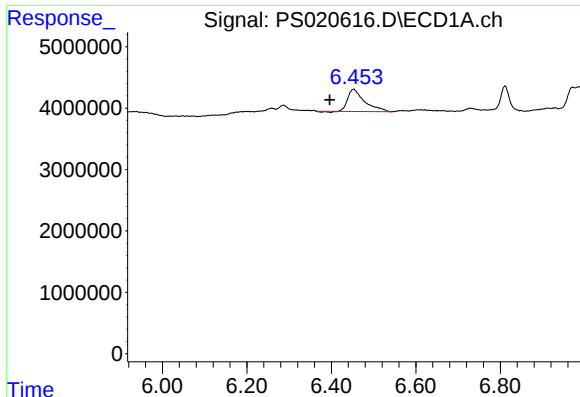

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.452 min
Delta R.T.: 0.056 min
Response: 9975835
Conc: 2.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

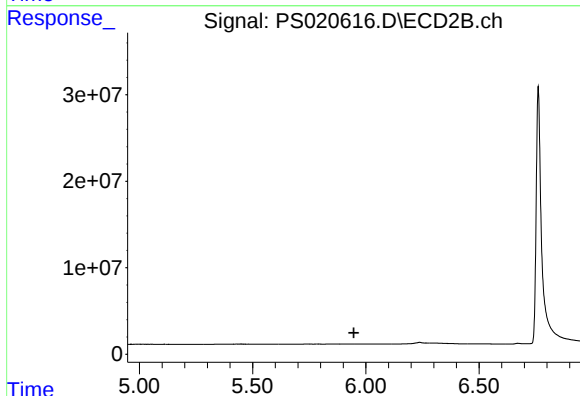


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

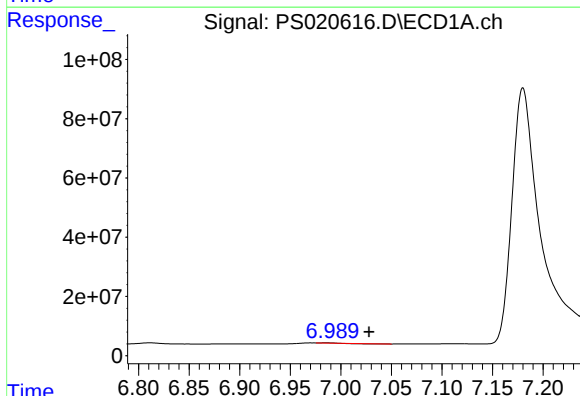


#3 4-Nitrophenol

R.T.: 6.985 min
Delta R.T.: -0.043 min
Response: -1280105
Conc: 126.44 ng/ml

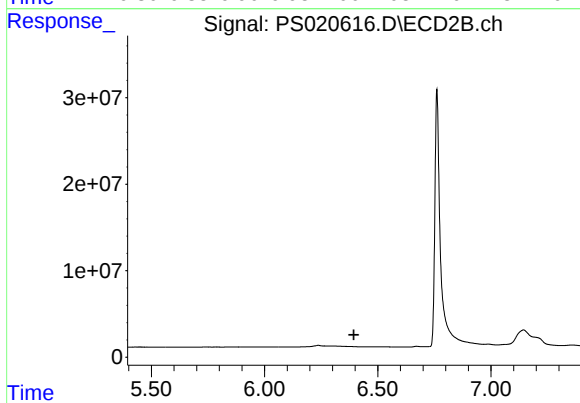

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

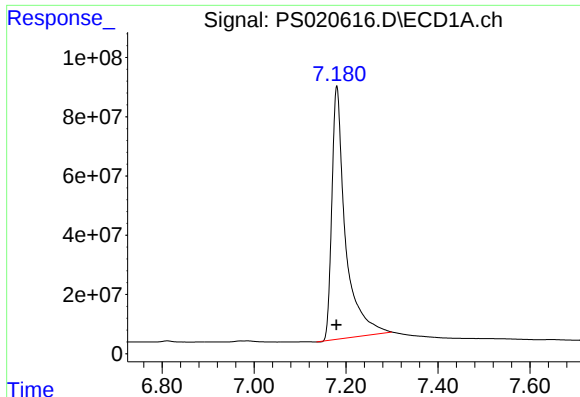

#4 2,4-DCAA


R.T.: 7.180 min
Delta R.T.: 0.001 min
Response: 1755160462
Conc: 510.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

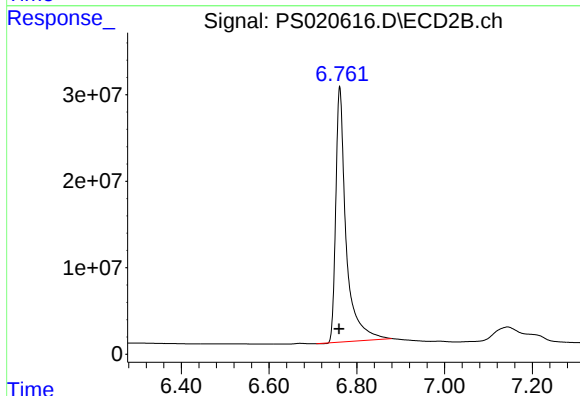


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: 0.001 min
Response: 484484588
Conc: 568.85 ng/ml

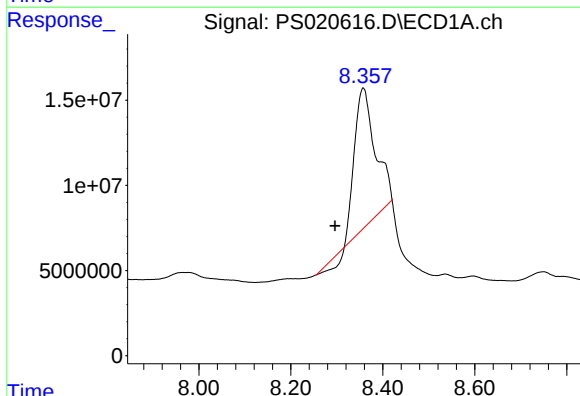


#9 2,4-D

R.T.: 8.357 min
Delta R.T.: 0.061 min
Response: 248245173
Conc: 53.41 ng/ml

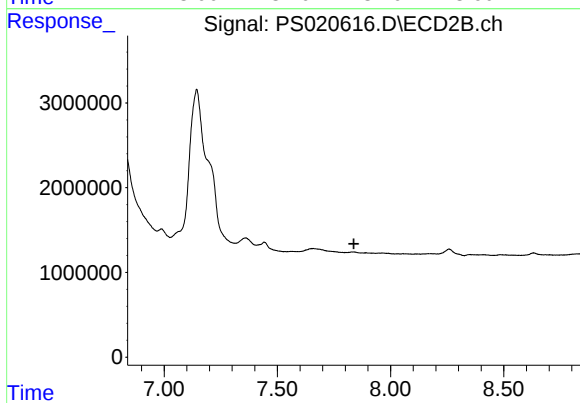

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

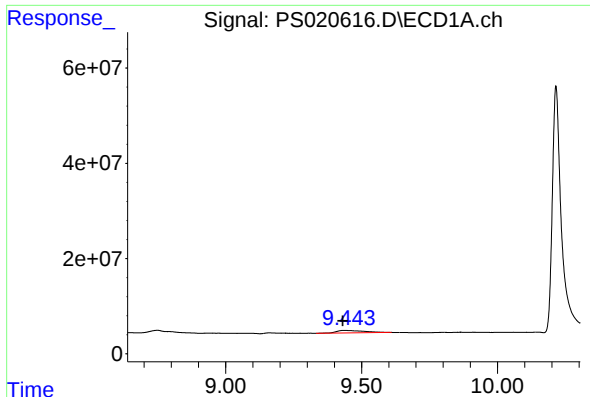

#12 2,4,5-T


R.T.: 9.441 min
Delta R.T.: 0.010 min
Response: 38434279
Conc: 1.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

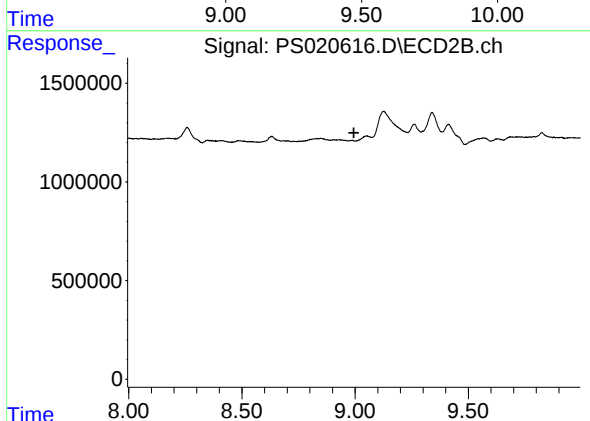


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.995 min
Response: 0
Conc: N.D.

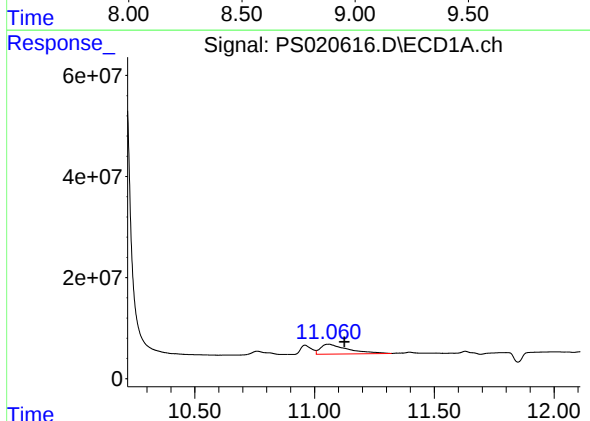


#14 DINOSEB

R.T.: 11.060 min
Delta R.T.: -0.065 min
Response: 157749510
Conc: 8.59 ng/ml

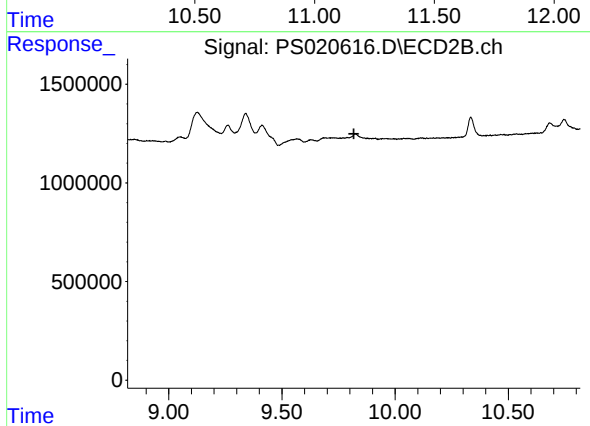

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

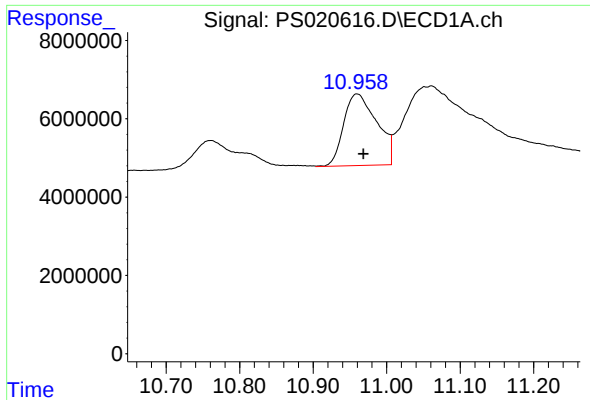

#15 Picloram

R.T.: 10.960 min
Delta R.T.: -0.009 min
Response: 57419805
Conc: 1.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

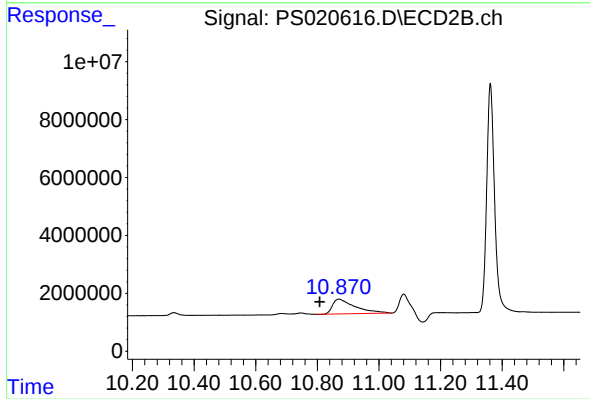

#15 Picloram

R.T.: 10.871 min
Delta R.T.: 0.063 min
Response: 26000390
Conc: 3.23 ng/ml