

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092022\
 Data File : PS020622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 12:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 15:23:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.760	1784.3E6	492.8E6	518.458	578.618
Target Compounds							
1) T	Dalapon	3.006	0.000	539279	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.450f	0.000	10614701	0	2.129	N.D. #
7) T	MCPA	7.643	0.000	1133615	0	<MDL	N.D. #
9) T	2,4-D	8.353f	0.000	223.4E6	0	48.069	N.D. #
10) T	Pentachlo...	8.590	0.000	576285	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.158	0.000	4338874	0	<MDL	N.D. #
12) T	2,4,5-T	9.427	0.000	21554998	0	<MDL	N.D. #
13) T	2,4-DB	10.009	0.000	2176082	0	<MDL	N.D. #
15) T	Picloram	10.952	10.867f	80406460	10485137	2.672	1.302 #
16) T	DCPA	11.399	10.679f	4784661	1176146	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092022\
Data File : PS020622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 12:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 15:23:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

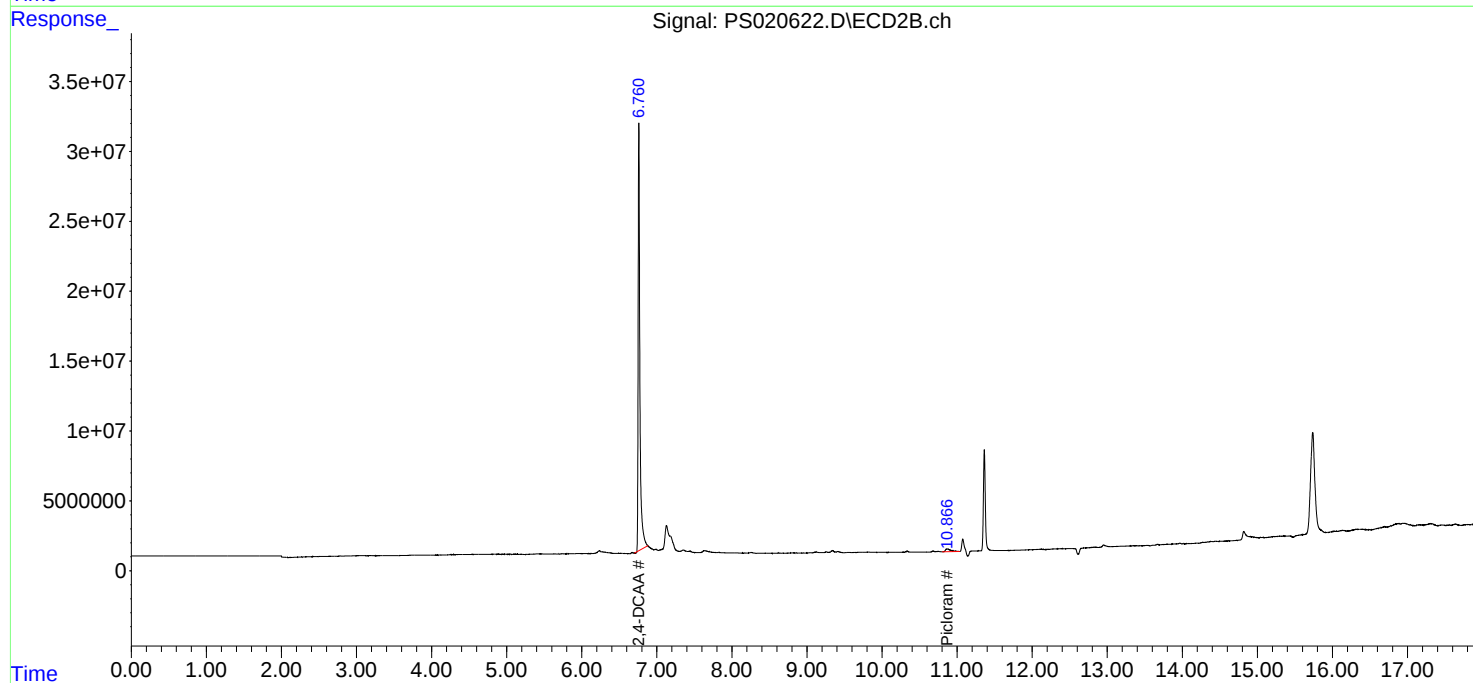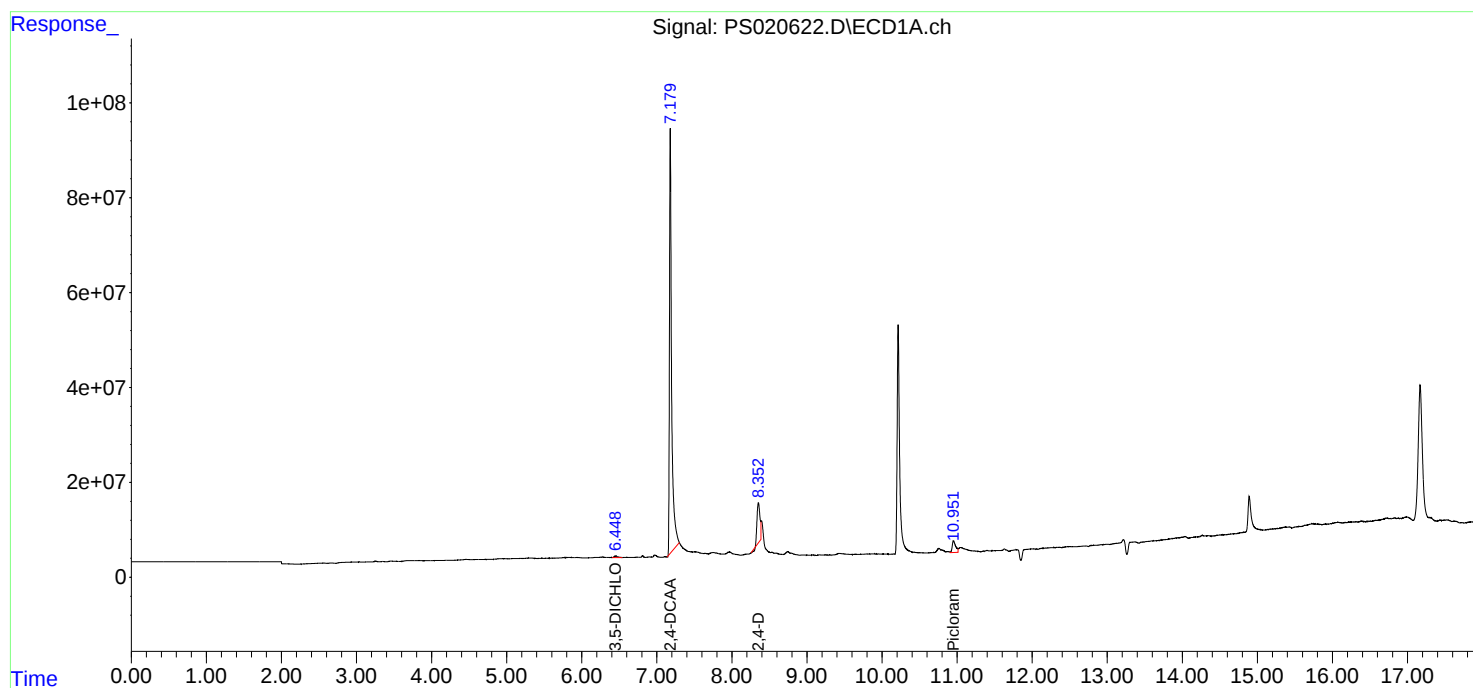


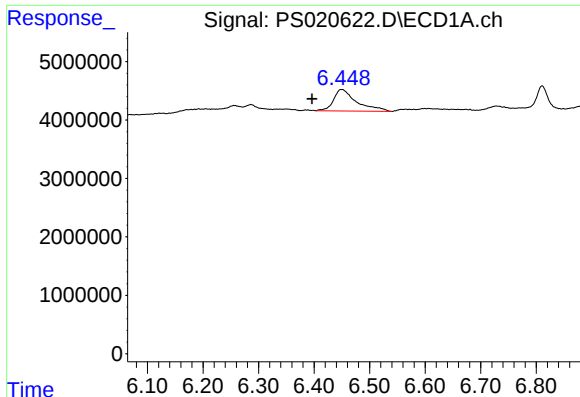

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.450 min
Delta R.T.: 0.054 min
Response: 10614701
Conc: 2.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

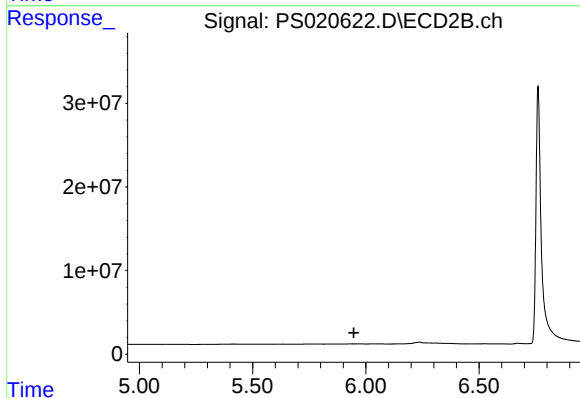


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

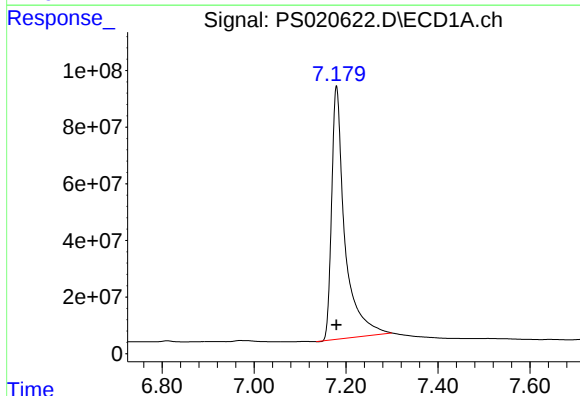


#4 2,4-DCAA

R.T.: 7.179 min
Delta R.T.: 0.000 min
Response: 1784267112
Conc: 518.46 ng/ml

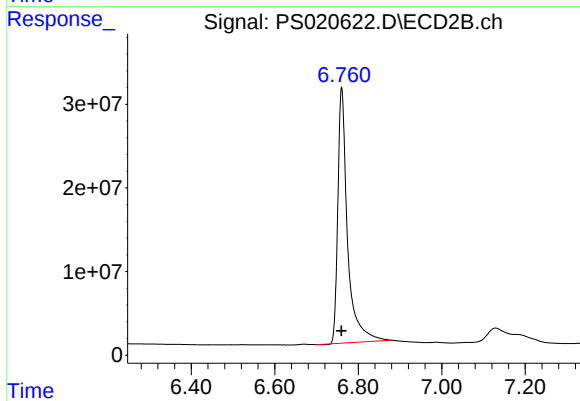

#4 2,4-DCAA


R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 492805775
Conc: 578.62 ng/ml

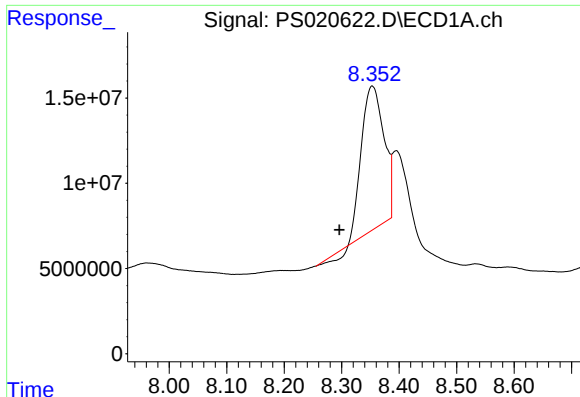

#9 2,4-D


R.T.: 8.353 min
Delta R.T.: 0.057 min
Response: 223429416
Conc: 48.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

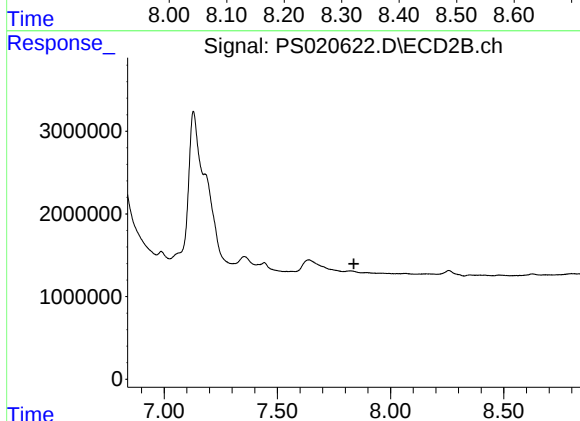


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

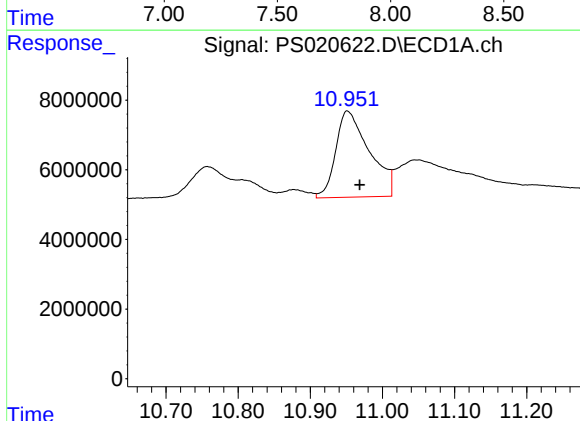

#15 Picloram

R.T.: 10.952 min
Delta R.T.: -0.017 min
Response: 80406460
Conc: 2.67 ng/ml

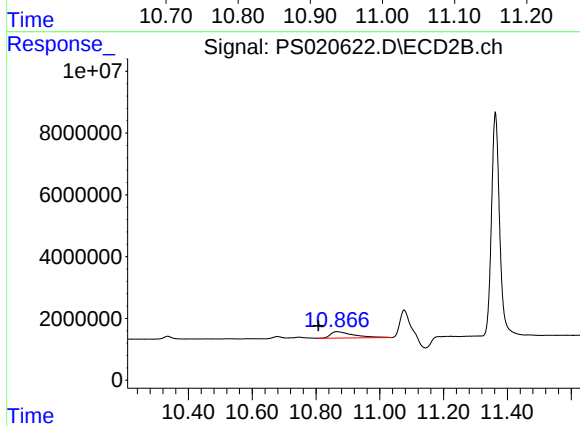

#15 Picloram

R.T.: 10.867 min
Delta R.T.: 0.059 min
Response: 10485137
Conc: 1.30 ng/ml