

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092024\
 Data File : PS027744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 11:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 22:24:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.114	0.000	1190878	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.523f	0.000	177.0E6	0	42.731	N.D. #
2) T	3,5-DICHL...	0.000	6.644f	0	1073162	N.D.	<MDL
3) T	4-Nitroph...	6.894	0.000	8540508	0	5.044	N.D. #
5) T	DICAMBA	0.000	7.834	0	1268356	N.D.	<MDL
6) T	MCP	7.520f	7.927	13192390	255767	1.914	<MDL #
8) T	DICHLORPROP	0.000	8.578f	0	1477719	N.D.	1.323
9) T	2,4-D	0.000	8.811f	0	1844222	N.D.	1.654
10) T	Pentachlo...	8.512	9.371	3130526	794634	<MDL	<MDL #
11) T	2,4,5-TP ...	9.025f	9.737	8602375	3455321	<MDL	<MDL #
12) T	2,4,5-T	9.364	10.156	2362240	5130801	<MDL	<MDL #
13) T	2,4-DB	9.889	0.000	3886882	0	1.674	N.D. #
15) T	Picloram	10.901	12.189	58175126	12772219	3.110	2.748
16) T	DCPA	11.378	12.122	6026845	9499645	<MDL	1.474 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092024\
Data File : PS027744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 11:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 22:24:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

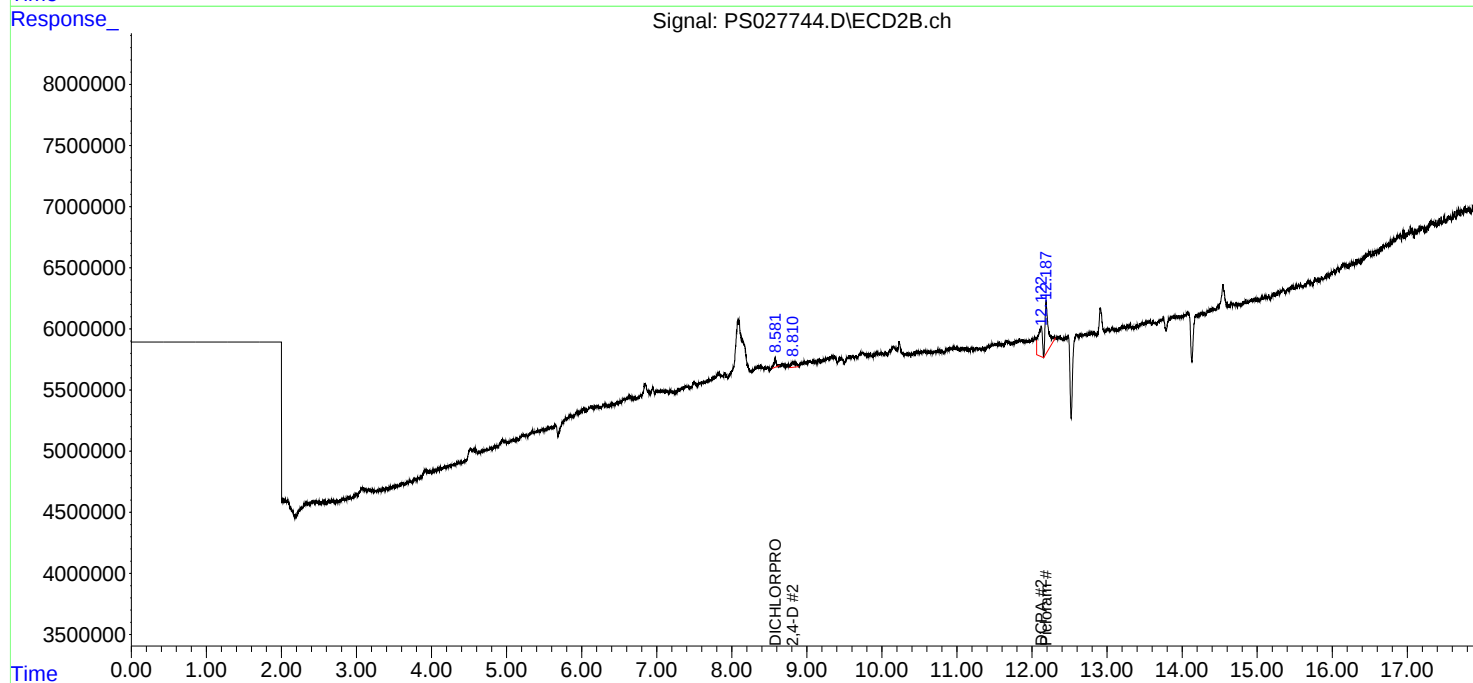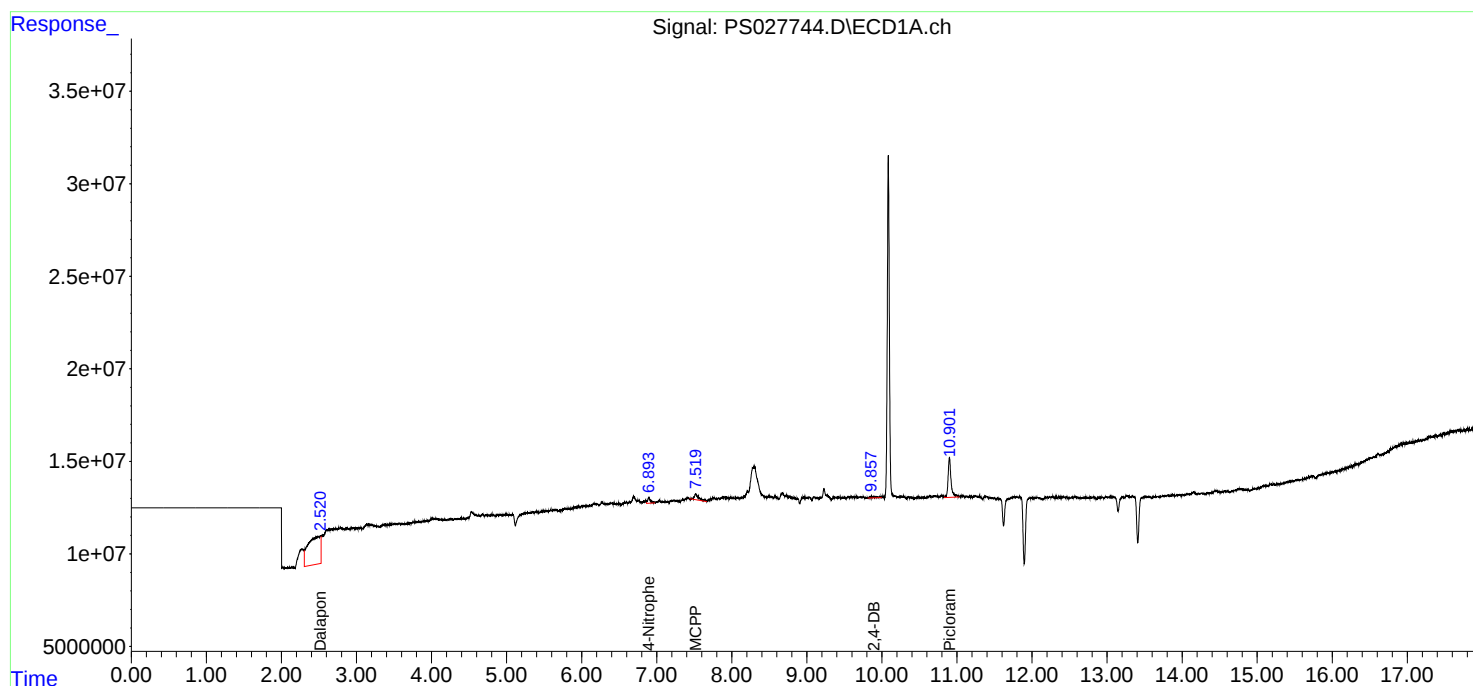


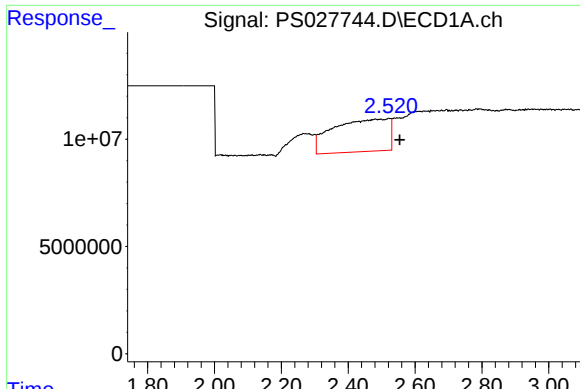

#1 Dalapon


R.T.: 2.523 min
Delta R.T.: -0.031 min
Response: 177039911
Conc: 42.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

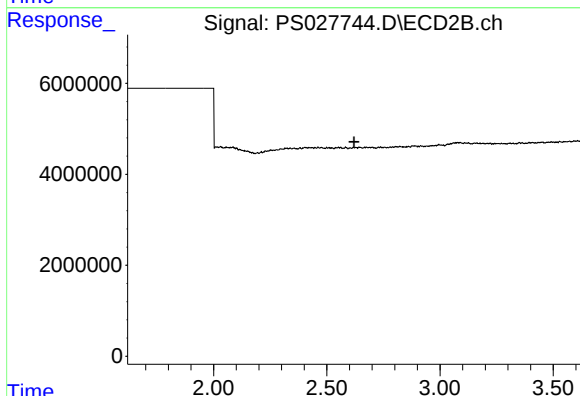


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

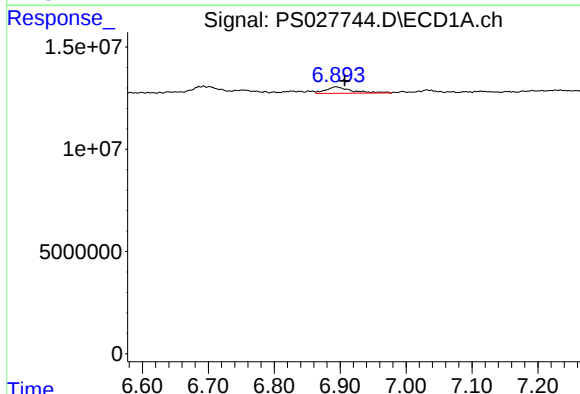


#3 4-Nitrophenol

R.T.: 6.894 min
Delta R.T.: -0.013 min
Response: 8540508
Conc: 5.04 ng/ml

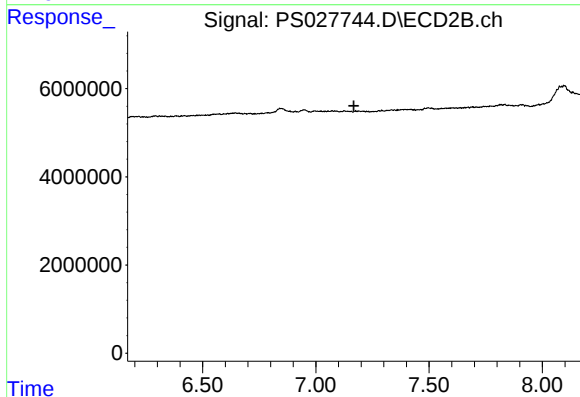

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

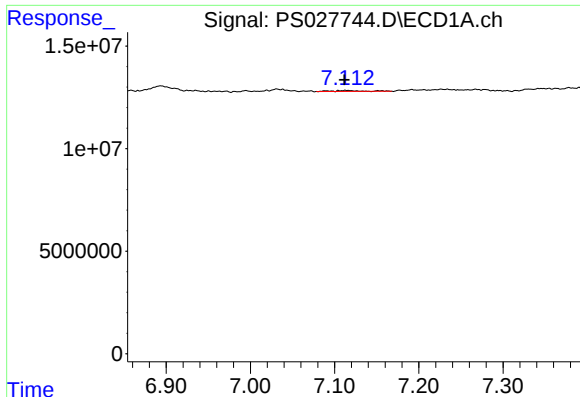

#4 2,4-DCAA


R.T.: 7.114 min
Delta R.T.: 0.002 min
Response: 1190878
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

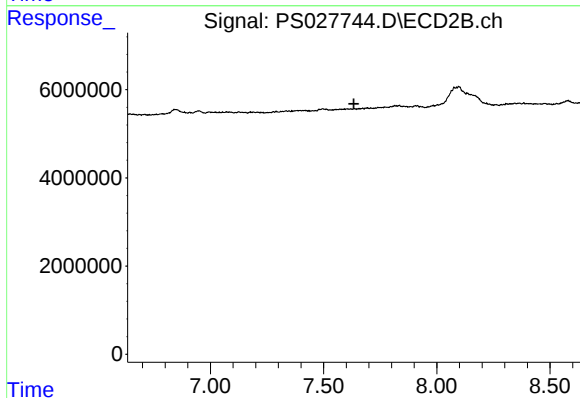


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.633 min
Response: 0
Conc: N.D.

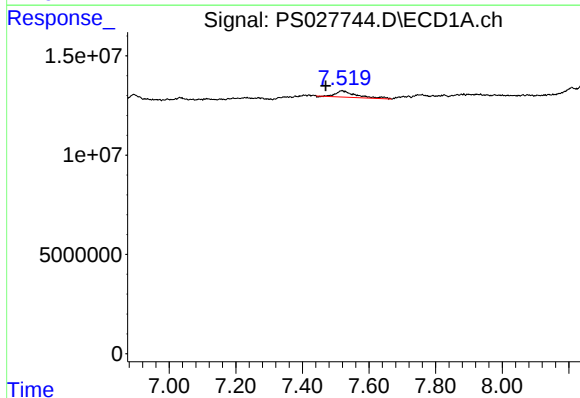


#6 MCP

R.T.: 7.520 min
Delta R.T.: 0.049 min
Response: 13192390
Conc: 1.91 ug/ml

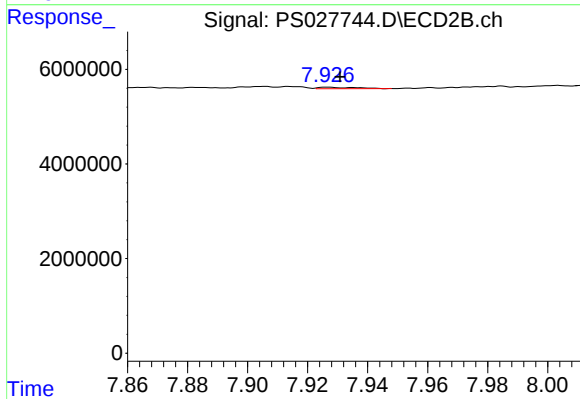

#6 MCP


R.T.: 7.927 min
Delta R.T.: -0.004 min
Response: 255767
Conc: N.D.

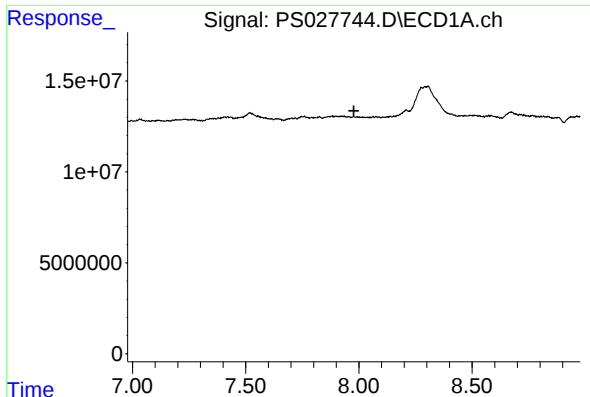

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

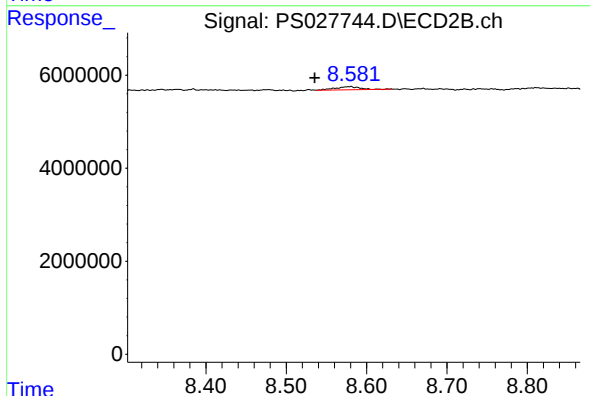


#8 DICHLORPROP

R.T.: 8.578 min
Delta R.T.: 0.043 min
Response: 1477719
Conc: 1.32 ng/ml

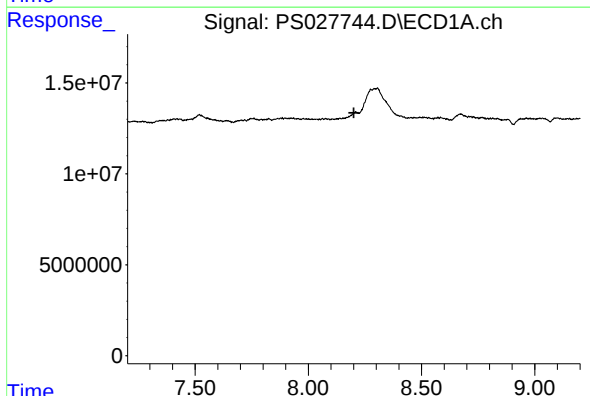


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.201 min
Response: 0
Conc: N.D.

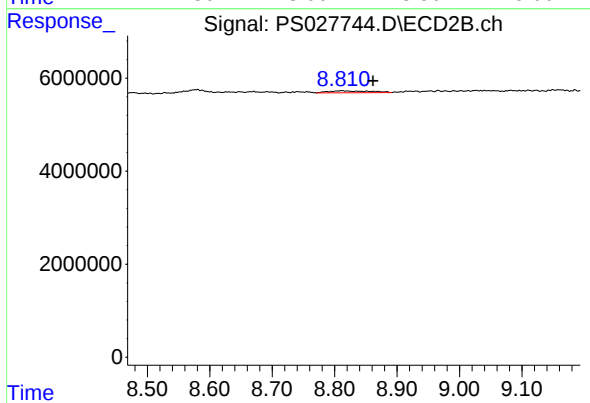

#9 2,4-D


R.T.: 8.811 min
Delta R.T.: -0.050 min
Response: 1844222
Conc: 1.65 ng/ml

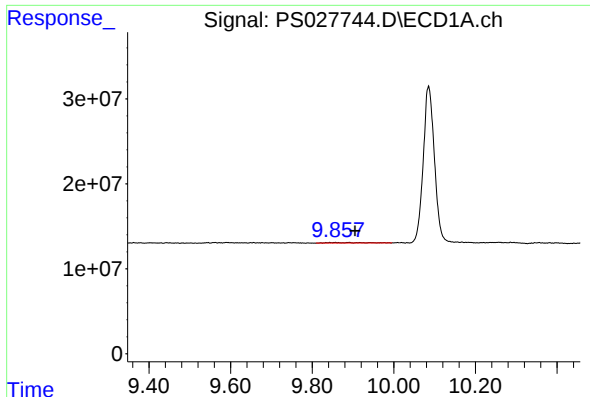

#13 2,4-DB


R.T.: 9.889 min
Delta R.T.: -0.017 min
Response: 3886882
Conc: 1.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

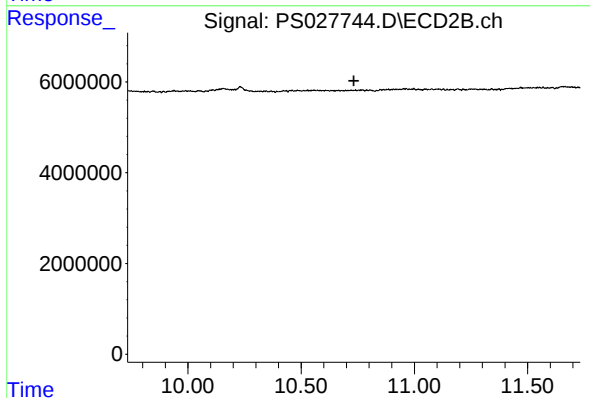


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.733 min
Response: 0
Conc: N.D.

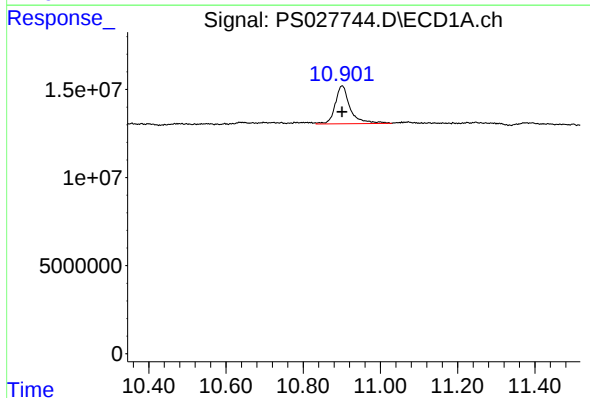


#15 Picloram

R.T.: 10.901 min
Delta R.T.: 0.000 min
Response: 58175126
Conc: 3.11 ng/ml

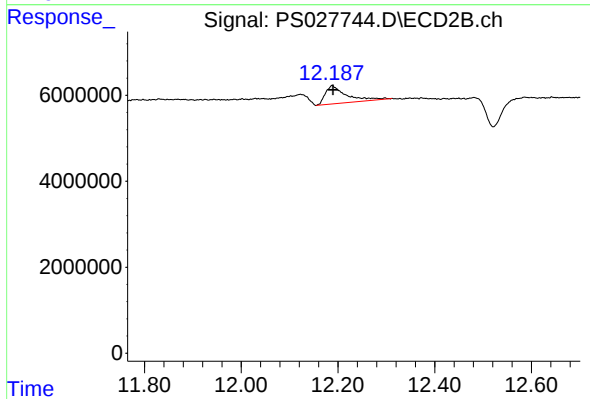

#15 Picloram


R.T.: 12.189 min
Delta R.T.: -0.001 min
Response: 12772219
Conc: 2.75 ng/ml

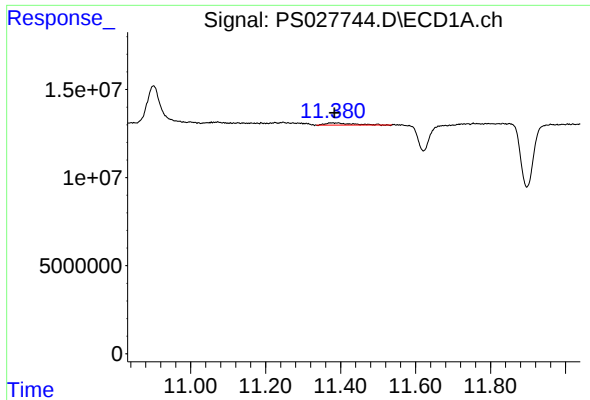

#16 DCPA

R.T.: 11.378 min
Delta R.T.: -0.005 min
Response: 6026845
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

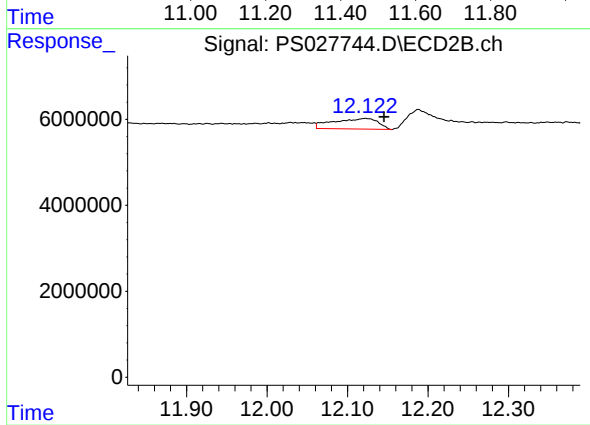

#16 DCPA

R.T.: 12.122 min
Delta R.T.: -0.024 min
Response: 9499645
Conc: 1.47 ng/ml