

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092120\
 Data File : PS012411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2020 20:28
 Operator : DD\AJ
 Sample : L4062-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EROC-CF-1

Manual Integrations
 APPROVED

Ankita
 9/22/2020 9:32:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 02:43:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.214	6.910	475.7E6	208.7E6	438.910	395.623m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092120\
Data File : PS012411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2020 20:28
Operator : DD\AJ
Sample : L4062-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
ERO-CF-1


Manual Integrations
APPROVED

Ankita
9/22/2020 9:32:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 02:43:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

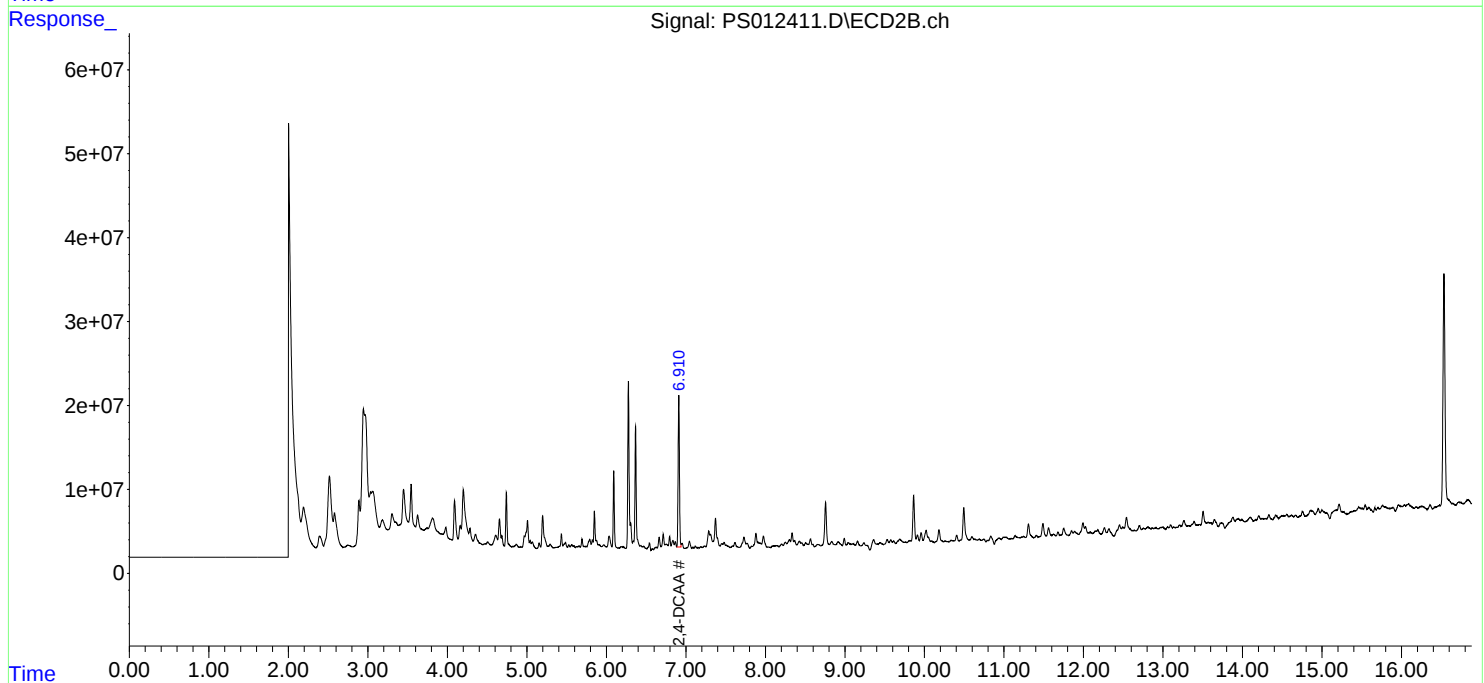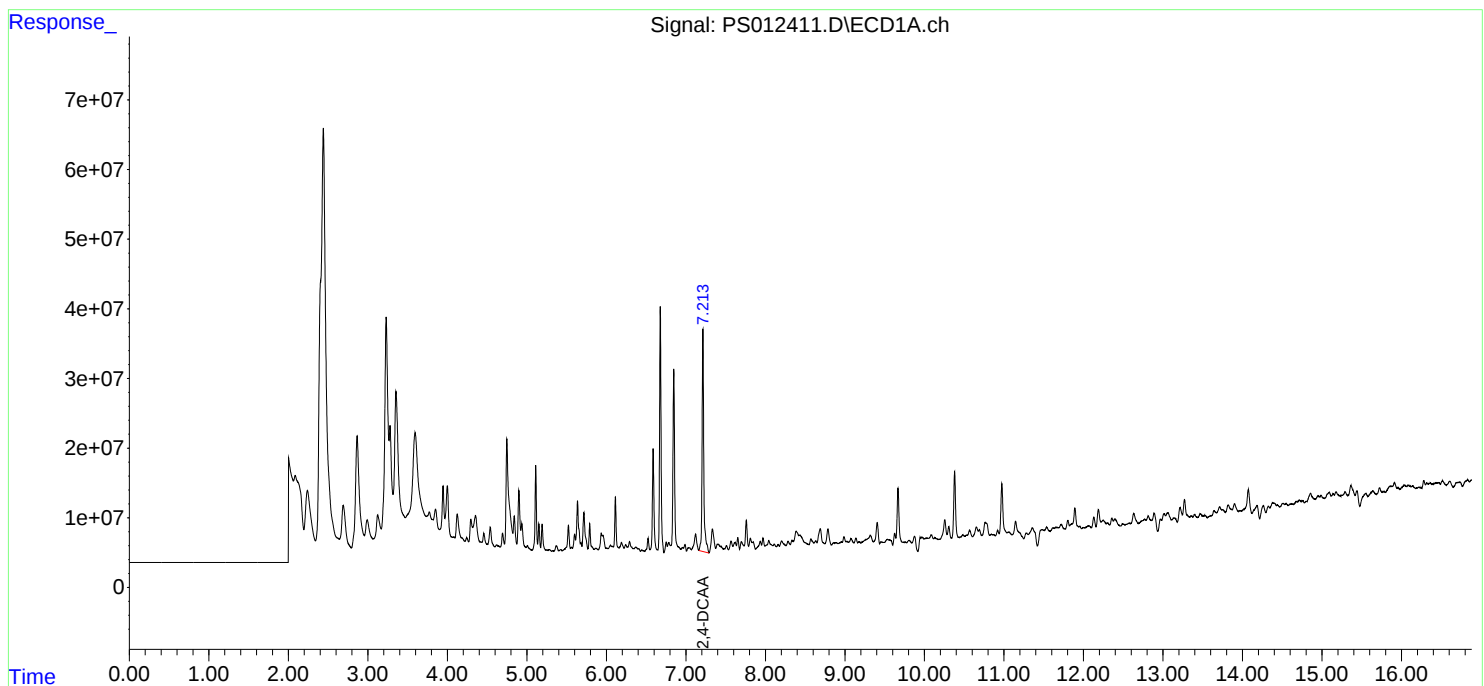

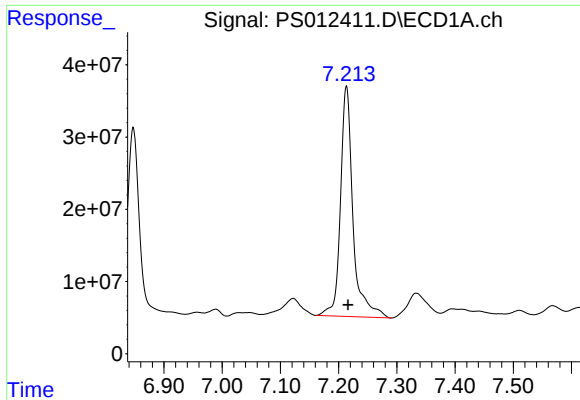


#4 2,4-DCAA

R.T.: 7.214 min
Delta R.T.: -0.003 min
Response: 475732960
Conc: 438.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
EROC-CF-1

Manual Integrations
APPROVED

Ankita
9/22/2020 9:32:28 AM

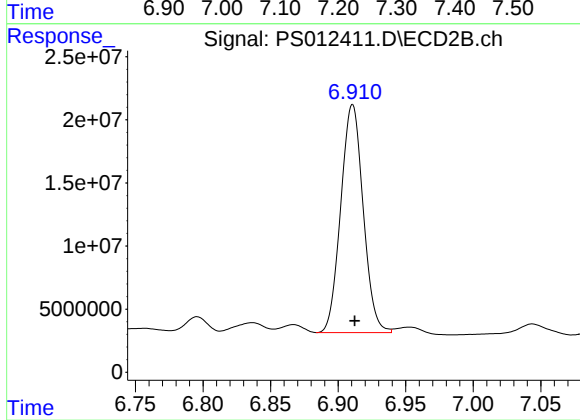

#4 2,4-DCAA

R.T.: 6.910 min
Delta R.T.: -0.002 min
Response: 208732829
Conc: 395.62 ng/ml m