

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092121\
 Data File : PS016853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2021 09:51
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 03:48:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.171	6.755	613.6E6	271.0E6	402.715	462.138
Target Compounds							
9) T	2,4-D	8.348f	0.000	57679960	0	32.805	N.D. #
15) T	Picloram	11.006f	10.818	21947828	8336090	1.844	1.943
16) T	DCPA	0.000	10.818f	0	8336090	N.D.	1.912



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092121\
Data File : PS016853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2021 09:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 03:48:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

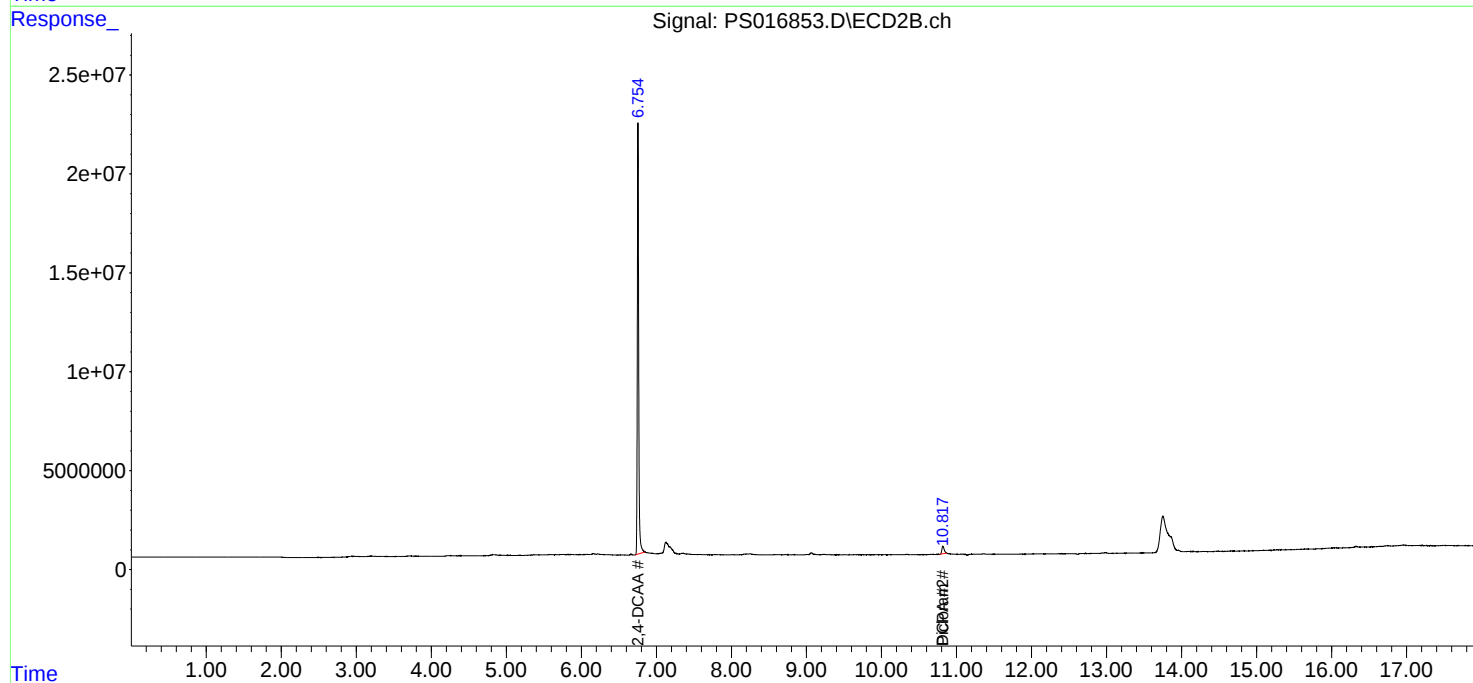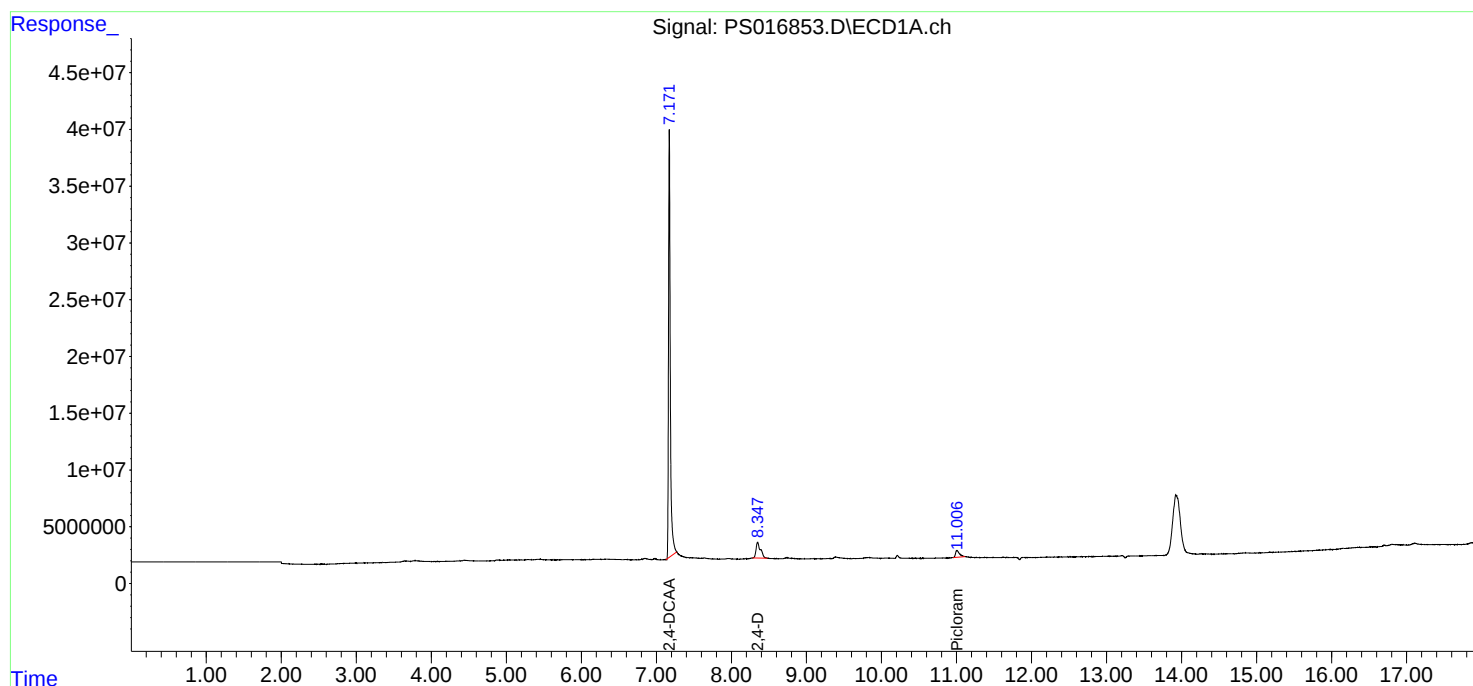


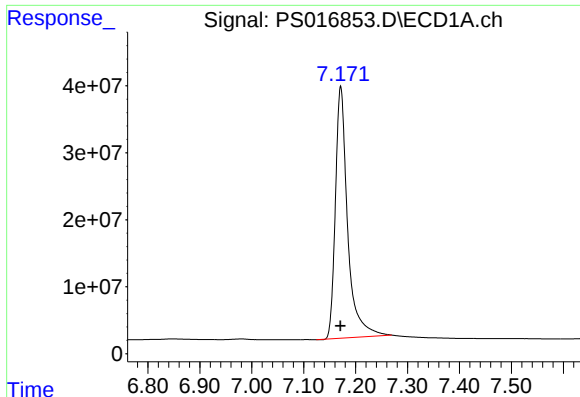

#4 2,4-DCAA


R.T.: 7.171 min
Delta R.T.: 0.000 min
Response: 613556131
Conc: 402.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

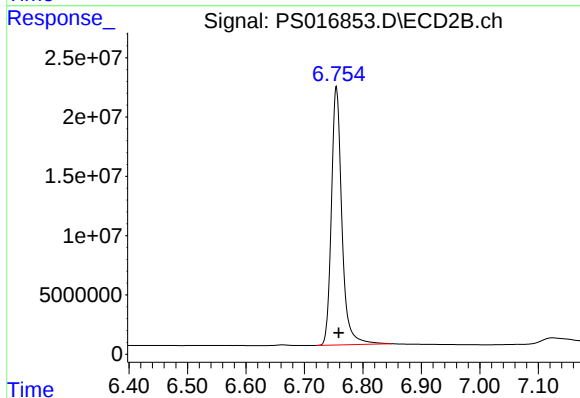


#4 2,4-DCAA

R.T.: 6.755 min
Delta R.T.: -0.004 min
Response: 270980757
Conc: 462.14 ng/ml

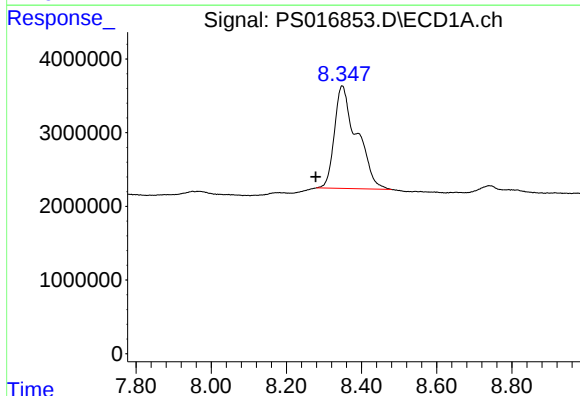


#9 2,4-D

R.T.: 8.348 min
Delta R.T.: 0.069 min
Response: 57679960
Conc: 32.81 ng/ml

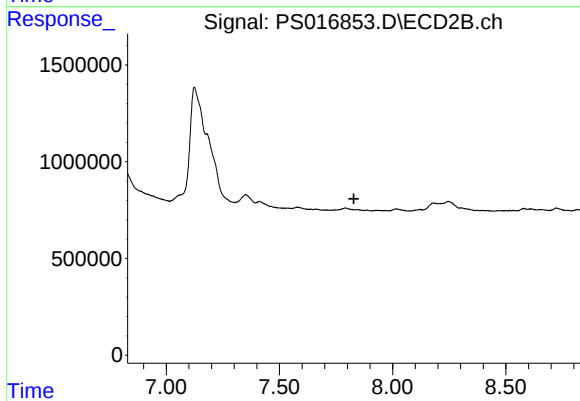

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.829 min
Response: 0
Conc: N.D.

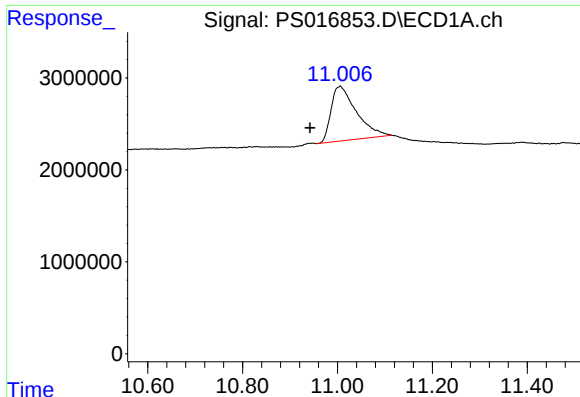

#15 Picloram


R.T.: 11.006 min
Delta R.T.: 0.063 min
Response: 21947828
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

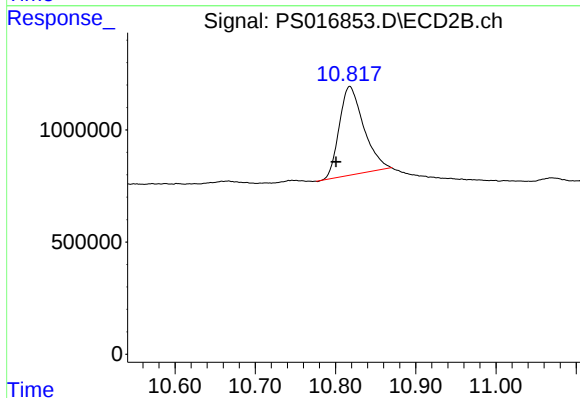


#15 Picloram

R.T.: 10.818 min
Delta R.T.: 0.017 min
Response: 8336090
Conc: 1.94 ng/ml

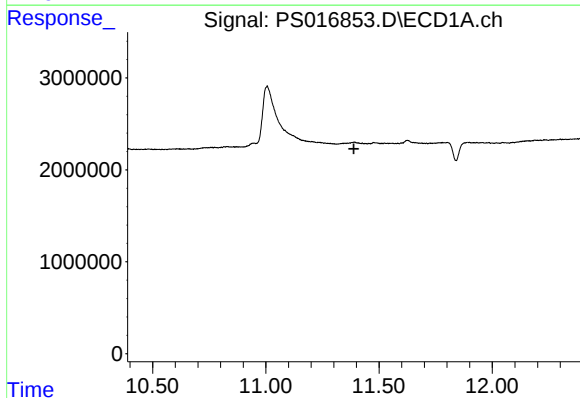

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.389 min
Response: 0
Conc: N.D.

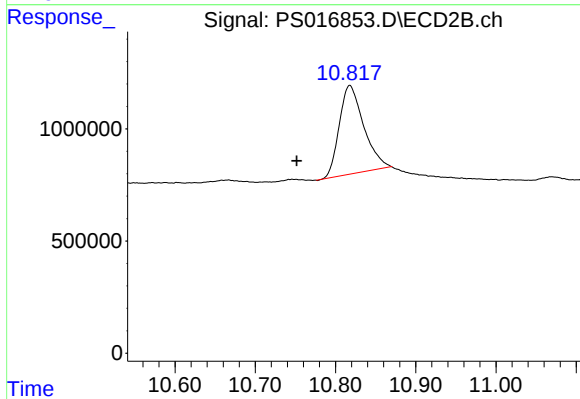

#16 DCPA

R.T.: 10.818 min
Delta R.T.: 0.066 min
Response: 8336090
Conc: 1.91 ng/ml