

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092121\
 Data File : PS016874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2021 21:57
 Operator : DD\AJ
 Sample : M3786-05 (Sig #1); PB139239BS (Sig #2)
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CHRT-26414

Manual Integrations
 APPROVED

mohammad
 9/22/2021 2:57:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 03:54:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.161	6.751	591.8E6	251.9E6	388.436	429.611m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092121\
Data File : PS016874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2021 21:57
Operator : DD\AJ
Sample : M3786-05 (Sig #1); PB139239BS (Sig #2)
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CHRT-26414


Manual Integrations
APPROVED

mohammad
9/22/2021 2:57:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 03:54:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

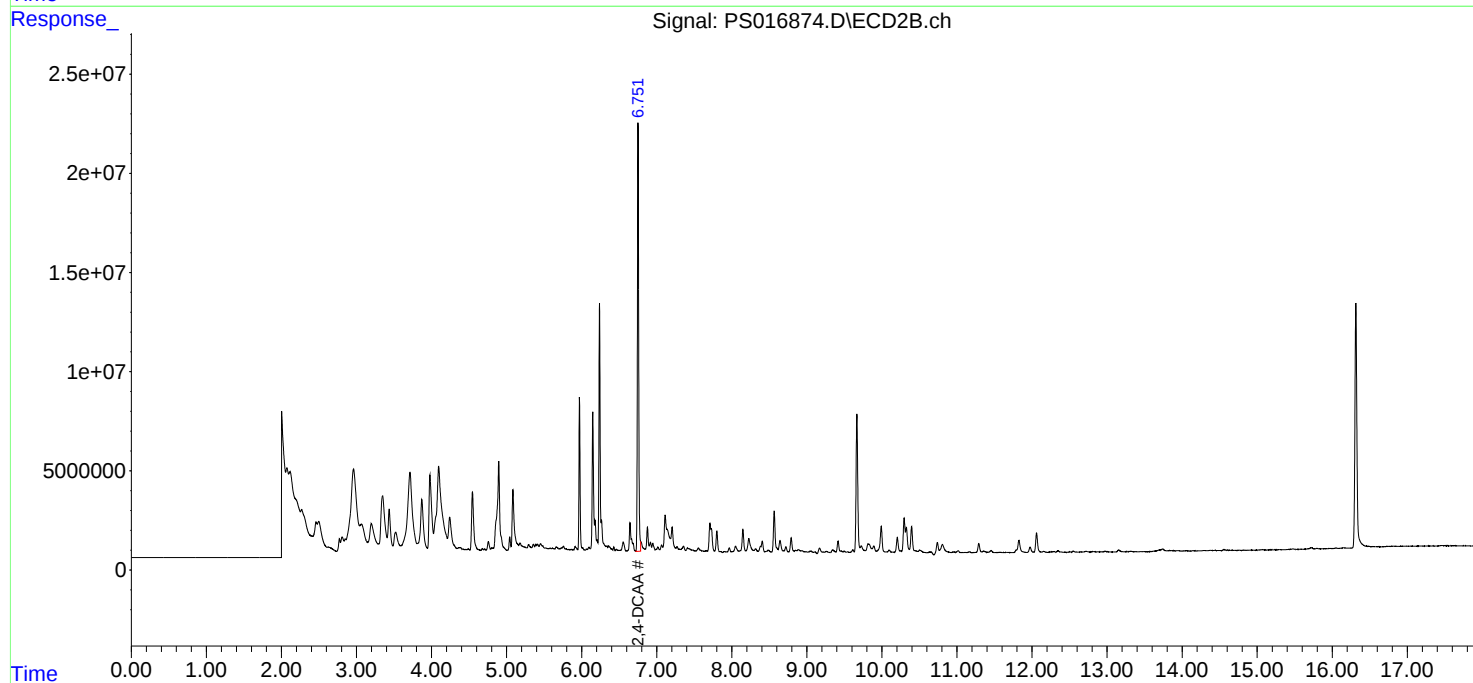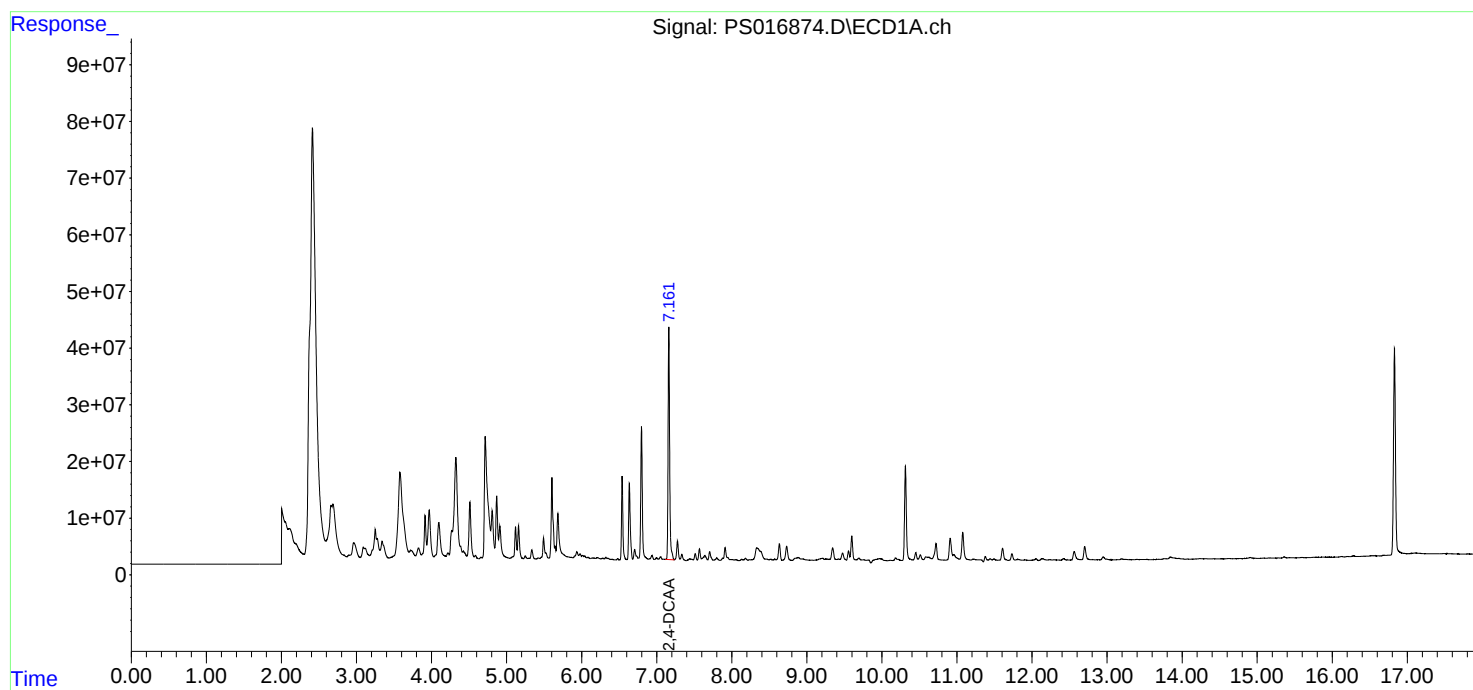

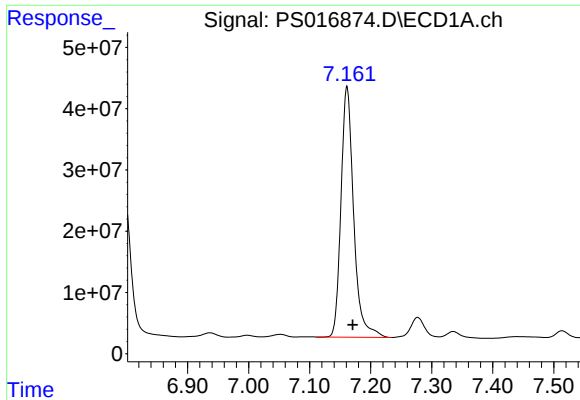


#4 2,4-DCAA

R.T.: 7.161 min
Delta R.T.: -0.009 min
Response: 591801761
Conc: 388.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
CHRT-26414

Manual Integrations
APPROVED

mohammad
9/22/2021 2:57:07 PM

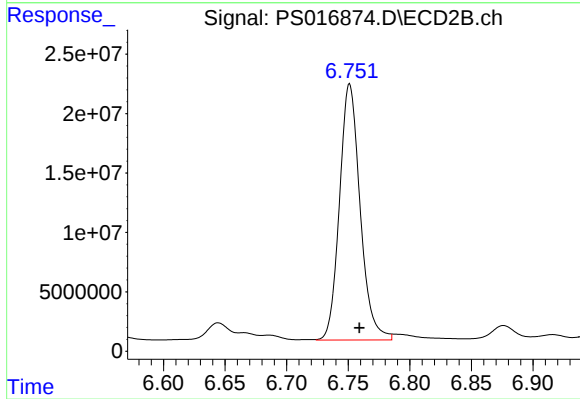

#4 2,4-DCAA

R.T.: 6.751 min
Delta R.T.: -0.008 min
Response: 251907885
Conc: 429.61 ng/ml m