

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092220\
 Data File : PS012425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2020 13:44
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 05:05:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds						
6) T	MCP	0.000	7.227	0	3480397	N.D. 2.301
7) T	MCPA	0.000	7.350	0	9183303	N.D. 3.831
9) T	2,4-D	8.394	7.965	65595575	6834148	57.772 10.913 #
13) T	2,4-DB	0.000	9.708	0	7246710	N.D. 19.357


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092220\
Data File : PS012425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2020 13:44
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 05:05:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

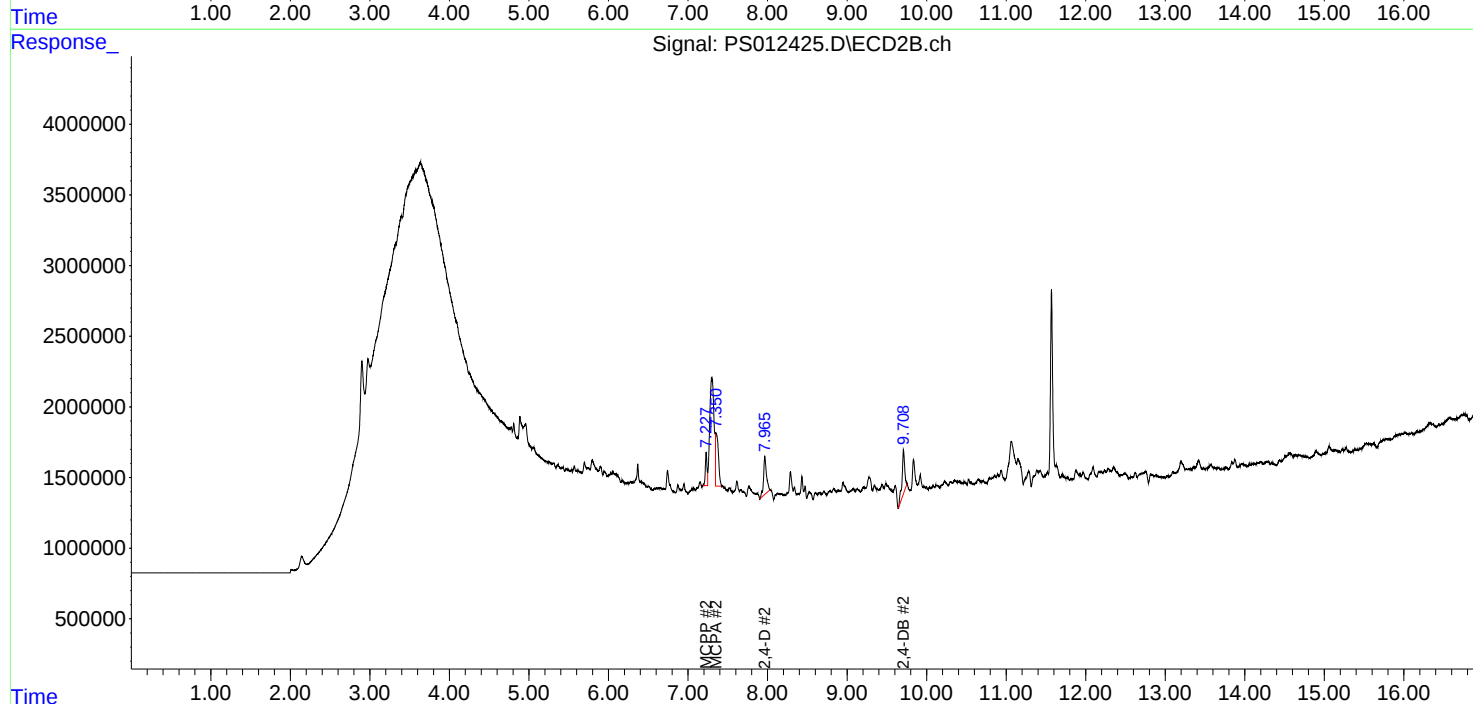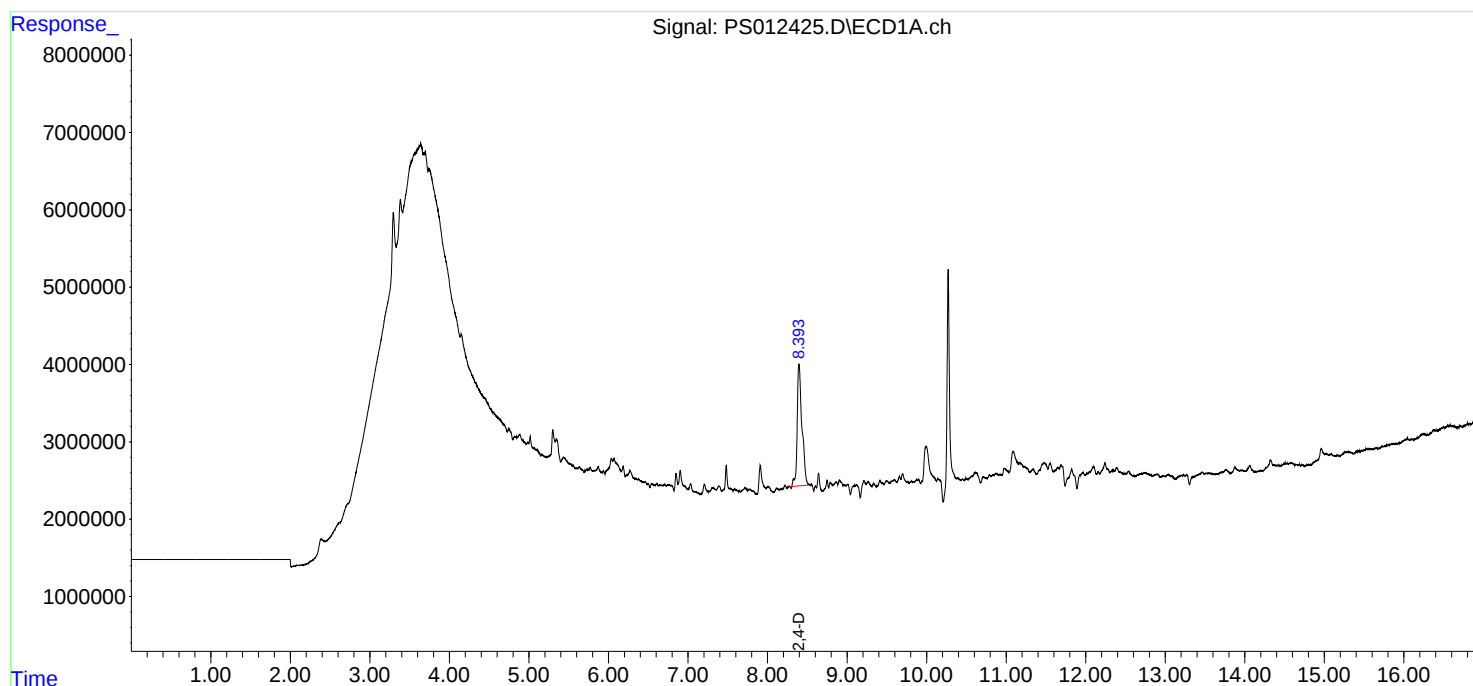

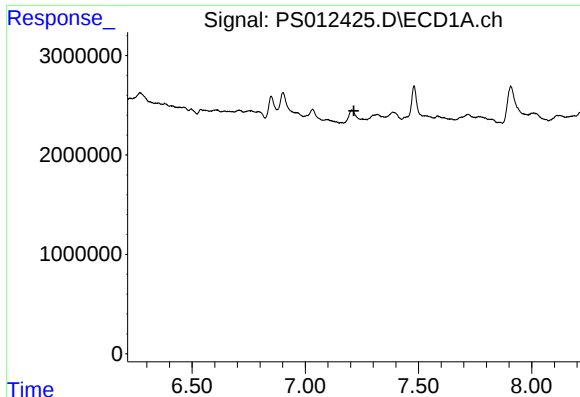


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.

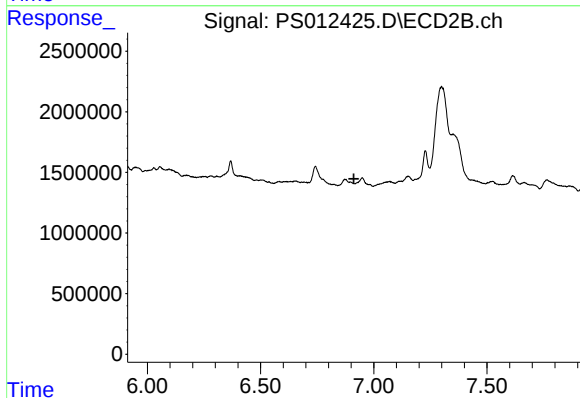


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

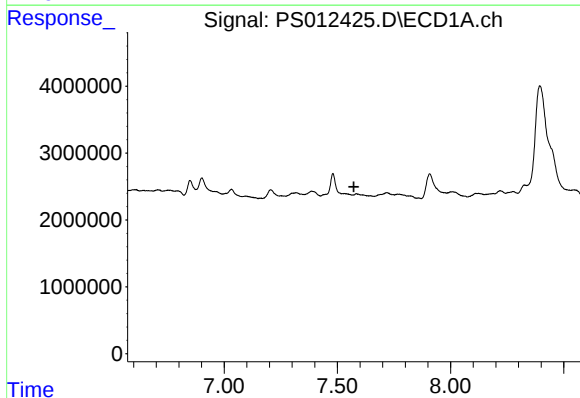


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

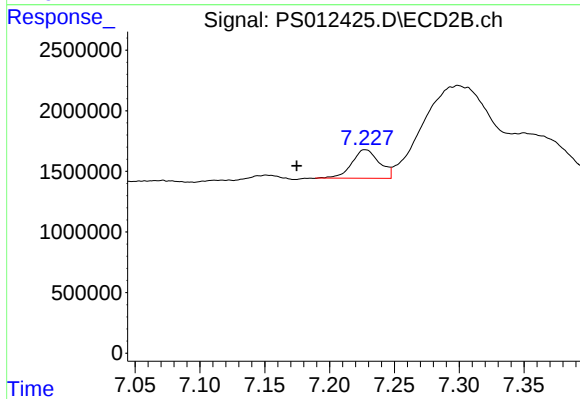


#6 MCPP

R.T.: 7.227 min
Delta R.T.: 0.053 min
Response: 3480397
Conc: 2.30 ug/ml

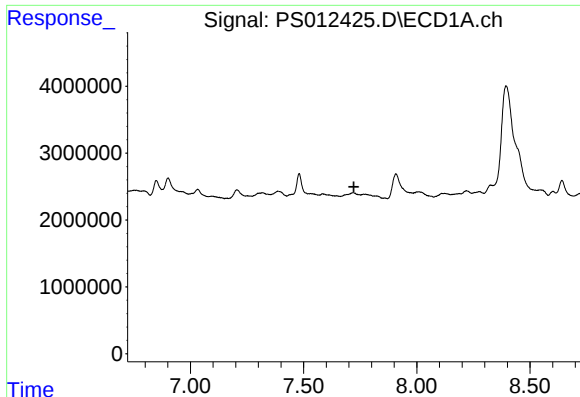


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.722 min
Response: 0
Conc: N.D.

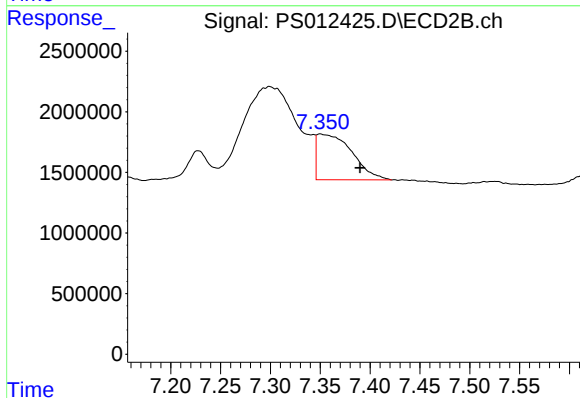


#7 MCPA

R.T.: 7.350 min
Delta R.T.: -0.040 min
Response: 9183303
Conc: 3.83 ug/ml

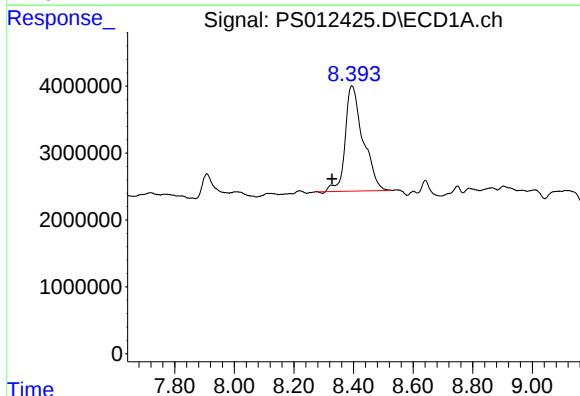


#9 2,4-D

R.T.: 8.394 min
Delta R.T.: 0.066 min
Response: 65595575
Conc: 57.77 ng/ml

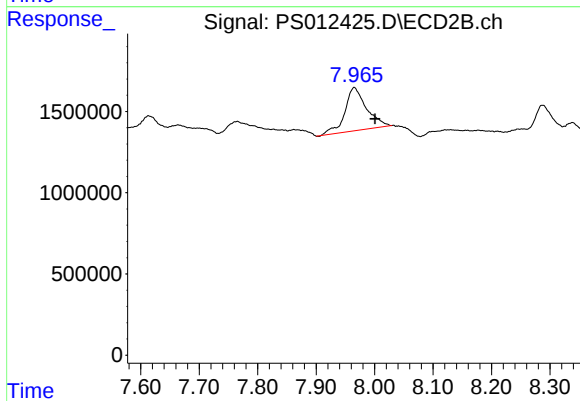


#9 2,4-D

R.T.: 7.965 min
Delta R.T.: -0.036 min
Response: 6834148
Conc: 10.91 ng/ml

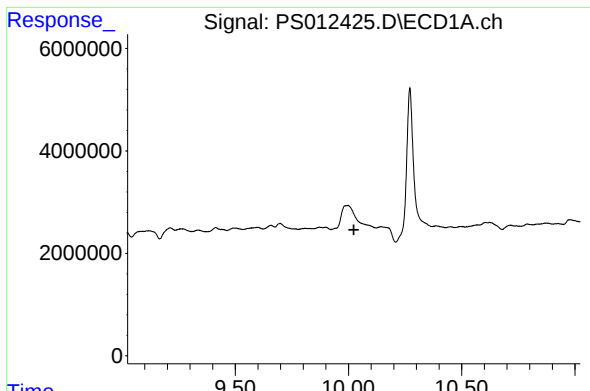

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.024 min
Response: 0
Conc: N.D.

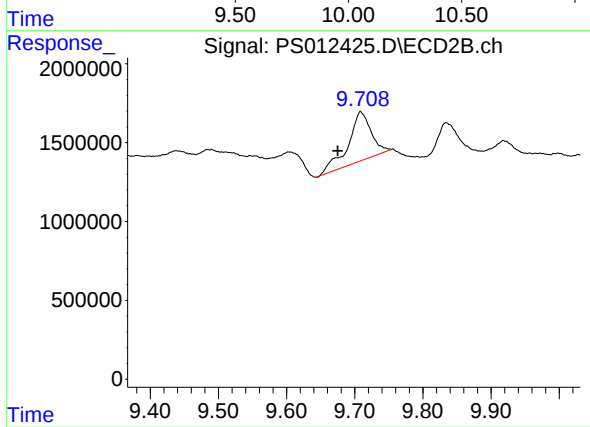

#13 2,4-DB

R.T.: 9.708 min
Delta R.T.: 0.033 min
Response: 7246710
Conc: 19.36 ng/ml