

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092220\
 Data File : PS012426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2020 14:07
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 05:05:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	412.2E6	230.4E6	420.859	500.892
Target Compounds							
9) T	2,4-D	8.397	0.000	61846033	0	54.470	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092220\
Data File : PS012426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2020 14:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 05:05:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

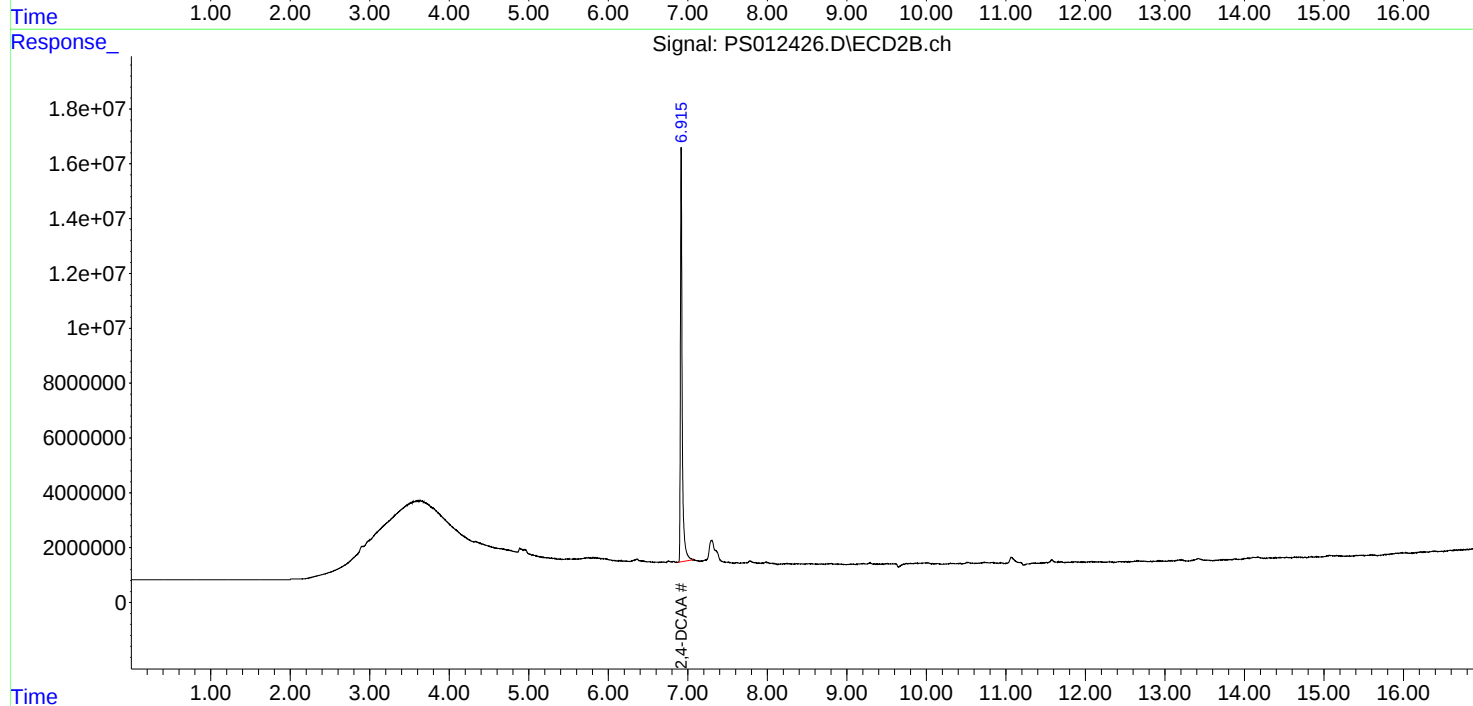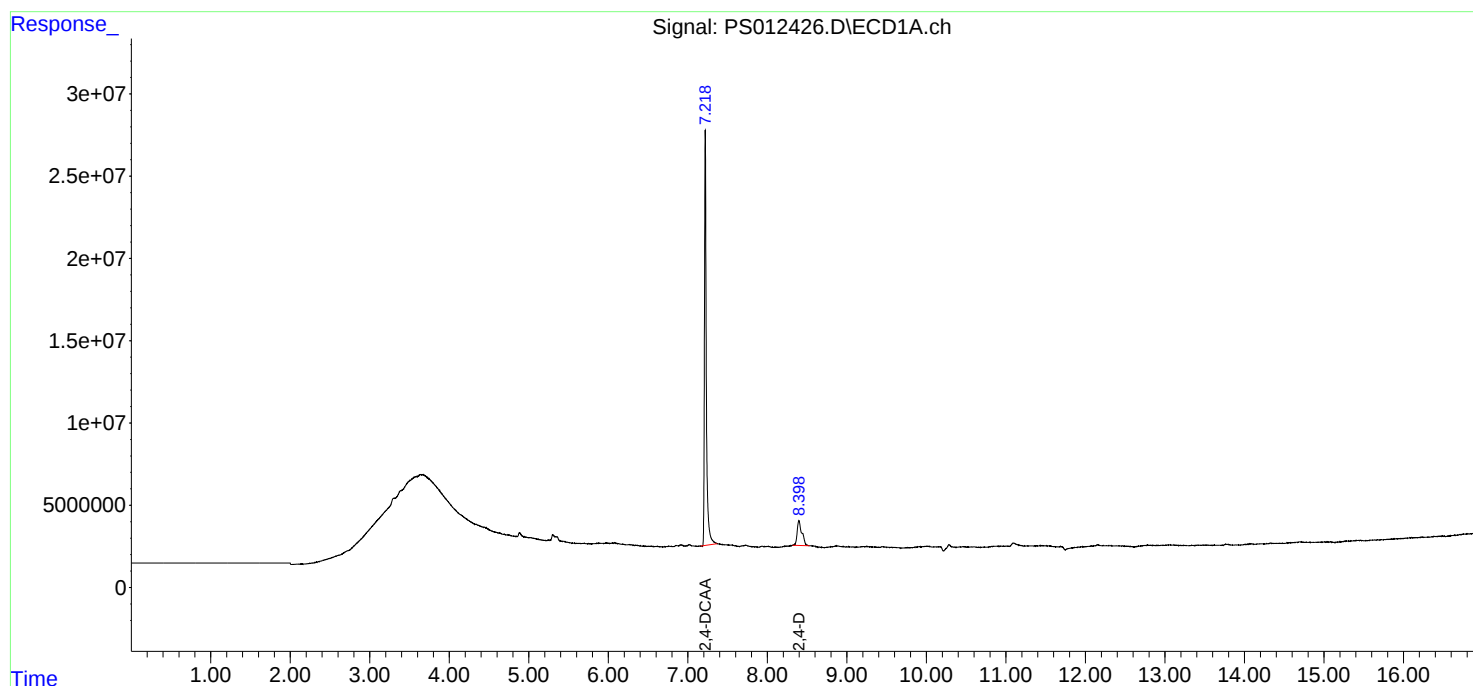

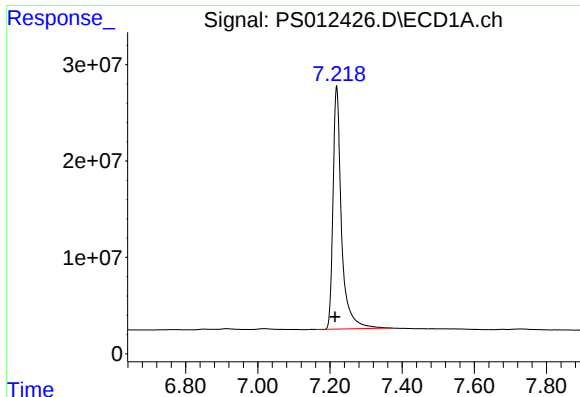


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.004 min
Response: 412209811
Conc: 420.86 ng/ml

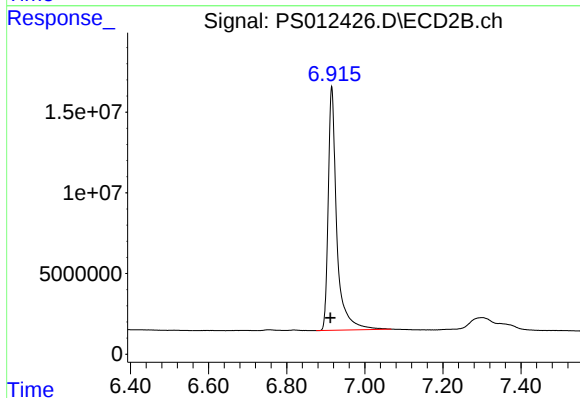


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.003 min
Response: 230418587
Conc: 500.89 ng/ml

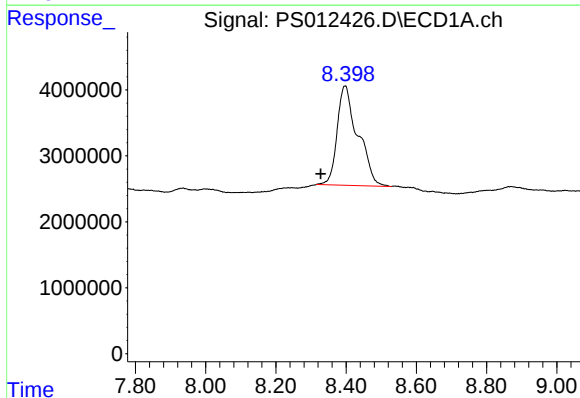

#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.069 min
Response: 61846033
Conc: 54.47 ng/ml

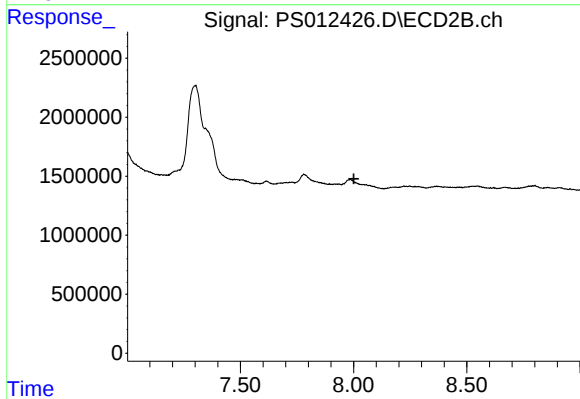

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.