

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092220\
 Data File : PS012429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2020 15:15
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 04:48:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:46:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.215	6.912	709.8E6	331.6E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.032	2.620	757.4E6	398.3E6	682.500	682.500
2) T	3,5-DICHL...	6.430	6.064	910.1E6	481.2E6	697.500	697.500
3) T	4-Nitroph...	7.047	6.522	323.4E6	186.9E6	682.500	682.500
5) T	DICAMBA	7.405	7.079	2649.6E6	1306.5E6	705.000	705.000
6) T	MCPD	7.573	7.175	202.6E6	103.6E6	70.500	70.500
7) T	MCPA	7.722	7.390	284.7E6	158.9E6	69.750	69.750
8) T	DICHLORPROP	8.097	7.705	657.4E6	347.3E6	705.000	705.000
9) T	2,4-D	8.328	8.001	770.2E6	426.4E6	705.000	705.000
10) T	Pentachlo...	8.636	8.428	9577.0E6	4219.3E6	712.500	712.500
11) T	2,4,5-TP ...	9.185	8.789	3840.3E6	1817.9E6	712.500	712.500
12) T	2,4,5-T	9.472	9.169	3895.2E6	1788.5E6	712.500	712.500
13) T	2,4-DB	10.024	9.675	662.8E6	255.8E6	712.500	712.500
14) T	DINOSEB	11.181	10.006	3078.7E6	1306.3E6	705.000	705.000
15) T	Picloram	11.009	10.995	5073.1E6	2741.7E6	712.500	712.500
16) T	DCPA	11.447	10.933	4919.6E6	2303.5E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092220\
Data File : PS012429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2020 15:15
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 04:48:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:46:44 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

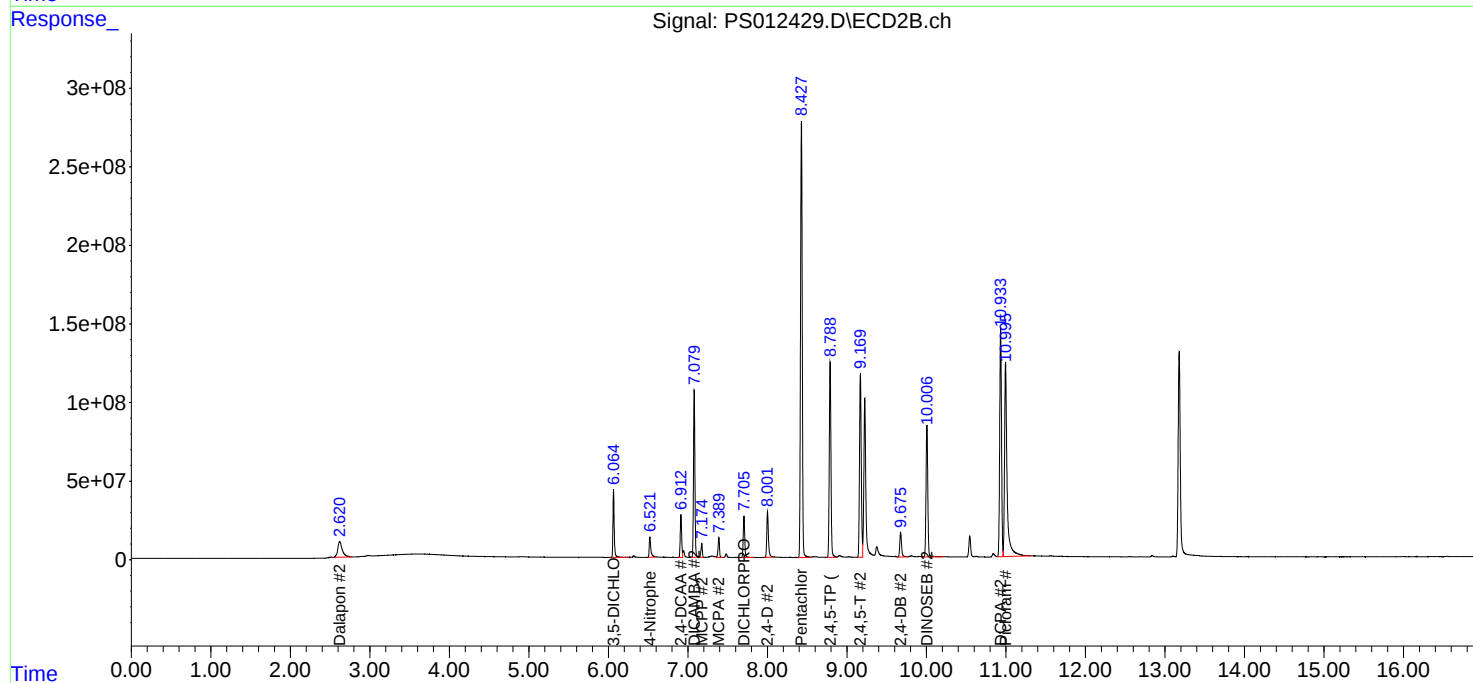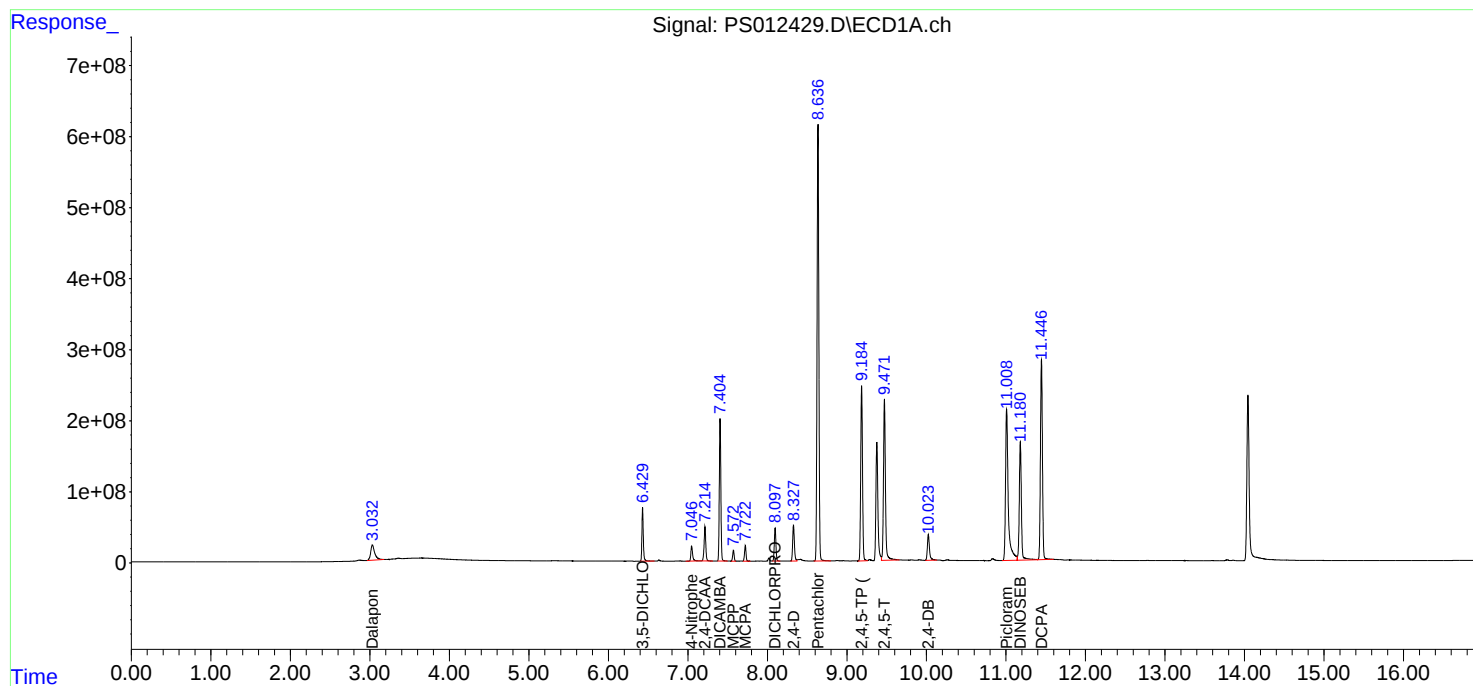


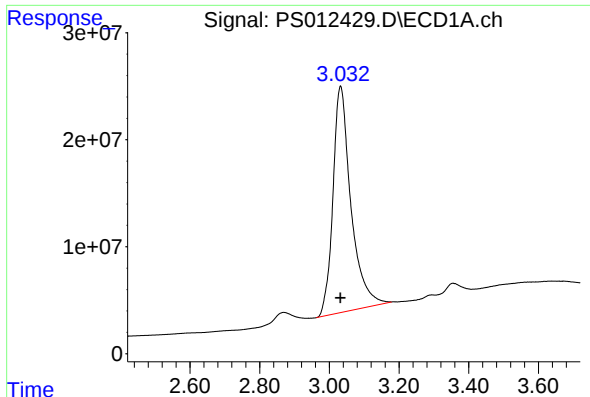

#1 Dalapon


R.T.: 3.032 min
Delta R.T.: 0.000 min
Response: 757440341
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

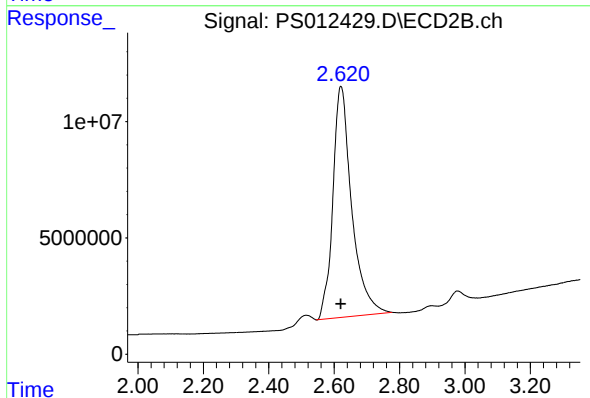


#1 Dalapon

R.T.: 2.620 min
Delta R.T.: 0.000 min
Response: 398275602
Conc: 682.50 ng/ml

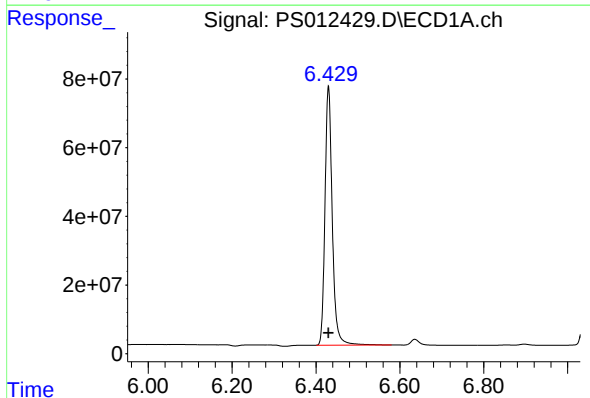


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.430 min
Delta R.T.: 0.000 min
Response: 910102878
Conc: 697.50 ng/ml

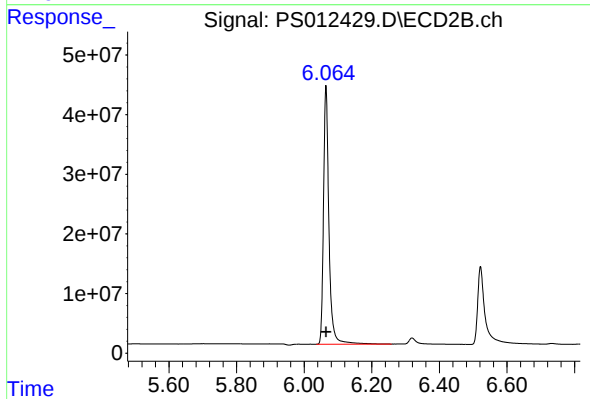

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 481169334
Conc: 697.50 ng/ml

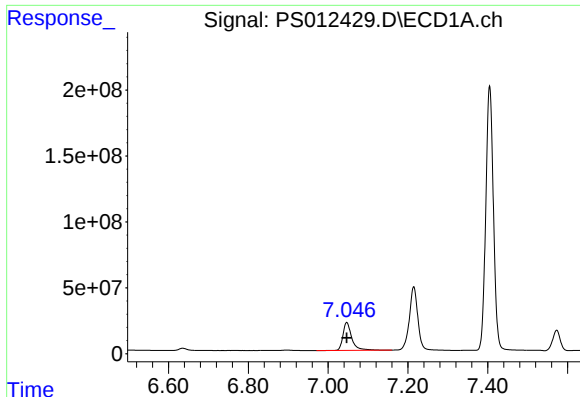

#3 4-Nitrophenol


R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 323401760
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

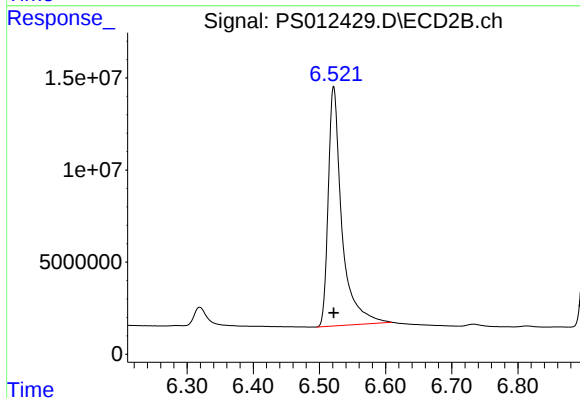


#3 4-Nitrophenol

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 186858053
Conc: 682.50 ng/ml

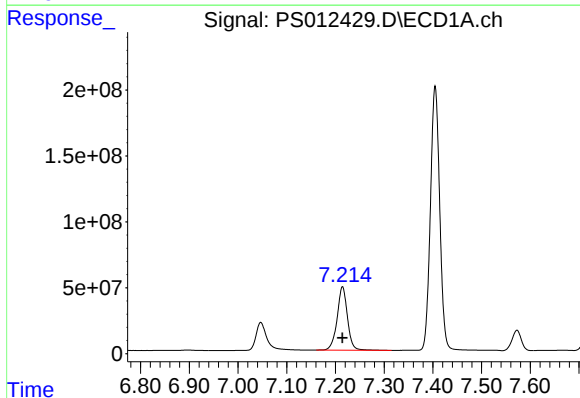


#4 2,4-DCAA

R.T.: 7.215 min
Delta R.T.: 0.000 min
Response: 709804356
Conc: 750.00 ng/ml

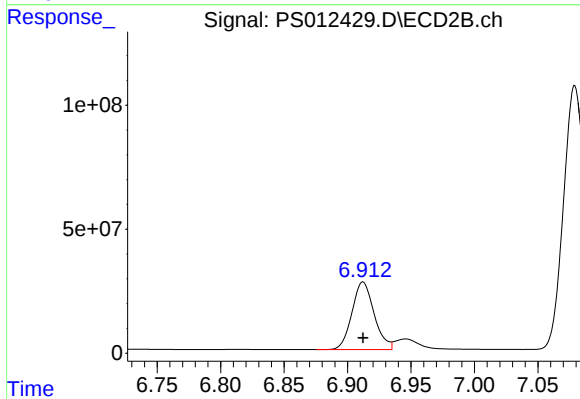

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 331565069
Conc: 750.00 ng/ml

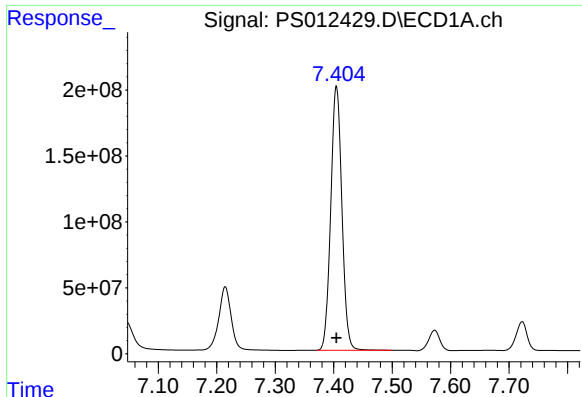

#5 DICAMBA


R.T.: 7.405 min
Delta R.T.: 0.000 min
Response: 2649643556
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

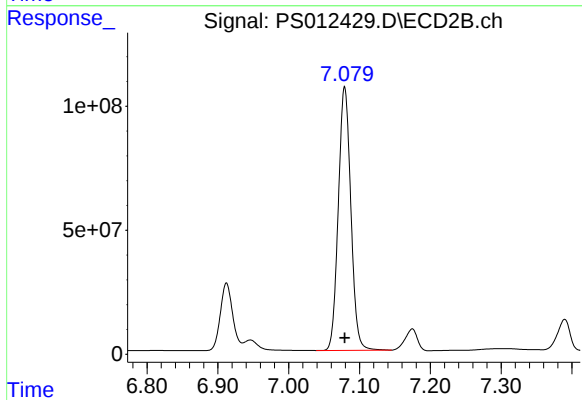


#5 DICAMBA

R.T.: 7.079 min
Delta R.T.: 0.000 min
Response: 1306547863
Conc: 705.00 ng/ml

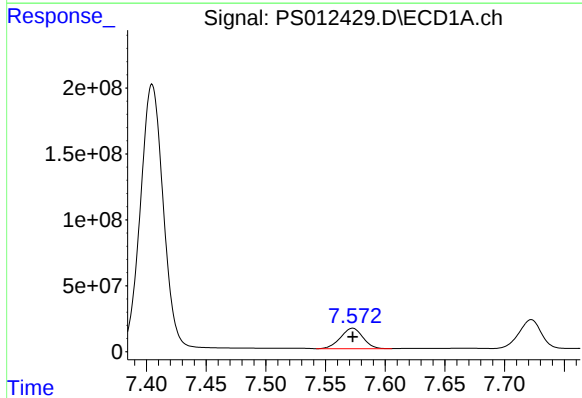


#6 MCP

R.T.: 7.573 min
Delta R.T.: 0.000 min
Response: 202564022
Conc: 70.50 ug/ml

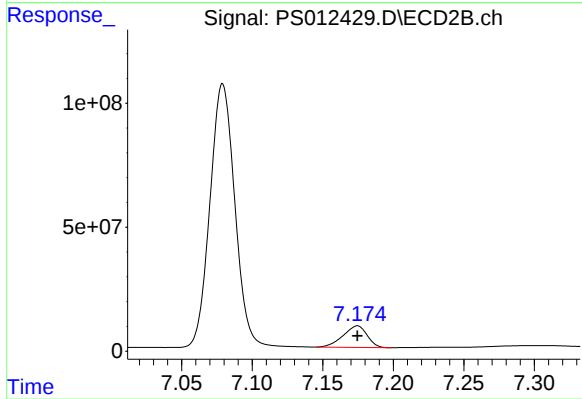

#6 MCP


R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 103614153
Conc: 70.50 ug/ml

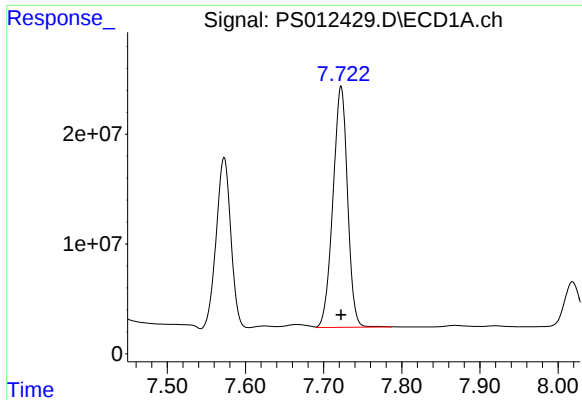

#7 MCPA


R.T.: 7.722 min
Delta R.T.: 0.000 min
Response: 284676630
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

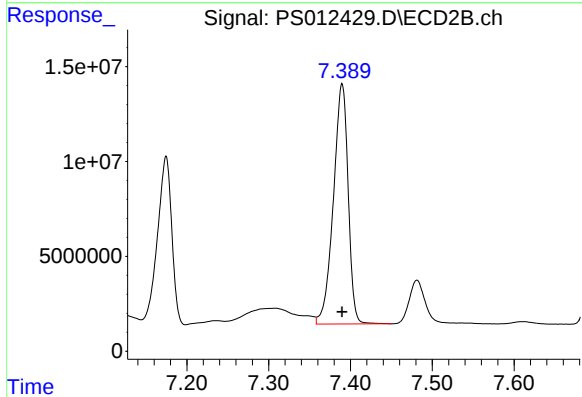


#7 MCPA

R.T.: 7.390 min
Delta R.T.: 0.000 min
Response: 158887987
Conc: 69.75 ug/ml

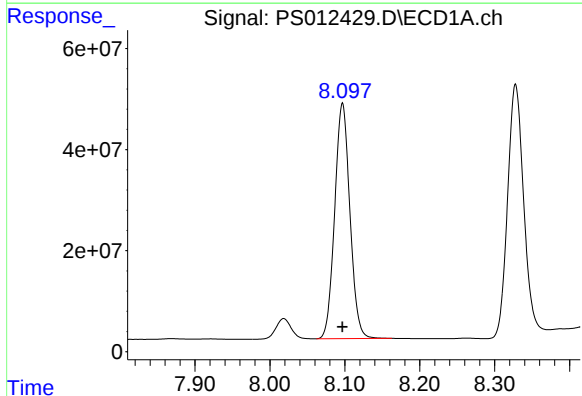


#8 DICHLORPROP

R.T.: 8.097 min
Delta R.T.: 0.000 min
Response: 657426284
Conc: 705.00 ng/ml

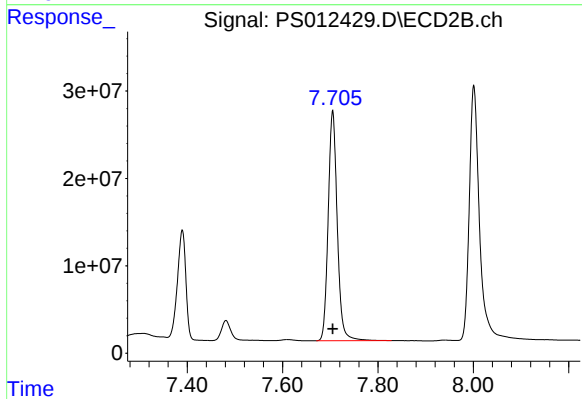

#8 DICHLORPROP


R.T.: 7.705 min
Delta R.T.: 0.000 min
Response: 347330038
Conc: 705.00 ng/ml

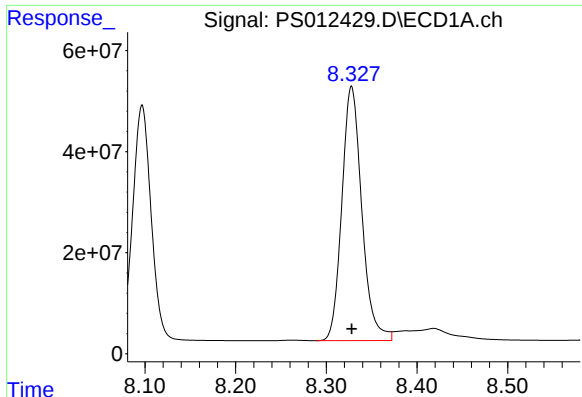

#9 2,4-D


R.T.: 8.328 min
Delta R.T.: 0.000 min
Response: 770158950
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

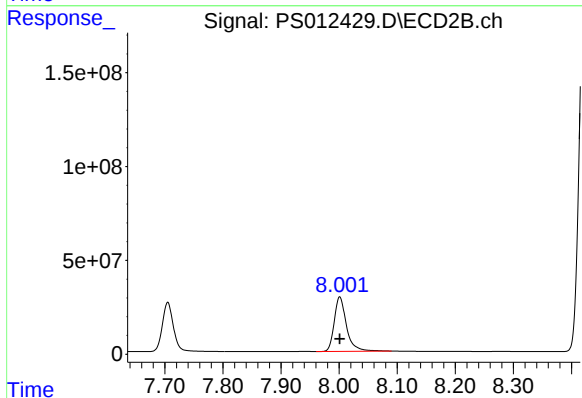


#9 2,4-D

R.T.: 8.001 min
Delta R.T.: 0.000 min
Response: 426392224
Conc: 705.00 ng/ml

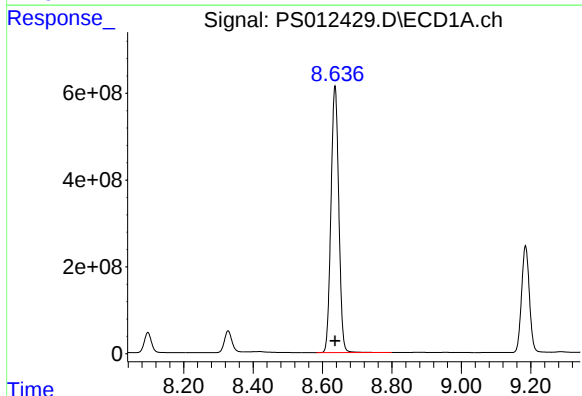


#10 Pentachlorophenol

R.T.: 8.636 min
Delta R.T.: 0.000 min
Response: 9576962242
Conc: 712.50 ng/ml

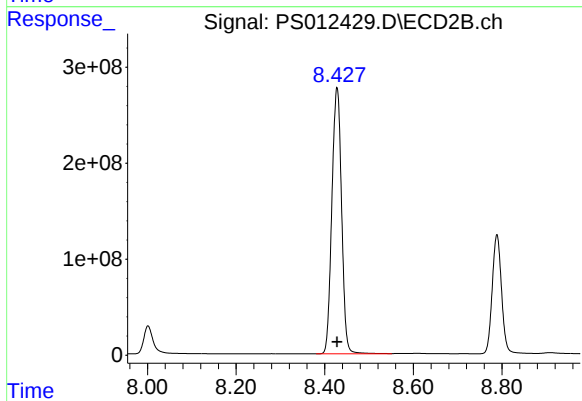

#10 Pentachlorophenol


R.T.: 8.428 min
Delta R.T.: 0.000 min
Response: 4219324223
Conc: 712.50 ng/ml

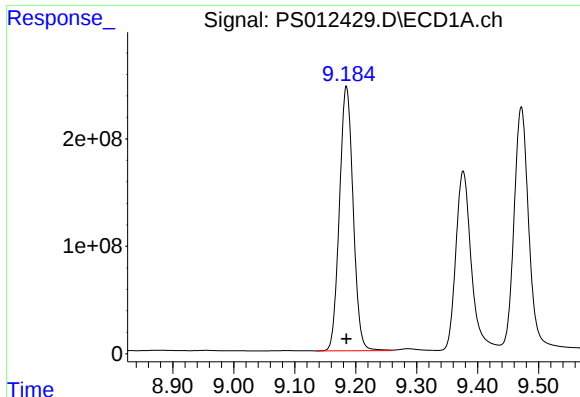

#11 2,4,5-TP (SILVEX)


R.T.: 9.185 min
Delta R.T.: 0.000 min
Response: 3840345090
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

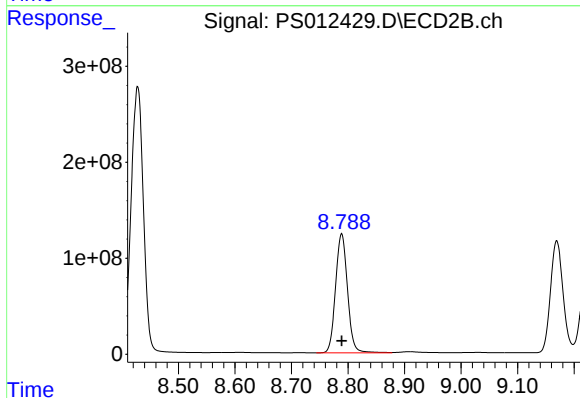


#11 2,4,5-TP (SILVEX)

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 1817883137
Conc: 712.50 ng/ml

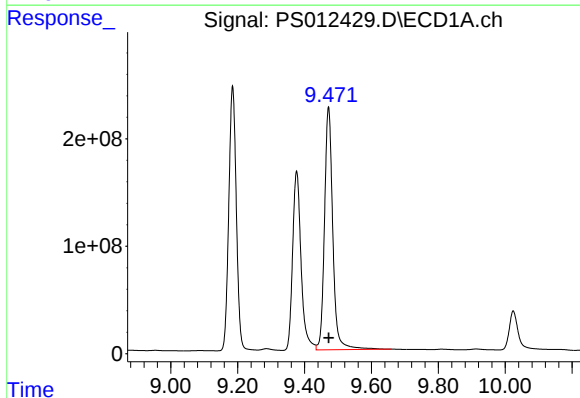


#12 2,4,5-T

R.T.: 9.472 min
Delta R.T.: 0.000 min
Response: 3895187960
Conc: 712.50 ng/ml

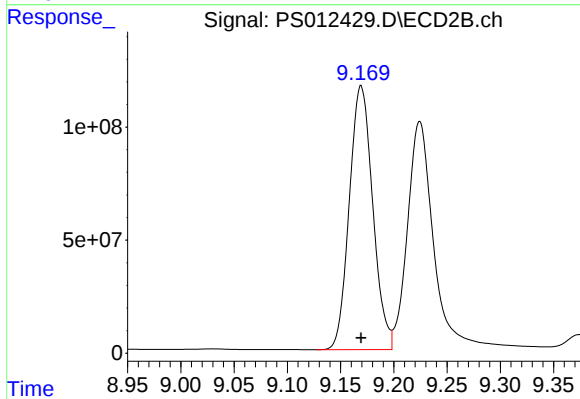

#12 2,4,5-T


R.T.: 9.169 min
Delta R.T.: 0.000 min
Response: 1788499666
Conc: 712.50 ng/ml

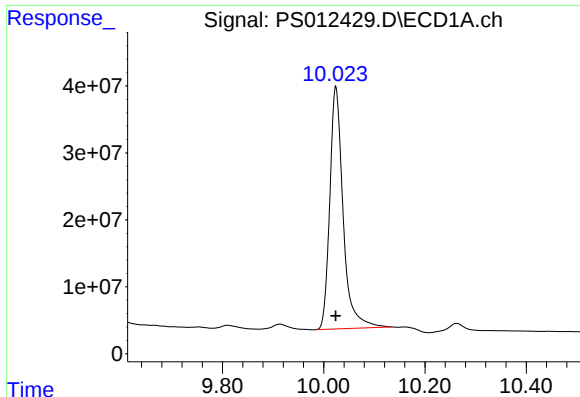

#13 2,4-DB


R.T.: 10.024 min
Delta R.T.: 0.000 min
Response: 662805324
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

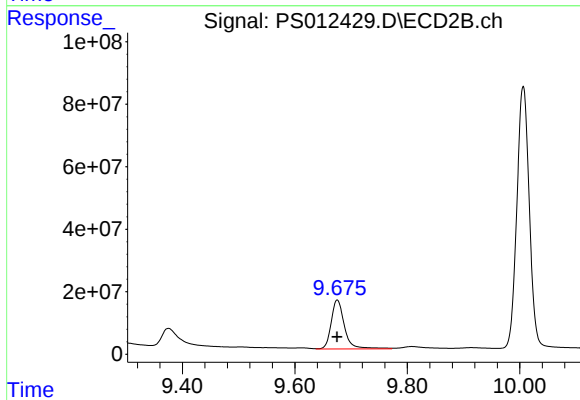


#13 2,4-DB

R.T.: 9.675 min
Delta R.T.: 0.000 min
Response: 255778421
Conc: 712.50 ng/ml

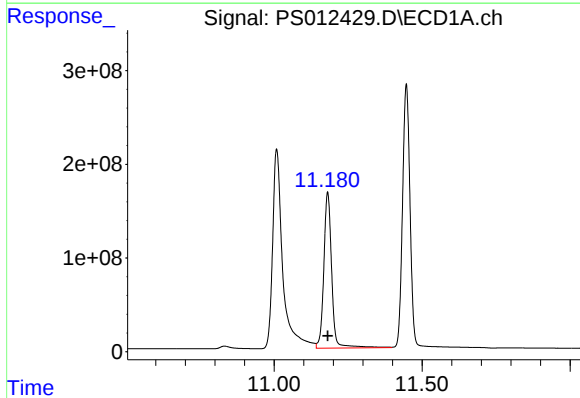


#14 DINOSEB

R.T.: 11.181 min
Delta R.T.: 0.000 min
Response: 3078665201
Conc: 705.00 ng/ml

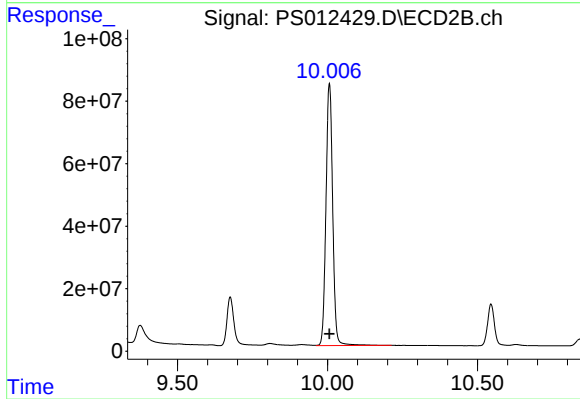

#14 DINOSEB


R.T.: 10.006 min
Delta R.T.: 0.000 min
Response: 1306292514
Conc: 705.00 ng/ml

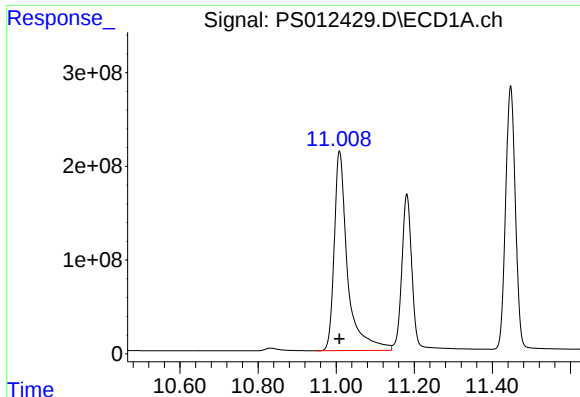

#15 Picloram


R.T.: 11.009 min
Delta R.T.: 0.000 min
Response: 5073089530
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

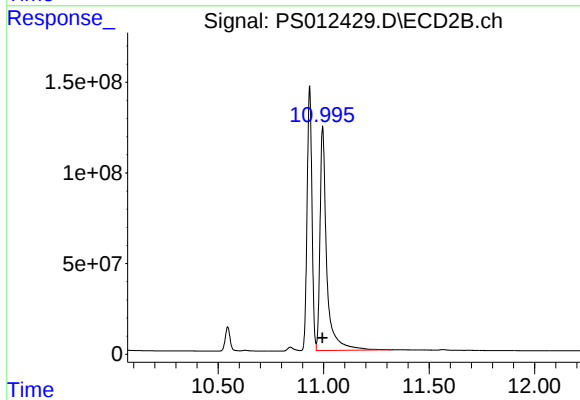


#15 Picloram

R.T.: 10.995 min
Delta R.T.: 0.000 min
Response: 2741672300
Conc: 712.50 ng/ml

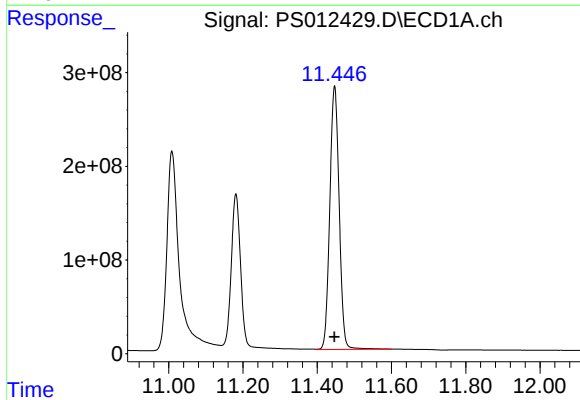

#16 DCPA

R.T.: 11.447 min
Delta R.T.: 0.000 min
Response: 4919570134
Conc: 720.00 ng/ml

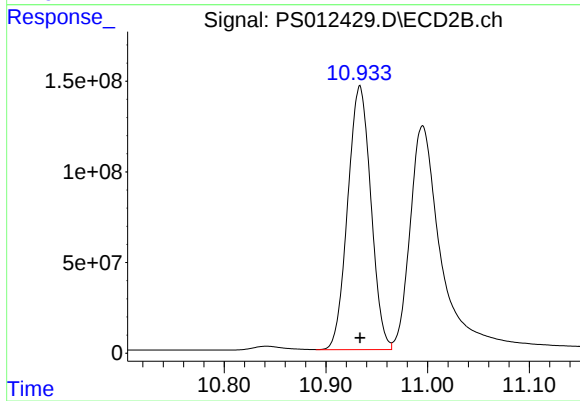

#16 DCPA

R.T.: 10.933 min
Delta R.T.: 0.000 min
Response: 2303533406
Conc: 720.00 ng/ml