

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092223\
 Data File : PS024351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2023 07:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 12:12:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.347	0.000	831196	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.516	2.567	7360521	4696202	3.386	4.453 #
2) T	3,5-DICHL...	5.702	5.942	11598258	105857	3.815	<MDL #
3) T	4-Nitroph...	6.198	6.357f	13520598	91779	10.883	<MDL #
6) T	MCP	6.681	7.070	3793192	34802	<MDL	<MDL #
7) T	MCPA	6.783	0.000	893527	0	<MDL	N.D. #
8) T	DICHLORPROP	7.086	7.574	2805586	2104586	1.234	2.897 #
9) T	2,4-D	7.313	7.915f	17689407	61544	6.650	<MDL #
10) T	Pentachlo...	7.520	8.331f	1065859	114993	<MDL	<MDL #
11) T	2,4,5-TP ...	8.078	8.625	2448469	730733	<MDL	<MDL #
12) T	2,4,5-T	8.296	9.042	1306654	1312859	<MDL	<MDL #
14) T	DINOSEB	9.859	0.000	2213981	0	<MDL	N.D. #
15) T	Picloram	9.661	10.786	49278985	17085453	3.017	2.877
16) T	DCPA	10.111	10.786	2205386	17085453	<MDL	3.331 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092223\
Data File : PS024351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2023 07:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 12:12:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

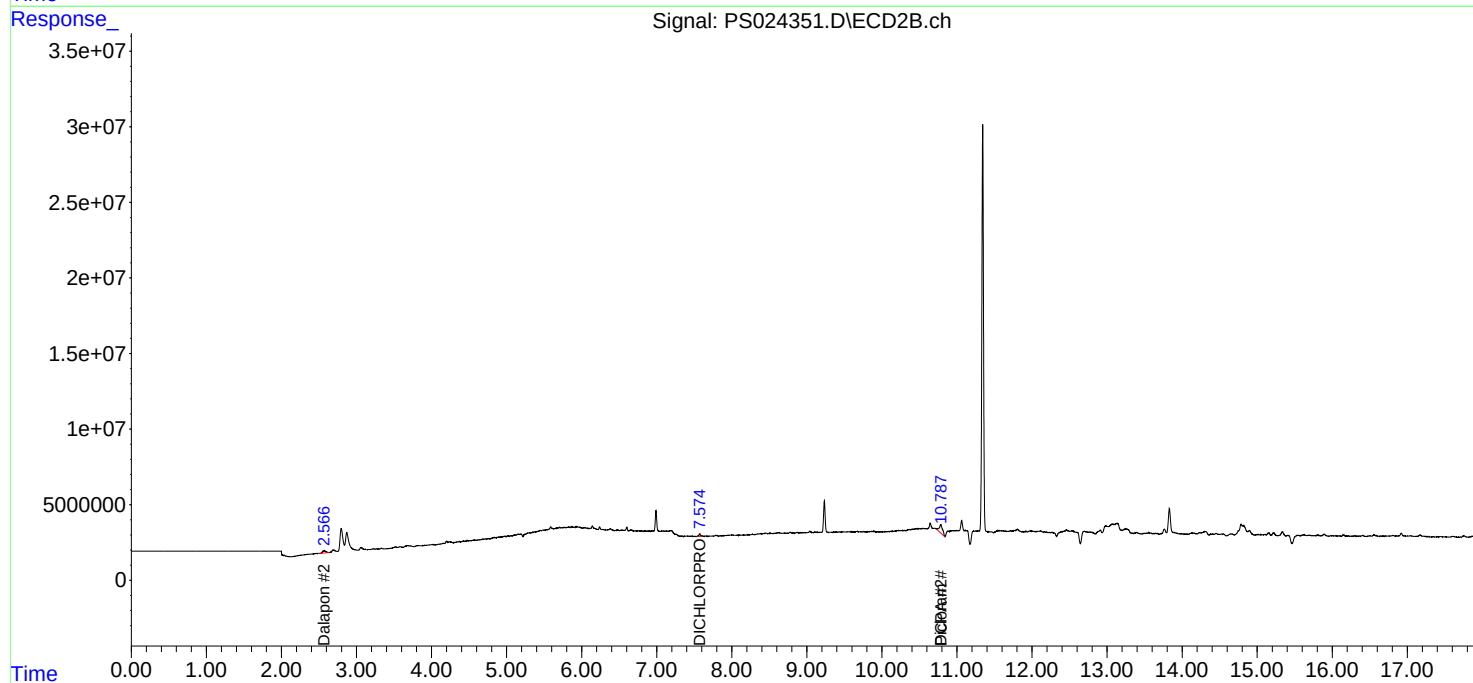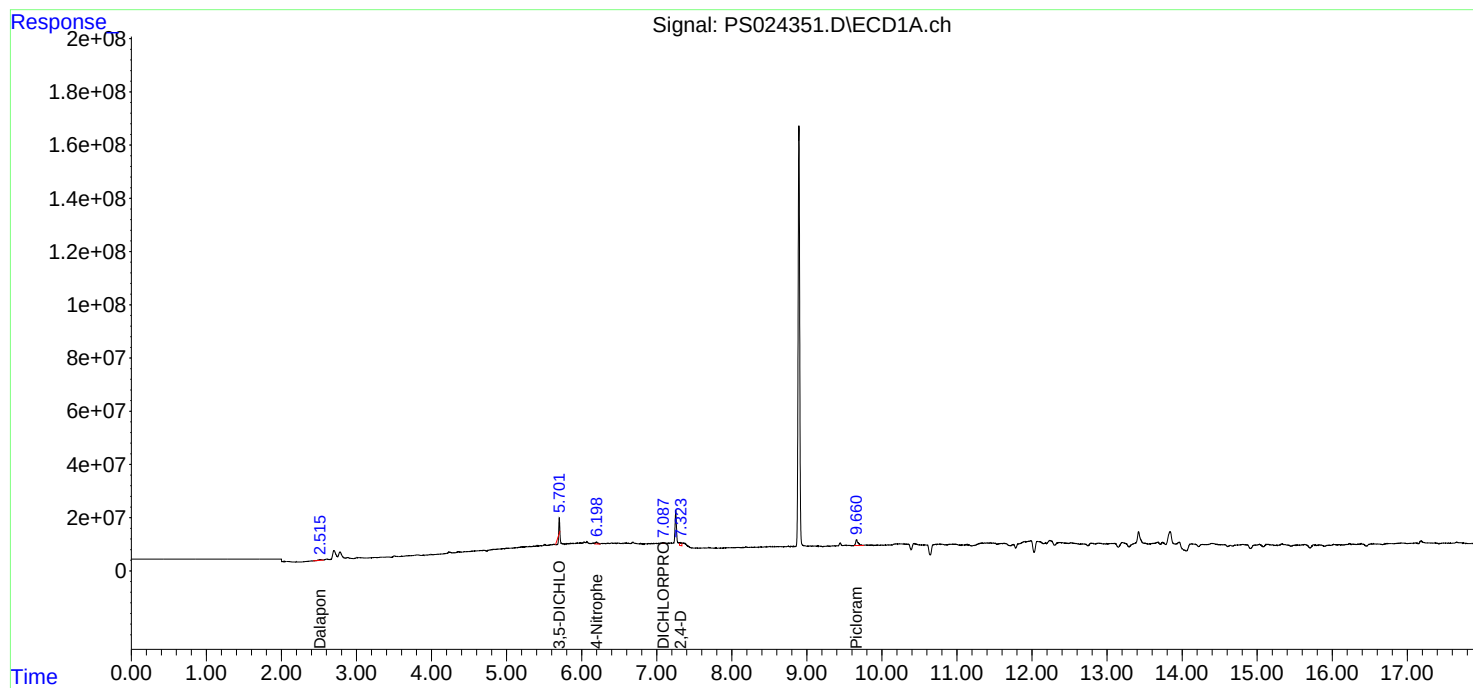


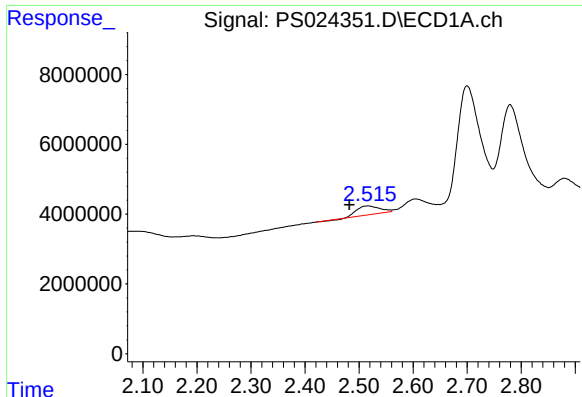

#1 Dalapon


R.T.: 2.516 min
Delta R.T.: 0.034 min
Response: 7360521
Conc: 3.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

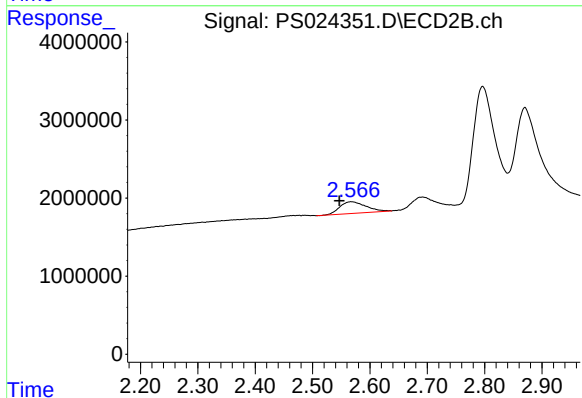


#1 Dalapon

R.T.: 2.567 min
Delta R.T.: 0.020 min
Response: 4696202
Conc: 4.45 ng/ml

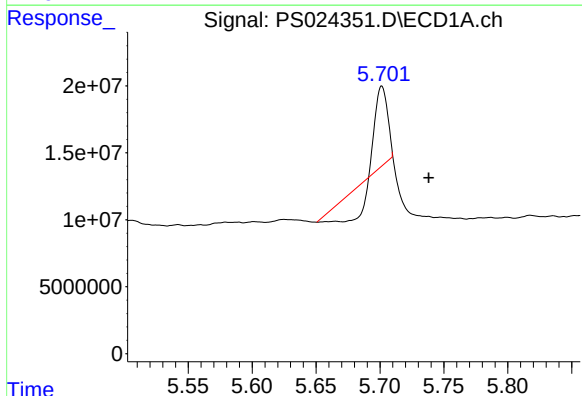


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.702 min
Delta R.T.: -0.036 min
Response: 11598258
Conc: 3.82 ng/ml

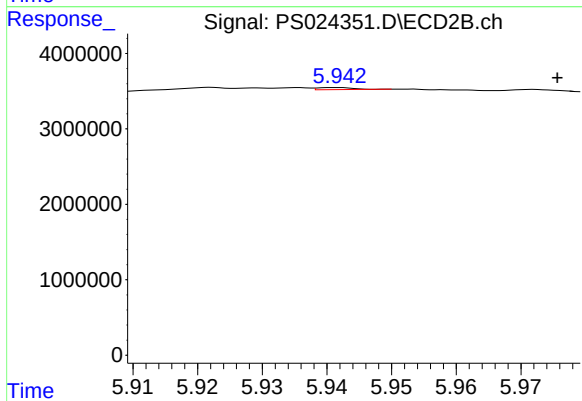

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.942 min
Delta R.T.: -0.034 min
Response: 105857
Conc: N.D.

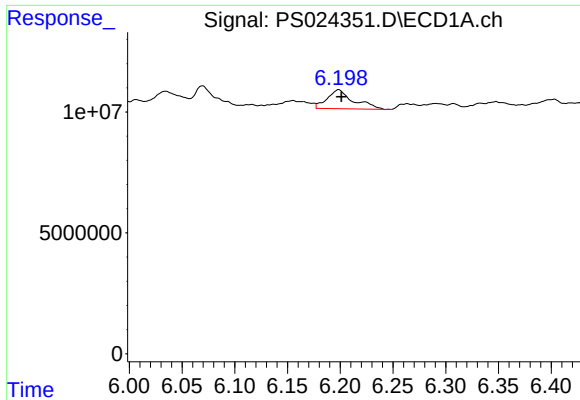

#3 4-Nitrophenol


R.T.: 6.198 min
Delta R.T.: -0.003 min
Response: 13520598
Conc: 10.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

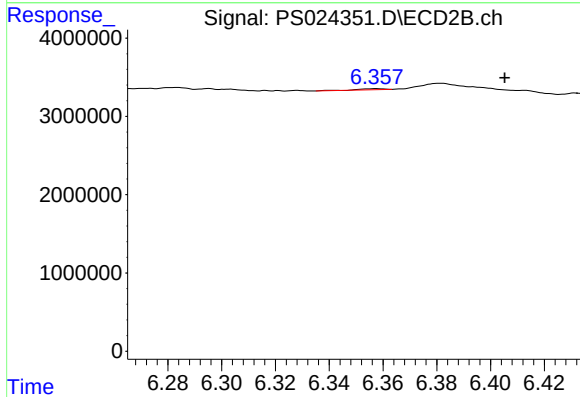


#3 4-Nitrophenol

R.T.: 6.357 min
Delta R.T.: -0.048 min
Response: 91779
Conc: N.D.

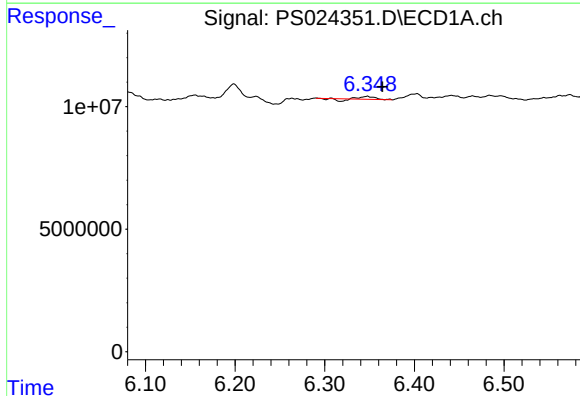


#4 2,4-DCAA

R.T.: 6.347 min
Delta R.T.: -0.017 min
Response: 831196
Conc: N.D.

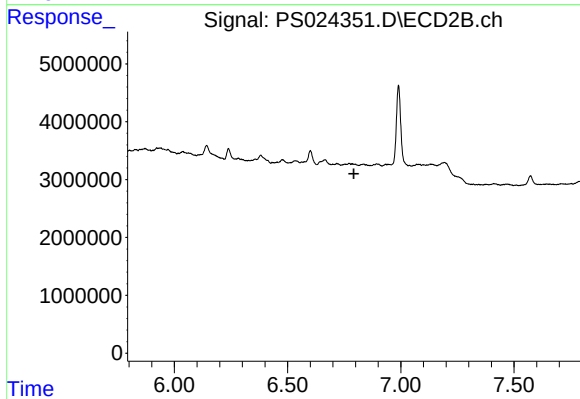

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.793 min
Response: 0
Conc: N.D.

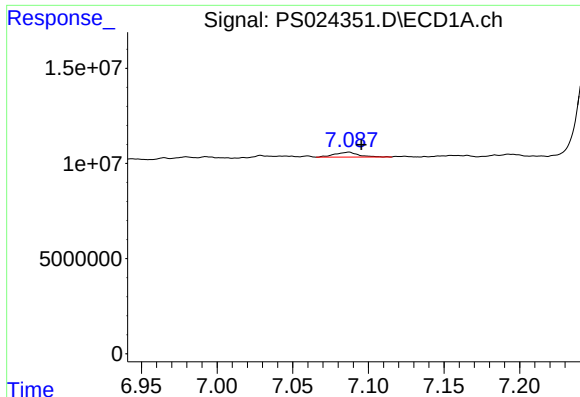

#8 DICHLORPROP


R.T.: 7.086 min
Delta R.T.: -0.009 min
Response: 2805586
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

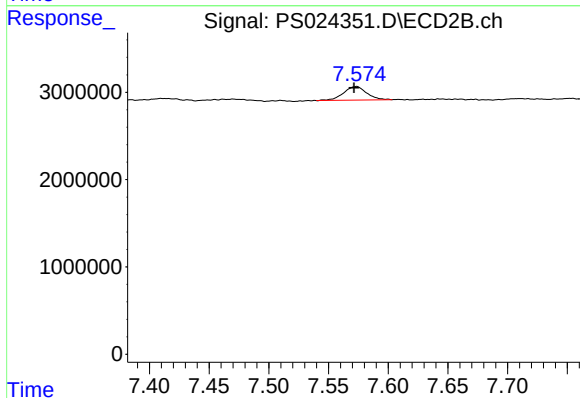


#8 DICHLORPROP

R.T.: 7.574 min
Delta R.T.: 0.002 min
Response: 2104586
Conc: 2.90 ng/ml

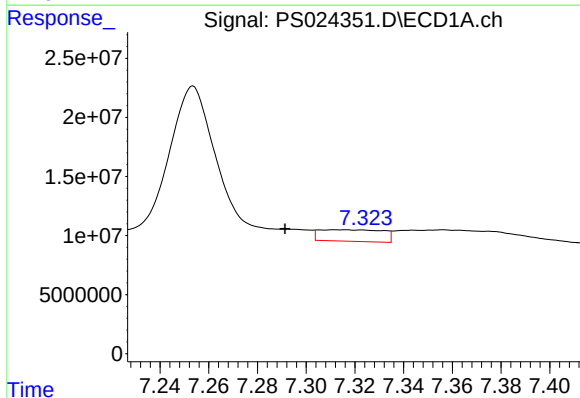


#9 2,4-D

R.T.: 7.313 min
Delta R.T.: 0.022 min
Response: 17689407
Conc: 6.65 ng/ml

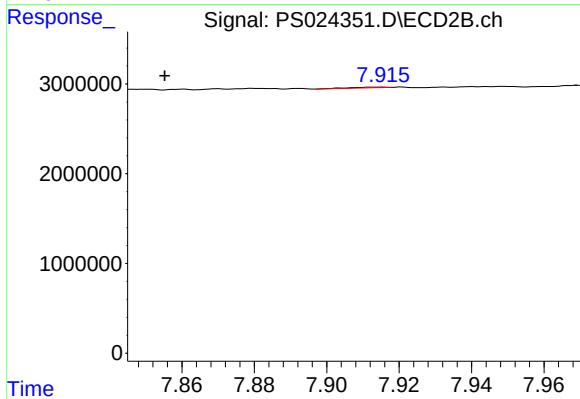

#9 2,4-D


R.T.: 7.915 min
Delta R.T.: 0.060 min
Response: 61544
Conc: N.D.

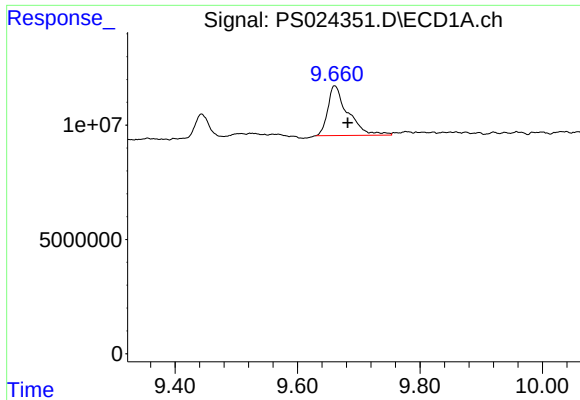

#15 Picloram


R.T.: 9.661 min
Delta R.T.: -0.021 min
Response: 49278985
Conc: 3.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

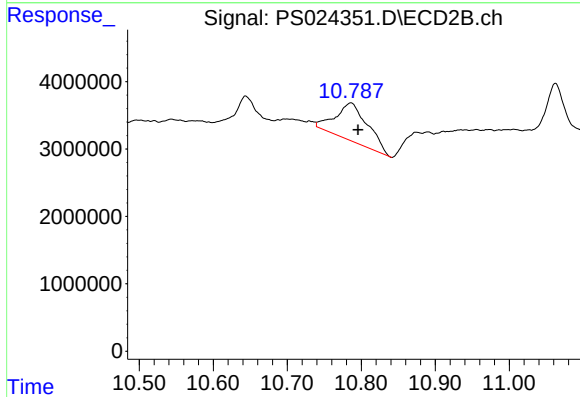


#15 Picloram

R.T.: 10.786 min
Delta R.T.: -0.010 min
Response: 17085453
Conc: 2.88 ng/ml

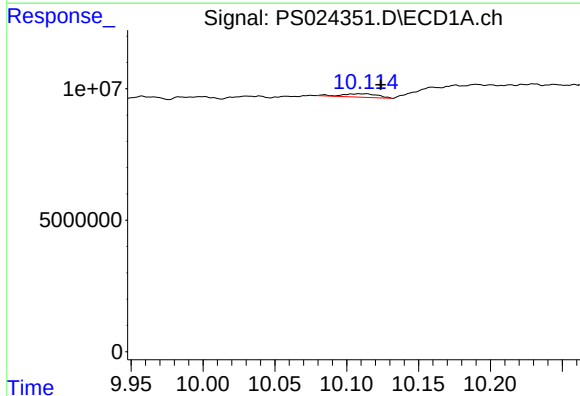

#16 DCPA

R.T.: 10.111 min
Delta R.T.: -0.013 min
Response: 2205386
Conc: N.D.

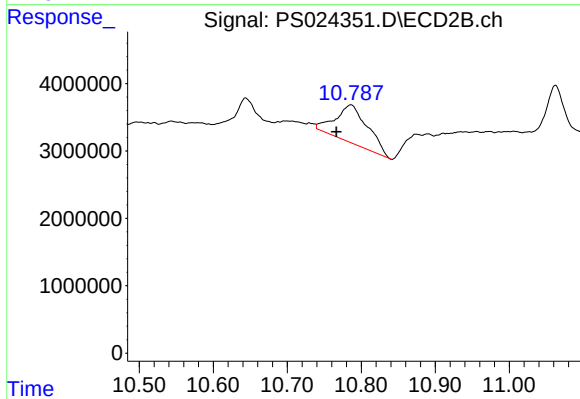

#16 DCPA

R.T.: 10.786 min
Delta R.T.: 0.020 min
Response: 17085453
Conc: 3.33 ng/ml