

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092225\
 Data File : PS031812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2025 05:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 05:59:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.747	1831.4E6	503.4E6	508.518	553.907
Target Compounds							
1) T	Dalapon	0.000	2.661f	0	72307590	N.D.	25.663
2) T	3,5-DICHL...	6.449	0.000	5562675	0	1.043	N.D. #
3) T	4-Nitroph...	7.074	0.000	7670130	0	6.953	N.D. #
7) T	MCPA	7.759f	8.244f	36431645	33539743	3.279	11.973 #
8) T	DICHLORPROP	8.194	0.000	1424335	0	<MDL	N.D. #
10) T	Pentachlo...	8.710	9.514	10059578	5756025	<MDL	<MDL #
11) T	2,4,5-TP ...	9.295	9.911	7844719	3237673	<MDL	<MDL #
12) T	2,4,5-T	9.627f	0.000	5712882	0	<MDL	N.D. #
13) T	2,4-DB	10.117f	0.000	4322055	0	1.853	N.D. #
14) T	DINOSEB	11.356	0.000	4788471	0	<MDL	N.D. #
15) T	Picloram	11.177	0.000	6312756	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092225\
Data File : PS031812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2025 05:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 05:59:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

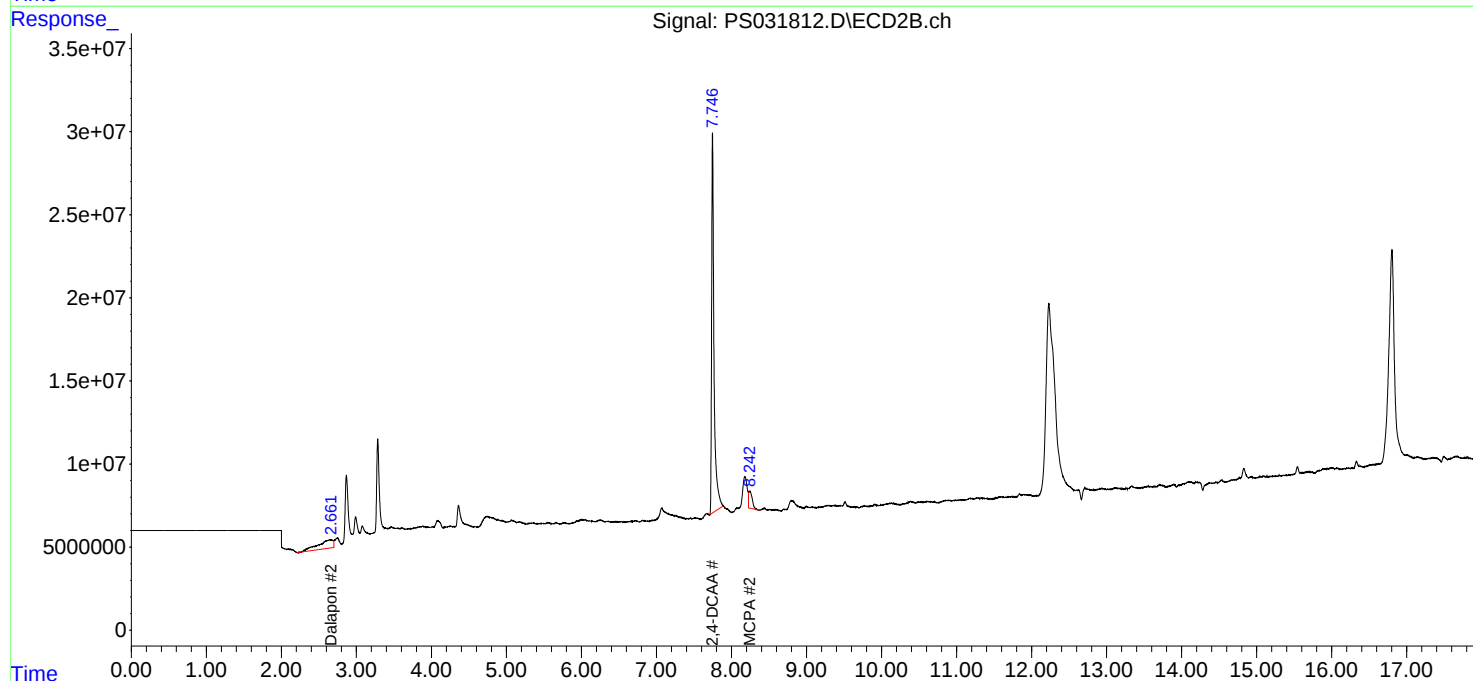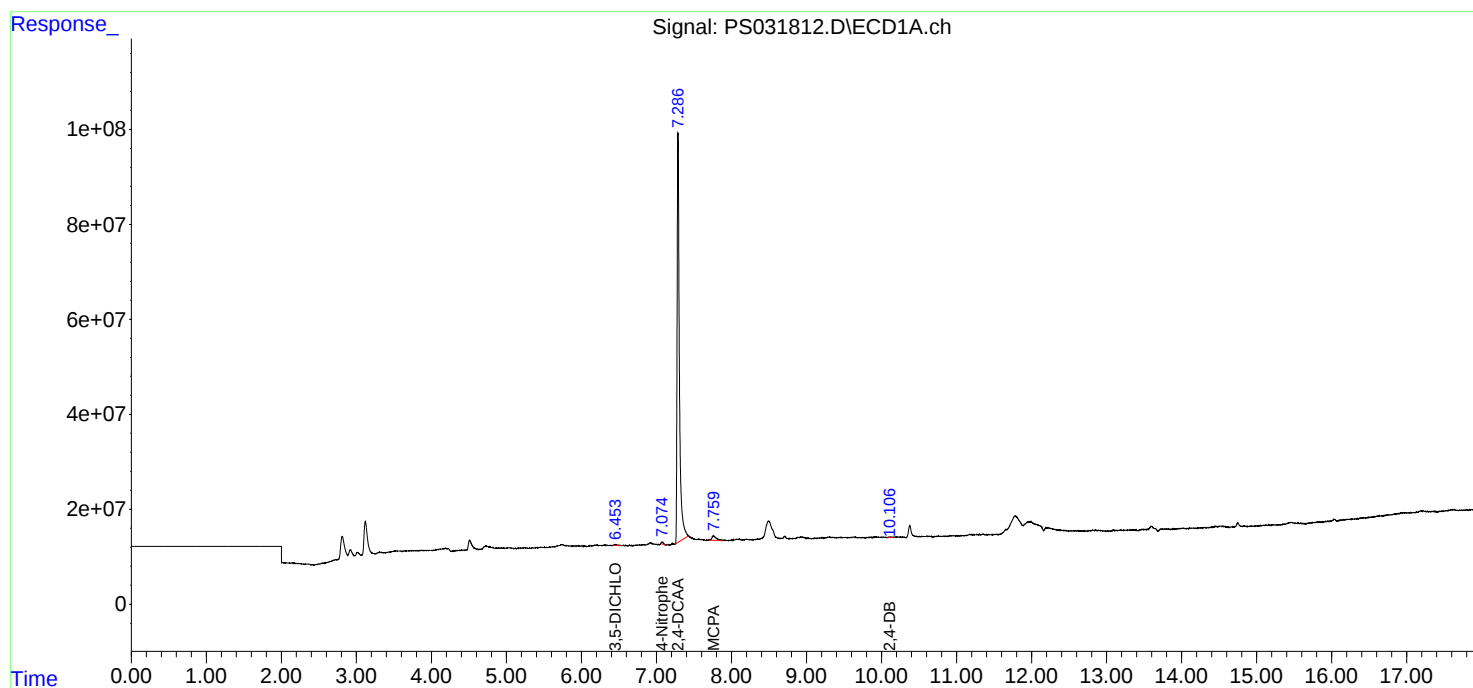


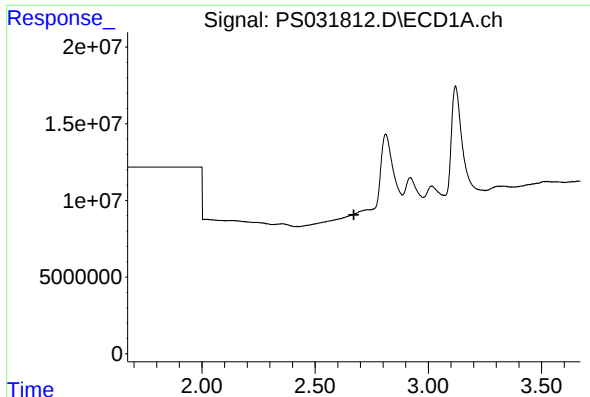

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

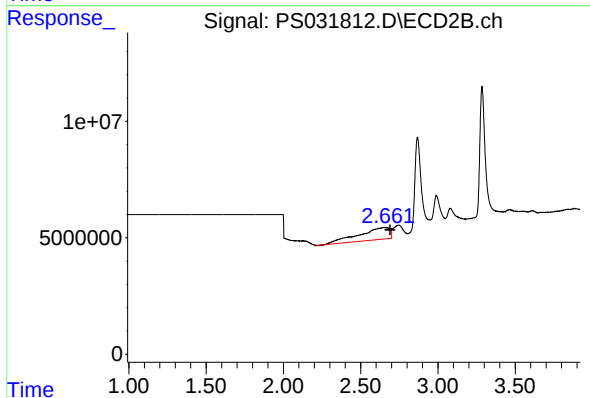


#1 Dalapon

R.T.: 2.661 min
Delta R.T.: -0.031 min
Response: 72307590
Conc: 25.66 ng/ml

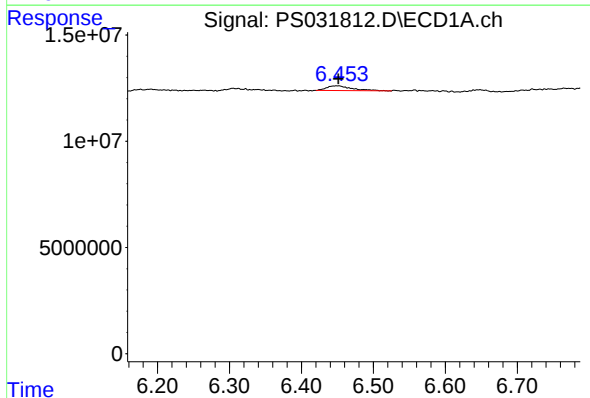


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.449 min
Delta R.T.: -0.002 min
Response: 5562675
Conc: 1.04 ng/ml

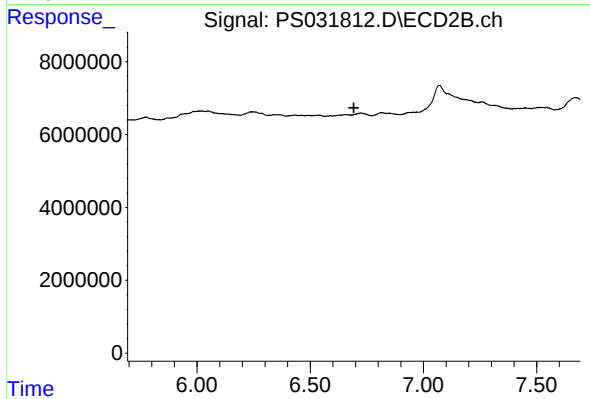

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

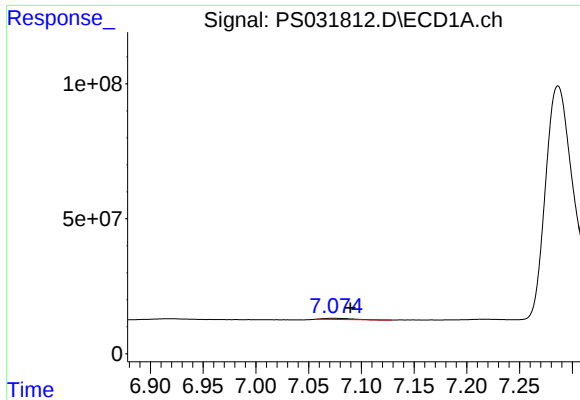

#3 4-Nitrophenol


R.T.: 7.074 min
Delta R.T.: -0.016 min
Response: 7670130
Conc: 6.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

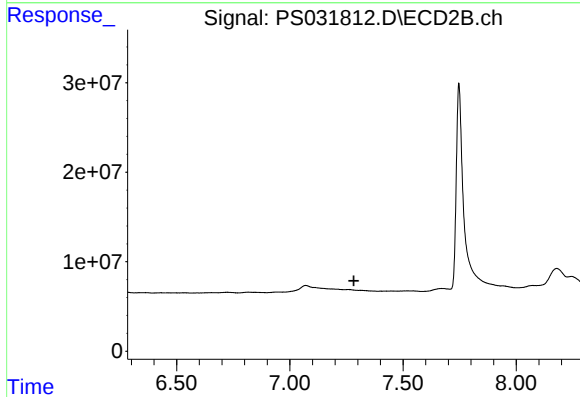


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

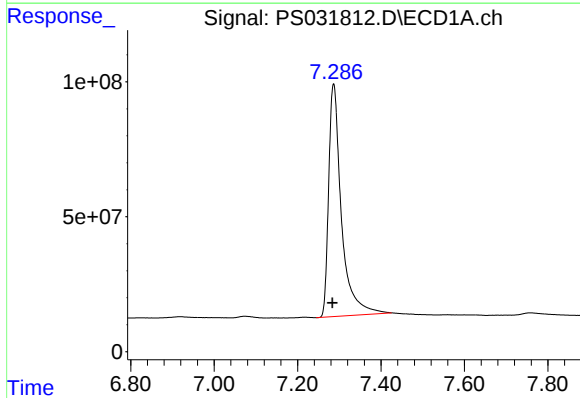


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: 0.003 min
Response: 1831440303
Conc: 508.52 ng/ml

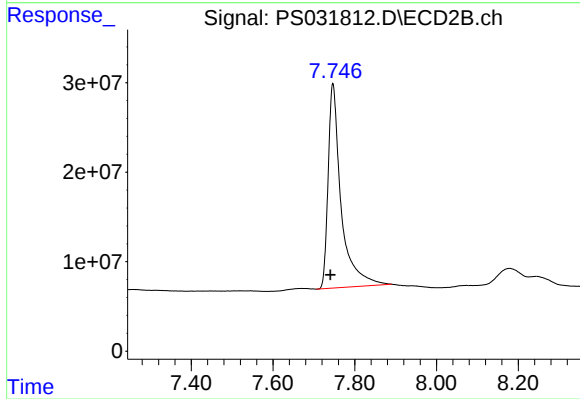

#4 2,4-DCAA


R.T.: 7.747 min
Delta R.T.: 0.006 min
Response: 503445981
Conc: 553.91 ng/ml

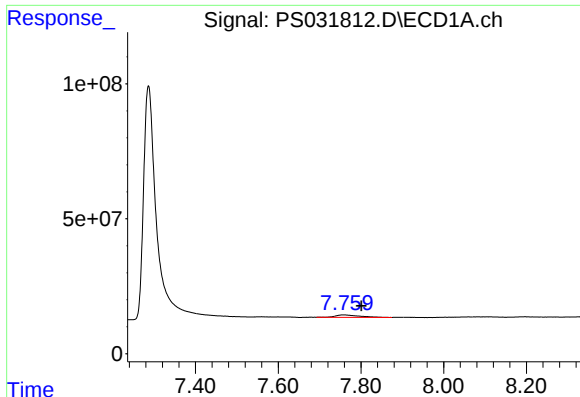

#7 MCPA


R.T.: 7.759 min
Delta R.T.: -0.043 min
Response: 36431645
Conc: 3.28 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

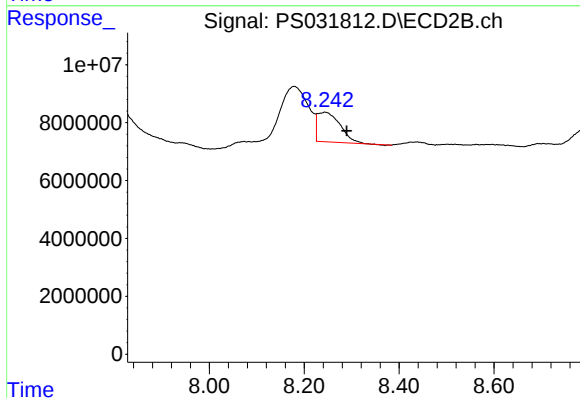


#7 MCPA

R.T.: 8.244 min
Delta R.T.: -0.046 min
Response: 33539743
Conc: 11.97 ug/ml

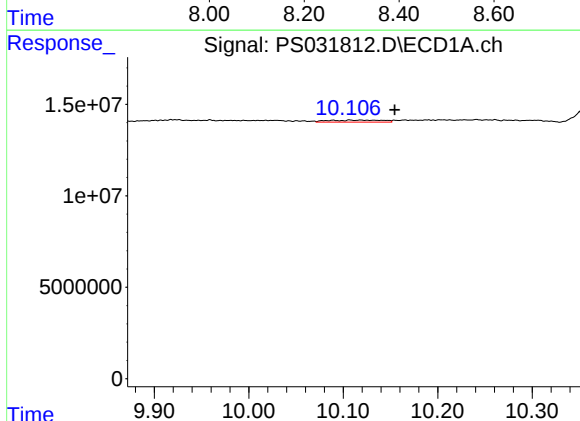

#13 2,4-DB

R.T.: 10.117 min
Delta R.T.: -0.038 min
Response: 4322055
Conc: 1.85 ng/ml

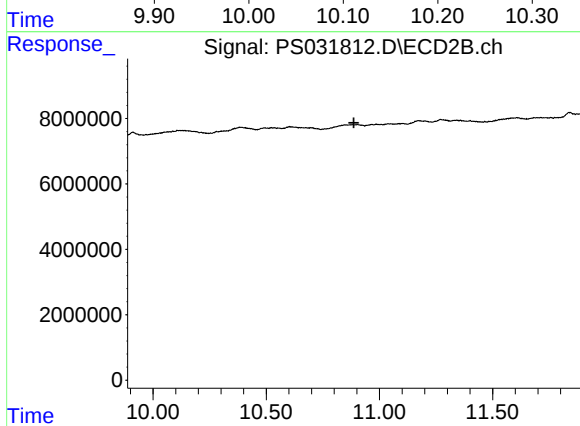

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.887 min
Response: 0
Conc: N.D.