

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
 Data File : PS001799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2018 14:57
 Operator : EI\SJ
 Sample : PB113122BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:26:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.463	10.953	105.4E6	107.0E6	469.773	421.408
Target Compounds							
1) T	Dalapon	2.891	2.364	14270048	35817157	43.885	121.243 #
2) T	3,5-DICHL...	0.000	9.190	0	17114108	N.D.	54.222 #
6) T	MCP	12.152	0.000	19606313	0	30.768	N.D. #
9) T	2,4-D	13.327	0.000	687677	0	2.495	N.D. #
15) T	Picloram	16.979	16.890	11528841	28029038	6.621	16.480 #
16) T	DCPA	0.000	16.890	0	28029038	N.D.	15.197 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
Data File : PS001799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2018 14:57
Operator : EI\SJ
Sample : PB113122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:26:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

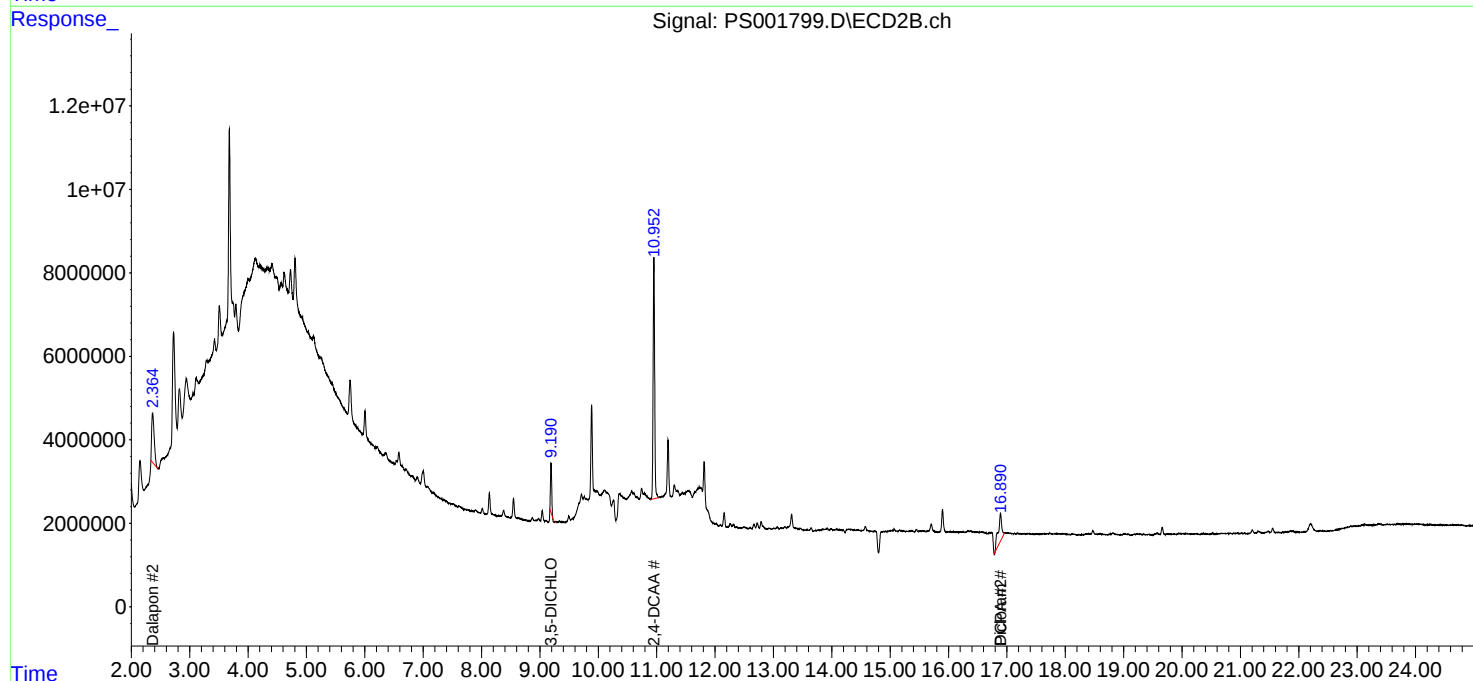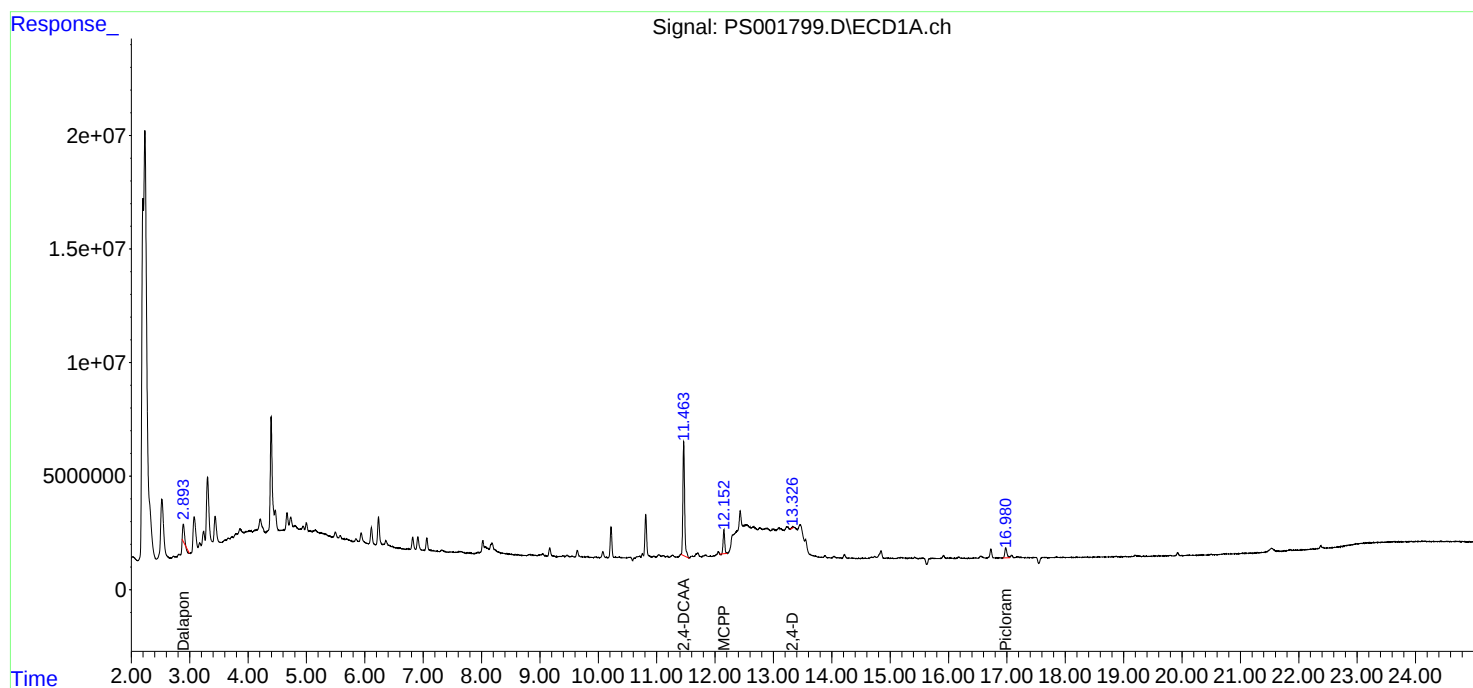


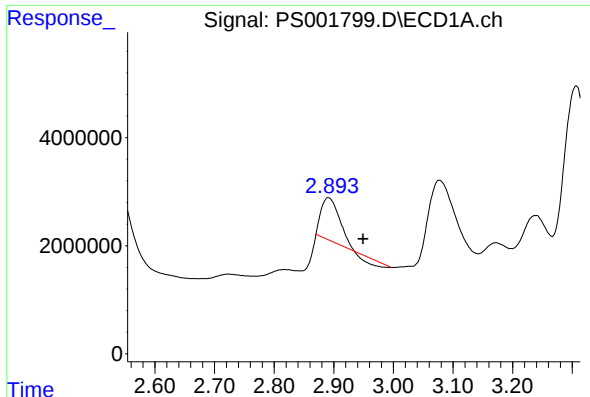

#1 Dalapon


R.T.: 2.891 min
Delta R.T.: -0.058 min
Response: 14270048
Conc: 43.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

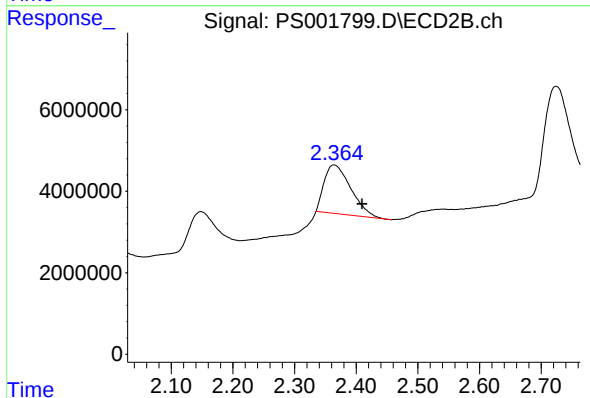


#1 Dalapon

R.T.: 2.364 min
Delta R.T.: -0.045 min
Response: 35817157
Conc: 121.24 ng/ml

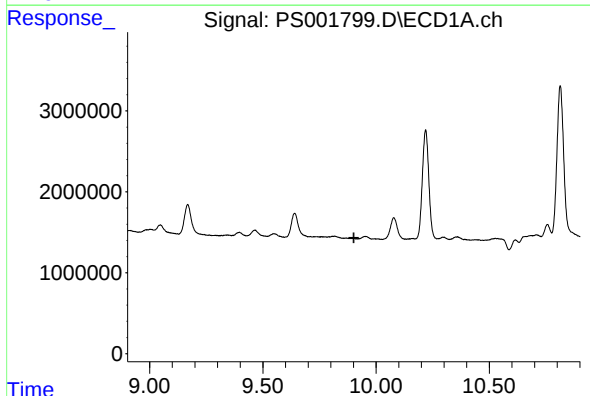


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

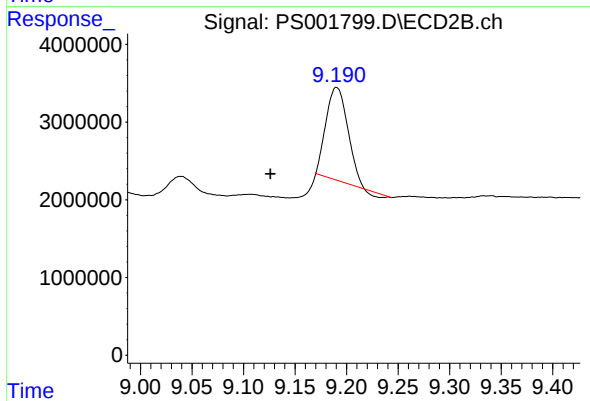

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.190 min
Delta R.T.: 0.064 min
Response: 17114108
Conc: 54.22 ng/ml

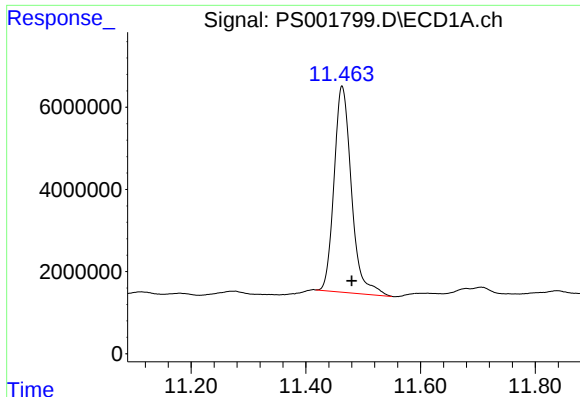

#4 2,4-DCAA


R.T.: 11.463 min
Delta R.T.: -0.016 min
Response: 105377453
Conc: 469.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

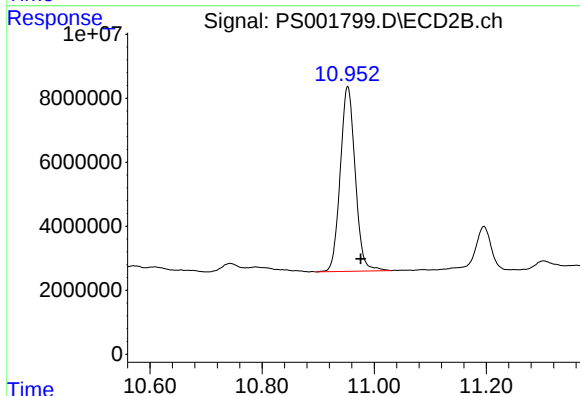


#4 2,4-DCAA

R.T.: 10.953 min
Delta R.T.: -0.023 min
Response: 107044613
Conc: 421.41 ng/ml

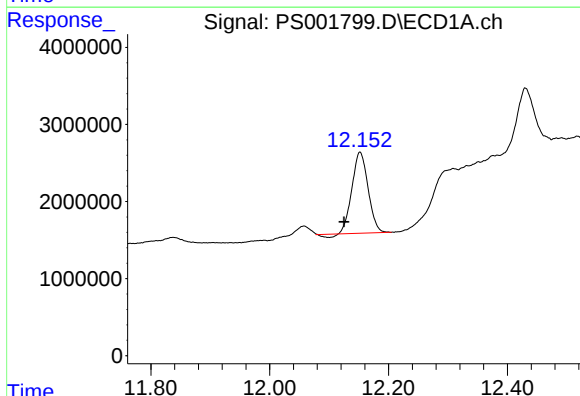


#6 MCP

R.T.: 12.152 min
Delta R.T.: 0.027 min
Response: 19606313
Conc: 30.77 ug/ml

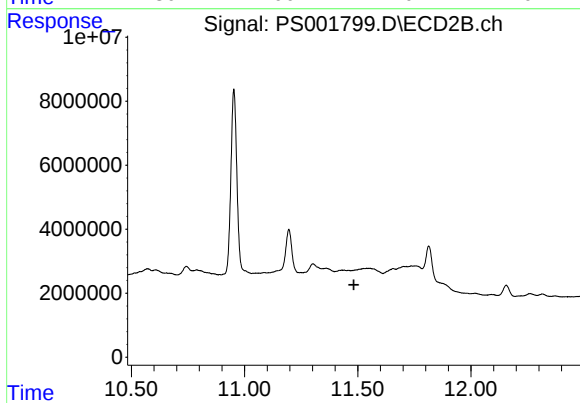

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

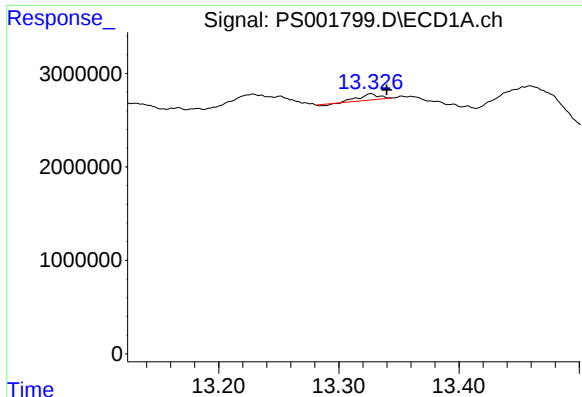

#9 2,4-D


R.T.: 13.327 min
Delta R.T.: -0.013 min
Response: 687677
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

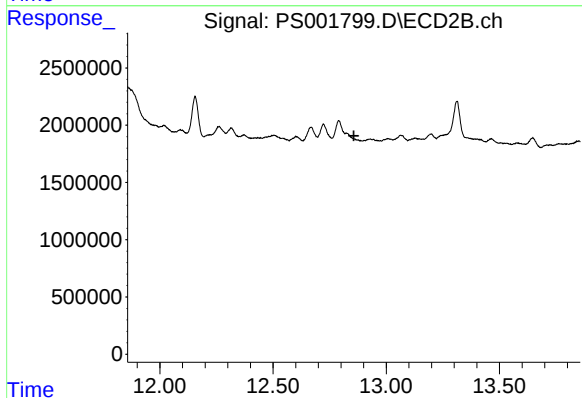


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.857 min
Response: 0
Conc: N.D.

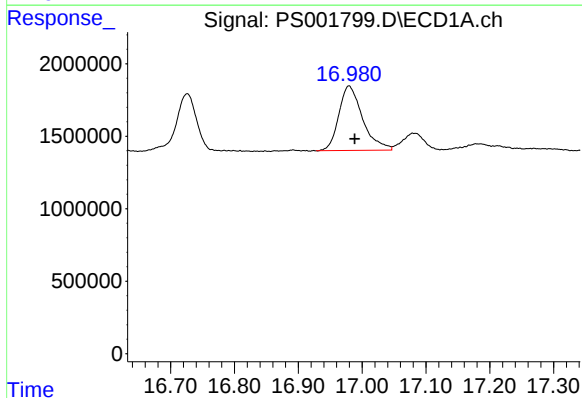


#15 Picloram

R.T.: 16.979 min
Delta R.T.: -0.009 min
Response: 11528841
Conc: 6.62 ng/ml

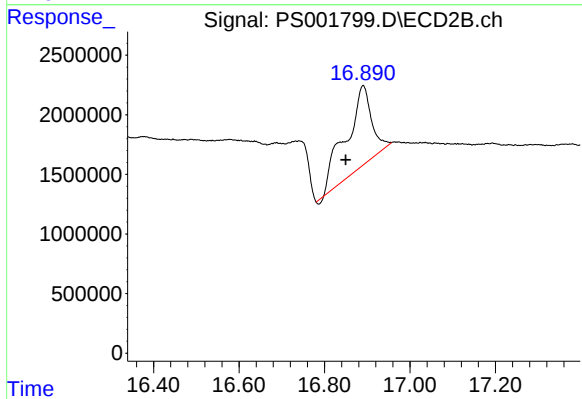

#15 Picloram


R.T.: 16.890 min
Delta R.T.: 0.040 min
Response: 28029038
Conc: 16.48 ng/ml

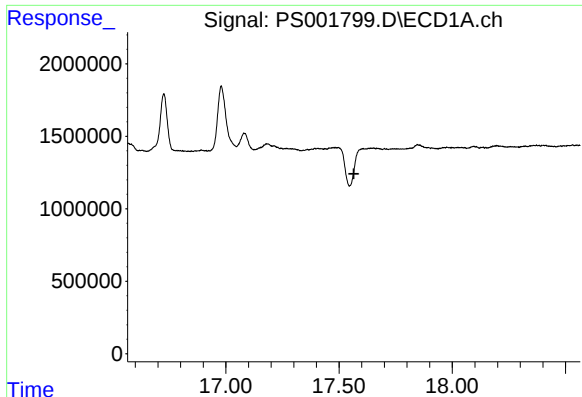

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

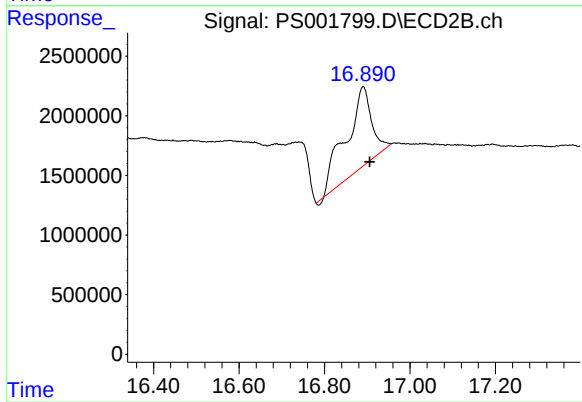

#16 DCPA

R.T.: 16.890 min
Delta R.T.: -0.016 min
Response: 28029038
Conc: 15.20 ng/ml