

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
 Data File : PS001811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2018 21:11
 Operator : EI\SJ
 Sample : J4777-22
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:30:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.487	10.985	59115778	59066158	263.538	232.529
Target Compounds							
1) T	Dalapon	2.918	2.400	30409246	31463449	93.519	106.505
2) T	3,5-DICHL...	0.000	9.076	0	4108525	N.D.	13.017 #
5) T	DICAMBA	0.000	11.228	0	27455974	N.D.	30.784 #
6) T	MCP	12.174	0.000	23096330	0	36.245	N.D. #
7) T	MCPA	0.000	11.792	0	8033047	N.D.	9.267 #
9) T	2,4-D	0.000	12.820	0	5408369	N.D.	17.384 #
11) T	2,4,5-TP ...	0.000	13.956	0	1971038	N.D.	1.438 #
15) T	Picloram	0.000	16.918	0	5085349	N.D.	2.990 #
16) T	DCPA	0.000	16.918	0	5085349	N.D.	2.757 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
Data File : PS001811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2018 21:11
Operator : EI\SJ
Sample : J4777-22
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:30:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

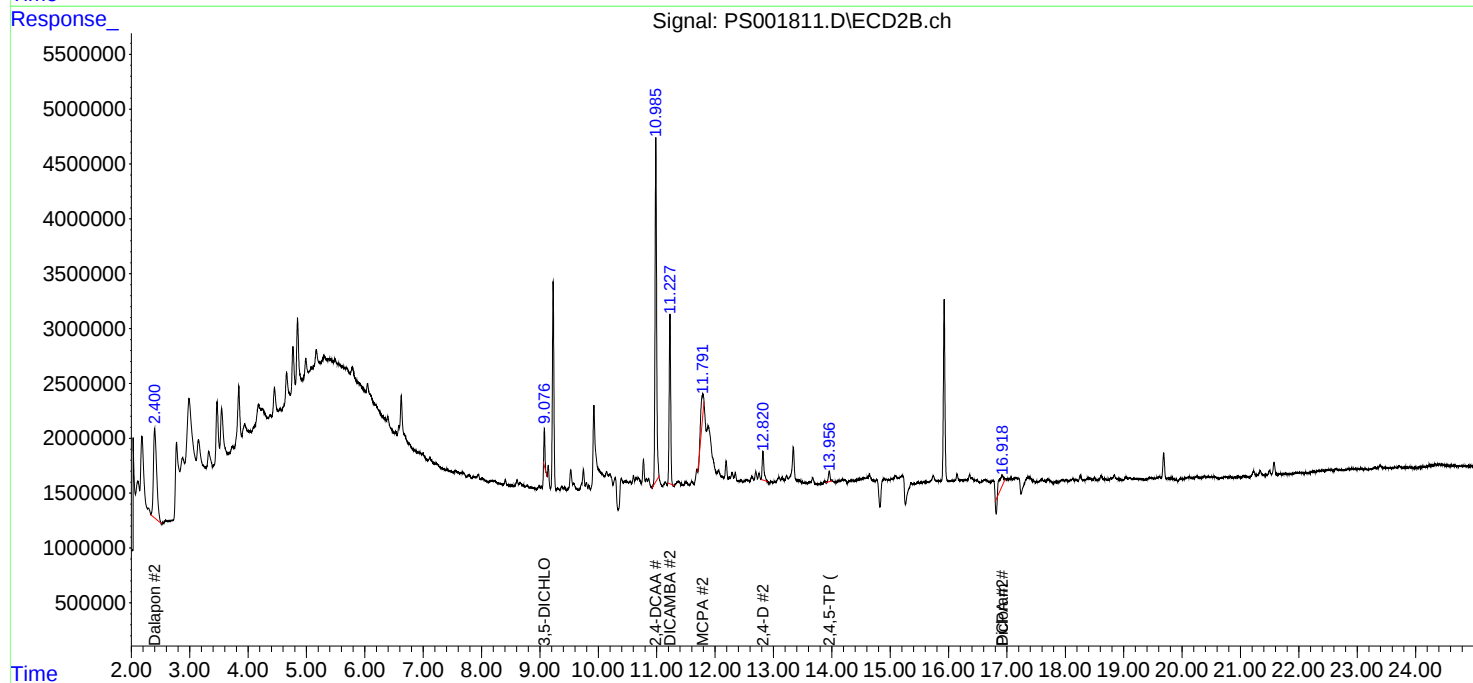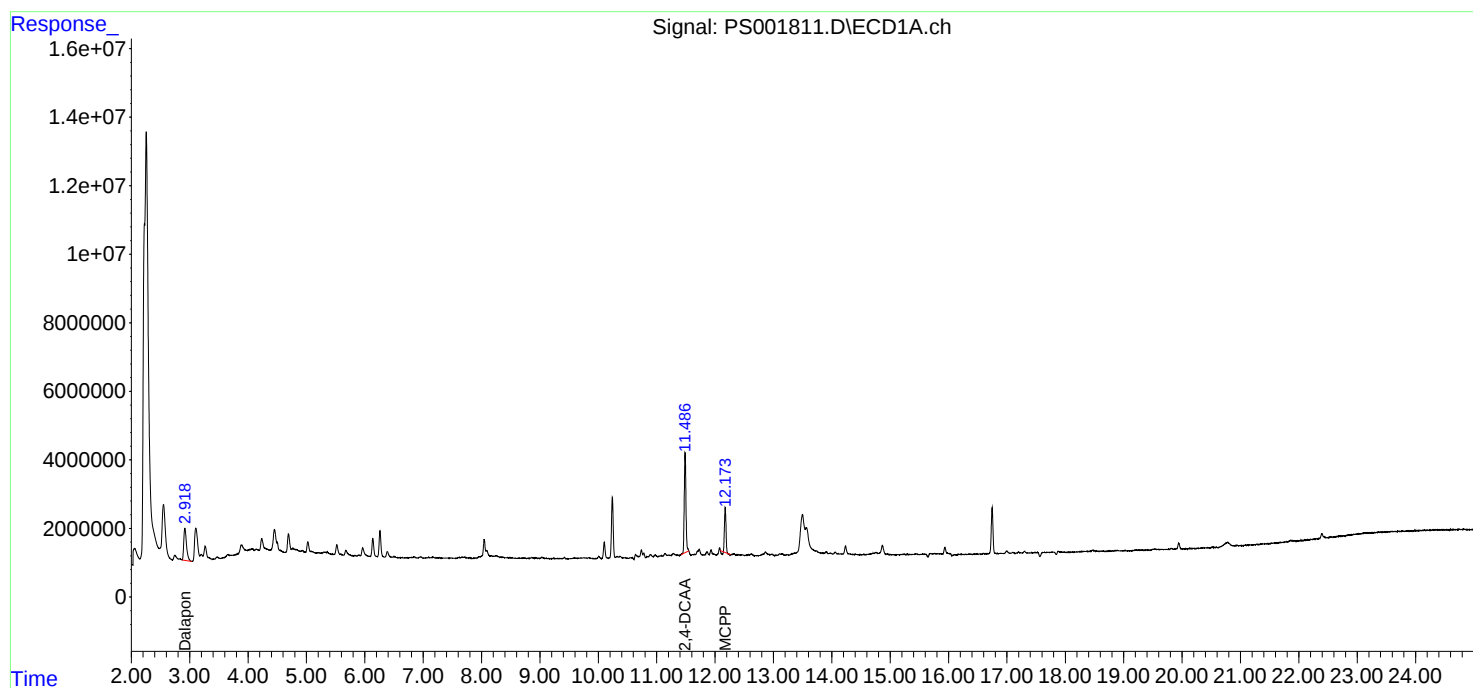


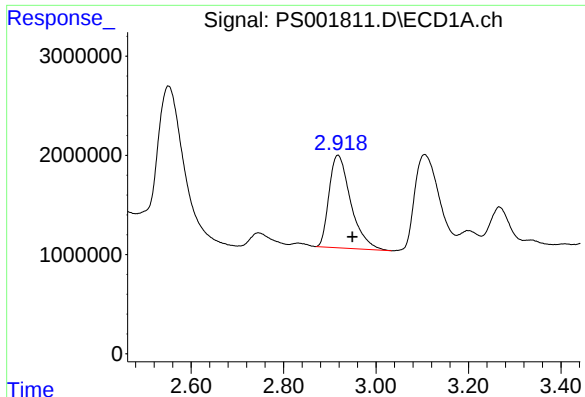

#1 Dalapon


R.T.: 2.918 min
Delta R.T.: -0.031 min
Response: 30409246
Conc: 93.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

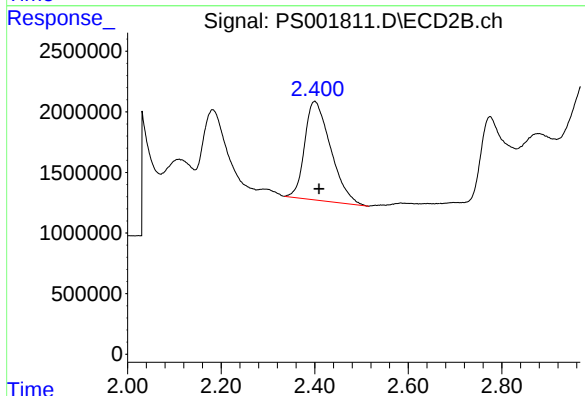


#1 Dalapon

R.T.: 2.400 min
Delta R.T.: -0.009 min
Response: 31463449
Conc: 106.51 ng/ml

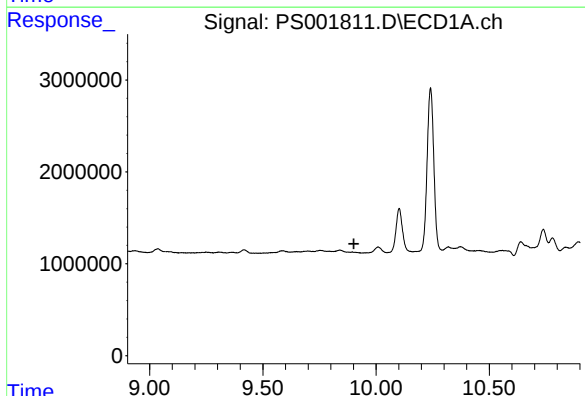


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

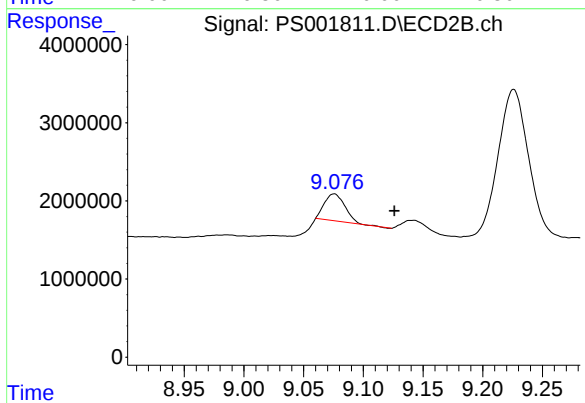

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.076 min
Delta R.T.: -0.050 min
Response: 4108525
Conc: 13.02 ng/ml

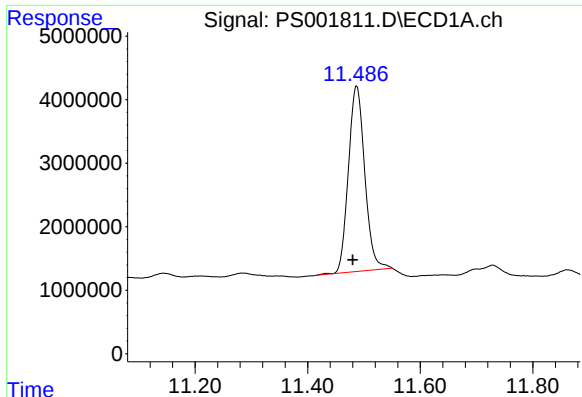

#4 2,4-DCAA


R.T.: 11.487 min
Delta R.T.: 0.007 min
Response: 59115778
Conc: 263.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

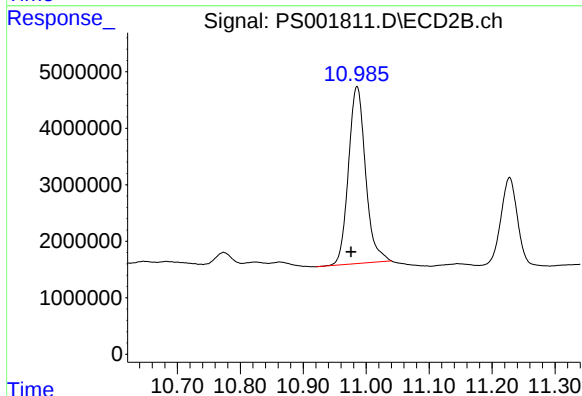


#4 2,4-DCAA

R.T.: 10.985 min
Delta R.T.: 0.009 min
Response: 59066158
Conc: 232.53 ng/ml

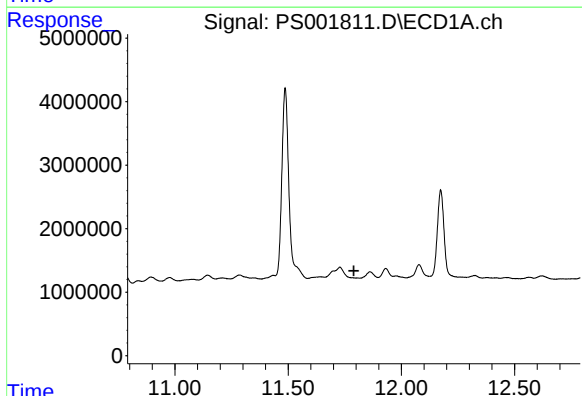


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.790 min
Response: 0
Conc: N.D.

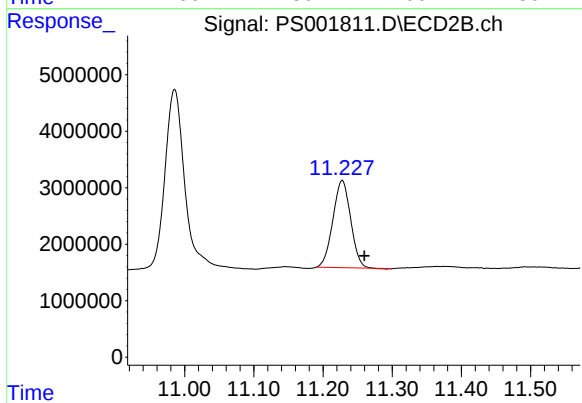

#5 DICAMBA


R.T.: 11.228 min
Delta R.T.: -0.032 min
Response: 27455974
Conc: 30.78 ng/ml

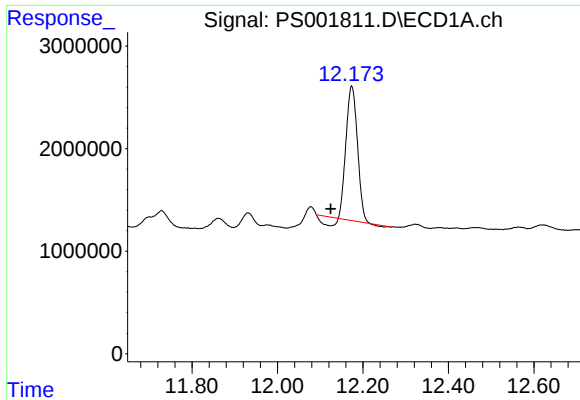

#6 MCPP


R.T.: 12.174 min
Delta R.T.: 0.049 min
Response: 23096330
Conc: 36.24 ug/ml

Instrument :
ECD_S
ClientSampleId :

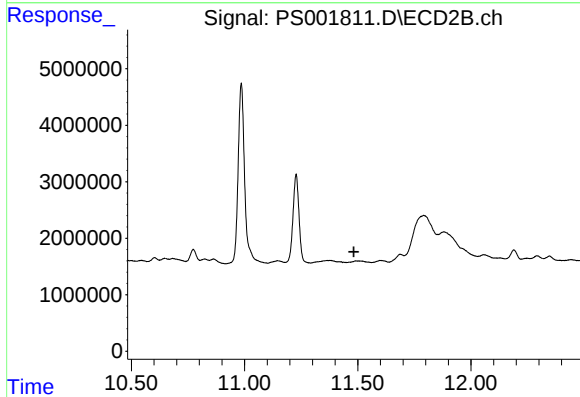


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

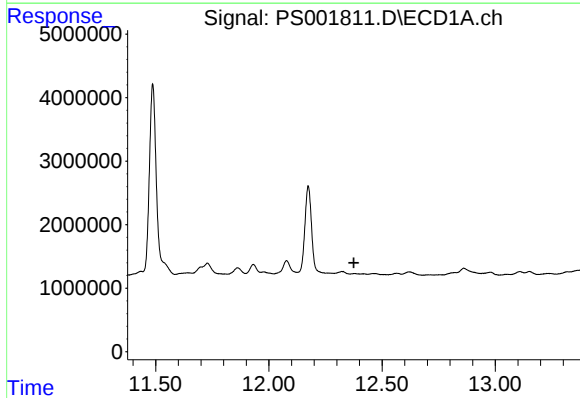


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.375 min
Response: 0
Conc: N.D.

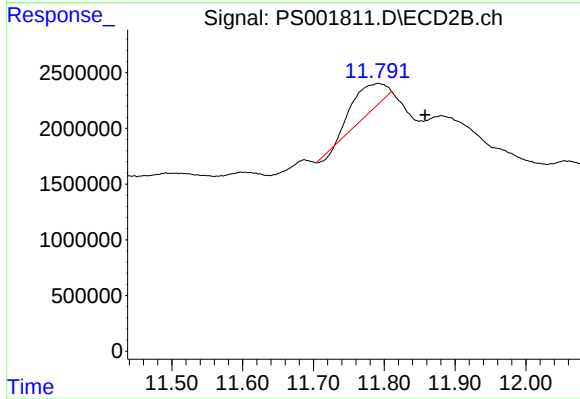

#7 MCPA


R.T.: 11.792 min
Delta R.T.: -0.066 min
Response: 8033047
Conc: 9.27 ug/ml

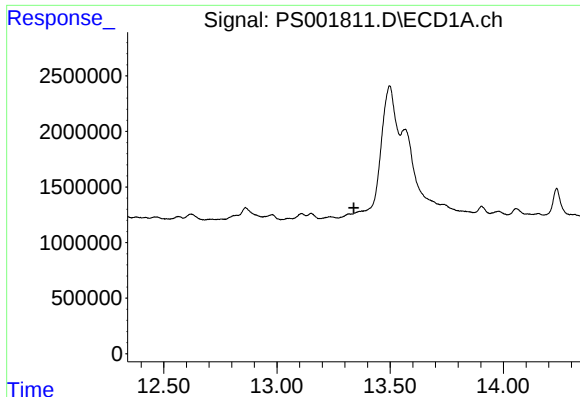

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

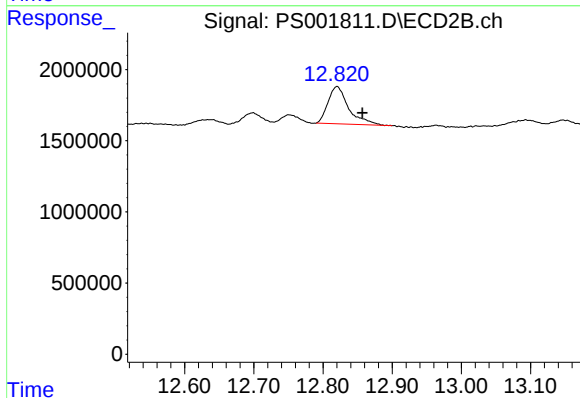


#9 2,4-D

R.T.: 12.820 min
Delta R.T.: -0.037 min
Response: 5408369
Conc: 17.38 ng/ml

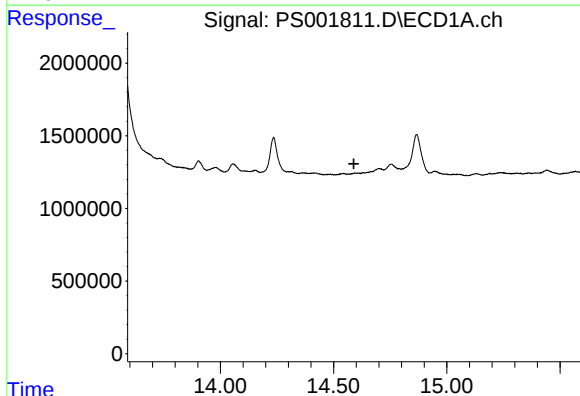


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.590 min
Response: 0
Conc: N.D.

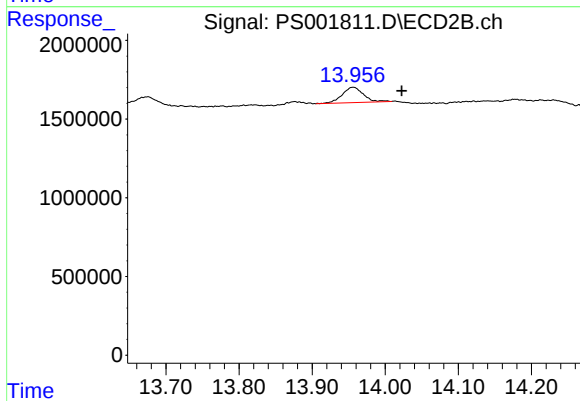

#11 2,4,5-TP (SILVEX)


R.T.: 13.956 min
Delta R.T.: -0.067 min
Response: 1971038
Conc: 1.44 ng/ml

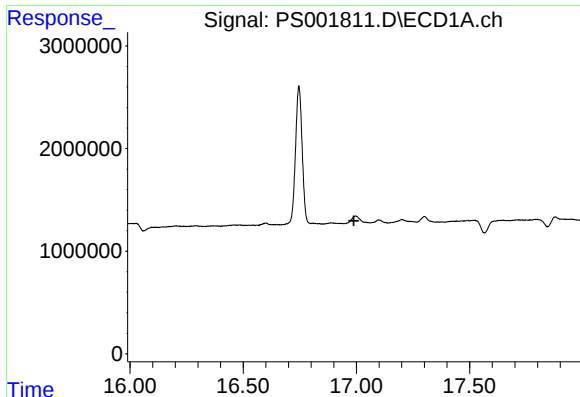

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

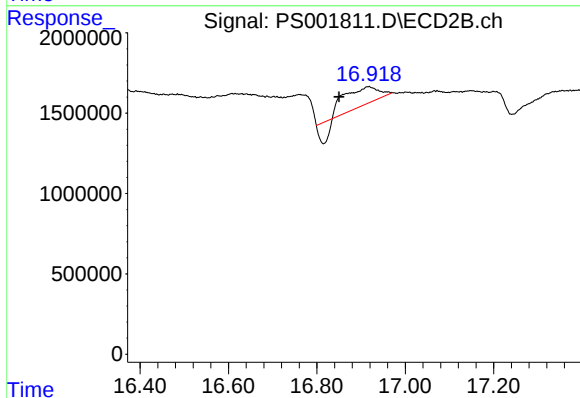


#15 Picloram

R.T.: 16.918 min
Delta R.T.: 0.068 min
Response: 5085349
Conc: 2.99 ng/ml

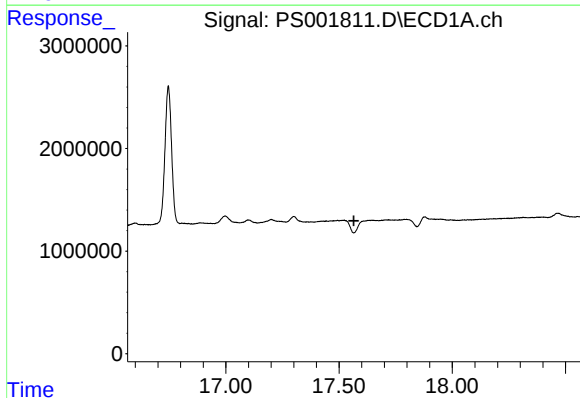

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

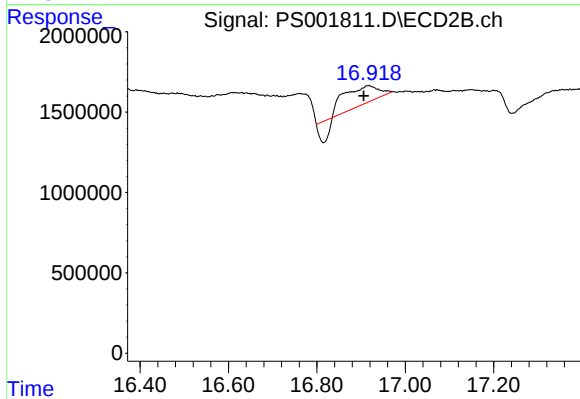

#16 DCPA

R.T.: 16.918 min
Delta R.T.: 0.012 min
Response: 5085349
Conc: 2.76 ng/ml